

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112118\
 Data File : P0051705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2018 12:08
 Operator : SM/SJ
 Sample : J5981-05RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DTW-03(8-10)RE

Manual Integrations
 APPROVED

mohammad
 11/23/2018 11:40:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:45:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 21 00:55:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.321	8750926	3148712	11.625m	13.155m
2) SA Decachlor...	9.937	8.043	1708095	864093	3.682	3.997

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112118\
Data File : PO051705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2018 12:08
Operator : SM/SJ
Sample : J5981-05RE
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DTW-03(8-10)RE


Manual Integrations
APPROVED

mohammad
11/23/2018 11:40:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:45:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 21 00:55:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

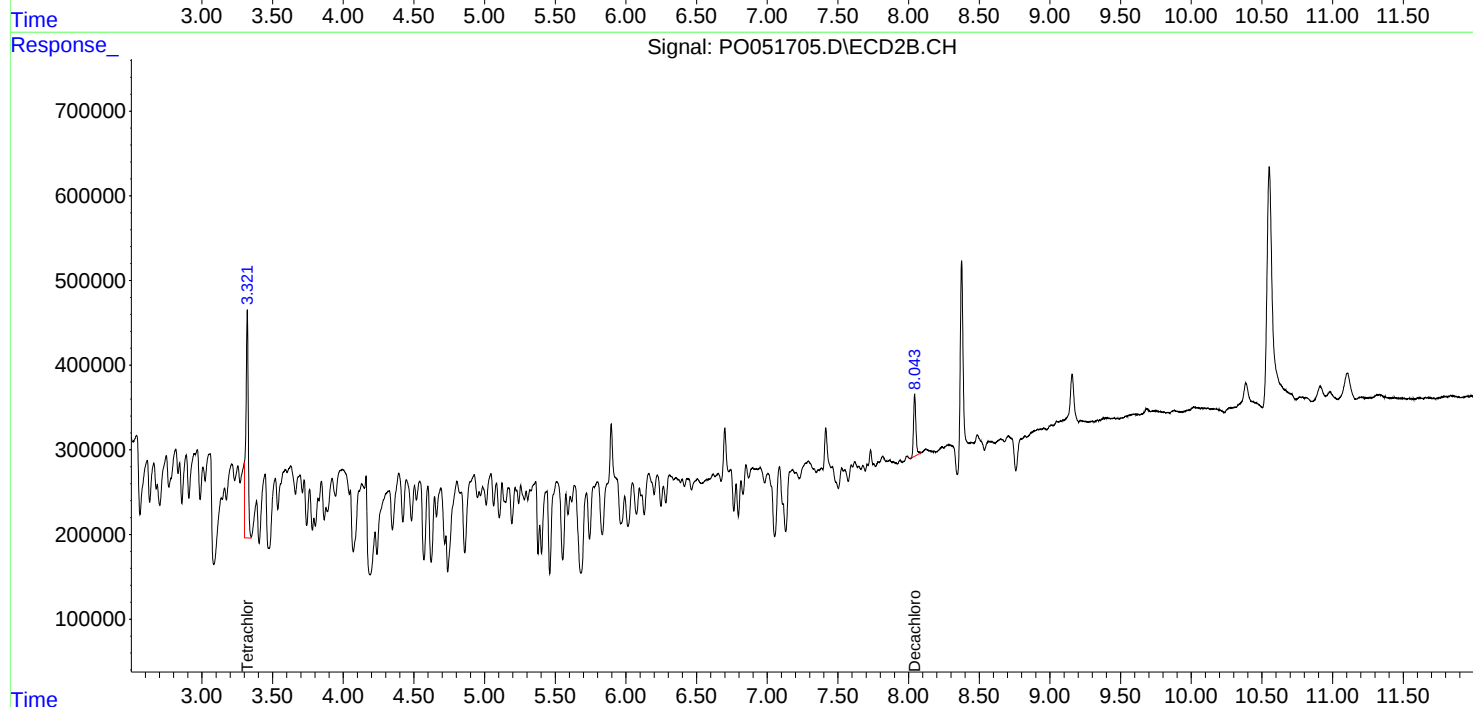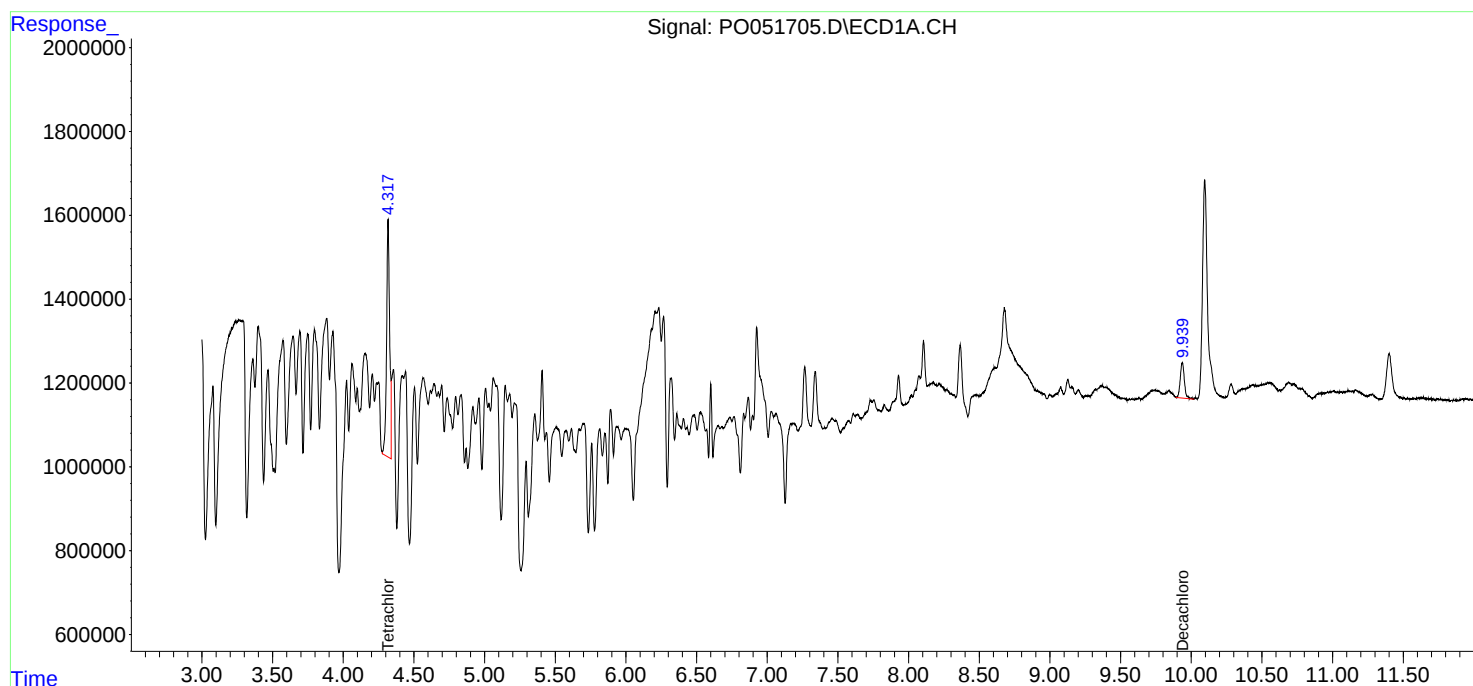

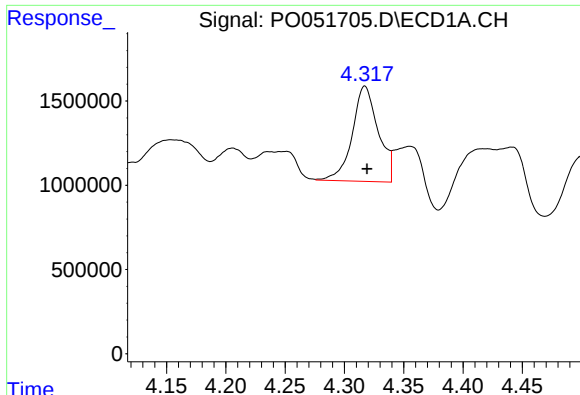


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: -0.002 min
Response: 8750926
Conc: 11.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DTW-03(8-10)RE


Manual Integrations
APPROVED

mohammad
11/23/2018 11:40:15 AM

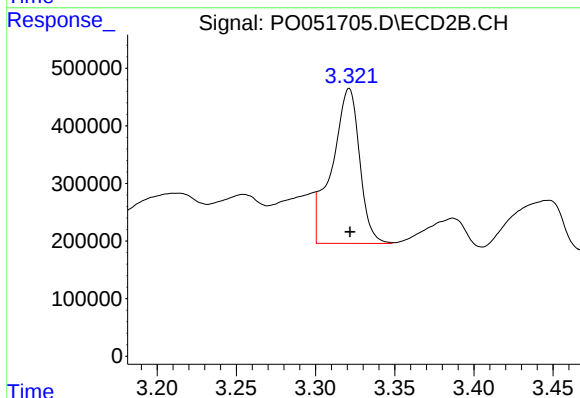


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: 0.000 min
Response: 3148712
Conc: 13.15 ng/ml m

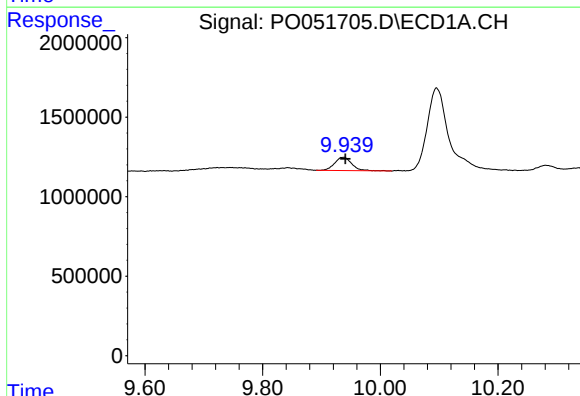

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.004 min
Response: 1708095
Conc: 3.68 ng/ml

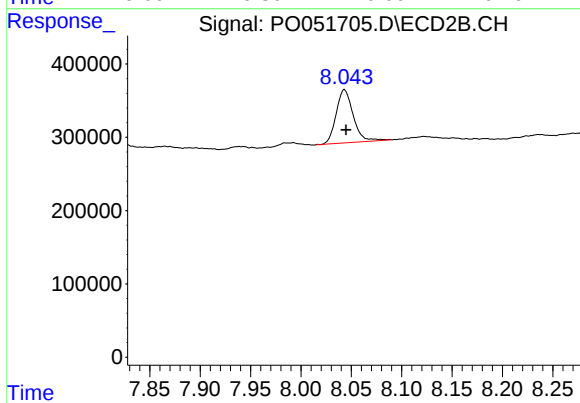

#2 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.002 min
Response: 864093
Conc: 4.00 ng/ml