

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112118\
 Data File : P0051727.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2018 19:05
 Operator : SM/SJ
 Sample : J6023-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 111918-JETT-E-D-S

Manual Integrations
 APPROVED

mohammad
 11/23/2018 11:40:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:56:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 21 00:55:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.310	3.313	19764531	6533321	26.255	27.295
2) SA Decachlor...	9.931	8.038	16947442	7744702	36.534	35.826m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112118\
Data File : PO051727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2018 19:05
Operator : SM/SJ
Sample : J6023-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
111918-JETT-E-D-S


Manual Integrations
APPROVED

mohammad
11/23/2018 11:40:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:56:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 21 00:55:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

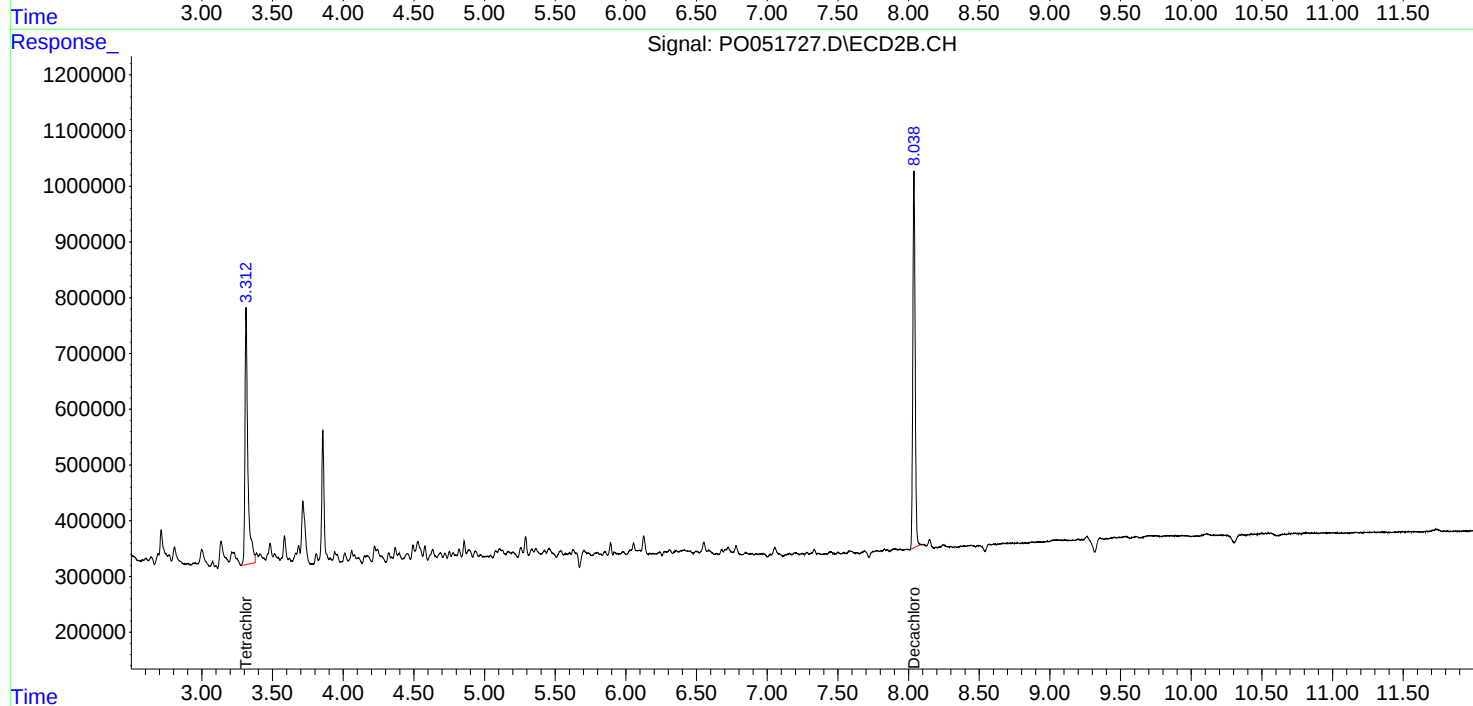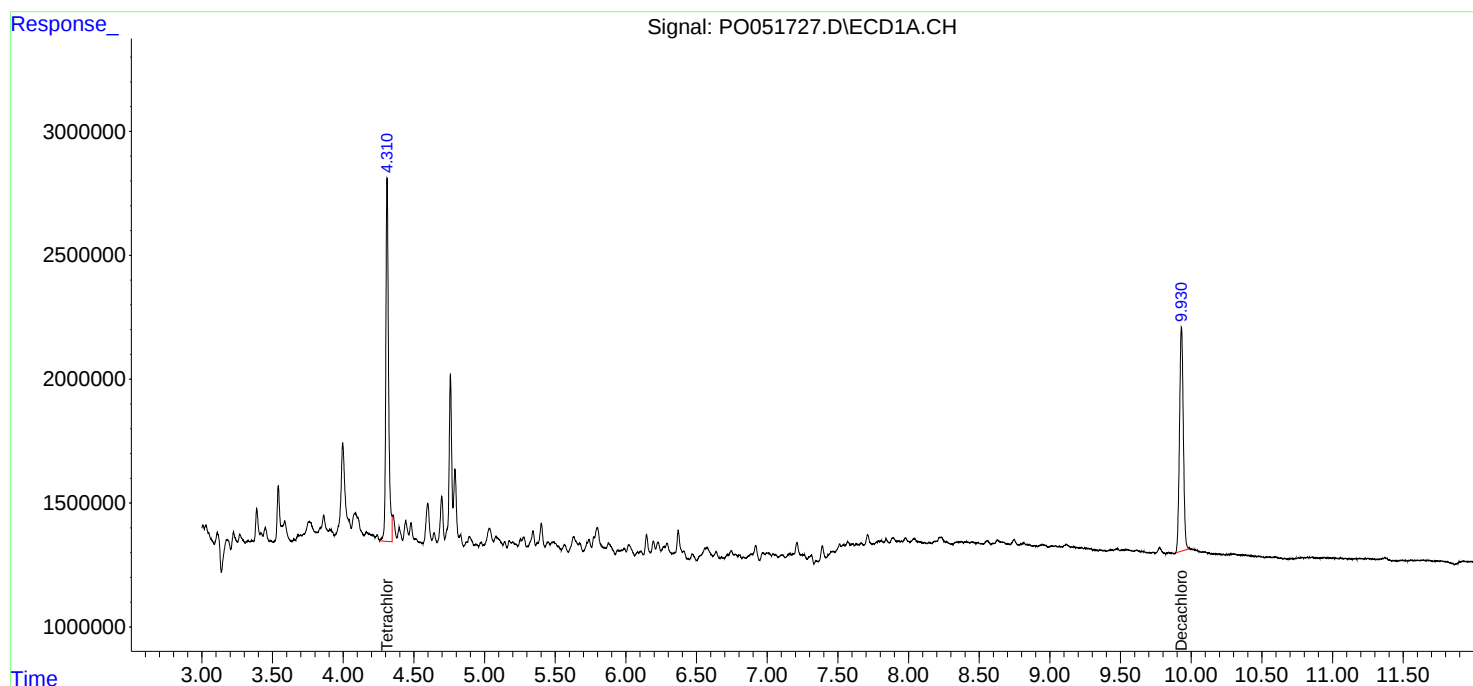

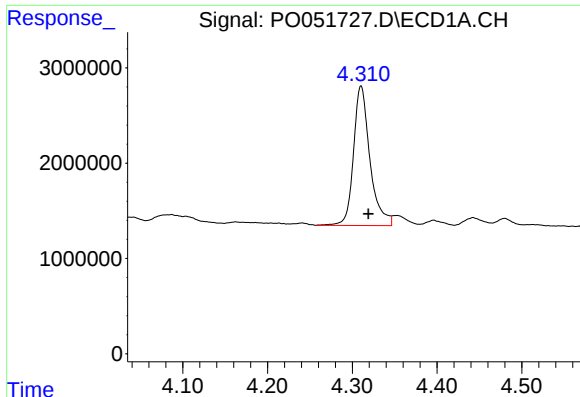


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: -0.009 min
Response: 19764531
Conc: 26.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
111918-JETT-E-D-S


Manual Integrations
APPROVED

mohammad
11/23/2018 11:40:39 AM

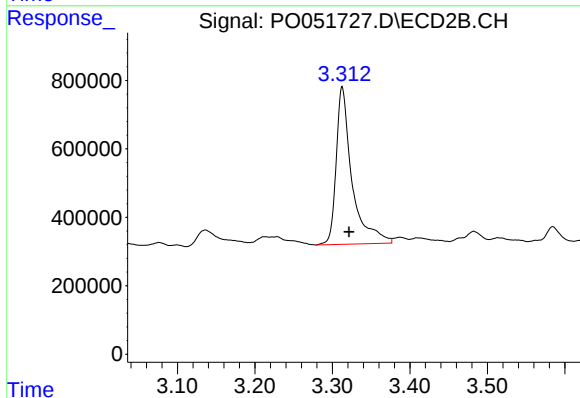


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.009 min
Response: 6533321
Conc: 27.29 ng/ml

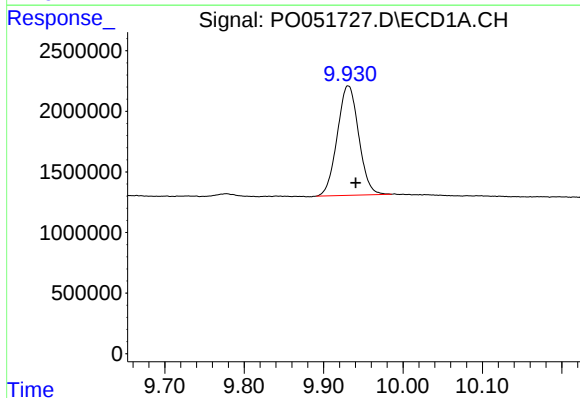

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.010 min
Response: 16947442
Conc: 36.53 ng/ml

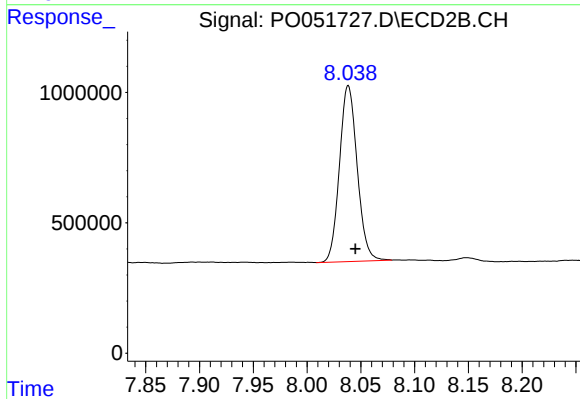

#2 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.007 min
Response: 7744702
Conc: 35.83 ng/ml m