

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063972.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2019 20:25
 Operator : SM/AJ
 Sample : K5955-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:47:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.566	783810	607322	25.636	27.343
2)	SA Decachlor...	9.939	8.533	837334	676727	20.606	23.138
Target Compounds							
3)	L1 AR-1016-1	5.476	4.643	258760	185482	186.318	180.998
4)	L1 AR-1016-2	5.498	4.662	384777	274934	196.041	201.792
5)	L1 AR-1016-3	5.559	4.836	272545	171284	218.181	230.028
6)	L1 AR-1016-4	5.658	4.877	248657	111014	241.763	178.191 #
7)	L1 AR-1016-5	5.949	5.089	249024	144794	234.027	182.308
9)	L2 AR-1221-2	4.617	3.863	21508	12959	68.571	61.632
10)	L2 AR-1221-3	4.684	3.938	46901	28648	49.449	42.976
11)	L3 AR-1232-1	4.684	3.938	46901	28648	35.262	30.391
12)	L3 AR-1232-2	5.209	4.662	162572	274934	227.972	272.839
13)	L3 AR-1232-3	5.498	4.836	384777	171284	268.930	323.609
14)	L3 AR-1232-4	5.658	4.918	248657	136846	334.952	291.474
15)	L3 AR-1232-5	5.746	5.089	184780	144794	315.225	280.881
16)	L4 AR-1242-1	5.476	4.643	258760	185482	244.570	235.135
17)	L4 AR-1242-2	5.498	4.662	384777	274934	256.529	259.711
18)	L4 AR-1242-3	5.559	4.836	272545	171284	285.195	298.961
19)	L4 AR-1242-4	5.658	4.918	248657	136846	316.608	239.682
20)	L4 AR-1242-5	6.389	5.439	439425	309978	422.871	398.251
21)	L5 AR-1248-1	5.476	4.643	258760	185482	296.292	287.839
22)	L5 AR-1248-2	5.746	4.877	184780	111014	145.835	128.804
23)	L5 AR-1248-3	5.949	4.918	249024	136846	174.564	154.672
24)	L5 AR-1248-4	6.351	5.089	347633	144794	200.840	134.499 #
25)	L5 AR-1248-5	6.389	5.480	439425	246855	260.531	221.324
26)	L6 AR-1254-1	6.324	5.439	297586	309978	170.339	174.953
27)	L6 AR-1254-2	6.545	5.585	483741	117559	173.526	74.558 #
28)	L6 AR-1254-3	6.908	5.988	428359	229914	136.445	85.744 #
29)	L6 AR-1254-4	7.191	6.214	169359	78502	68.494	44.268 #
30)	L6 AR-1254-5	7.607	6.631	187326	145928	69.109	58.401
31)	L7 AR-1260-1	7.069	6.117	400453	185429	198.430	118.077 #
32)	L7 AR-1260-2	7.324	6.303	228542	134652	90.713	68.451
33)	L7 AR-1260-3	7.682	6.458	84915	127738	41.909	71.623 #
34)	L7 AR-1260-4	7.906	6.928	138113	61206	57.995	38.874 #
35)	L7 AR-1260-5	8.217	7.168	214805	130506	45.759	33.662 #
36)	L8 AR-1262-1	7.682	6.721	84915	40995	26.375	39.210 #
37)	L8 AR-1262-2	8.217	7.168	214805	130506	36.461	27.514
38)	L8 AR-1262-3	8.528	7.451	43114	92493	10.522	49.350 #
39)	L8 AR-1262-4	8.604	7.514	67103	166614	21.457	47.193 #
40)	L8 AR-1262-5	9.190	8.006	255198	8086	117.151	5.296 #
41)	L9 AR-1268-1	8.528	7.451	43114	92493	6.378	17.326 #
42)	L9 AR-1268-2	8.604	7.514	67103	166614	10.694	33.434 #
43)	L9 AR-1268-3	8.871	0.000	31889	0	6.143	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063972.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2019 20:25
 Operator : SM/AJ
 Sample : K5955-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:47:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.190	8.006	255198	8086	104.985	4.773 #
45) L9	AR-1268-5	9.622	8.284	13137	150306	0.854	12.708 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063972.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2019 20:25
Operator : SM/AJ
Sample : K5955-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:47:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

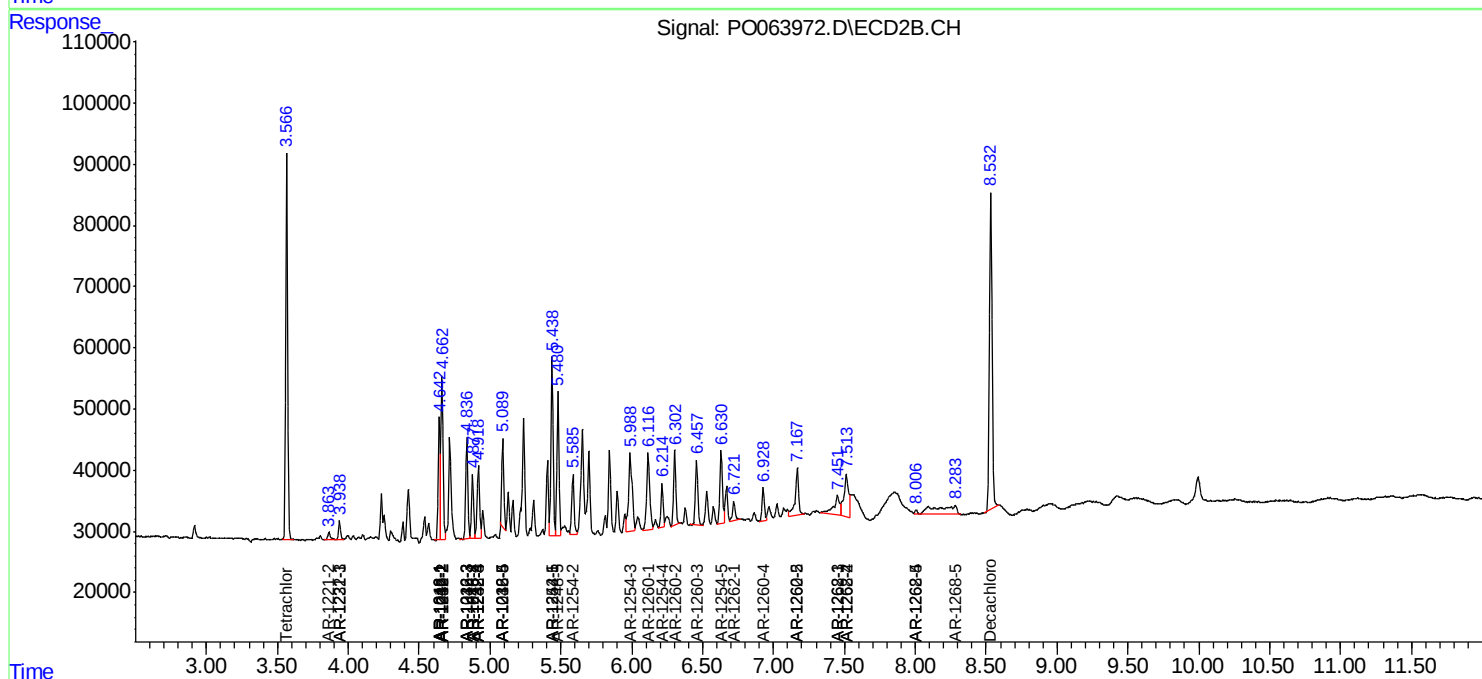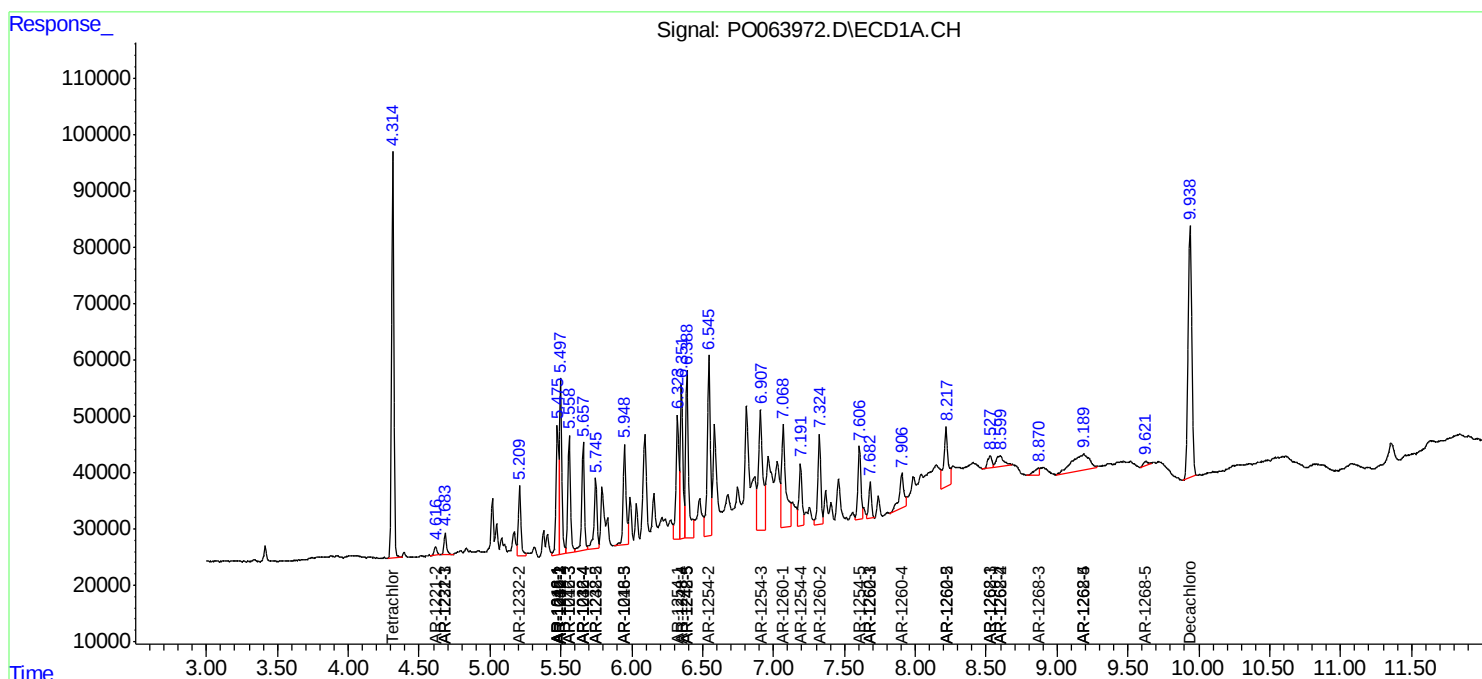


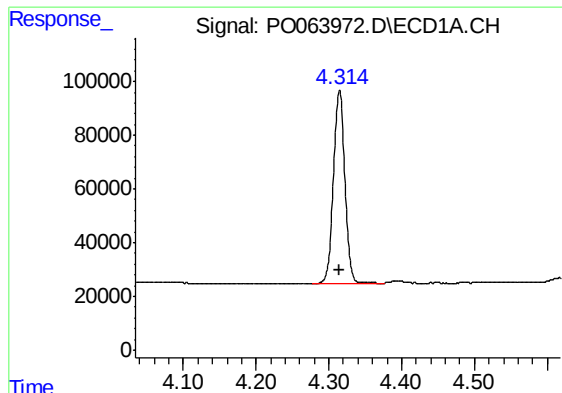

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.000 min
Response: 783810
Conc: 25.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

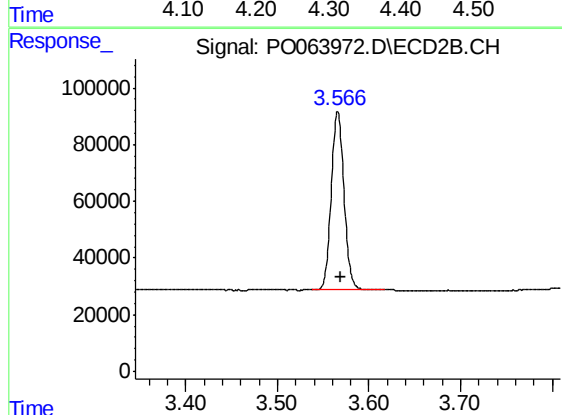


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 607322
Conc: 27.34 ng/ml

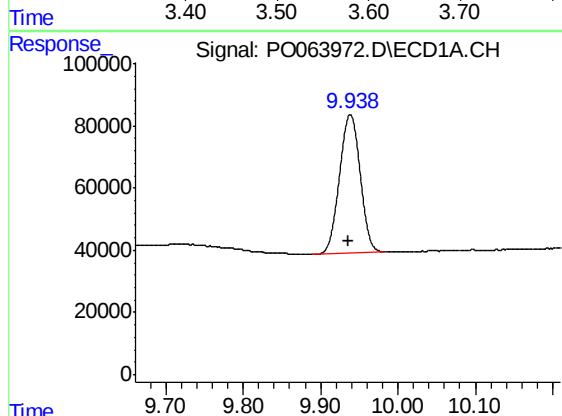


#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: 0.003 min
Response: 837334
Conc: 20.61 ng/ml

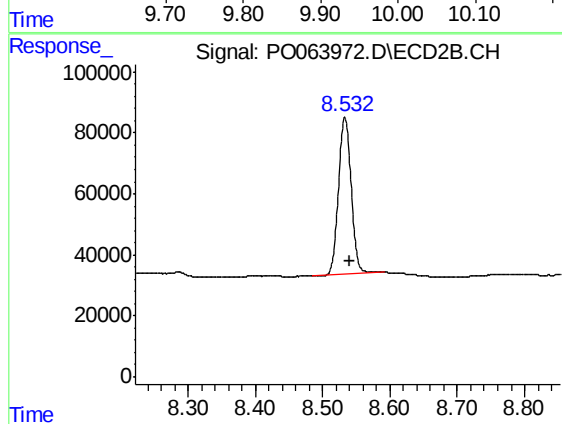

#2 Decachlorobiphenyl


R.T.: 8.533 min
Delta R.T.: -0.007 min
Response: 676727
Conc: 23.14 ng/ml

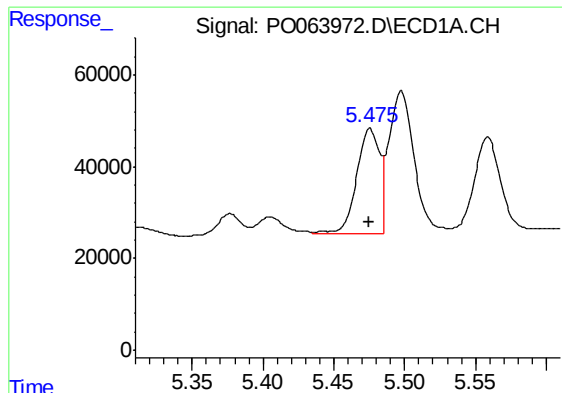

#3 AR-1016-1


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 258760
Conc: 186.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

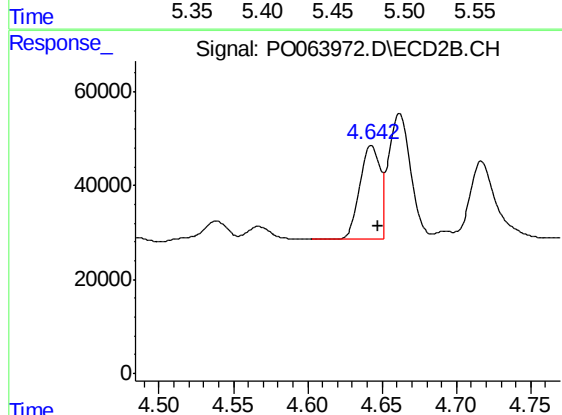


#3 AR-1016-1

R.T.: 4.643 min
Delta R.T.: -0.005 min
Response: 185482
Conc: 181.00 ng/ml

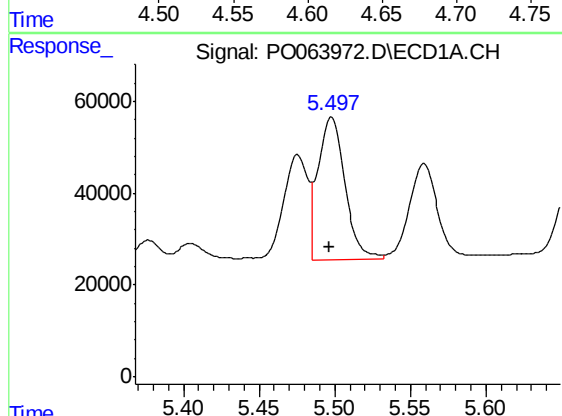


#4 AR-1016-2

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 384777
Conc: 196.04 ng/ml

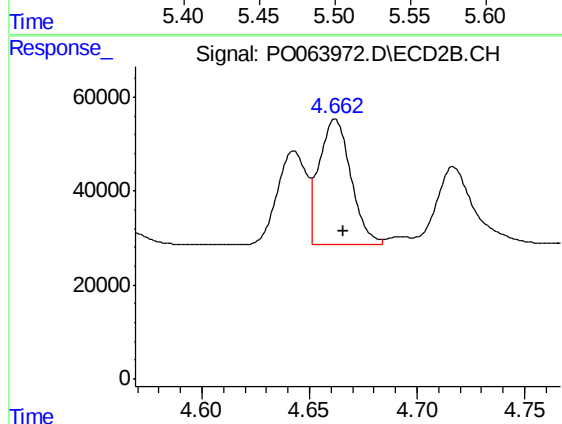

#4 AR-1016-2


R.T.: 4.662 min
Delta R.T.: -0.004 min
Response: 274934
Conc: 201.79 ng/ml



#5 AR-1016-3


R.T.: 5.559 min
Delta R.T.: 0.000 min
Response: 272545
Conc: 218.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

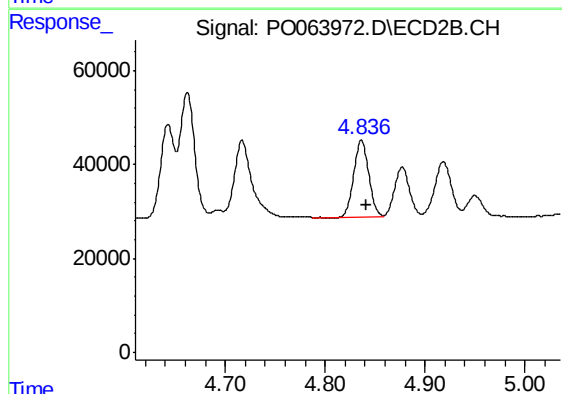


#5 AR-1016-3

R.T.: 4.836 min
Delta R.T.: -0.004 min
Response: 171284
Conc: 230.03 ng/ml

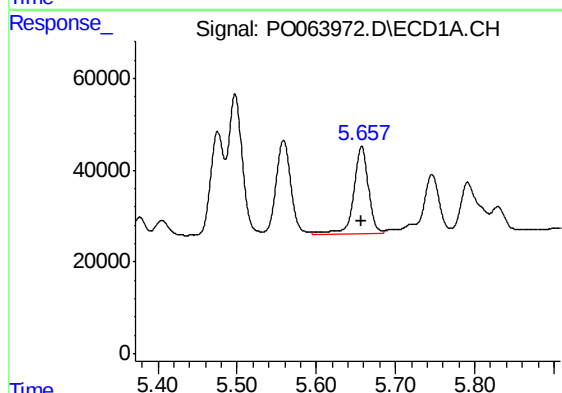


#6 AR-1016-4

R.T.: 5.658 min
Delta R.T.: 0.001 min
Response: 248657
Conc: 241.76 ng/ml

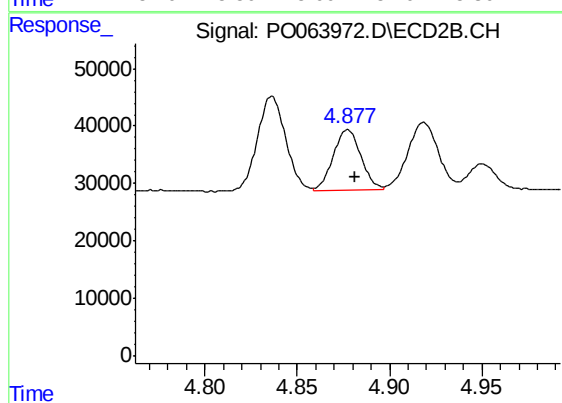

#6 AR-1016-4


R.T.: 4.877 min
Delta R.T.: -0.004 min
Response: 111014
Conc: 178.19 ng/ml



#7 AR-1016-5


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 249024
Conc: 234.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

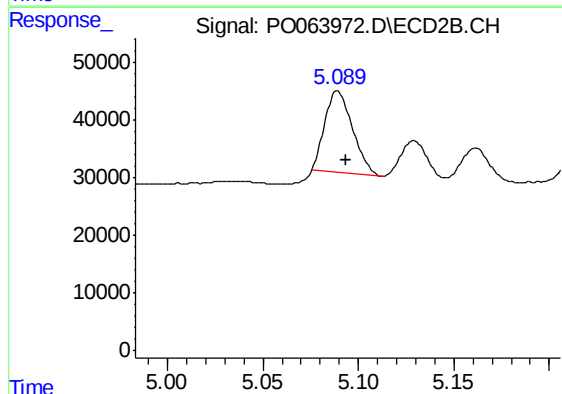


#7 AR-1016-5

R.T.: 5.089 min
Delta R.T.: -0.005 min
Response: 144794
Conc: 182.31 ng/ml




#9 AR-1221-2

R.T.: 4.617 min
Delta R.T.: 0.007 min
Response: 21508
Conc: 68.57 ng/ml

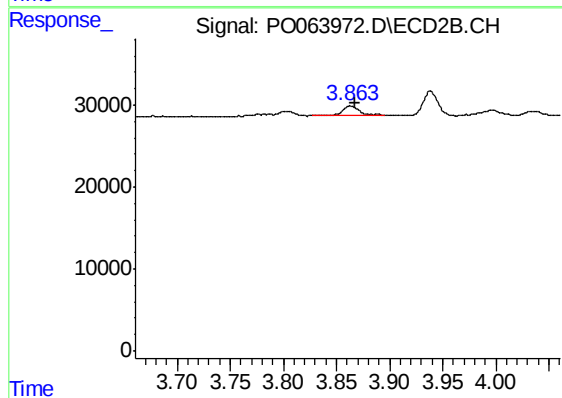

#9 AR-1221-2


R.T.: 3.863 min
Delta R.T.: -0.004 min
Response: 12959
Conc: 61.63 ng/ml



#10 AR-1221-3


R.T.: 4.684 min
Delta R.T.: -0.001 min
Response: 46901
Conc: 49.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

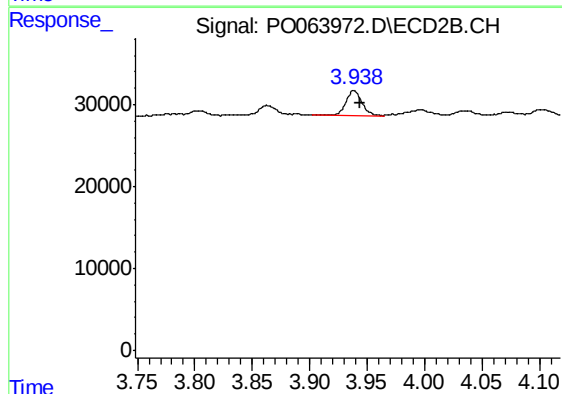


#10 AR-1221-3

R.T.: 3.938 min
Delta R.T.: -0.005 min
Response: 28648
Conc: 42.98 ng/ml




#11 AR-1232-1

R.T.: 4.684 min
Delta R.T.: -0.001 min
Response: 46901
Conc: 35.26 ng/ml

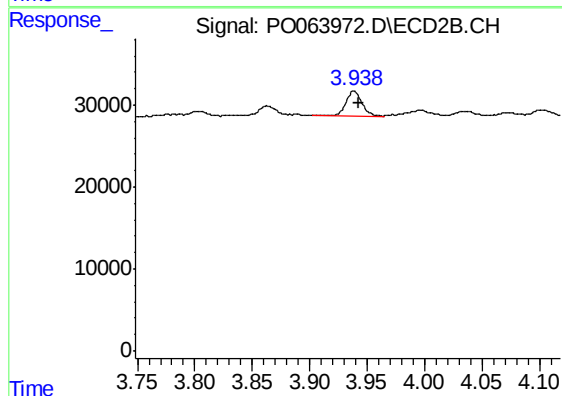

#11 AR-1232-1


R.T.: 3.938 min
Delta R.T.: -0.005 min
Response: 28648
Conc: 30.39 ng/ml

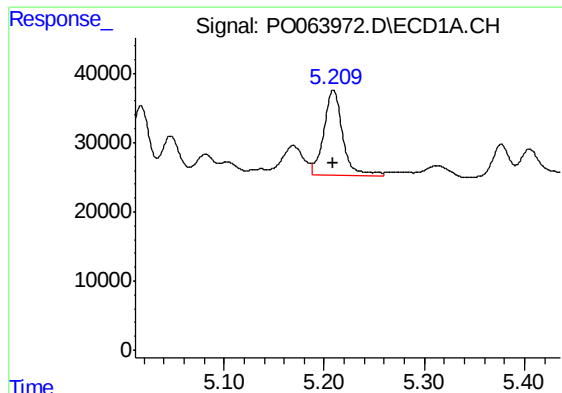

#12 AR-1232-2


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 162572
Conc: 227.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

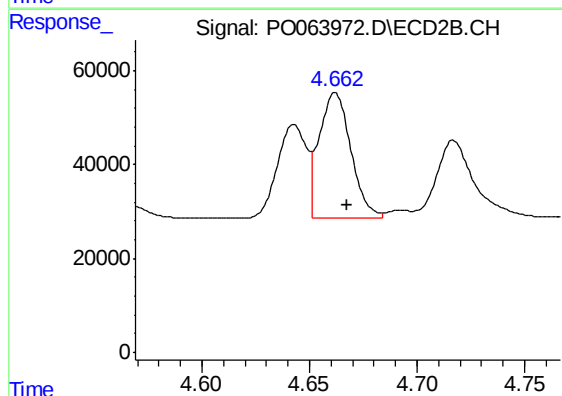


#12 AR-1232-2

R.T.: 4.662 min
Delta R.T.: -0.005 min
Response: 274934
Conc: 272.84 ng/ml

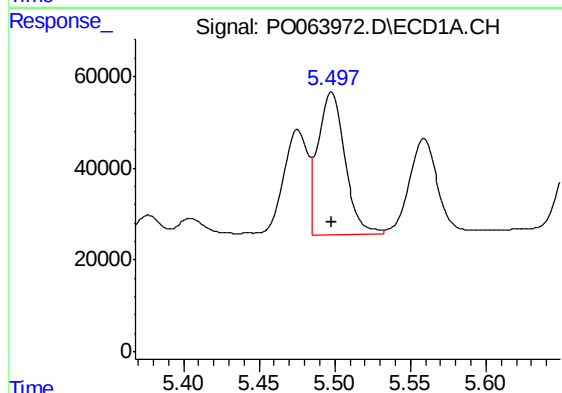


#13 AR-1232-3

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 384777
Conc: 268.93 ng/ml

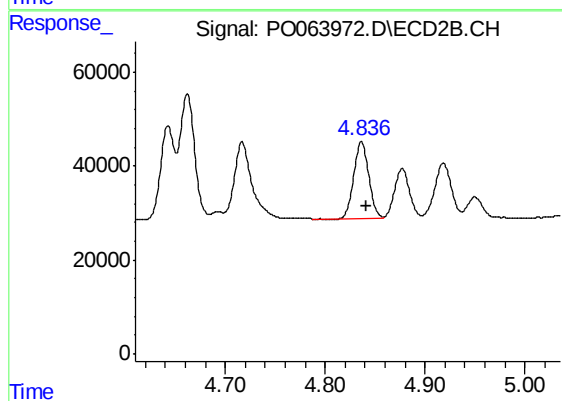

#13 AR-1232-3


R.T.: 4.836 min
Delta R.T.: -0.005 min
Response: 171284
Conc: 323.61 ng/ml

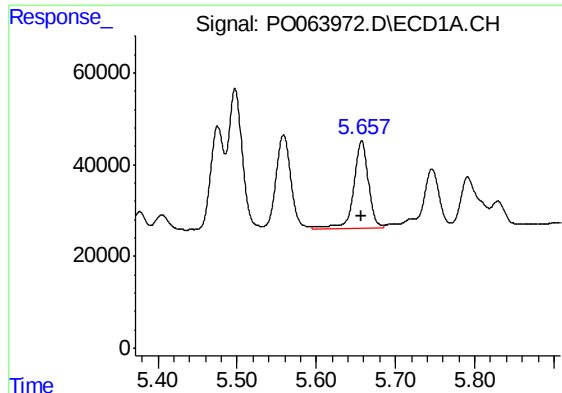

#14 AR-1232-4


R.T.: 5.658 min
Delta R.T.: 0.000 min
Response: 248657
Conc: 334.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

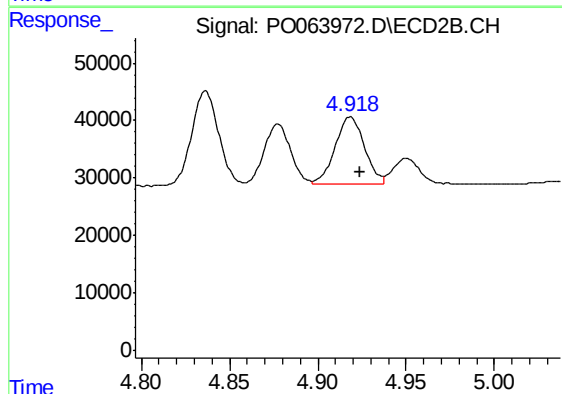


#14 AR-1232-4

R.T.: 4.918 min
Delta R.T.: -0.006 min
Response: 136846
Conc: 291.47 ng/ml

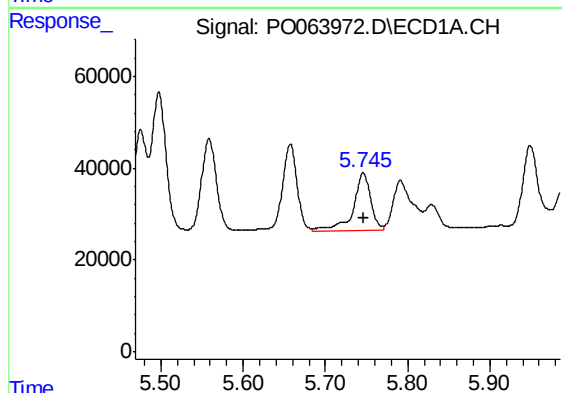


#15 AR-1232-5

R.T.: 5.746 min
Delta R.T.: -0.002 min
Response: 184780
Conc: 315.22 ng/ml

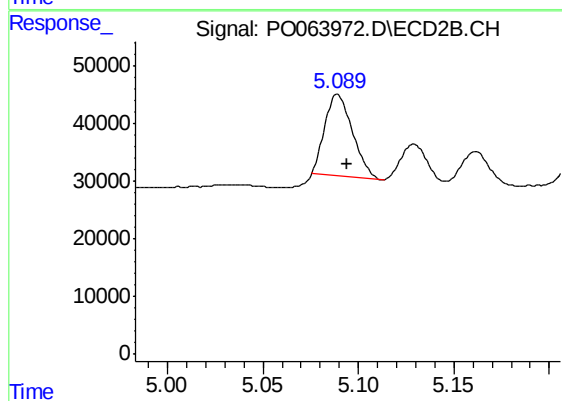

#15 AR-1232-5


R.T.: 5.089 min
Delta R.T.: -0.005 min
Response: 144794
Conc: 280.88 ng/ml



#16 AR-1242-1


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 258760
Conc: 244.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

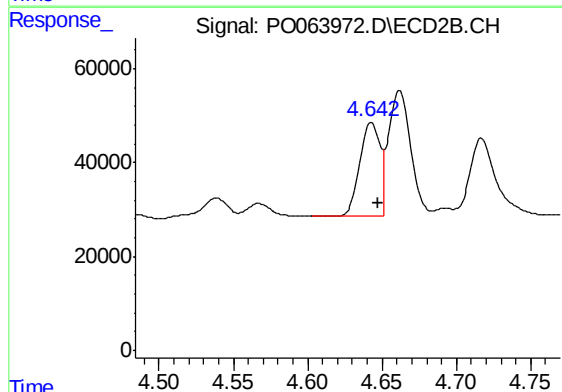


#16 AR-1242-1

R.T.: 4.643 min
Delta R.T.: -0.005 min
Response: 185482
Conc: 235.14 ng/ml




#17 AR-1242-2

R.T.: 5.498 min
Delta R.T.: 0.000 min
Response: 384777
Conc: 256.53 ng/ml

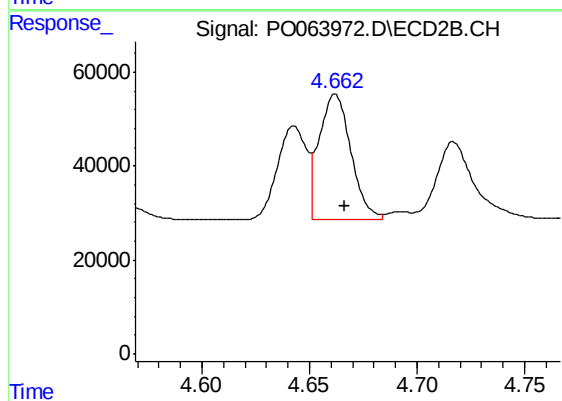

#17 AR-1242-2


R.T.: 4.662 min
Delta R.T.: -0.005 min
Response: 274934
Conc: 259.71 ng/ml



#18 AR-1242-3


R.T.: 5.559 min
Delta R.T.: 0.000 min
Response: 272545
Conc: 285.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

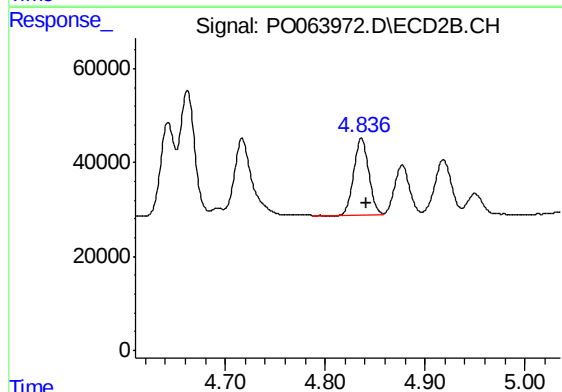


#18 AR-1242-3

R.T.: 4.836 min
Delta R.T.: -0.005 min
Response: 171284
Conc: 298.96 ng/ml




#19 AR-1242-4

R.T.: 5.658 min
Delta R.T.: 0.000 min
Response: 248657
Conc: 316.61 ng/ml

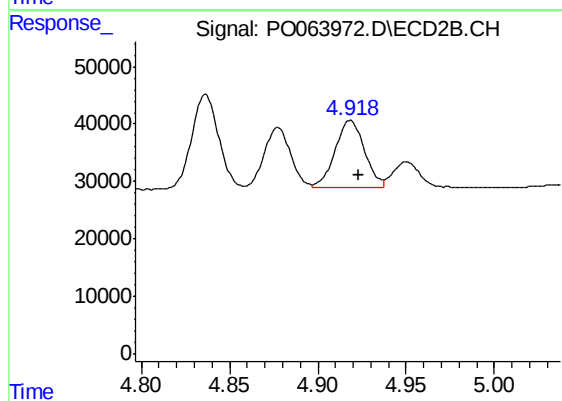

#19 AR-1242-4


R.T.: 4.918 min
Delta R.T.: -0.005 min
Response: 136846
Conc: 239.68 ng/ml

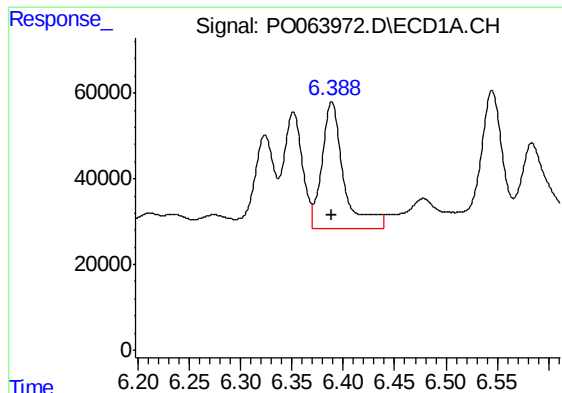

#20 AR-1242-5


R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 439425
Conc: 422.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

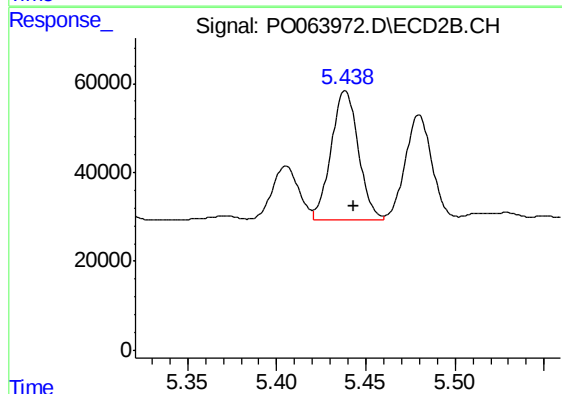


#20 AR-1242-5

R.T.: 5.439 min
Delta R.T.: -0.005 min
Response: 309978
Conc: 398.25 ng/ml




#21 AR-1248-1

R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 258760
Conc: 296.29 ng/ml

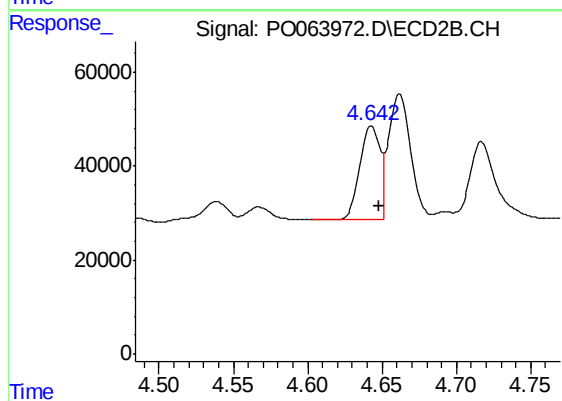

#21 AR-1248-1


R.T.: 4.643 min
Delta R.T.: -0.005 min
Response: 185482
Conc: 287.84 ng/ml



#22 AR-1248-2


R.T.: 5.746 min
Delta R.T.: -0.001 min
Response: 184780
Conc: 145.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

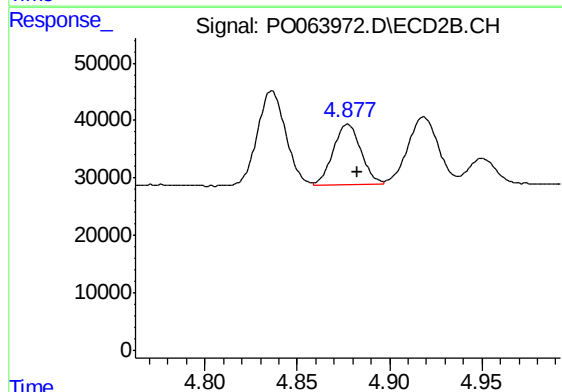


#22 AR-1248-2

R.T.: 4.877 min
Delta R.T.: -0.005 min
Response: 111014
Conc: 128.80 ng/ml




#23 AR-1248-3

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 249024
Conc: 174.56 ng/ml

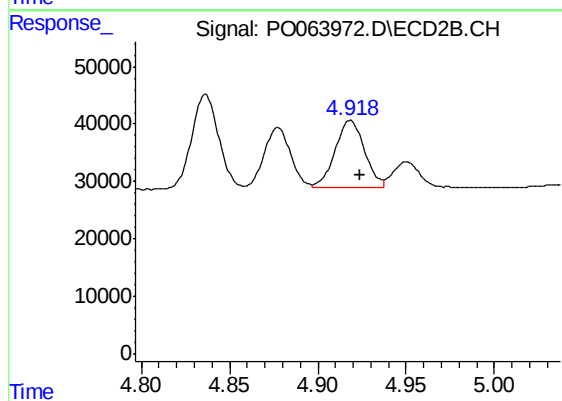

#23 AR-1248-3


R.T.: 4.918 min
Delta R.T.: -0.006 min
Response: 136846
Conc: 154.67 ng/ml



#24 AR-1248-4


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 347633
Conc: 200.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

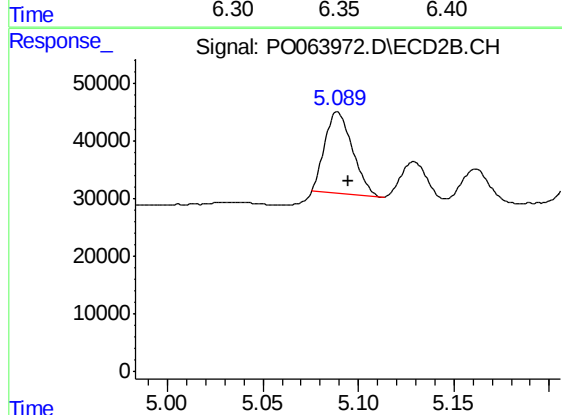


#24 AR-1248-4

R.T.: 5.089 min
Delta R.T.: -0.005 min
Response: 144794
Conc: 134.50 ng/ml

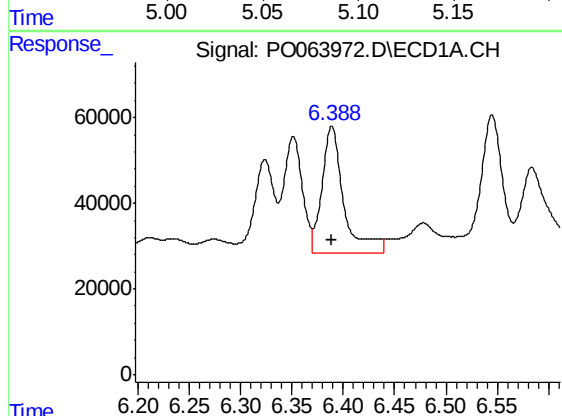


#25 AR-1248-5

R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 439425
Conc: 260.53 ng/ml

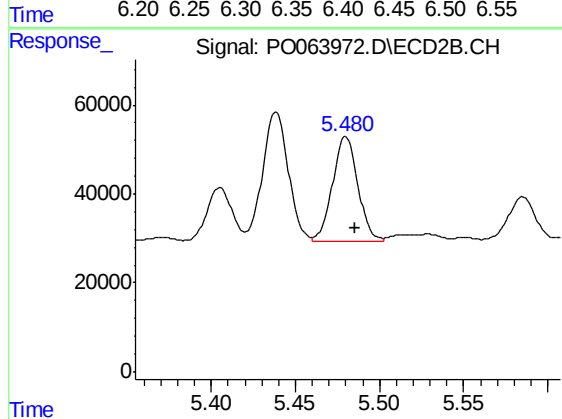

#25 AR-1248-5


R.T.: 5.480 min
Delta R.T.: -0.005 min
Response: 246855
Conc: 221.32 ng/ml



#26 AR-1254-1


R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 297586
Conc: 170.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

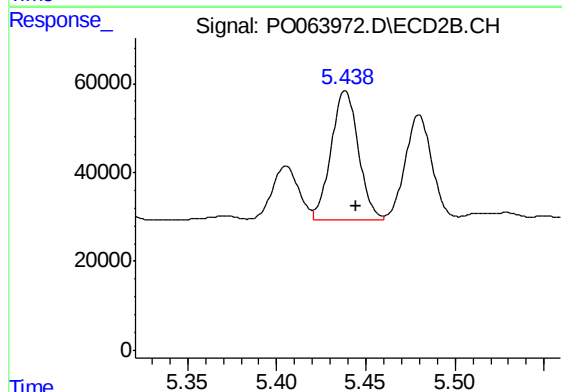


#26 AR-1254-1

R.T.: 5.439 min
Delta R.T.: -0.006 min
Response: 309978
Conc: 174.95 ng/ml

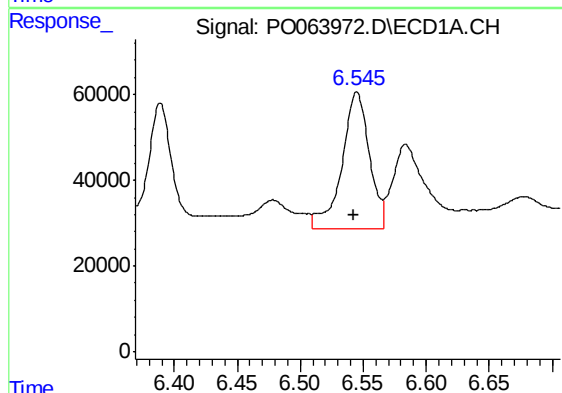


#27 AR-1254-2

R.T.: 6.545 min
Delta R.T.: 0.003 min
Response: 483741
Conc: 173.53 ng/ml

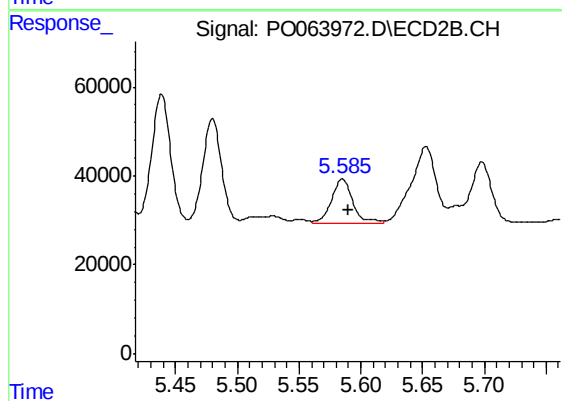

#27 AR-1254-2


R.T.: 5.585 min
Delta R.T.: -0.005 min
Response: 117559
Conc: 74.56 ng/ml

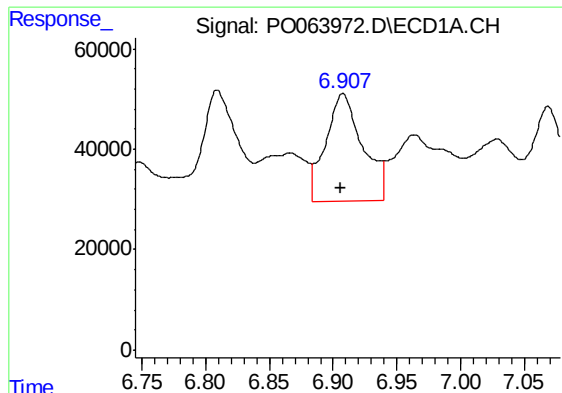

#28 AR-1254-3


R.T.: 6.908 min
Delta R.T.: 0.002 min
Response: 428359
Conc: 136.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

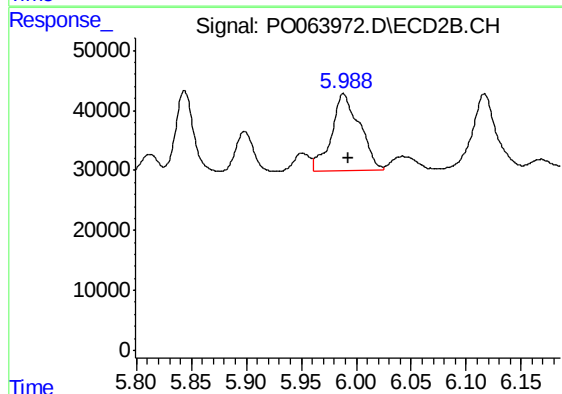


#28 AR-1254-3

R.T.: 5.988 min
Delta R.T.: -0.005 min
Response: 229914
Conc: 85.74 ng/ml

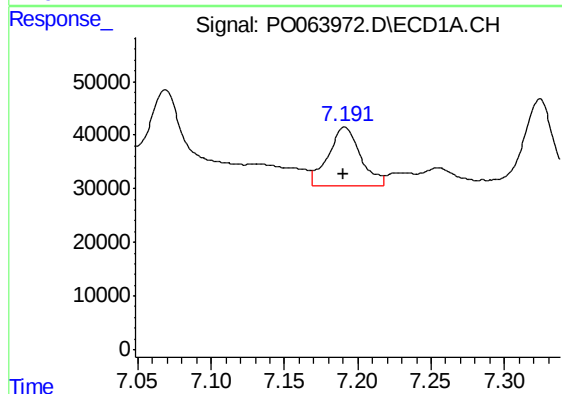


#29 AR-1254-4

R.T.: 7.191 min
Delta R.T.: 0.000 min
Response: 169359
Conc: 68.49 ng/ml

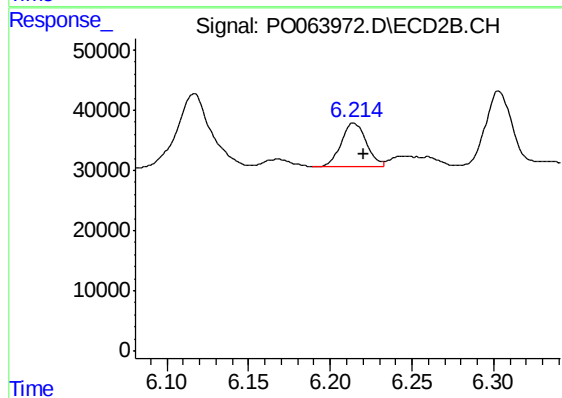

#29 AR-1254-4


R.T.: 6.214 min
Delta R.T.: -0.006 min
Response: 78502
Conc: 44.27 ng/ml



#30 AR-1254-5


R.T.: 7.607 min
Delta R.T.: -0.001 min
Response: 187326
Conc: 69.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

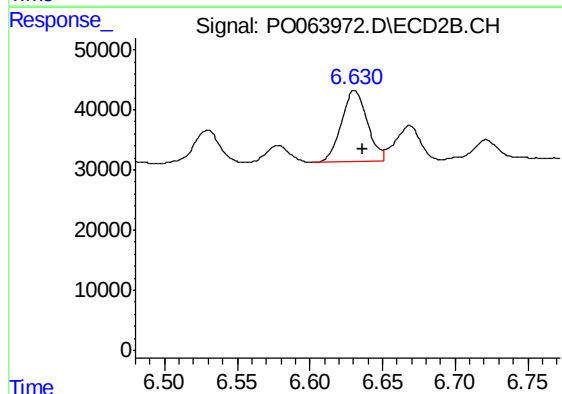


#30 AR-1254-5

R.T.: 6.631 min
Delta R.T.: -0.006 min
Response: 145928
Conc: 58.40 ng/ml




#31 AR-1260-1

R.T.: 7.069 min
Delta R.T.: 0.001 min
Response: 400453
Conc: 198.43 ng/ml

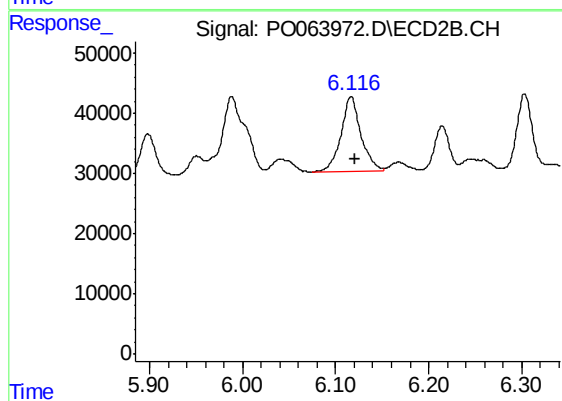

#31 AR-1260-1


R.T.: 6.117 min
Delta R.T.: -0.005 min
Response: 185429
Conc: 118.08 ng/ml

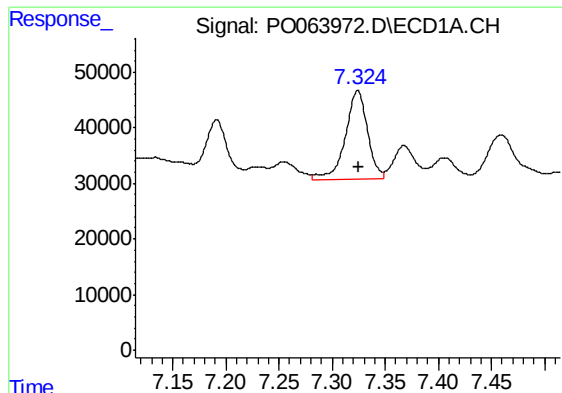

#32 AR-1260-2


R.T.: 7.324 min
Delta R.T.: 0.000 min
Response: 228542
Conc: 90.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

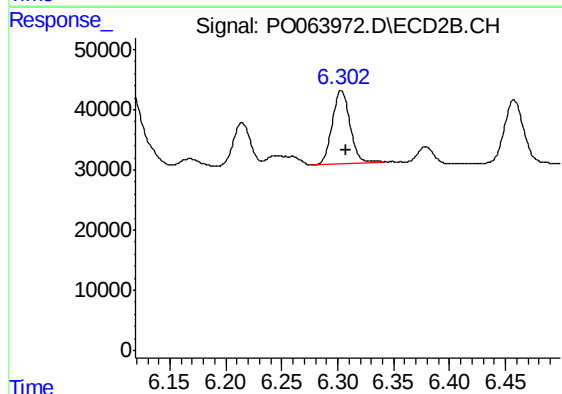


#32 AR-1260-2

R.T.: 6.303 min
Delta R.T.: -0.005 min
Response: 134652
Conc: 68.45 ng/ml




#33 AR-1260-3

R.T.: 7.682 min
Delta R.T.: 0.000 min
Response: 84915
Conc: 41.91 ng/ml

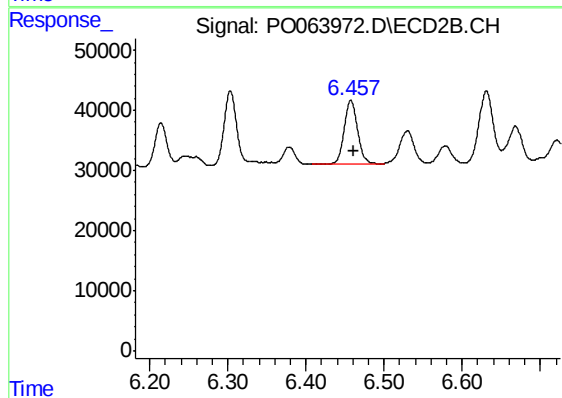

#33 AR-1260-3


R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 127738
Conc: 71.62 ng/ml

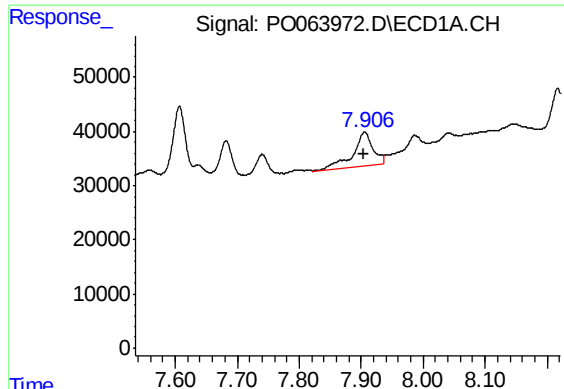

#34 AR-1260-4


R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 138113
Conc: 57.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

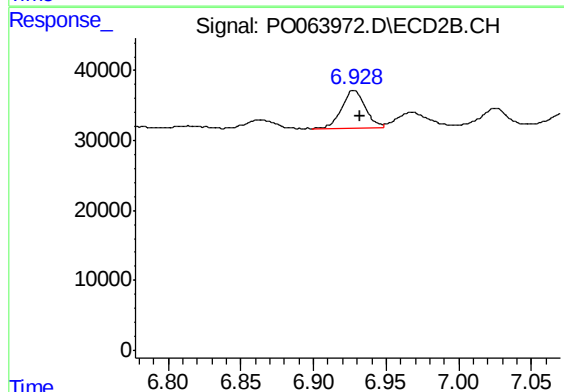


#34 AR-1260-4

R.T.: 6.928 min
Delta R.T.: -0.005 min
Response: 61206
Conc: 38.87 ng/ml

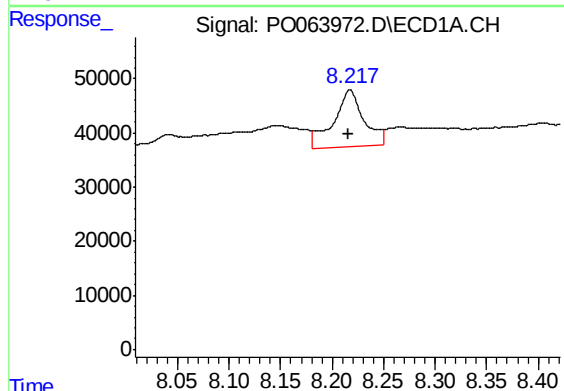


#35 AR-1260-5

R.T.: 8.217 min
Delta R.T.: 0.002 min
Response: 214805
Conc: 45.76 ng/ml

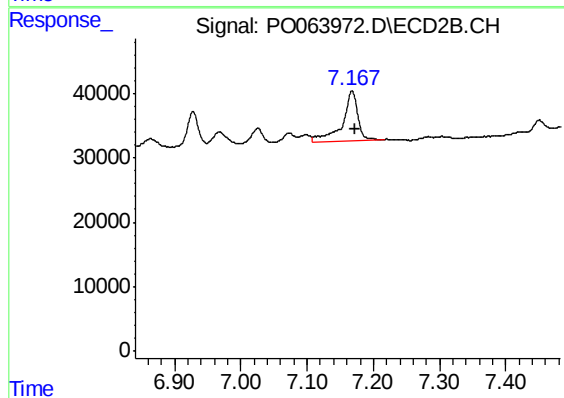

#35 AR-1260-5


R.T.: 7.168 min
Delta R.T.: -0.004 min
Response: 130506
Conc: 33.66 ng/ml



#36 AR-1262-1


R.T.: 7.682 min
Delta R.T.: 0.000 min
Response: 84915
Conc: 26.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

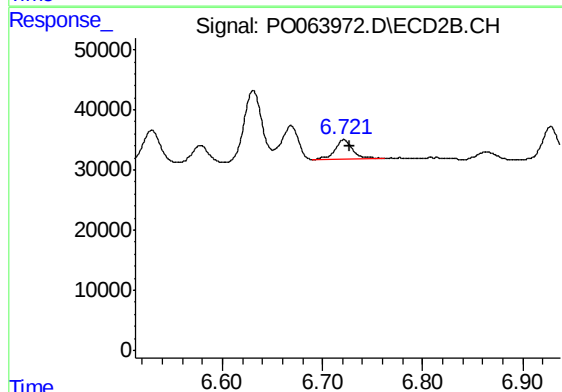


#36 AR-1262-1

R.T.: 6.721 min
Delta R.T.: -0.006 min
Response: 40995
Conc: 39.21 ng/ml




#37 AR-1262-2

R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 214805
Conc: 36.46 ng/ml

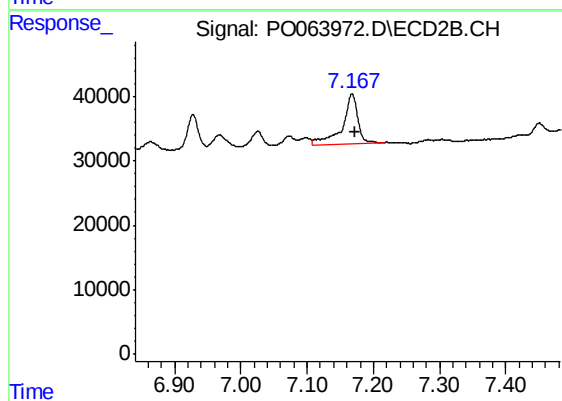

#37 AR-1262-2


R.T.: 7.168 min
Delta R.T.: -0.005 min
Response: 130506
Conc: 27.51 ng/ml

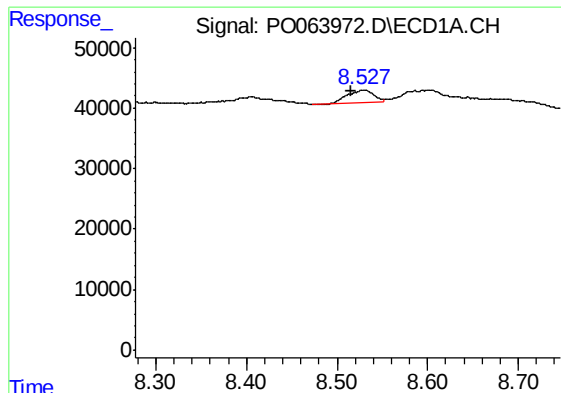

#38 AR-1262-3


R.T.: 8.528 min
Delta R.T.: 0.012 min
Response: 43114
Conc: 10.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

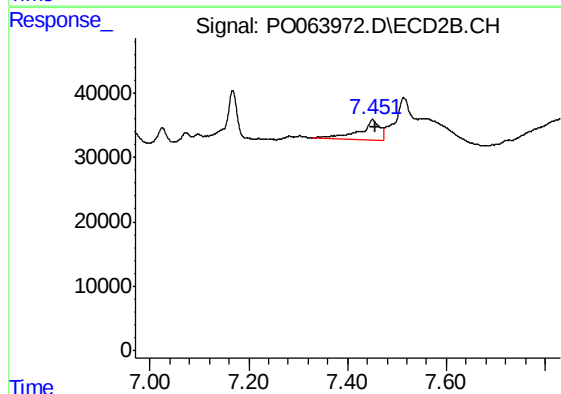


#38 AR-1262-3

R.T.: 7.451 min
Delta R.T.: -0.005 min
Response: 92493
Conc: 49.35 ng/ml

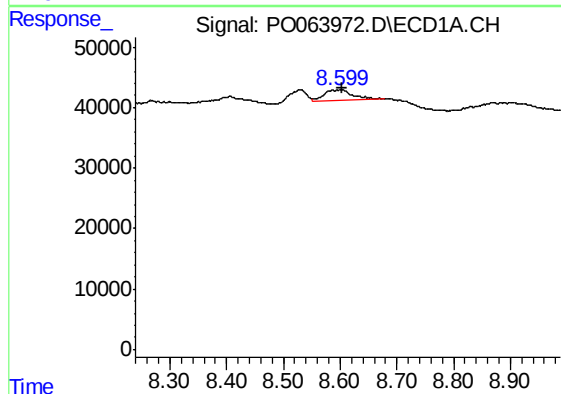


#39 AR-1262-4

R.T.: 8.604 min
Delta R.T.: 0.001 min
Response: 67103
Conc: 21.46 ng/ml

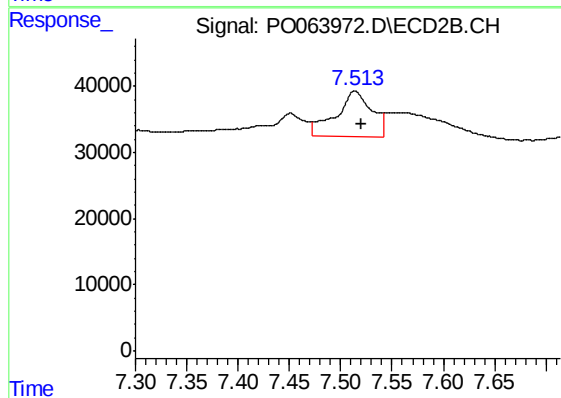

#39 AR-1262-4


R.T.: 7.514 min
Delta R.T.: -0.006 min
Response: 166614
Conc: 47.19 ng/ml

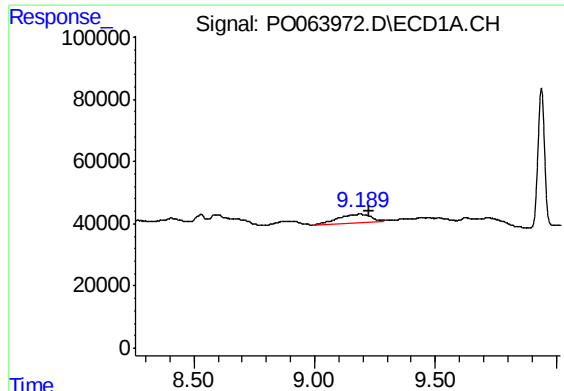

#40 AR-1262-5


R.T.: 9.190 min
Delta R.T.: -0.038 min
Response: 255198
Conc: 117.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

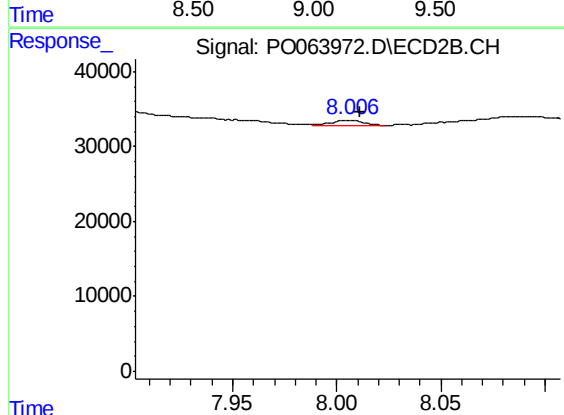


#40 AR-1262-5

R.T.: 8.006 min
Delta R.T.: -0.005 min
Response: 8086
Conc: 5.30 ng/ml

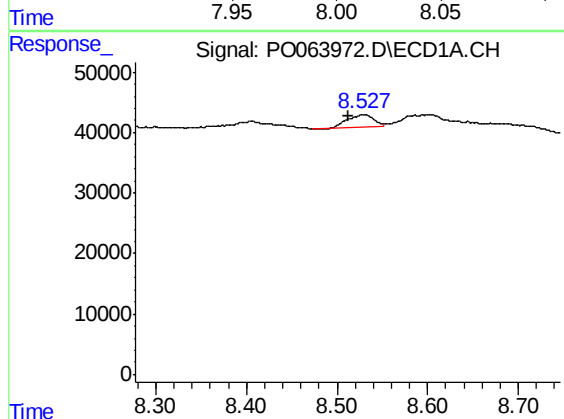


#41 AR-1268-1

R.T.: 8.528 min
Delta R.T.: 0.015 min
Response: 43114
Conc: 6.38 ng/ml

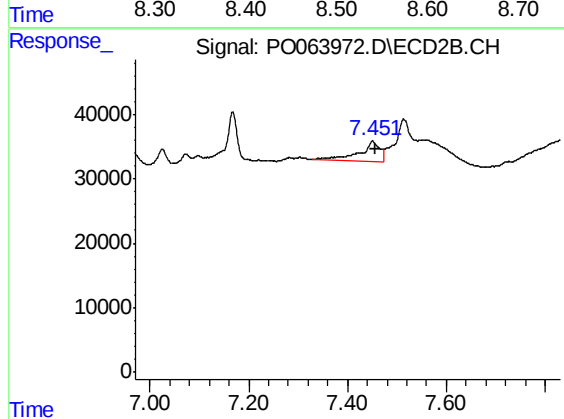

#41 AR-1268-1


R.T.: 7.451 min
Delta R.T.: -0.005 min
Response: 92493
Conc: 17.33 ng/ml

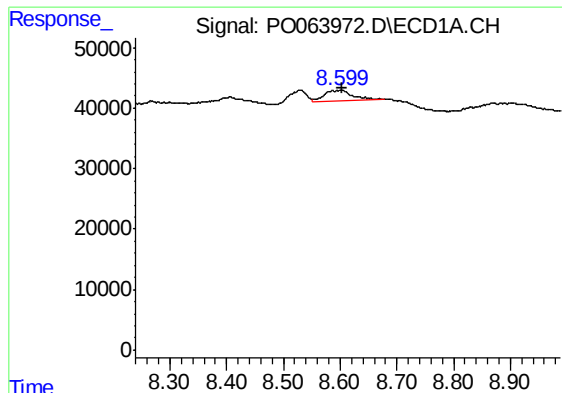

#42 AR-1268-2


R.T.: 8.604 min
Delta R.T.: 0.000 min
Response: 67103
Conc: 10.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

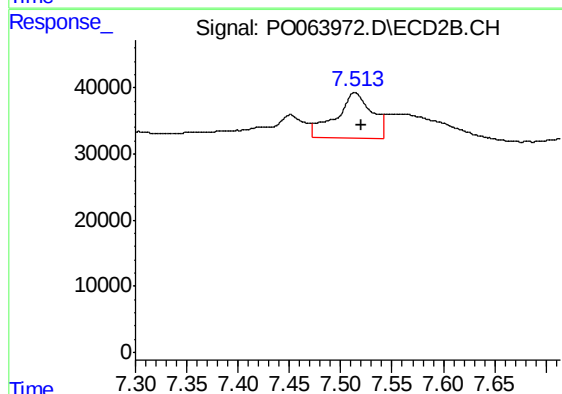


#42 AR-1268-2

R.T.: 7.514 min
Delta R.T.: -0.006 min
Response: 166614
Conc: 33.43 ng/ml

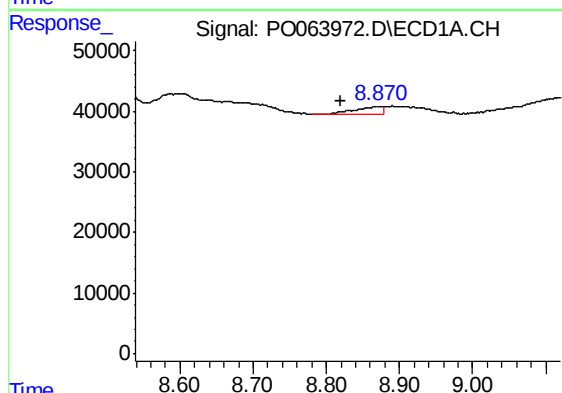


#43 AR-1268-3

R.T.: 8.871 min
Delta R.T.: 0.050 min
Response: 31889
Conc: 6.14 ng/ml

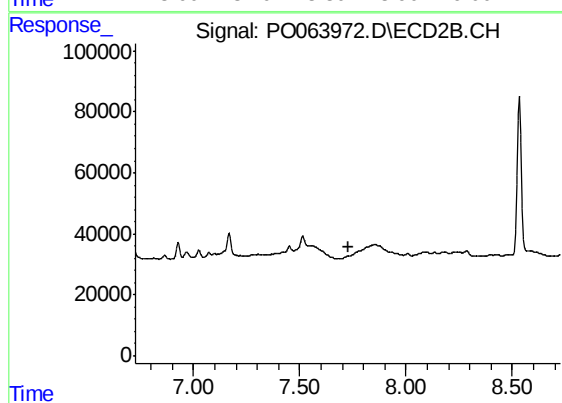

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 7.727 min
Response: 0
Conc: N.D.

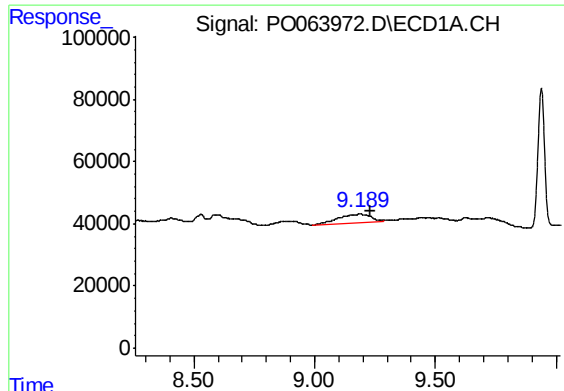

#44 AR-1268-4


R.T.: 9.190 min
Delta R.T.: -0.039 min
Response: 255198
Conc: 104.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE

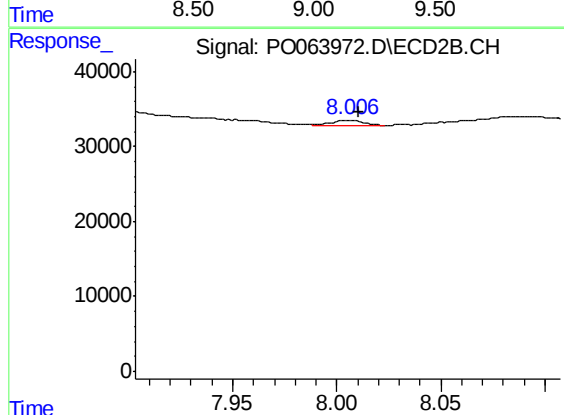


#44 AR-1268-4

R.T.: 8.006 min
Delta R.T.: -0.004 min
Response: 8086
Conc: 4.77 ng/ml

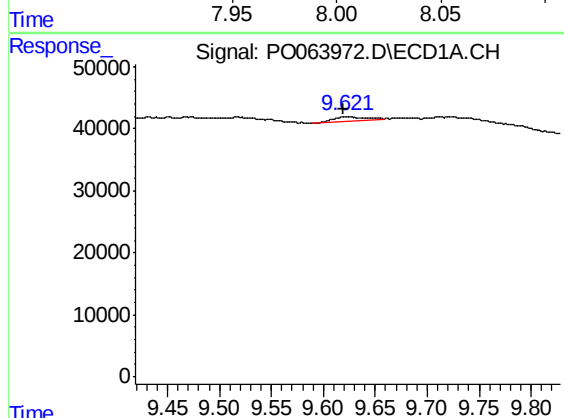

#45 AR-1268-5

R.T.: 9.622 min
Delta R.T.: 0.003 min
Response: 13137
Conc: 0.85 ng/ml

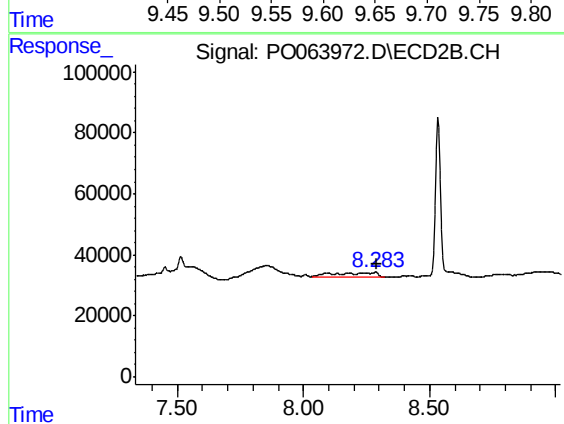

#45 AR-1268-5

R.T.: 8.284 min
Delta R.T.: -0.009 min
Response: 150306
Conc: 12.71 ng/ml