

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063987.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 2:15
 Operator : SM/AJ
 Sample : K5966-03 5X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110619-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:55:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.567	256735	186500	8.397	8.397
2)	SA Decachlor...	9.945	8.534	264692	196964	6.514	6.735
Target Compounds							
3)	L1 AR-1016-1	5.407	0.000	24247	0	17.459	N.D. #
5)	L1 AR-1016-3	5.615	4.815	432481	58263	346.215	78.245 #
6)	L1 AR-1016-4	5.682	4.815	386371	58263	375.659	93.520 #
7)	L1 AR-1016-5	5.950	0.000	84726	0	79.624	N.D. #
8)	L2 AR-1221-1	4.573	0.000	22858	0	56.727	N.D. #
9)	L2 AR-1221-2	4.573	3.868	22858	12193	72.876	57.987
10)	L2 AR-1221-3	4.702	3.981	8406	9335	8.862	14.004 #
11)	L3 AR-1232-1	4.702	3.981	8406	9335	6.320	9.903 #
12)	L3 AR-1232-2	5.207	0.000	10814	0	15.164	N.D. #
13)	L3 AR-1232-3	0.000	4.815	0	58263	N.D.	110.078 #
14)	L3 AR-1232-4	5.682	4.971	386371	13136	520.459	27.978 #
15)	L3 AR-1232-5	5.739	0.000	77316	0	131.897	N.D. #
16)	L4 AR-1242-1	5.407	0.000	24247	0	22.918	N.D. #
18)	L4 AR-1242-3	5.615	4.815	432481	58263	452.554	101.693 #
19)	L4 AR-1242-4	5.682	4.971	386371	13136	491.956	23.007 #
20)	L4 AR-1242-5	6.390	0.000	158003	0	152.051	N.D. #
21)	L5 AR-1248-1	5.407	0.000	24247	0	27.764	N.D. #
22)	L5 AR-1248-2	5.739	4.815	77316	58263	61.021	67.600
23)	L5 AR-1248-3	5.950	4.971	84726	13136	59.392	14.847 #
24)	L5 AR-1248-4	6.344	0.000	56744	0	32.783	N.D. #
25)	L5 AR-1248-5	6.390	0.000	158003	0	93.679	N.D. #
26)	L6 AR-1254-1	6.335	0.000	261065	0	149.434	N.D. #
27)	L6 AR-1254-2	6.543	5.589	63543	1048	22.794	0.665 #
28)	L6 AR-1254-3	6.916	5.988	188872	59373	60.161	22.143 #
29)	L6 AR-1254-4	7.191	6.222	32863	152408	13.291	85.944 #
30)	L6 AR-1254-5	0.000	6.619	0	48517650	N.D.	19416.950 #
31)	L7 AR-1260-1	7.075	6.084	44769	17581	22.184	11.195 #
32)	L7 AR-1260-2	7.327	6.302	149425	175154	59.310	89.041 #
33)	L7 AR-1260-3	7.716	0.000	68895222	0	34002.827	N.D. #
34)	L7 AR-1260-4	7.911	6.914	155369	20076	65.241	12.751 #
35)	L7 AR-1260-5	8.224	7.157	178678	34222	38.063	8.827 #
36)	L8 AR-1262-1	7.716	6.669	68895222	920317	21399.348	880.245 #
37)	L8 AR-1262-2	8.224	7.157	178678	34222	30.329	7.215 #
38)	L8 AR-1262-3	8.504	7.475	5386	603487	1.314	321.991 #
39)	L8 AR-1262-4	8.613	7.509	56965	339325	18.215	96.114 #
40)	L8 AR-1262-5	9.231	8.020	864355	972813	396.790	637.140 #
41)	L9 AR-1268-1	8.504	7.475	5386	603487	0.797	113.045 #
42)	L9 AR-1268-2	8.613	7.509	56965	339325	9.078	68.091 #
43)	L9 AR-1268-3	8.814	7.723	41710	924978	8.035	233.020 #
44)	L9 AR-1268-4	9.231	8.002	864355	3310883	355.585	1954.518 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063987.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 2:15
 Operator : SM/AJ
 Sample : K5966-03 5X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110619-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:55:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	9.611	8.309	1204294	489936	78.312	41.422 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063987.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 2:15
Operator : SM/AJ
Sample : K5966-03 5X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:55:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

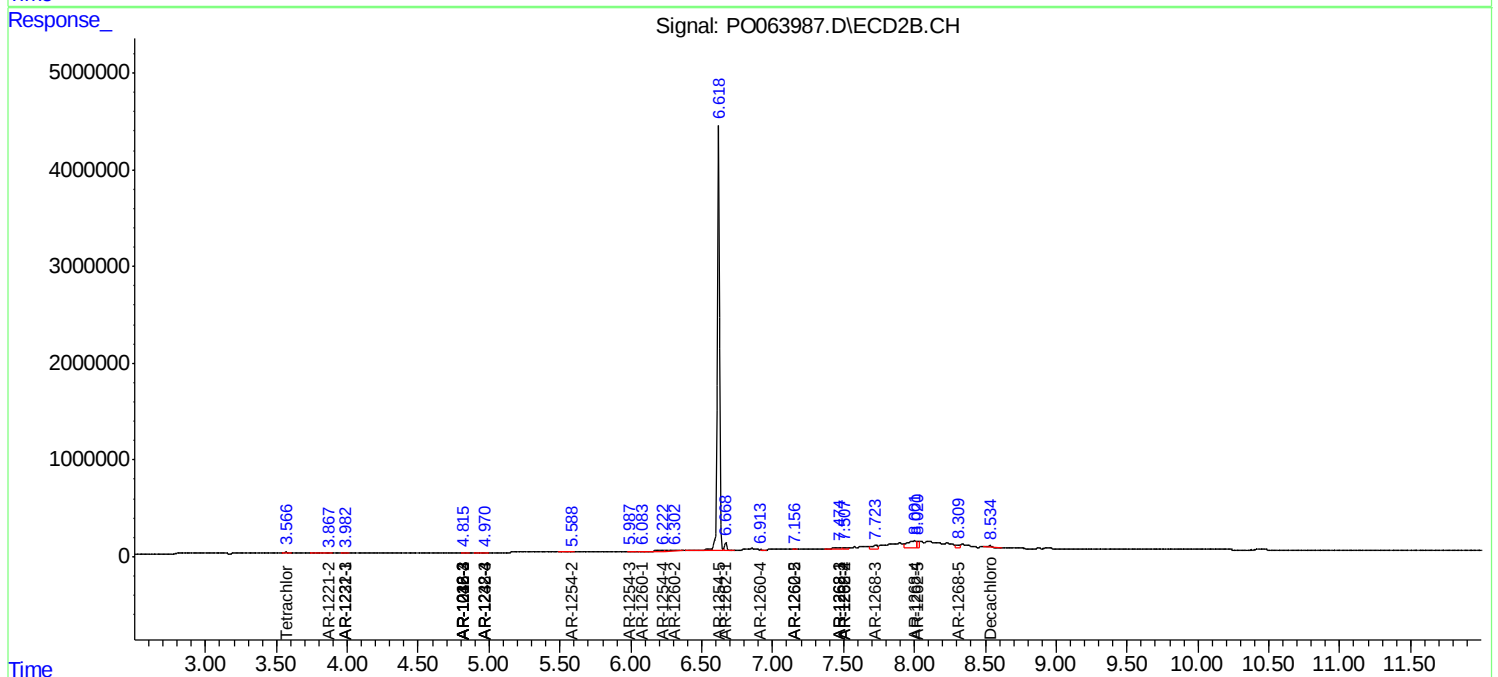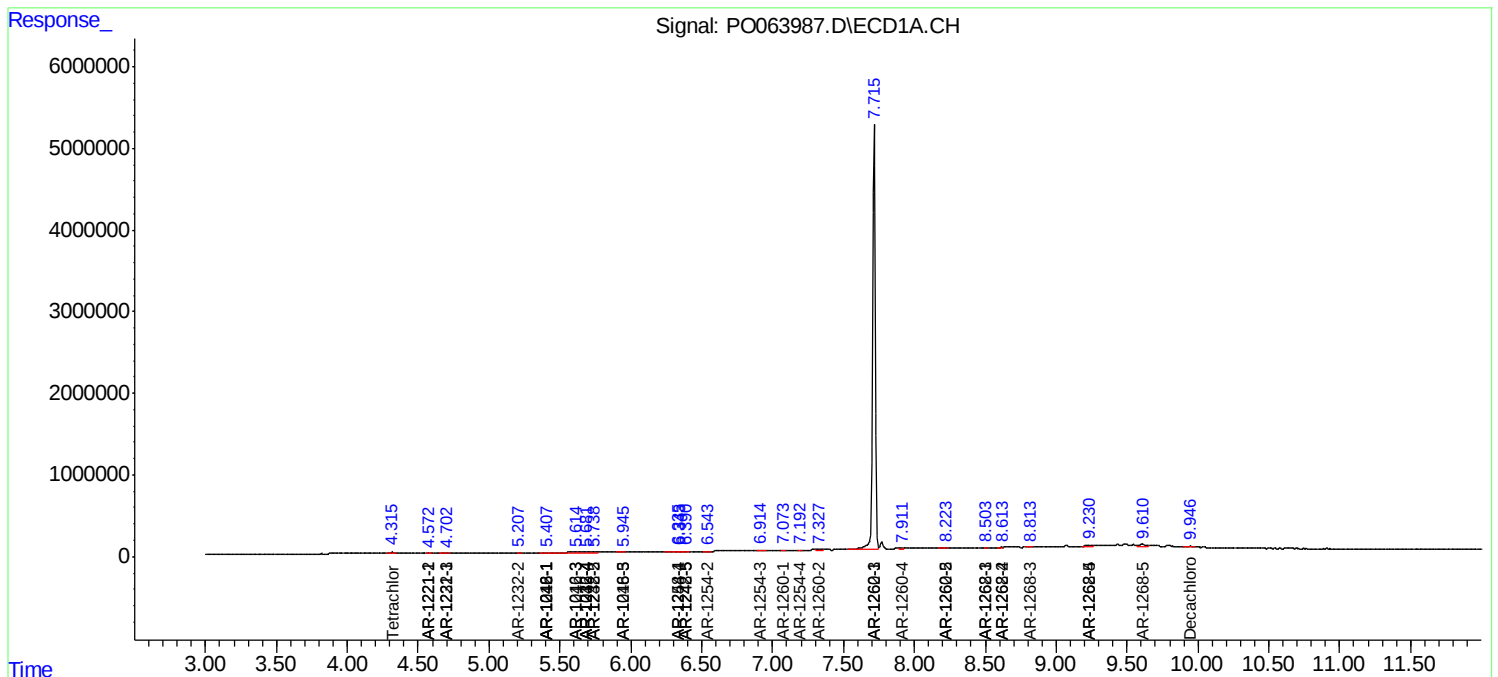


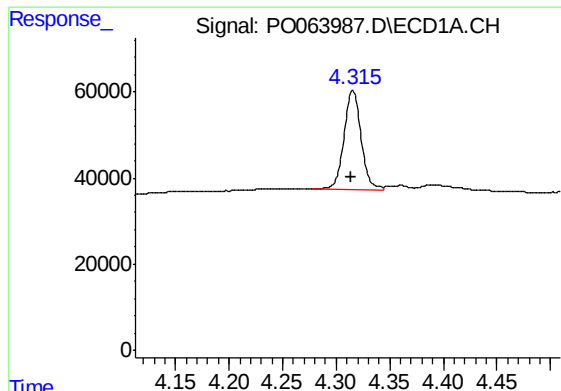

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 256735
Conc: 8.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

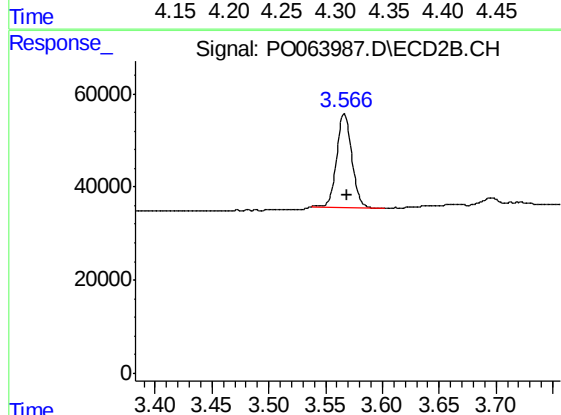


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.002 min
Response: 186500
Conc: 8.40 ng/ml

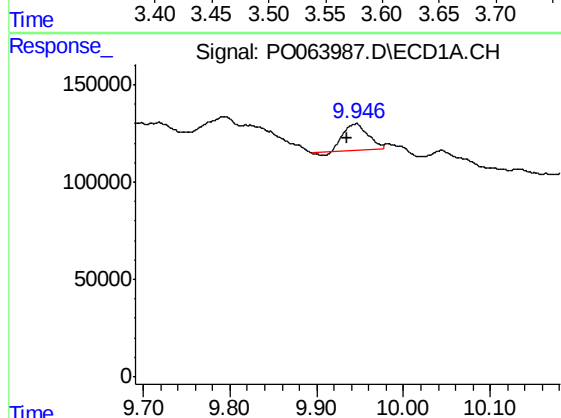


#2 Decachlorobiphenyl

R.T.: 9.945 min
Delta R.T.: 0.009 min
Response: 264692
Conc: 6.51 ng/ml

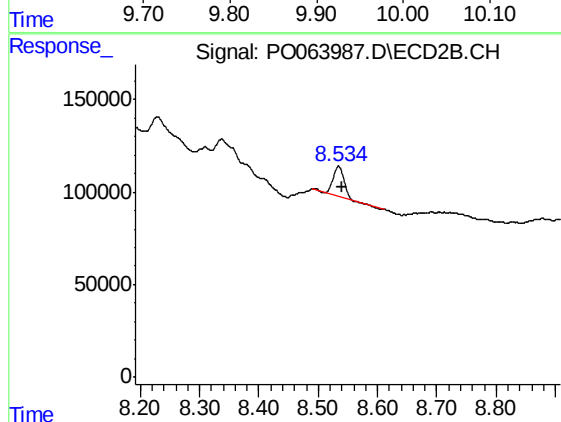

#2 Decachlorobiphenyl


R.T.: 8.534 min
Delta R.T.: -0.005 min
Response: 196964
Conc: 6.73 ng/ml

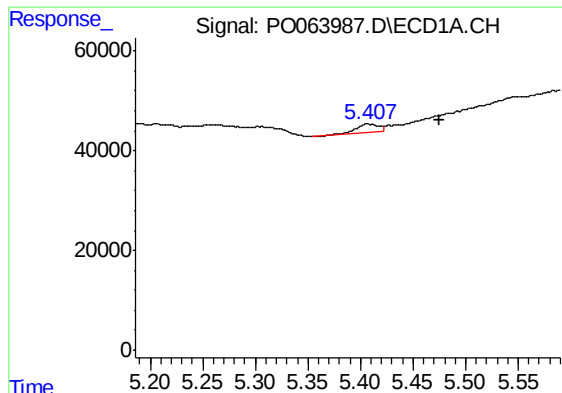

#3 AR-1016-1


R.T.: 5.407 min
Delta R.T.: -0.068 min
Response: 24247
Conc: 17.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

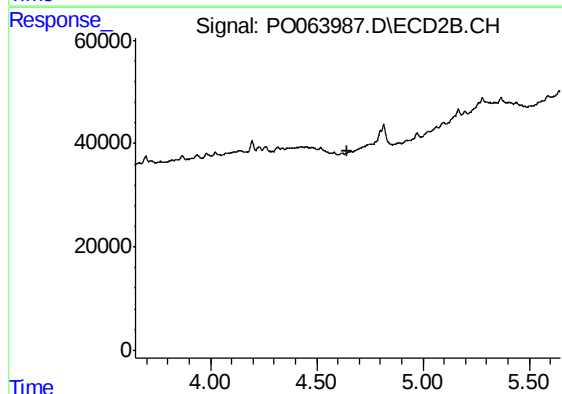


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.

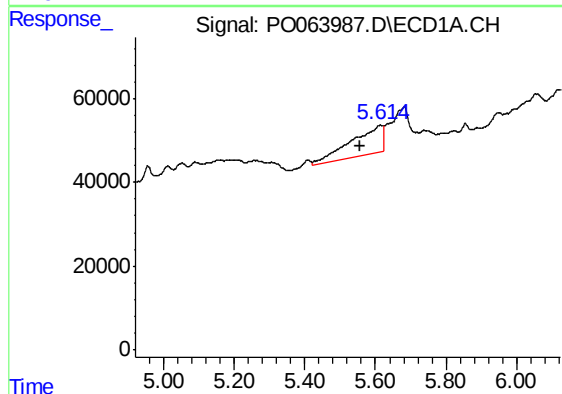


#5 AR-1016-3

R.T.: 5.615 min
Delta R.T.: 0.057 min
Response: 432481
Conc: 346.21 ng/ml

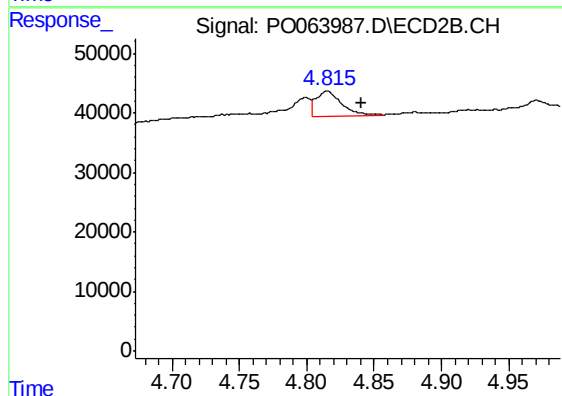

#5 AR-1016-3


R.T.: 4.815 min
Delta R.T.: -0.026 min
Response: 58263
Conc: 78.25 ng/ml

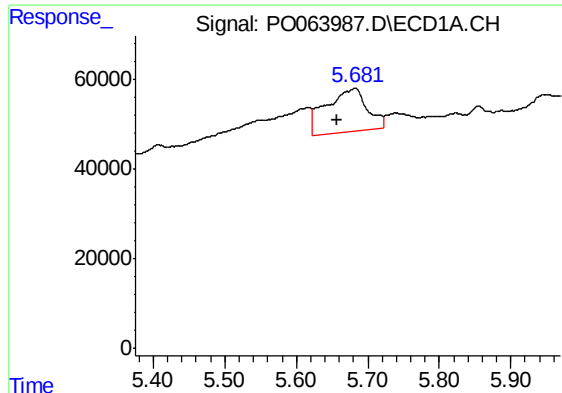

#6 AR-1016-4


R.T.: 5.682 min
Delta R.T.: 0.026 min
Response: 386371
Conc: 375.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

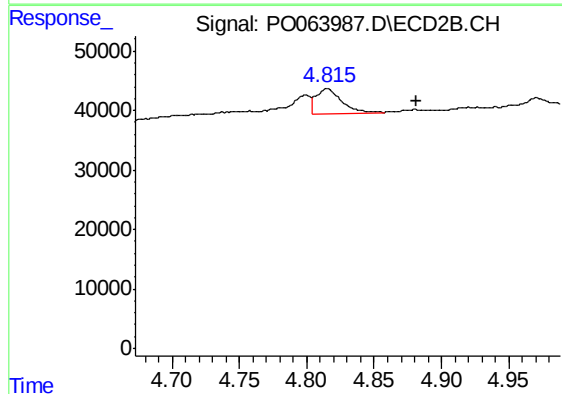


#6 AR-1016-4

R.T.: 4.815 min
Delta R.T.: -0.066 min
Response: 58263
Conc: 93.52 ng/ml

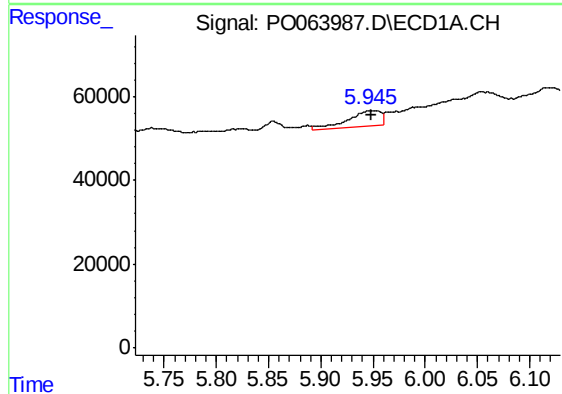


#7 AR-1016-5

R.T.: 5.950 min
Delta R.T.: 0.001 min
Response: 84726
Conc: 79.62 ng/ml

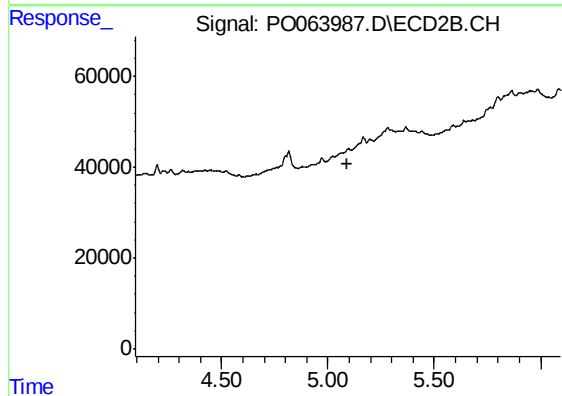

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.094 min
Response: 0
Conc: N.D.



#8 AR-1221-1


R.T.: 4.573 min
Delta R.T.: 0.050 min
Response: 22858
Conc: 56.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

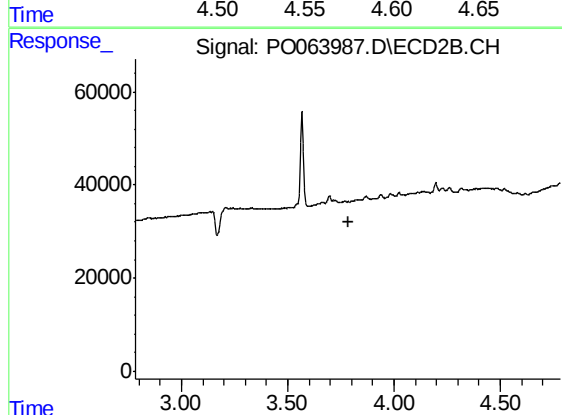


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.783 min
Response: 0
Conc: N.D.

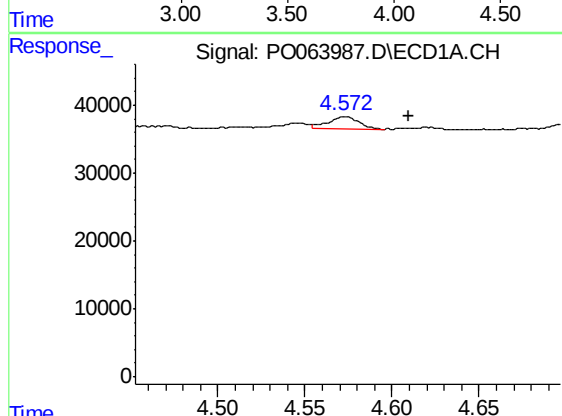


#9 AR-1221-2

R.T.: 4.573 min
Delta R.T.: -0.037 min
Response: 22858
Conc: 72.88 ng/ml

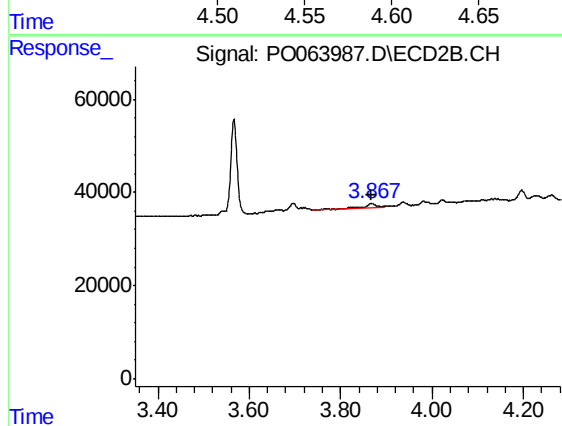

#9 AR-1221-2


R.T.: 3.868 min
Delta R.T.: 0.000 min
Response: 12193
Conc: 57.99 ng/ml



#10 AR-1221-3


R.T.: 4.702 min
Delta R.T.: 0.016 min
Response: 8406
Conc: 8.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#10 AR-1221-3

R.T.: 3.981 min
Delta R.T.: 0.038 min
Response: 9335
Conc: 14.00 ng/ml




#11 AR-1232-1

R.T.: 4.702 min
Delta R.T.: 0.016 min
Response: 8406
Conc: 6.32 ng/ml

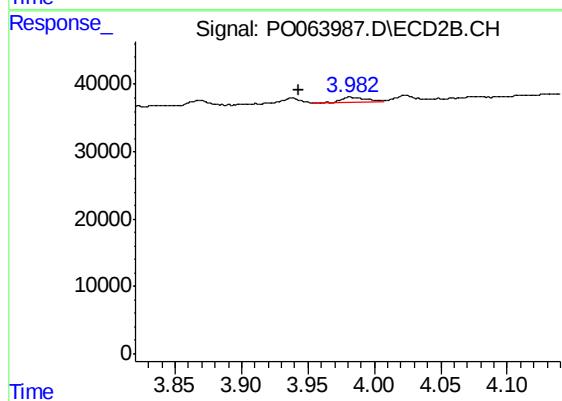

#11 AR-1232-1


R.T.: 3.981 min
Delta R.T.: 0.038 min
Response: 9335
Conc: 9.90 ng/ml



#12 AR-1232-2


R.T.: 5.207 min
Delta R.T.: -0.003 min
Response: 10814
Conc: 15.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.667 min
Response: 0
Conc: N.D.




#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.498 min
Response: 0
Conc: N.D.

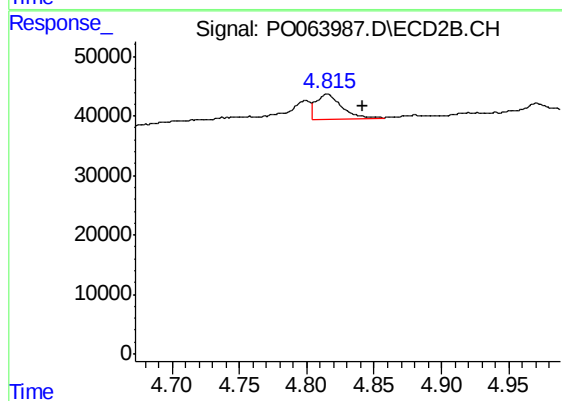

#13 AR-1232-3


R.T.: 4.815 min
Delta R.T.: -0.026 min
Response: 58263
Conc: 110.08 ng/ml



#14 AR-1232-4


R.T.: 5.682 min
Delta R.T.: 0.024 min
Response: 386371
Conc: 520.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#14 AR-1232-4

R.T.: 4.971 min
Delta R.T.: 0.047 min
Response: 13136
Conc: 27.98 ng/ml




#15 AR-1232-5

R.T.: 5.739 min
Delta R.T.: -0.009 min
Response: 77316
Conc: 131.90 ng/ml

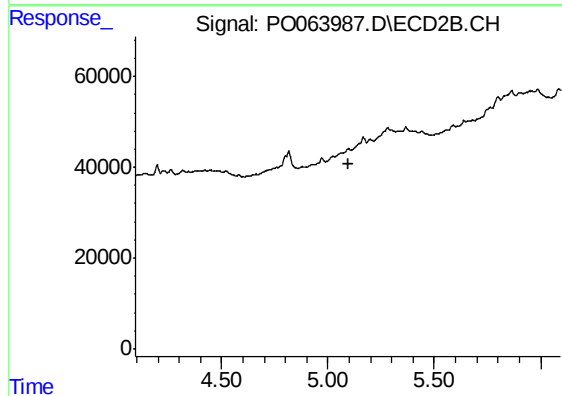

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.094 min
Response: 0
Conc: N.D.



#16 AR-1242-1


R.T.: 5.407 min
Delta R.T.: -0.069 min
Response: 24247
Conc: 22.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.




#18 AR-1242-3

R.T.: 5.615 min
Delta R.T.: 0.056 min
Response: 432481
Conc: 452.55 ng/ml

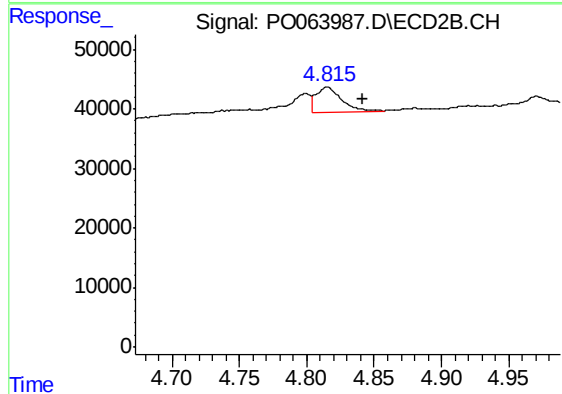

#18 AR-1242-3


R.T.: 4.815 min
Delta R.T.: -0.026 min
Response: 58263
Conc: 101.69 ng/ml



#19 AR-1242-4


R.T.: 5.682 min
Delta R.T.: 0.025 min
Response: 386371
Conc: 491.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#19 AR-1242-4

R.T.: 4.971 min
Delta R.T.: 0.047 min
Response: 13136
Conc: 23.01 ng/ml




#20 AR-1242-5

R.T.: 6.390 min
Delta R.T.: 0.001 min
Response: 158003
Conc: 152.05 ng/ml

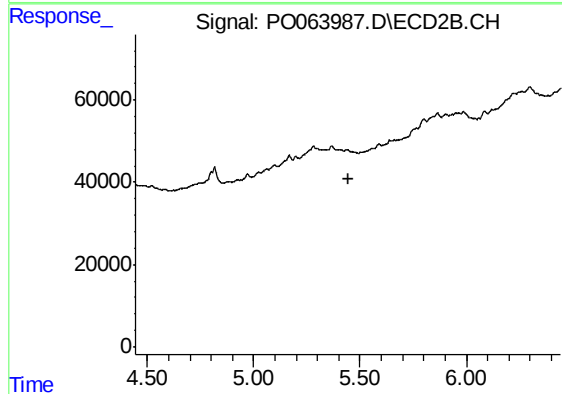

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.



#21 AR-1248-1


R.T.: 5.407 min
Delta R.T.: -0.068 min
Response: 24247
Conc: 27.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.




#22 AR-1248-2

R.T.: 5.739 min
Delta R.T.: -0.009 min
Response: 77316
Conc: 61.02 ng/ml

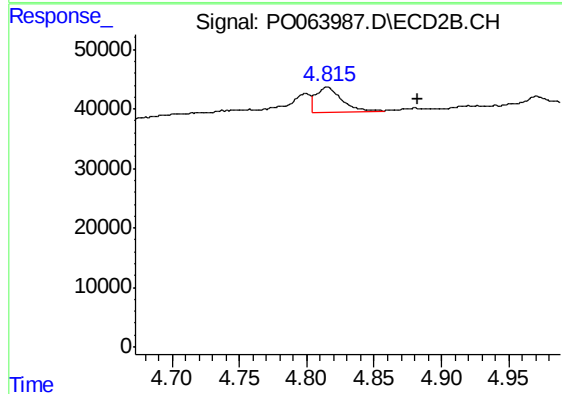

#22 AR-1248-2


R.T.: 4.815 min
Delta R.T.: -0.067 min
Response: 58263
Conc: 67.60 ng/ml

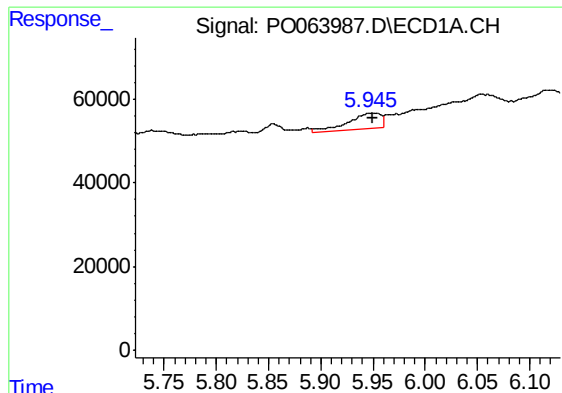

#23 AR-1248-3


R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 84726
Conc: 59.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

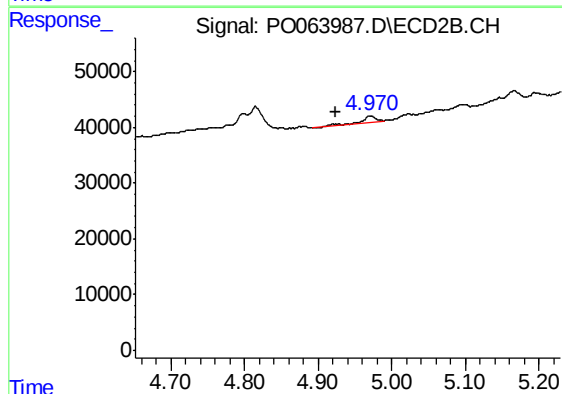


#23 AR-1248-3

R.T.: 4.971 min
Delta R.T.: 0.046 min
Response: 13136
Conc: 14.85 ng/ml




#24 AR-1248-4

R.T.: 6.344 min
Delta R.T.: -0.007 min
Response: 56744
Conc: 32.78 ng/ml

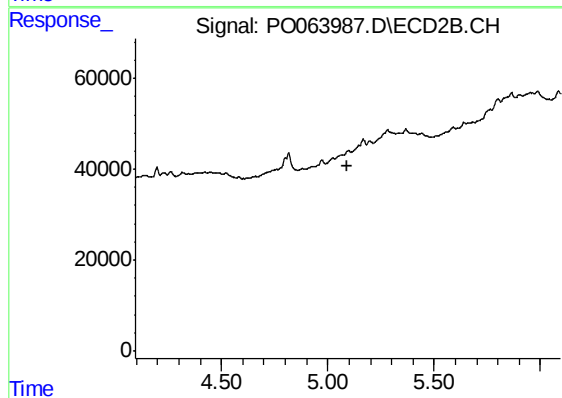

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.095 min
Response: 0
Conc: N.D.



#25 AR-1248-5


R.T.: 6.390 min
Delta R.T.: 0.001 min
Response: 158003
Conc: 93.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.485 min
Response: 0
Conc: N.D.

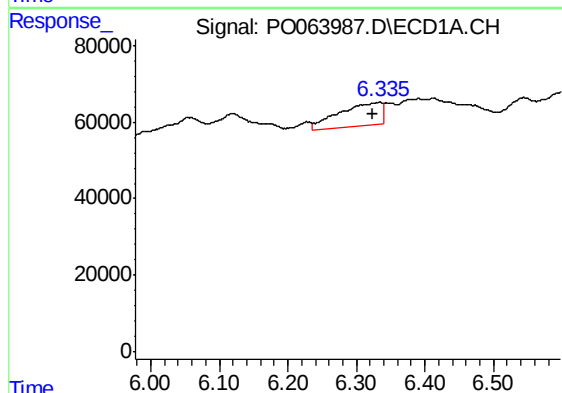


#26 AR-1254-1

R.T.: 6.335 min
Delta R.T.: 0.011 min
Response: 261065
Conc: 149.43 ng/ml

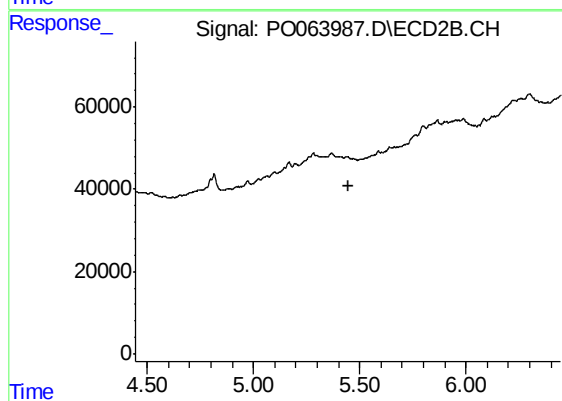

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.445 min
Response: 0
Conc: N.D.



#27 AR-1254-2


R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 63543
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#27 AR-1254-2

R.T.: 5.589 min
Delta R.T.: -0.001 min
Response: 1048
Conc: 0.66 ng/ml




#28 AR-1254-3

R.T.: 6.916 min
Delta R.T.: 0.009 min
Response: 188872
Conc: 60.16 ng/ml

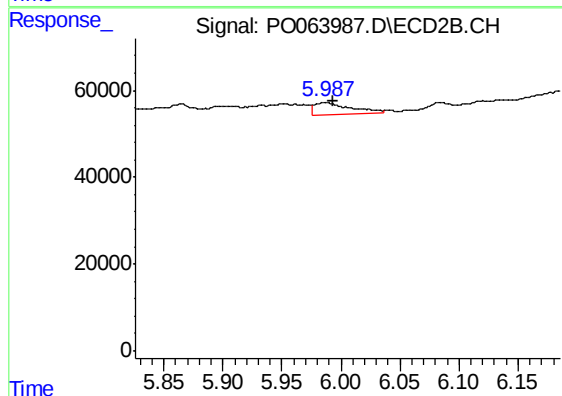

#28 AR-1254-3


R.T.: 5.988 min
Delta R.T.: -0.006 min
Response: 59373
Conc: 22.14 ng/ml



#29 AR-1254-4


R.T.: 7.191 min
Delta R.T.: 0.000 min
Response: 32863
Conc: 13.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

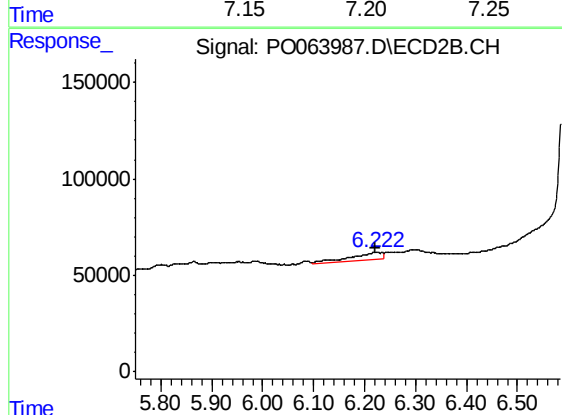


#29 AR-1254-4

R.T.: 6.222 min
Delta R.T.: 0.002 min
Response: 152408
Conc: 85.94 ng/ml

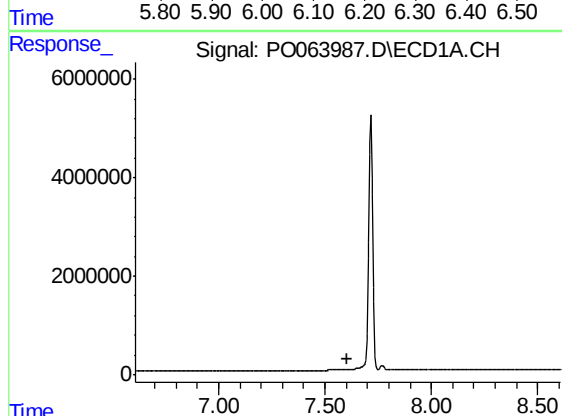


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.608 min
Response: 0
Conc: N.D.

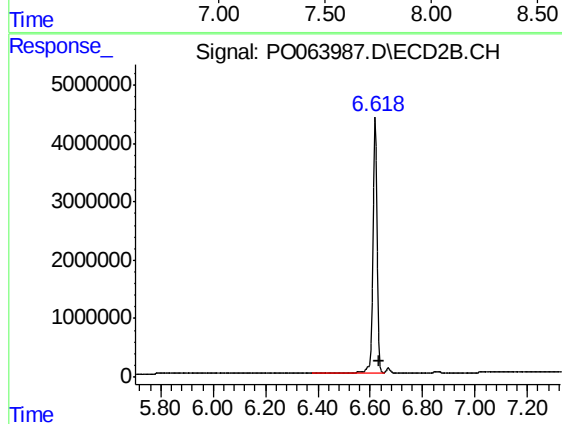

#30 AR-1254-5


R.T.: 6.619 min
Delta R.T.: -0.018 min
Response: 48517650
Conc: 19416.95 ng/ml



#31 AR-1260-1


R.T.: 7.075 min
Delta R.T.: 0.008 min
Response: 44769
Conc: 22.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

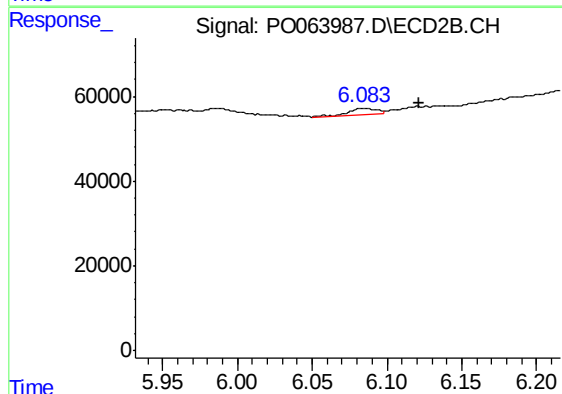


#31 AR-1260-1

R.T.: 6.084 min
Delta R.T.: -0.038 min
Response: 17581
Conc: 11.19 ng/ml




#32 AR-1260-2

R.T.: 7.327 min
Delta R.T.: 0.002 min
Response: 149425
Conc: 59.31 ng/ml

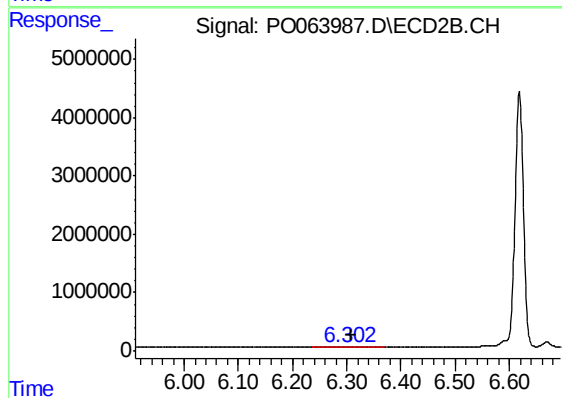

#32 AR-1260-2


R.T.: 6.302 min
Delta R.T.: -0.006 min
Response: 175154
Conc: 89.04 ng/ml



#33 AR-1260-3


R.T.: 7.716 min
Delta R.T.: 0.034 min
Response: 68895222
Conc: 34002.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.




#34 AR-1260-4

R.T.: 7.911 min
Delta R.T.: 0.006 min
Response: 155369
Conc: 65.24 ng/ml

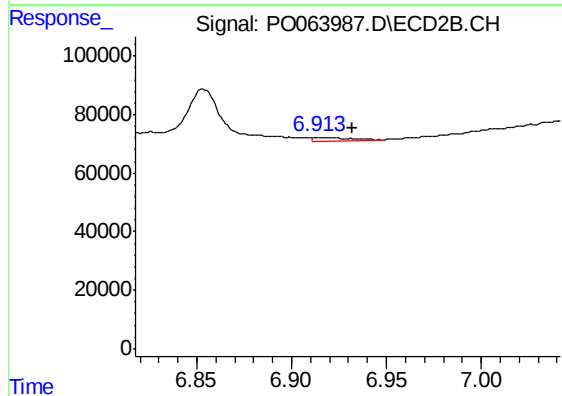

#34 AR-1260-4


R.T.: 6.914 min
Delta R.T.: -0.018 min
Response: 20076
Conc: 12.75 ng/ml

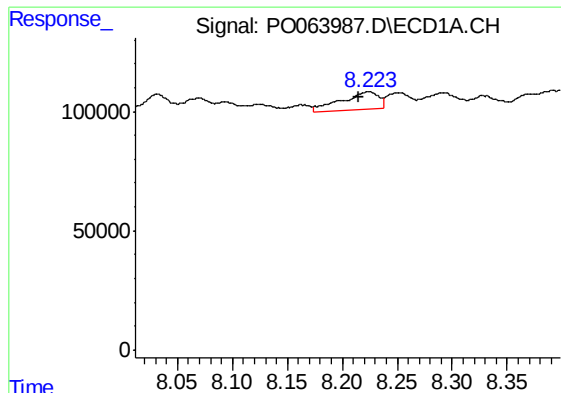

#35 AR-1260-5


R.T.: 8.224 min
Delta R.T.: 0.008 min
Response: 178678
Conc: 38.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

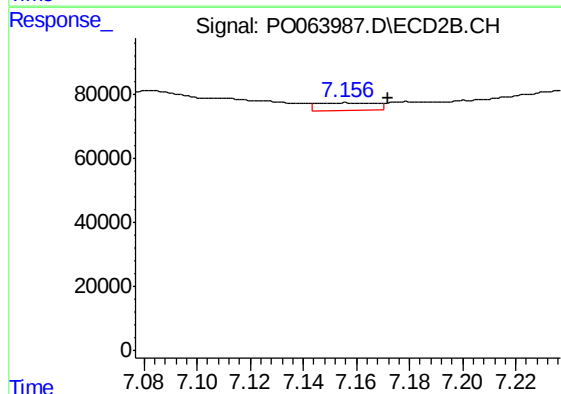


#35 AR-1260-5

R.T.: 7.157 min
Delta R.T.: -0.016 min
Response: 34222
Conc: 8.83 ng/ml

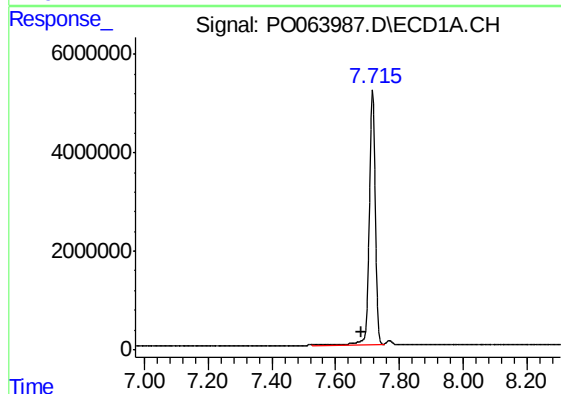


#36 AR-1262-1

R.T.: 7.716 min
Delta R.T.: 0.034 min
Response: 68895222
Conc: 21399.35 ng/ml

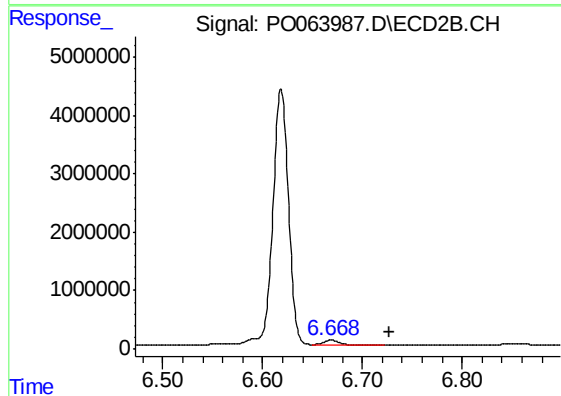

#36 AR-1262-1


R.T.: 6.669 min
Delta R.T.: -0.059 min
Response: 920317
Conc: 880.25 ng/ml

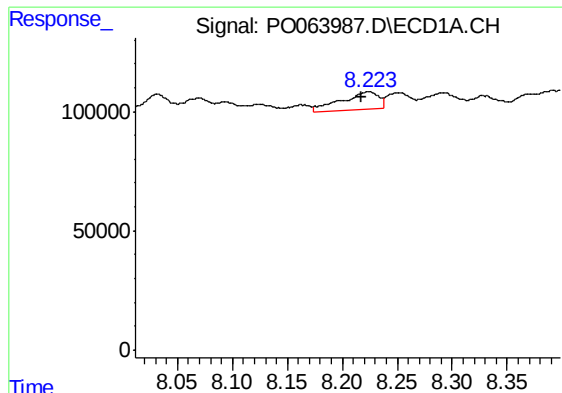

#37 AR-1262-2


R.T.: 8.224 min
Delta R.T.: 0.007 min
Response: 178678
Conc: 30.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

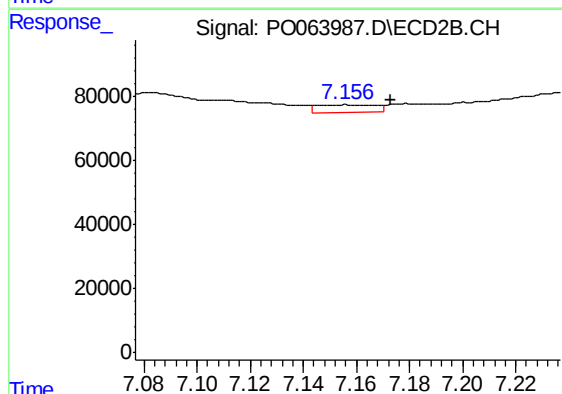


#37 AR-1262-2

R.T.: 7.157 min
Delta R.T.: -0.017 min
Response: 34222
Conc: 7.21 ng/ml

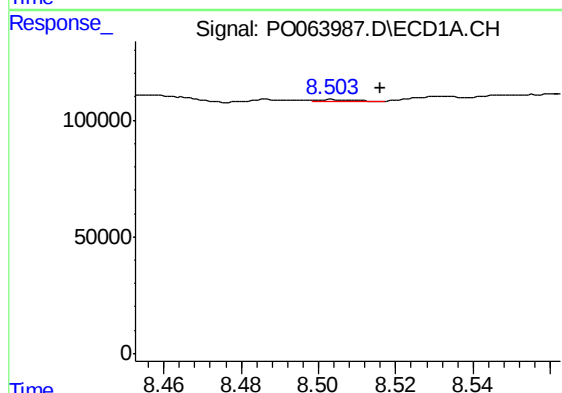


#38 AR-1262-3

R.T.: 8.504 min
Delta R.T.: -0.012 min
Response: 5386
Conc: 1.31 ng/ml

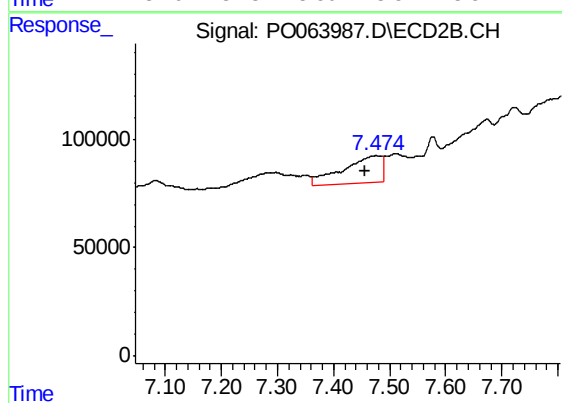

#38 AR-1262-3


R.T.: 7.475 min
Delta R.T.: 0.019 min
Response: 603487
Conc: 321.99 ng/ml

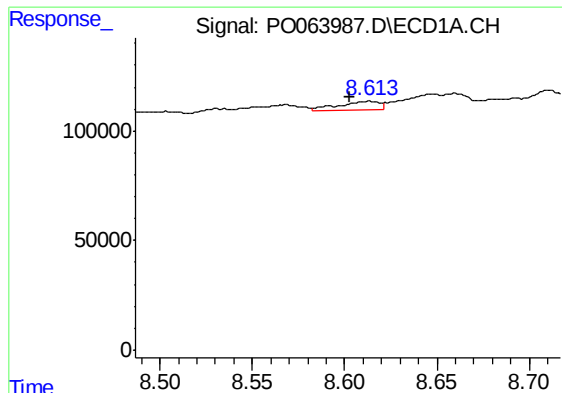

#39 AR-1262-4


R.T.: 8.613 min
Delta R.T.: 0.010 min
Response: 56965
Conc: 18.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

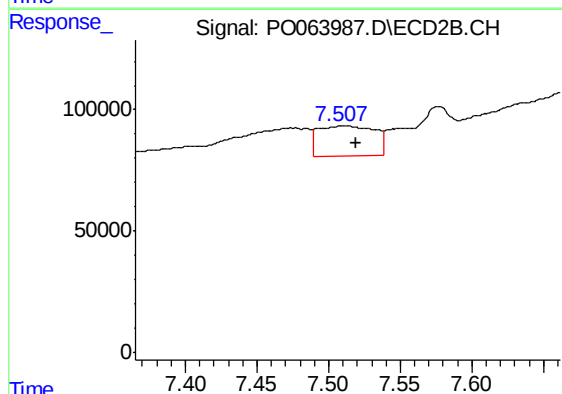


#39 AR-1262-4

R.T.: 7.509 min
Delta R.T.: -0.011 min
Response: 339325
Conc: 96.11 ng/ml

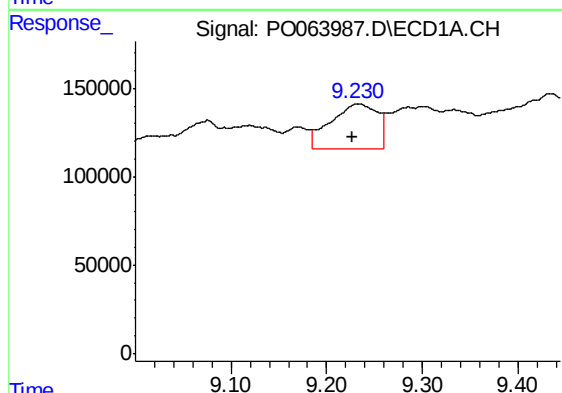


#40 AR-1262-5

R.T.: 9.231 min
Delta R.T.: 0.003 min
Response: 864355
Conc: 396.79 ng/ml

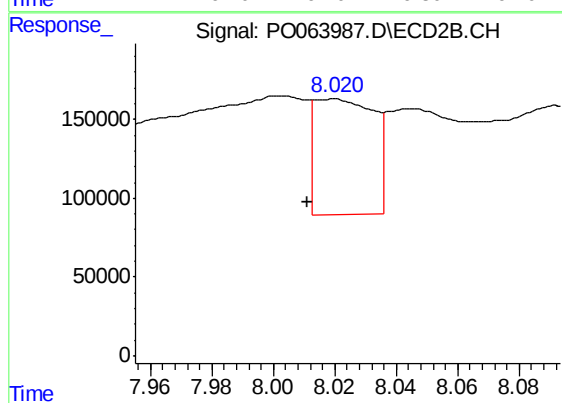

#40 AR-1262-5


R.T.: 8.020 min
Delta R.T.: 0.009 min
Response: 972813
Conc: 637.14 ng/ml



#41 AR-1268-1


R.T.: 8.504 min
Delta R.T.: -0.009 min
Response: 5386
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03




#41 AR-1268-1

R.T.: 7.475 min
Delta R.T.: 0.019 min
Response: 603487
Conc: 113.05 ng/ml




#42 AR-1268-2

R.T.: 8.613 min
Delta R.T.: 0.009 min
Response: 56965
Conc: 9.08 ng/ml

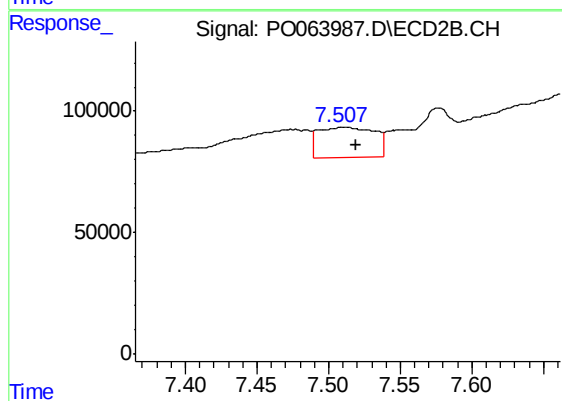

#42 AR-1268-2


R.T.: 7.509 min
Delta R.T.: -0.011 min
Response: 339325
Conc: 68.09 ng/ml



#43 AR-1268-3


R.T.: 8.814 min
Delta R.T.: -0.006 min
Response: 41710
Conc: 8.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

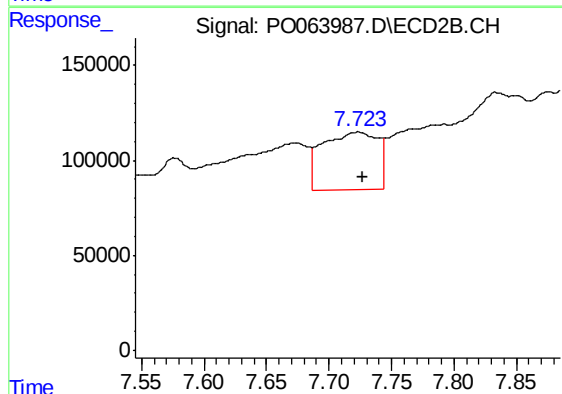


#43 AR-1268-3

R.T.: 7.723 min
Delta R.T.: -0.004 min
Response: 924978
Conc: 233.02 ng/ml

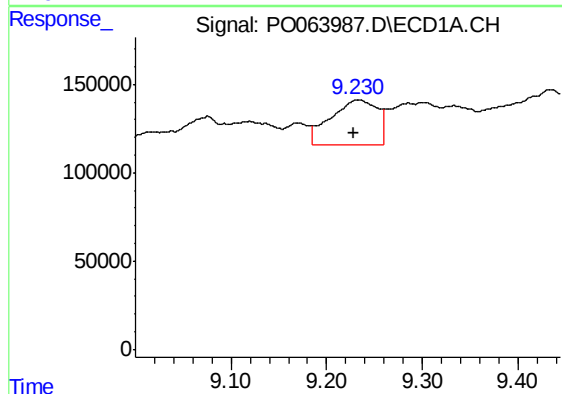


#44 AR-1268-4

R.T.: 9.231 min
Delta R.T.: 0.002 min
Response: 864355
Conc: 355.59 ng/ml

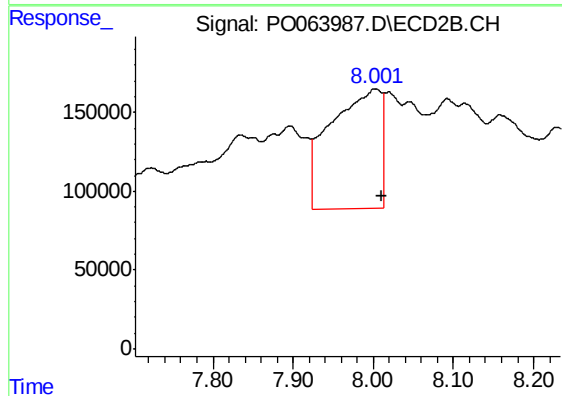

#44 AR-1268-4


R.T.: 8.002 min
Delta R.T.: -0.009 min
Response: 3310883
Conc: 1954.52 ng/ml

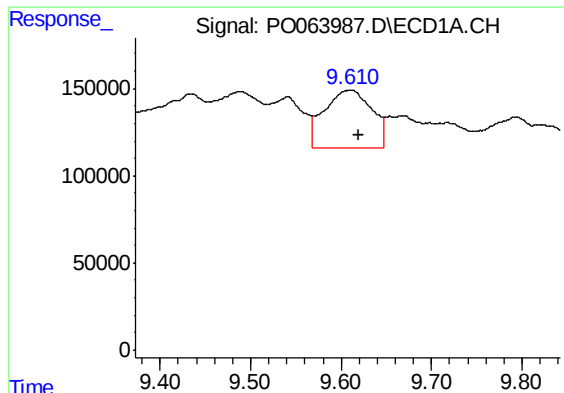

#45 AR-1268-5

R.T.: 9.611 min
Delta R.T.: -0.008 min
Response: 1204294
Conc: 78.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-03

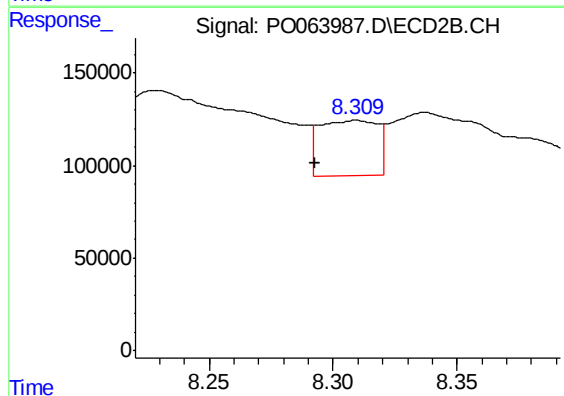

#45 AR-1268-5

R.T.: 8.309 min
Delta R.T.: 0.016 min
Response: 489936
Conc: 41.42 ng/ml