

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 2:49
 Operator : SM/AJ
 Sample : K5966-05 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110619-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:56:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.566	166995	128261	5.462	5.775
2)	SA Decachlor...	9.940	8.534	167574	150654	4.124	5.151
Target Compounds							
3)	L1 AR-1016-1	5.499	0.000	64156	0	46.195	N.D. #
4)	L1 AR-1016-2	5.499	0.000	64156	0	32.687	N.D. #
5)	L1 AR-1016-3	5.499	4.878	64156	22017	51.359	29.568 #
6)	L1 AR-1016-4	0.000	4.878	0	22017	N.D.	35.340 #
7)	L1 AR-1016-5	5.951	5.090	83816	11908	78.768	14.993 #
10)	L2 AR-1221-3	0.000	3.982	0	63339	N.D.	95.018 #
11)	L3 AR-1232-1	0.000	3.982	0	63339	N.D.	67.194 #
12)	L3 AR-1232-2	5.210	0.000	9499	0	13.320	N.D. #
13)	L3 AR-1232-3	5.499	4.878	64156	22017	44.840	41.598
14)	L3 AR-1232-4	0.000	4.878	0	22017	N.D.	46.895 #
15)	L3 AR-1232-5	5.748	5.090	426393	11908	727.402	23.100 #
16)	L4 AR-1242-1	5.499	0.000	64156	0	60.638	N.D. #
17)	L4 AR-1242-2	5.499	0.000	64156	0	42.773	N.D. #
18)	L4 AR-1242-3	5.499	4.878	64156	22017	67.134	38.429 #
19)	L4 AR-1242-4	0.000	4.878	0	22017	N.D.	38.563 #
20)	L4 AR-1242-5	6.391	5.440	159122	57865	153.128	74.344 #
21)	L5 AR-1248-1	5.499	0.000	64156	0	73.462	N.D. #
22)	L5 AR-1248-2	5.748	4.878	426393	22017	336.525	25.545 #
23)	L5 AR-1248-3	5.951	4.878	83816	22017	58.754	24.885 #
24)	L5 AR-1248-4	6.327	5.090	314526	11908	181.713	11.061 #
25)	L5 AR-1248-5	6.391	5.440	159122	57865	94.342	51.881 #
26)	L6 AR-1254-1	6.327	5.440	314526	57865	180.035	32.659 #
27)	L6 AR-1254-2	6.543	5.586	146403	57554	52.517	36.501 #
28)	L6 AR-1254-3	6.912	5.988	236169	63734	75.227	23.769 #
29)	L6 AR-1254-4	7.191	6.215	155504	43399	62.890	24.473 #
30)	L6 AR-1254-5	7.629	6.632	308137	137630	113.679	55.080 #
31)	L7 AR-1260-1	7.070	6.117	222238	40940	110.122	26.069 #
32)	L7 AR-1260-2	7.320	6.304	276289	60715	109.665	30.865 #
33)	L7 AR-1260-3	7.685	6.458	107778	36304	53.193	20.355 #
34)	L7 AR-1260-4	7.902	6.927	545367	14220	229.004	9.032 #
35)	L7 AR-1260-5	8.219	7.168	285136	37061	60.741	9.559 #
36)	L8 AR-1262-1	7.685	6.667	107778	15905	33.477	15.212 #
37)	L8 AR-1262-2	8.219	7.168	285136	37061	48.399	7.813 #
38)	L8 AR-1262-3	8.536	7.451	76396	7641	18.644	4.077 #
39)	L8 AR-1262-4	8.536	7.515	76396	22426	24.428	6.352 #
40)	L8 AR-1262-5	9.196	0.000	57695	0	26.486	N.D. #
41)	L9 AR-1268-1	8.536	7.451	76396	7641	11.301	1.431 #
42)	L9 AR-1268-2	8.536	7.515	76396	22426	12.175	4.500 #
43)	L9 AR-1268-3	8.823	0.000	35862	0	6.908	N.D. #
44)	L9 AR-1268-4	9.196	0.000	57695	0	23.735	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 2:49
 Operator : SM/AJ
 Sample : K5966-05 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110619-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:56:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	9.624	8.306	18516	168715	1.204	14.264 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 2:49
Operator : SM/AJ
Sample : K5966-05 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:56:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

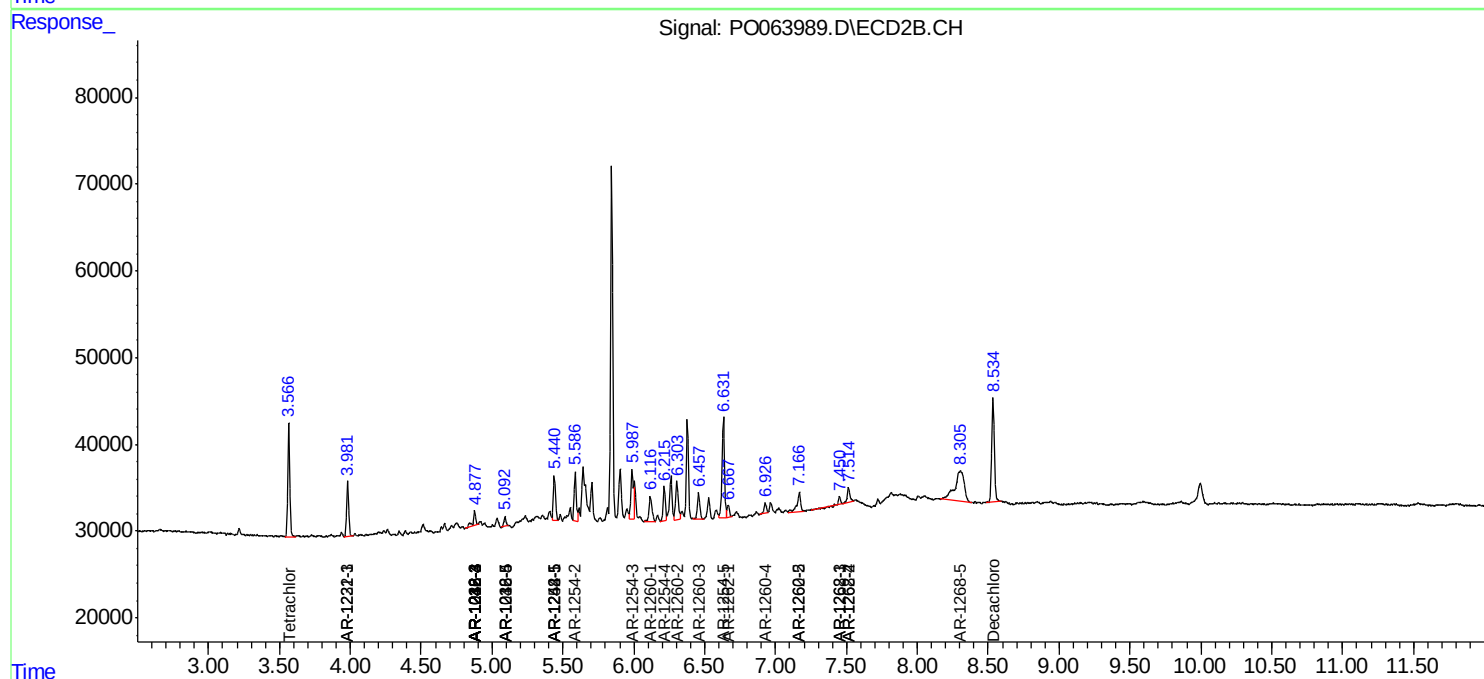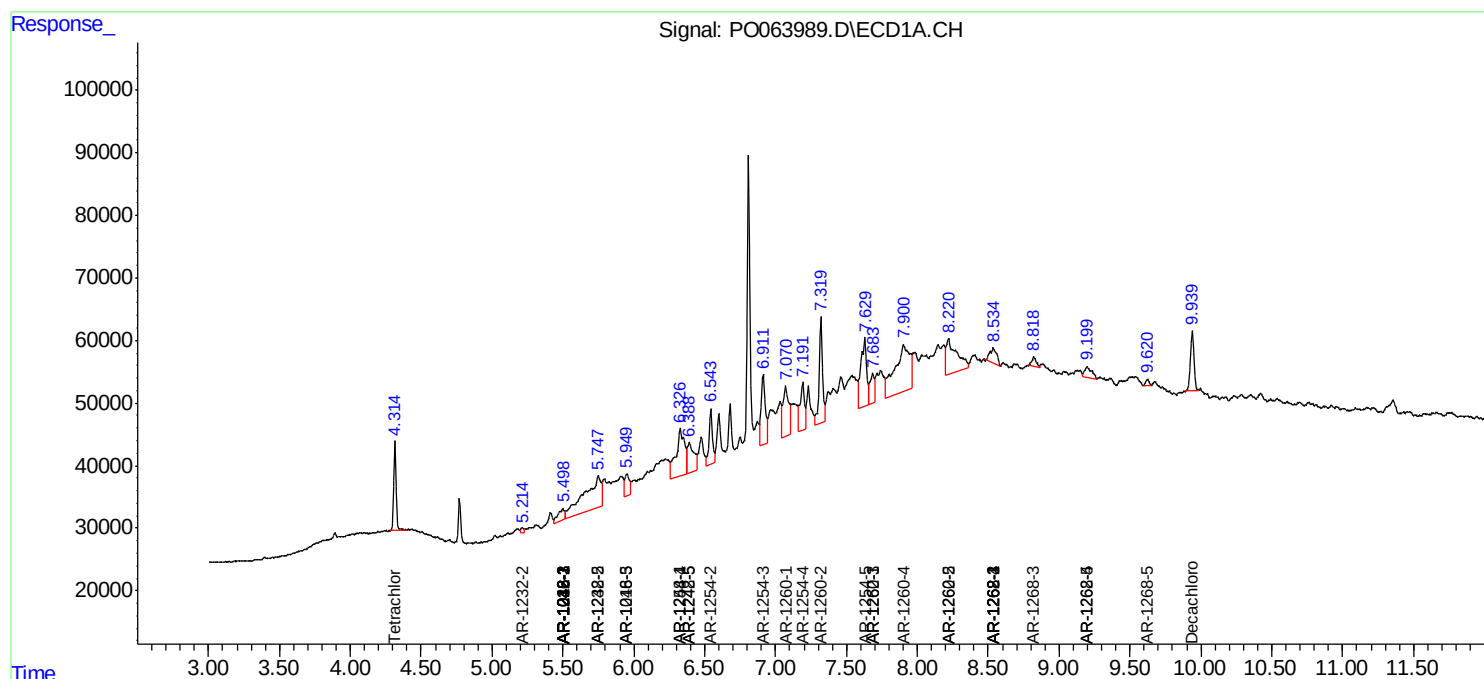




#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.001 min
Response: 166995
Conc: 5.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

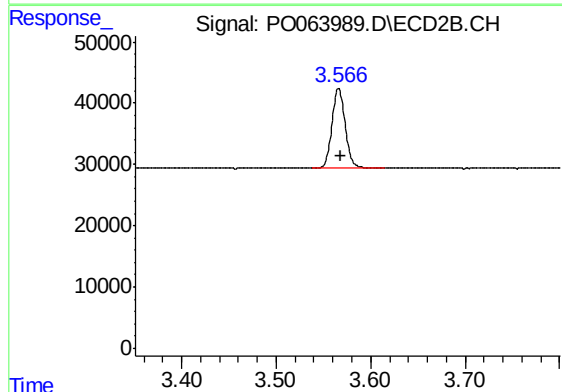


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 128261
Conc: 5.77 ng/ml

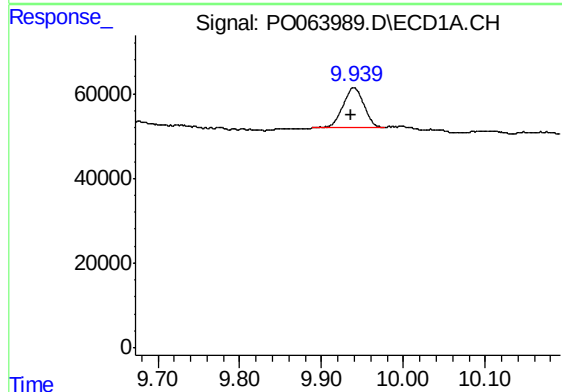


#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 167574
Conc: 4.12 ng/ml

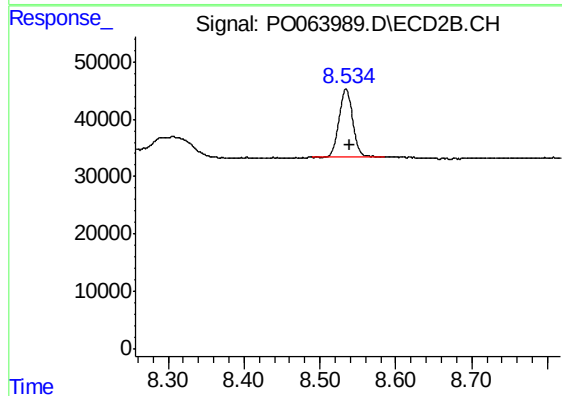

#2 Decachlorobiphenyl


R.T.: 8.534 min
Delta R.T.: -0.005 min
Response: 150654
Conc: 5.15 ng/ml

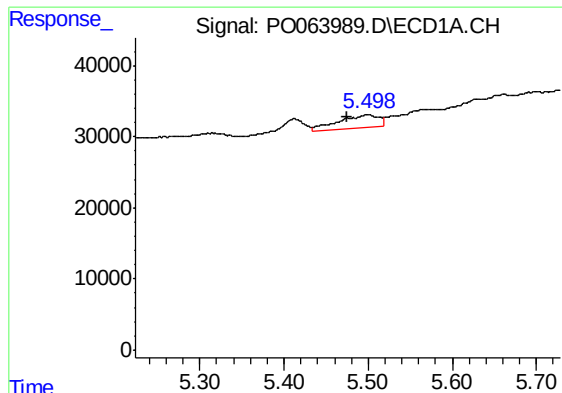

#3 AR-1016-1


R.T.: 5.499 min
Delta R.T.: 0.024 min
Response: 64156
Conc: 46.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

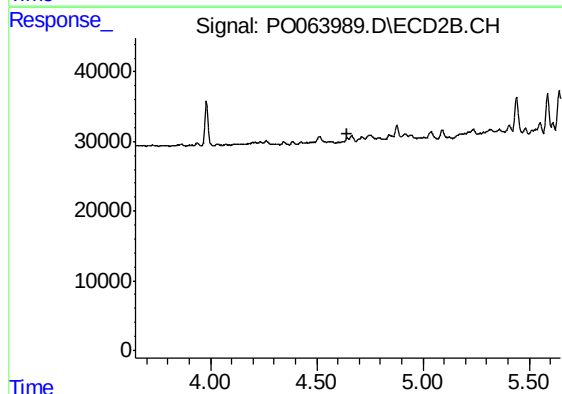


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.




#4 AR-1016-2

R.T.: 5.499 min
Delta R.T.: 0.003 min
Response: 64156
Conc: 32.69 ng/ml

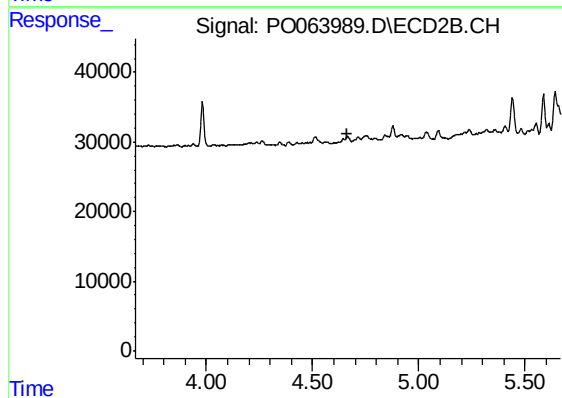

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

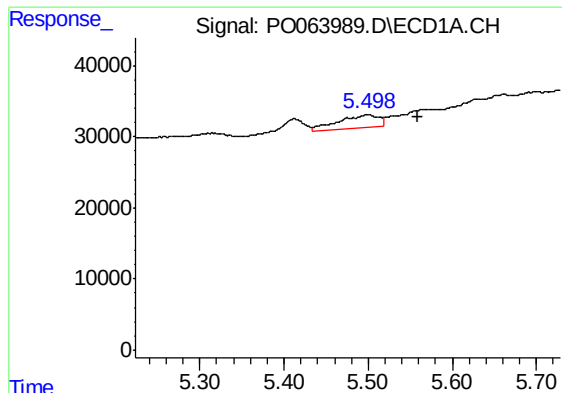

#5 AR-1016-3


R.T.: 5.499 min
Delta R.T.: -0.059 min
Response: 64156
Conc: 51.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

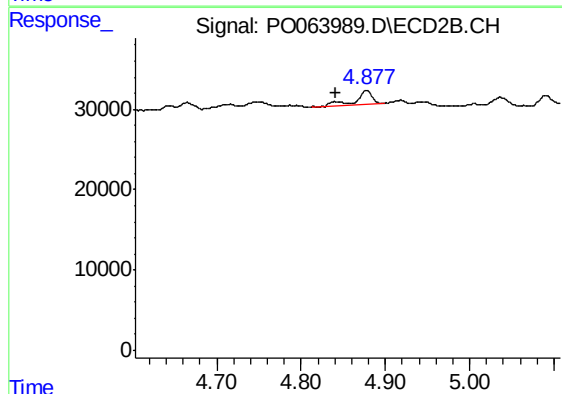


#5 AR-1016-3

R.T.: 4.878 min
Delta R.T.: 0.037 min
Response: 22017
Conc: 29.57 ng/ml

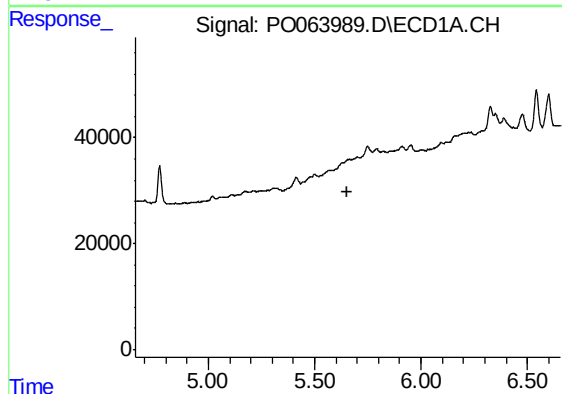


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.656 min
Response: 0
Conc: N.D.

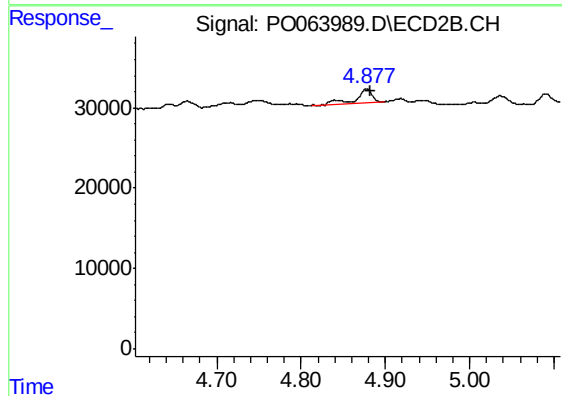

#6 AR-1016-4


R.T.: 4.878 min
Delta R.T.: -0.004 min
Response: 22017
Conc: 35.34 ng/ml



#7 AR-1016-5


R.T.: 5.951 min
Delta R.T.: 0.002 min
Response: 83816
Conc: 78.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

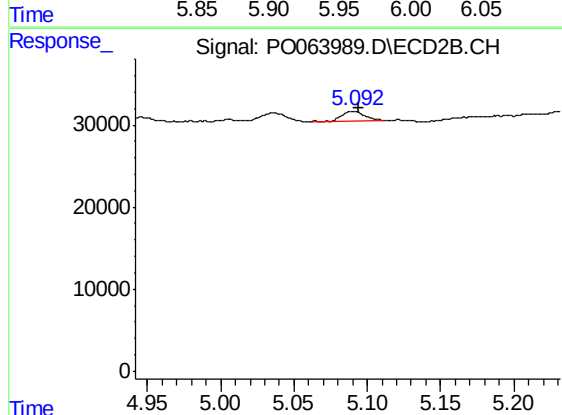


#7 AR-1016-5

R.T.: 5.090 min
Delta R.T.: -0.004 min
Response: 11908
Conc: 14.99 ng/ml

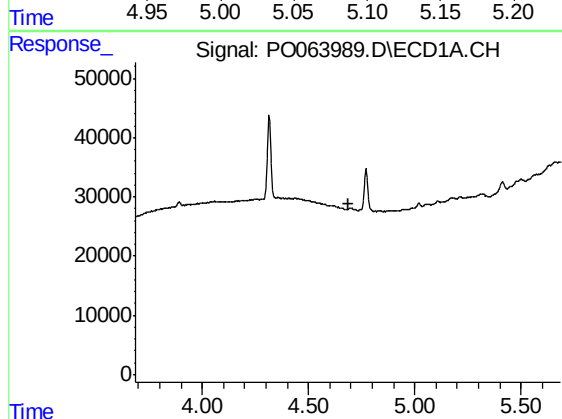


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

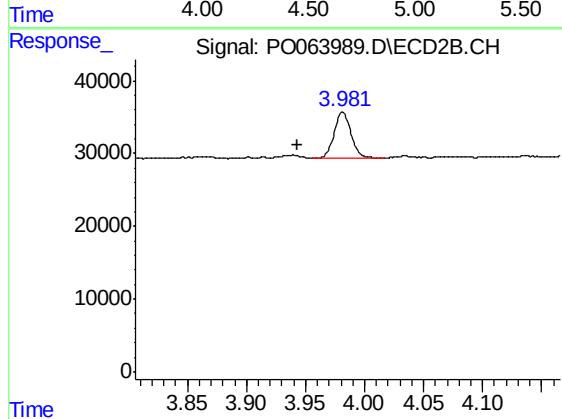

#10 AR-1221-3


R.T.: 3.982 min
Delta R.T.: 0.038 min
Response: 63339
Conc: 95.02 ng/ml

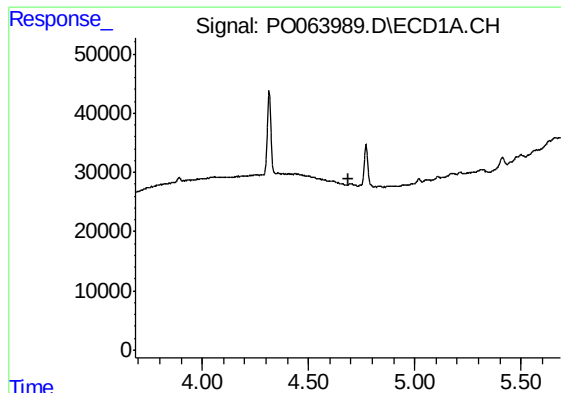

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

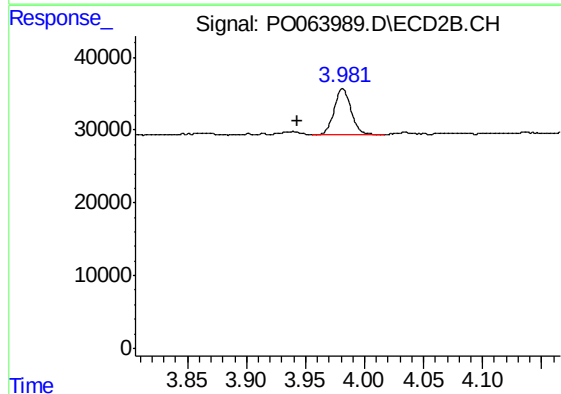


#11 AR-1232-1

R.T.: 3.982 min
Delta R.T.: 0.038 min
Response: 63339
Conc: 67.19 ng/ml

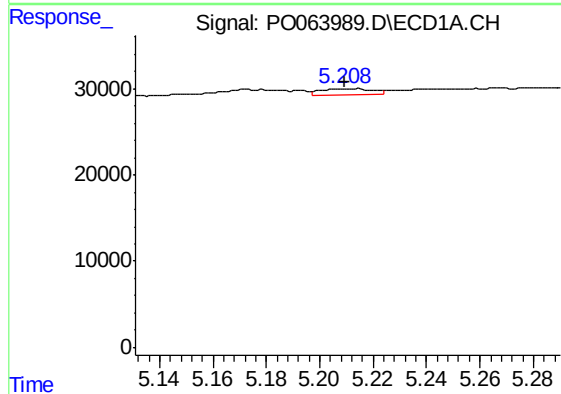


#12 AR-1232-2

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 9499
Conc: 13.32 ng/ml

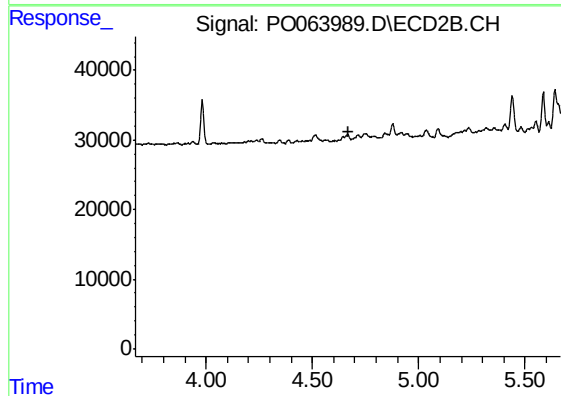

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.667 min
Response: 0
Conc: N.D.

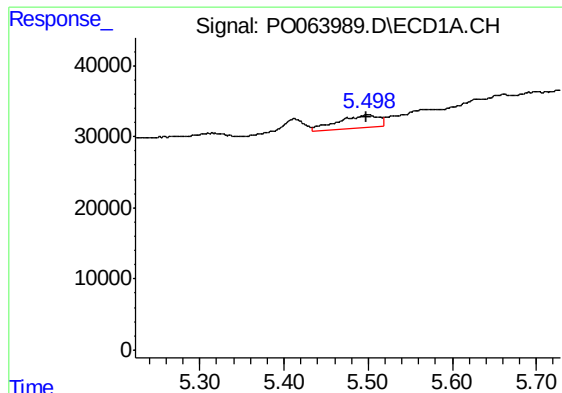

#13 AR-1232-3


R.T.: 5.499 min
Delta R.T.: 0.001 min
Response: 64156
Conc: 44.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

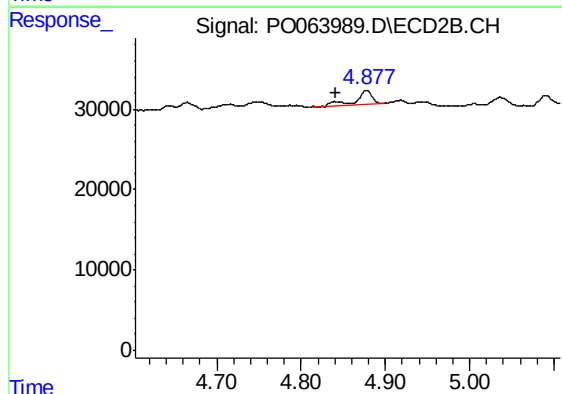


#13 AR-1232-3

R.T.: 4.878 min
Delta R.T.: 0.036 min
Response: 22017
Conc: 41.60 ng/ml

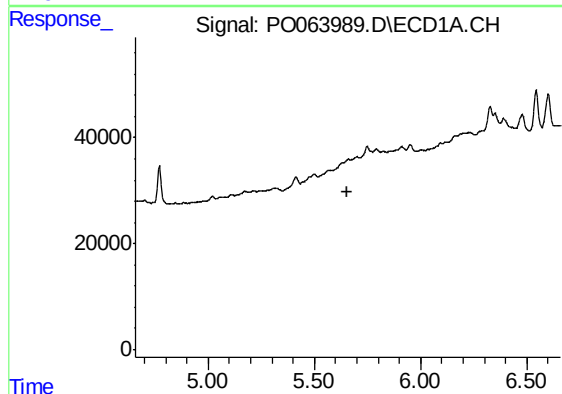


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

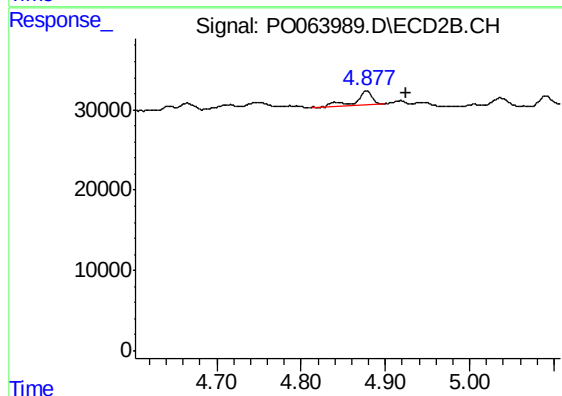

#14 AR-1232-4


R.T.: 4.878 min
Delta R.T.: -0.046 min
Response: 22017
Conc: 46.90 ng/ml



#15 AR-1232-5


R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 426393
Conc: 727.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

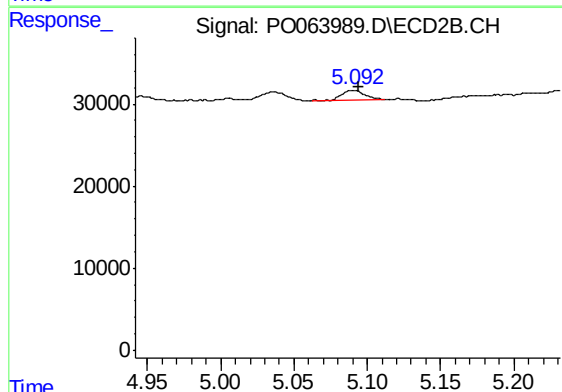


#15 AR-1232-5

R.T.: 5.090 min
Delta R.T.: -0.004 min
Response: 11908
Conc: 23.10 ng/ml




#16 AR-1242-1

R.T.: 5.499 min
Delta R.T.: 0.024 min
Response: 64156
Conc: 60.64 ng/ml

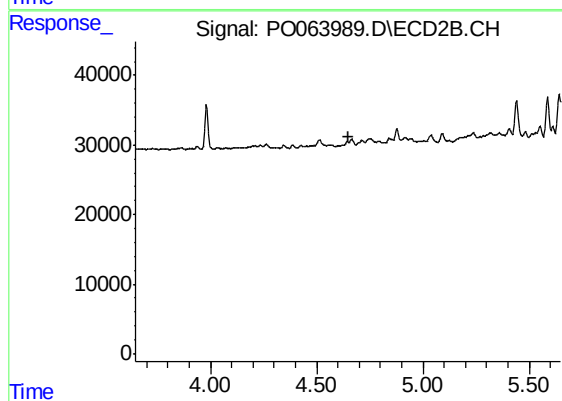

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.647 min
Response: 0
Conc: N.D.



#17 AR-1242-2


R.T.: 5.499 min
Delta R.T.: 0.002 min
Response: 64156
Conc: 42.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

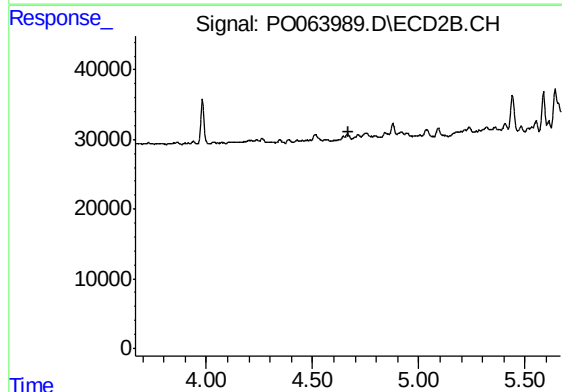


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.666 min
Response: 0
Conc: N.D.

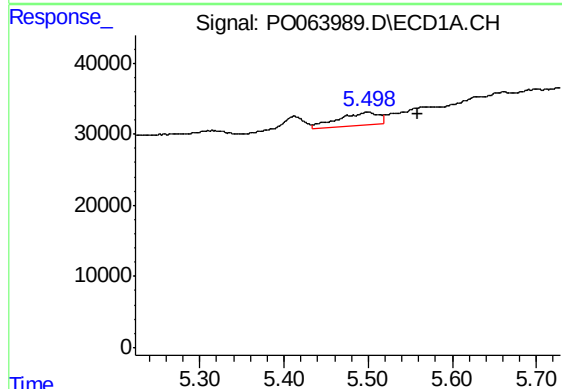


#18 AR-1242-3

R.T.: 5.499 min
Delta R.T.: -0.060 min
Response: 64156
Conc: 67.13 ng/ml

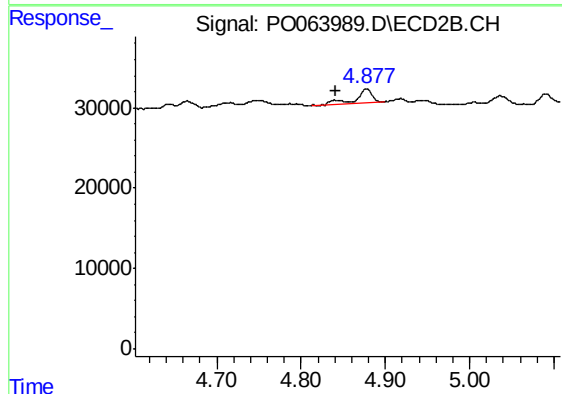

#18 AR-1242-3


R.T.: 4.878 min
Delta R.T.: 0.036 min
Response: 22017
Conc: 38.43 ng/ml



#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

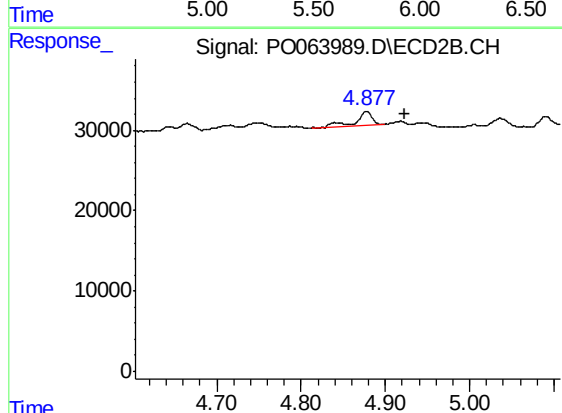


#19 AR-1242-4

R.T.: 4.878 min
Delta R.T.: -0.046 min
Response: 22017
Conc: 38.56 ng/ml

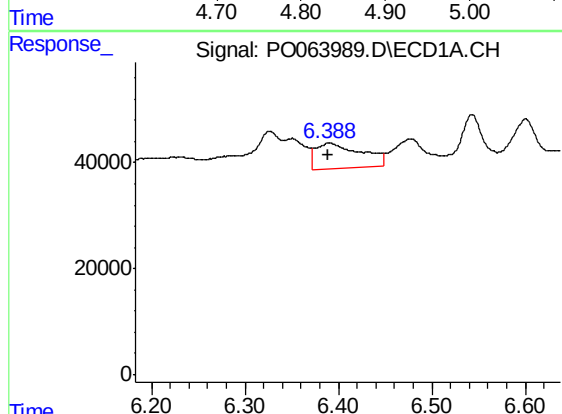


#20 AR-1242-5

R.T.: 6.391 min
Delta R.T.: 0.001 min
Response: 159122
Conc: 153.13 ng/ml

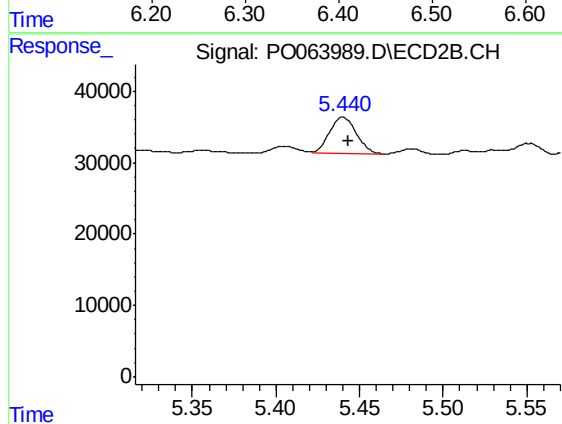

#20 AR-1242-5


R.T.: 5.440 min
Delta R.T.: -0.003 min
Response: 57865
Conc: 74.34 ng/ml

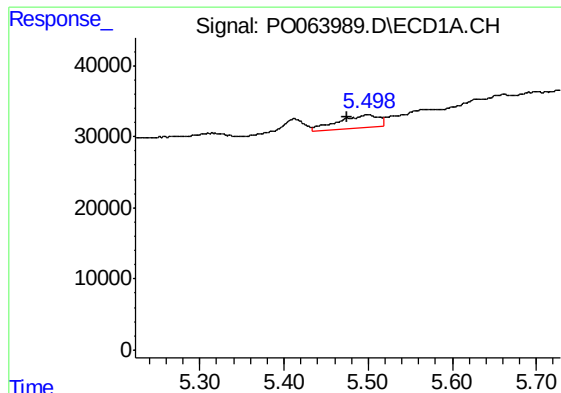

#21 AR-1248-1


R.T.: 5.499 min
Delta R.T.: 0.024 min
Response: 64156
Conc: 73.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

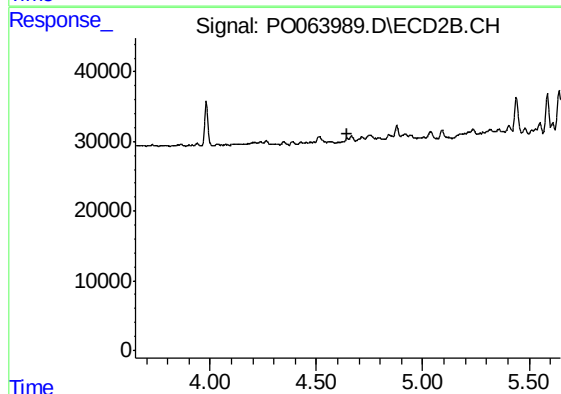


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

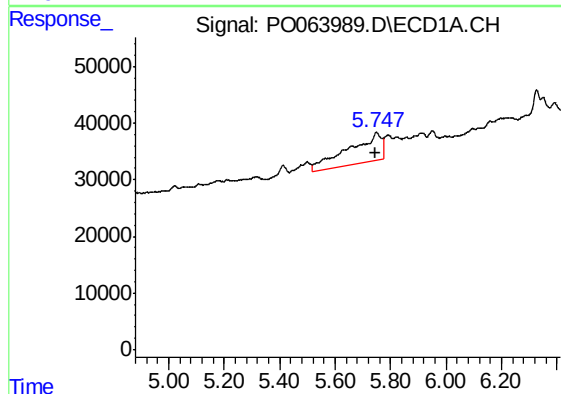


#22 AR-1248-2

R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 426393
Conc: 336.52 ng/ml

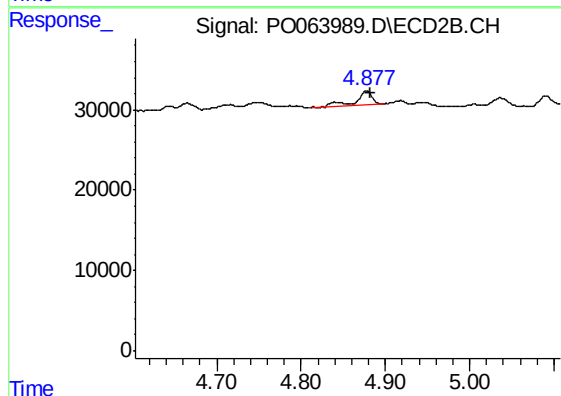

#22 AR-1248-2


R.T.: 4.878 min
Delta R.T.: -0.005 min
Response: 22017
Conc: 25.55 ng/ml



#23 AR-1248-3


R.T.: 5.951 min
Delta R.T.: 0.002 min
Response: 83816
Conc: 58.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

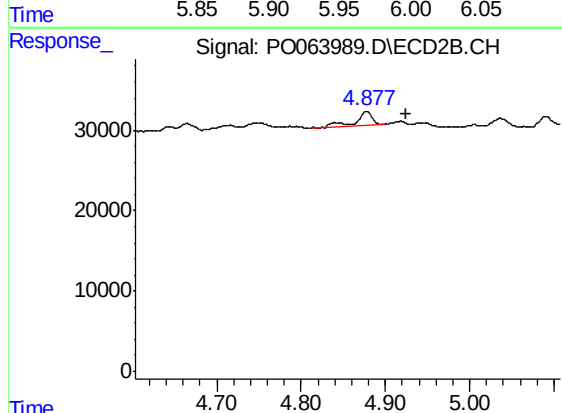


#23 AR-1248-3

R.T.: 4.878 min
Delta R.T.: -0.047 min
Response: 22017
Conc: 24.89 ng/ml

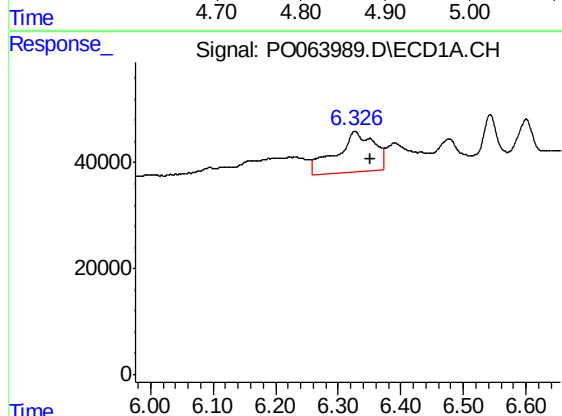


#24 AR-1248-4

R.T.: 6.327 min
Delta R.T.: -0.025 min
Response: 314526
Conc: 181.71 ng/ml

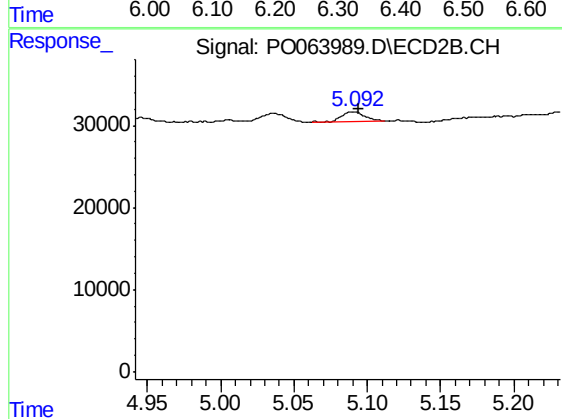

#24 AR-1248-4


R.T.: 5.090 min
Delta R.T.: -0.004 min
Response: 11908
Conc: 11.06 ng/ml

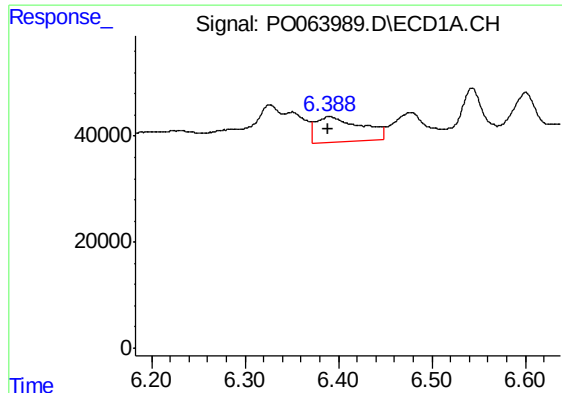

#25 AR-1248-5


R.T.: 6.391 min
Delta R.T.: 0.001 min
Response: 159122
Conc: 94.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

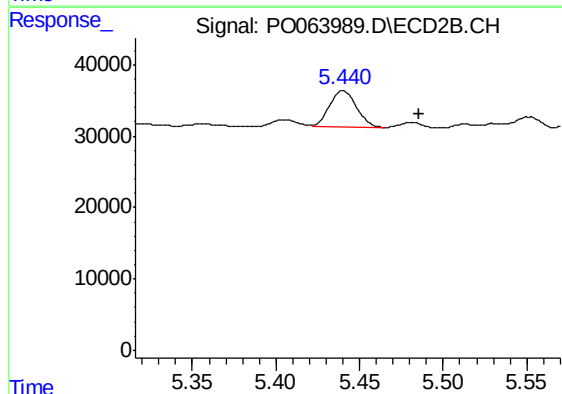


#25 AR-1248-5

R.T.: 5.440 min
Delta R.T.: -0.045 min
Response: 57865
Conc: 51.88 ng/ml

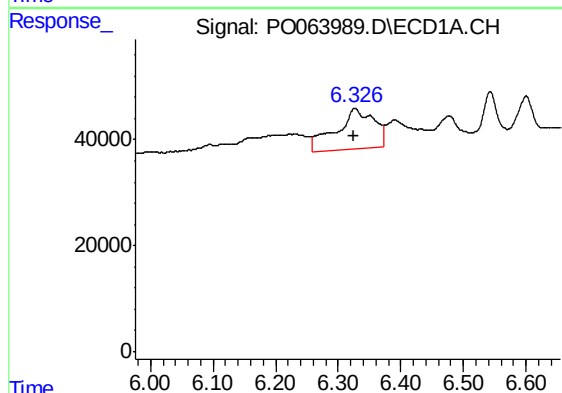


#26 AR-1254-1

R.T.: 6.327 min
Delta R.T.: 0.003 min
Response: 314526
Conc: 180.03 ng/ml

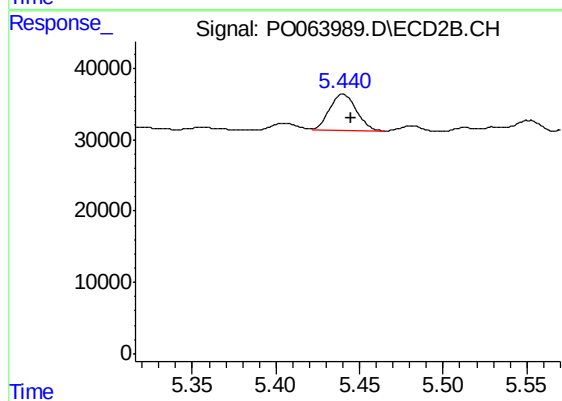

#26 AR-1254-1


R.T.: 5.440 min
Delta R.T.: -0.005 min
Response: 57865
Conc: 32.66 ng/ml

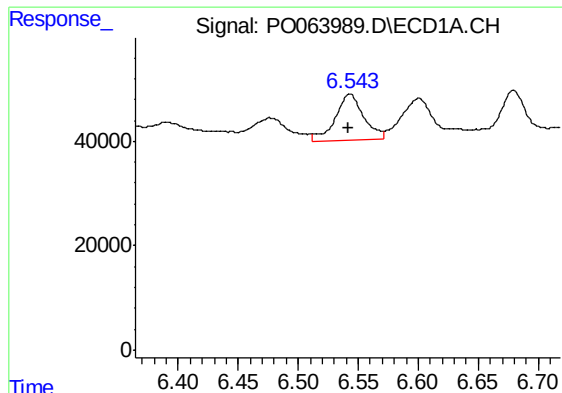

#27 AR-1254-2


R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 146403
Conc: 52.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

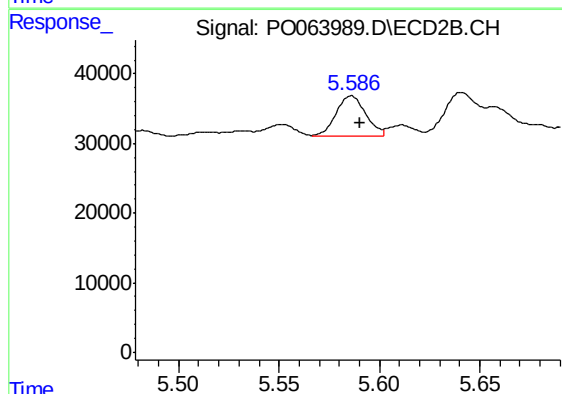


#27 AR-1254-2

R.T.: 5.586 min
Delta R.T.: -0.004 min
Response: 57554
Conc: 36.50 ng/ml

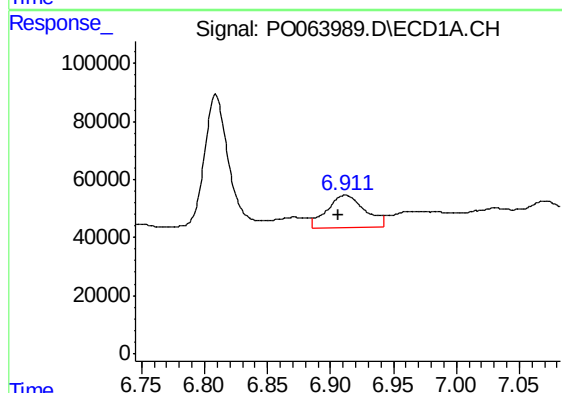


#28 AR-1254-3

R.T.: 6.912 min
Delta R.T.: 0.006 min
Response: 236169
Conc: 75.23 ng/ml

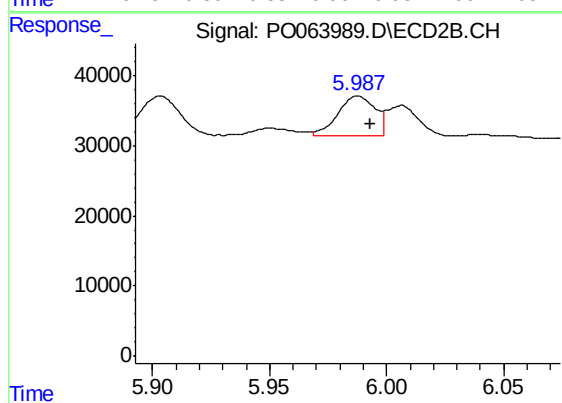

#28 AR-1254-3


R.T.: 5.988 min
Delta R.T.: -0.006 min
Response: 63734
Conc: 23.77 ng/ml

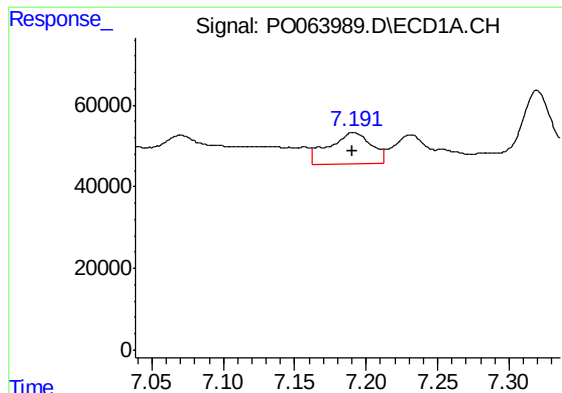

#29 AR-1254-4


R.T.: 7.191 min
Delta R.T.: 0.000 min
Response: 155504
Conc: 62.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

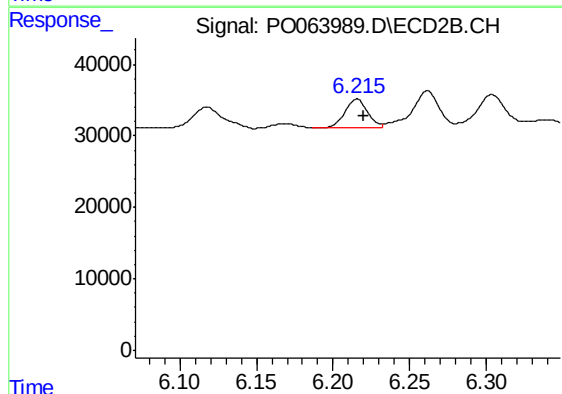


#29 AR-1254-4

R.T.: 6.215 min
Delta R.T.: -0.005 min
Response: 43399
Conc: 24.47 ng/ml

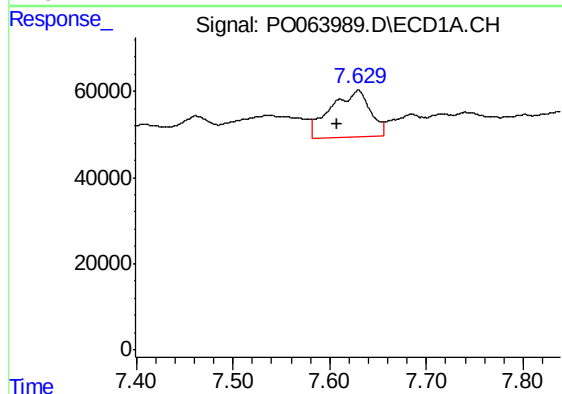


#30 AR-1254-5

R.T.: 7.629 min
Delta R.T.: 0.022 min
Response: 308137
Conc: 113.68 ng/ml

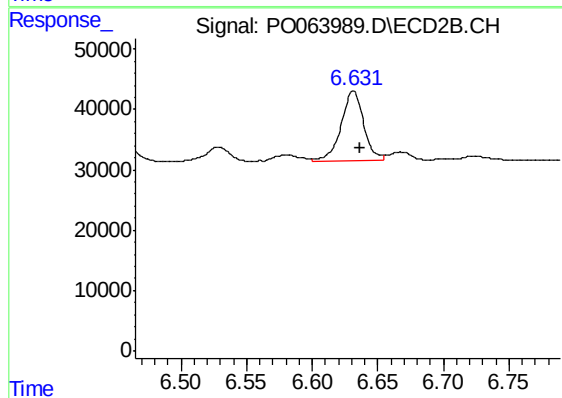

#30 AR-1254-5


R.T.: 6.632 min
Delta R.T.: -0.005 min
Response: 137630
Conc: 55.08 ng/ml

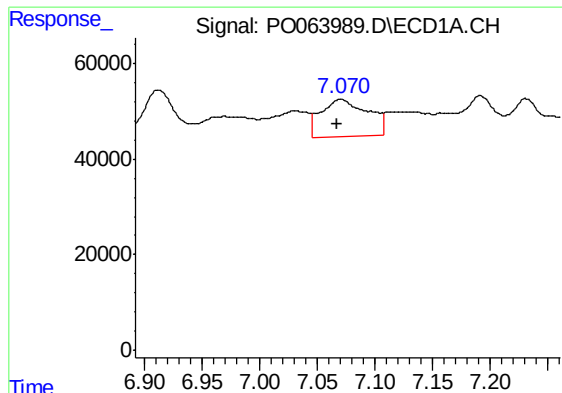

#31 AR-1260-1


R.T.: 7.070 min
Delta R.T.: 0.003 min
Response: 222238
Conc: 110.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

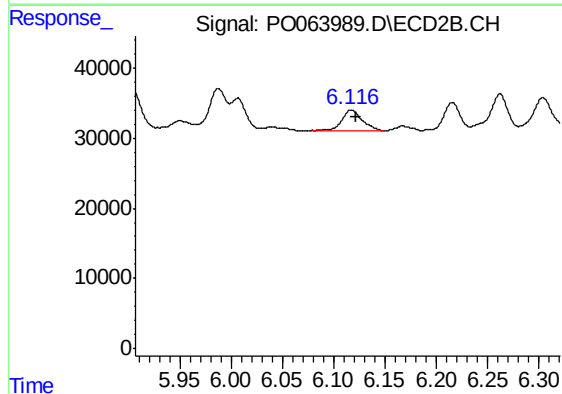


#31 AR-1260-1

R.T.: 6.117 min
Delta R.T.: -0.004 min
Response: 40940
Conc: 26.07 ng/ml

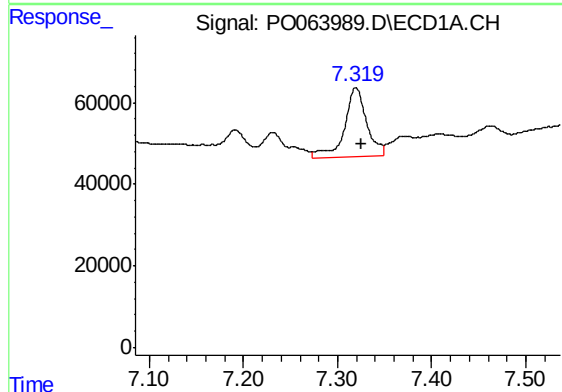


#32 AR-1260-2

R.T.: 7.320 min
Delta R.T.: -0.005 min
Response: 276289
Conc: 109.67 ng/ml

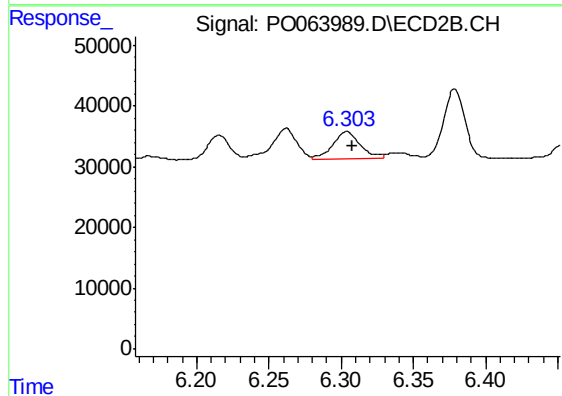

#32 AR-1260-2


R.T.: 6.304 min
Delta R.T.: -0.004 min
Response: 60715
Conc: 30.87 ng/ml

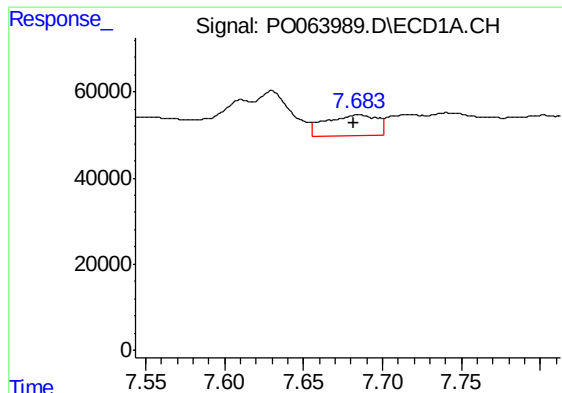

#33 AR-1260-3


R.T.: 7.685 min
Delta R.T.: 0.003 min
Response: 107778
Conc: 53.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

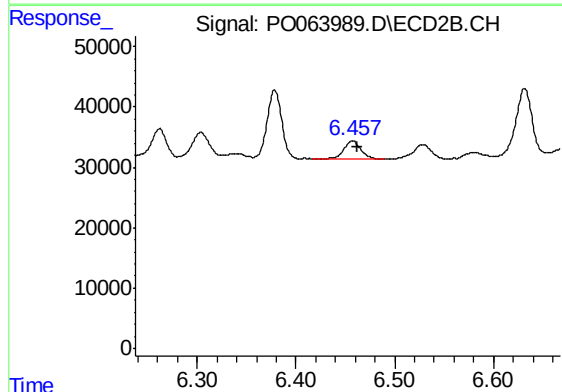


#33 AR-1260-3

R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 36304
Conc: 20.36 ng/ml

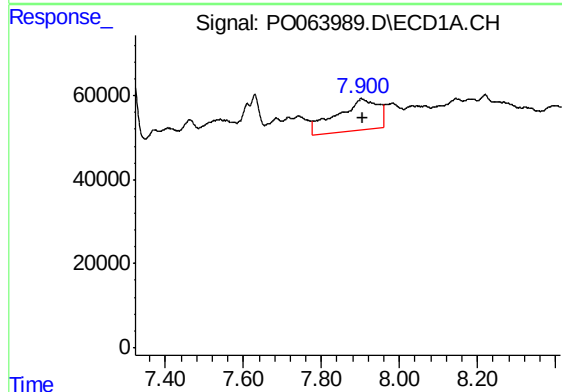


#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.003 min
Response: 545367
Conc: 229.00 ng/ml

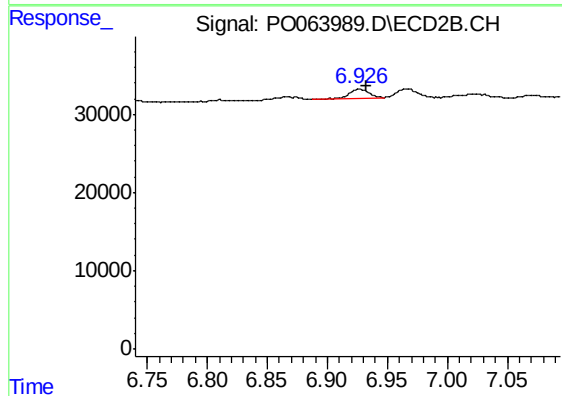

#34 AR-1260-4


R.T.: 6.927 min
Delta R.T.: -0.006 min
Response: 14220
Conc: 9.03 ng/ml

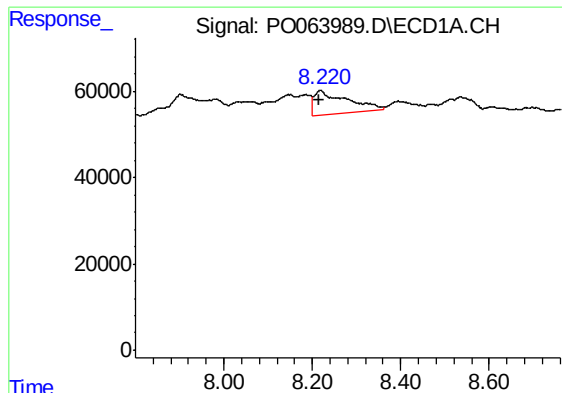

#35 AR-1260-5


R.T.: 8.219 min
Delta R.T.: 0.004 min
Response: 285136
Conc: 60.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

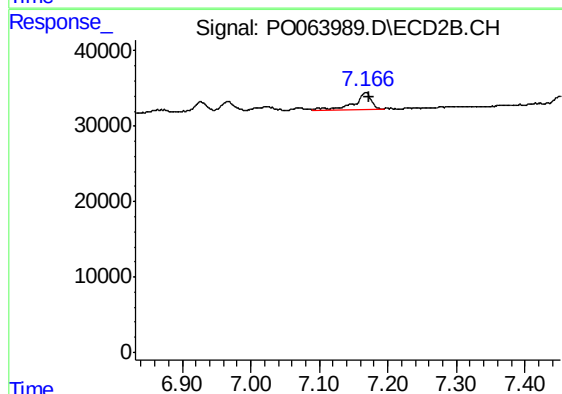


#35 AR-1260-5

R.T.: 7.168 min
Delta R.T.: -0.005 min
Response: 37061
Conc: 9.56 ng/ml

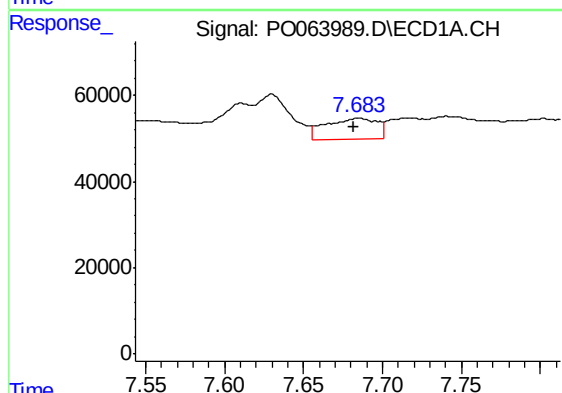


#36 AR-1262-1

R.T.: 7.685 min
Delta R.T.: 0.003 min
Response: 107778
Conc: 33.48 ng/ml

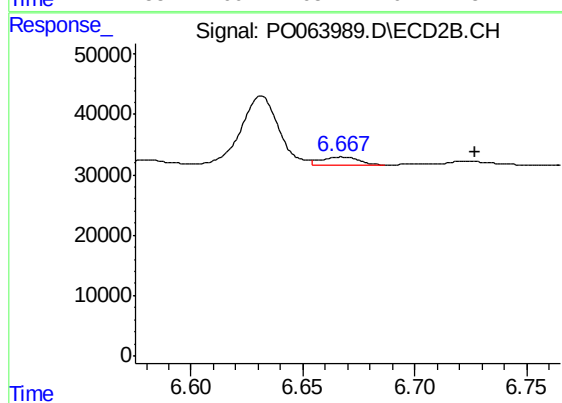

#36 AR-1262-1


R.T.: 6.667 min
Delta R.T.: -0.060 min
Response: 15905
Conc: 15.21 ng/ml

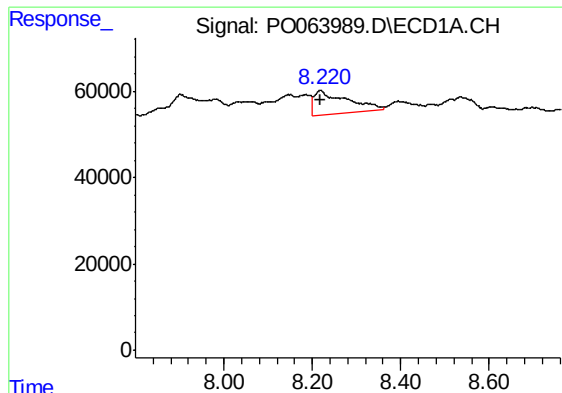

#37 AR-1262-2


R.T.: 8.219 min
Delta R.T.: 0.002 min
Response: 285136
Conc: 48.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

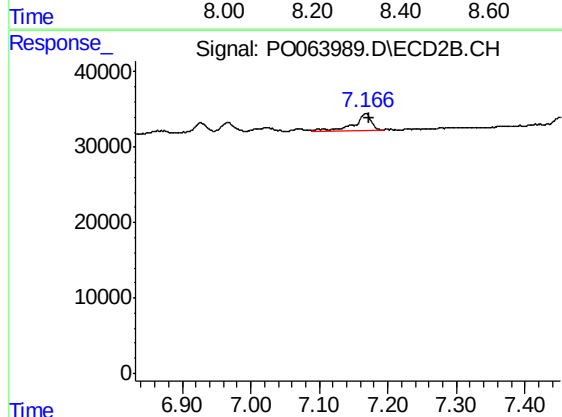


#37 AR-1262-2

R.T.: 7.168 min
Delta R.T.: -0.006 min
Response: 37061
Conc: 7.81 ng/ml

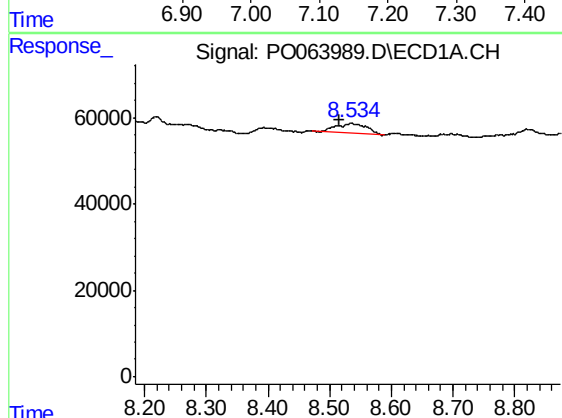


#38 AR-1262-3

R.T.: 8.536 min
Delta R.T.: 0.019 min
Response: 76396
Conc: 18.64 ng/ml

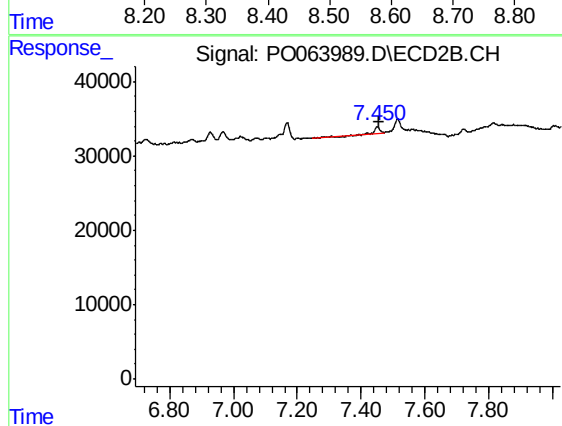

#38 AR-1262-3


R.T.: 7.451 min
Delta R.T.: -0.005 min
Response: 7641
Conc: 4.08 ng/ml

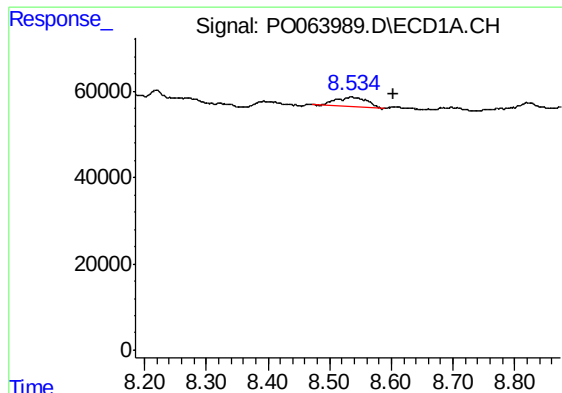

#39 AR-1262-4


R.T.: 8.536 min
Delta R.T.: -0.067 min
Response: 76396
Conc: 24.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

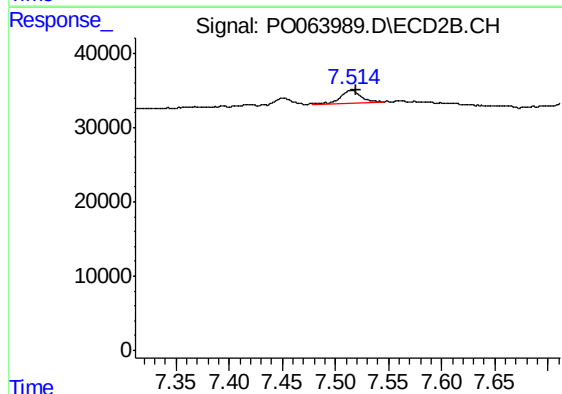


#39 AR-1262-4

R.T.: 7.515 min
Delta R.T.: -0.005 min
Response: 22426
Conc: 6.35 ng/ml

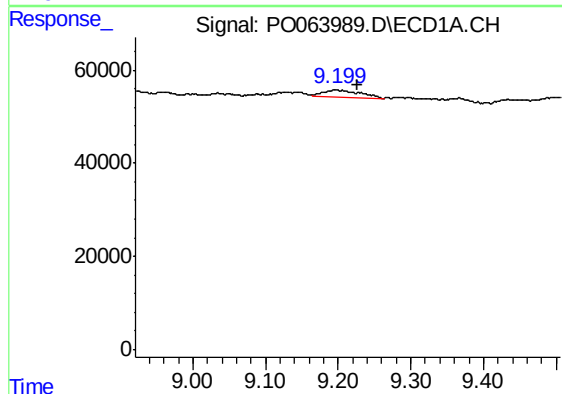


#40 AR-1262-5

R.T.: 9.196 min
Delta R.T.: -0.031 min
Response: 57695
Conc: 26.49 ng/ml

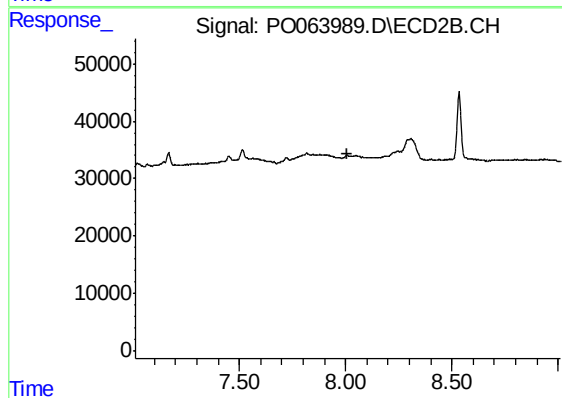

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.011 min
Response: 0
Conc: N.D.



#41 AR-1268-1


R.T.: 8.536 min
Delta R.T.: 0.023 min
Response: 76396
Conc: 11.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

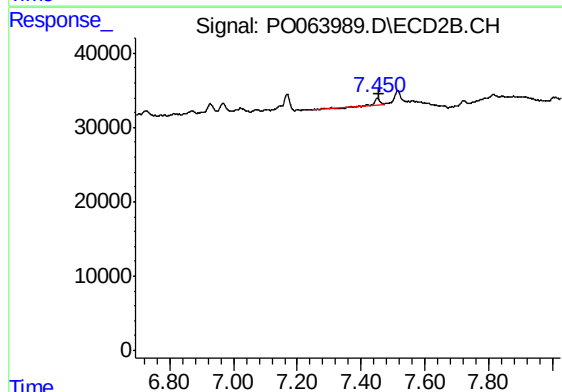


#41 AR-1268-1

R.T.: 7.451 min
Delta R.T.: -0.005 min
Response: 7641
Conc: 1.43 ng/ml

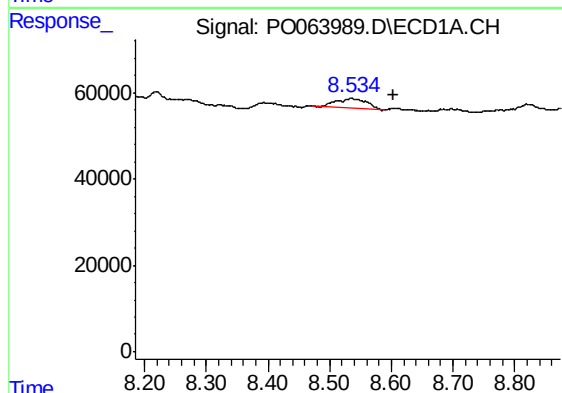


#42 AR-1268-2

R.T.: 8.536 min
Delta R.T.: -0.068 min
Response: 76396
Conc: 12.17 ng/ml

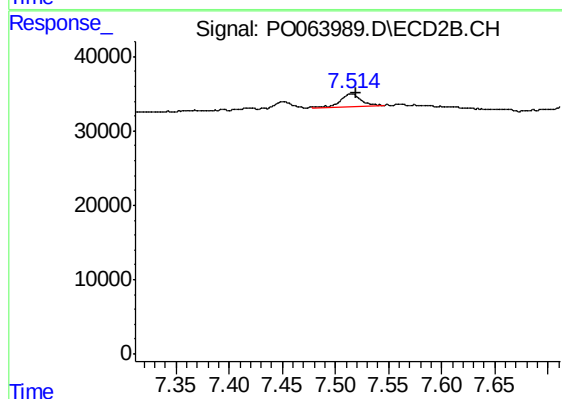

#42 AR-1268-2


R.T.: 7.515 min
Delta R.T.: -0.005 min
Response: 22426
Conc: 4.50 ng/ml

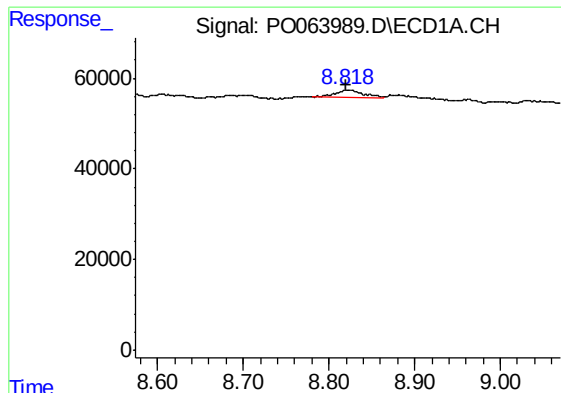

#43 AR-1268-3


R.T.: 8.823 min
Delta R.T.: 0.003 min
Response: 35862
Conc: 6.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

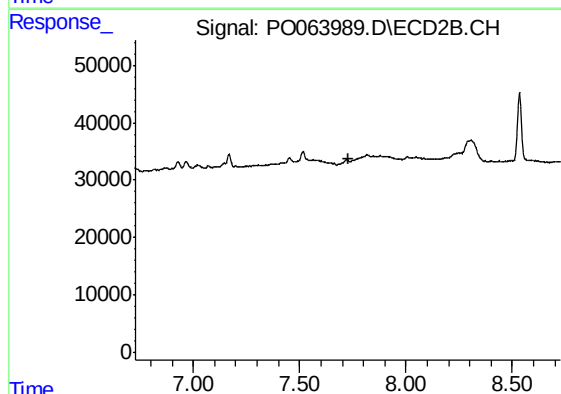


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.727 min
Response: 0
Conc: N.D.

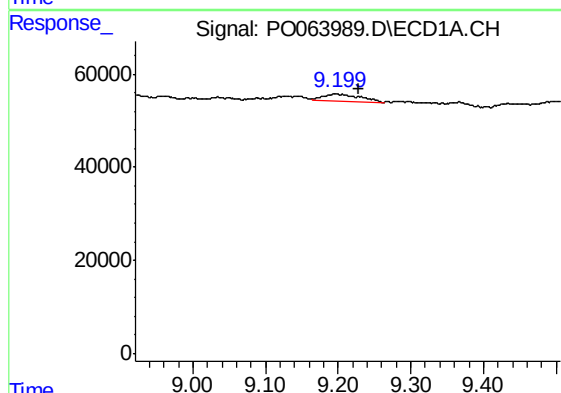


#44 AR-1268-4

R.T.: 9.196 min
Delta R.T.: -0.032 min
Response: 57695
Conc: 23.74 ng/ml

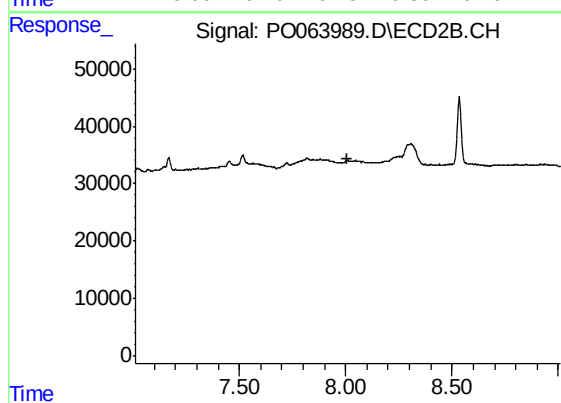

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.010 min
Response: 0
Conc: N.D.



#45 AR-1268-5

R.T.: 9.624 min
Delta R.T.: 0.005 min
Response: 18516
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

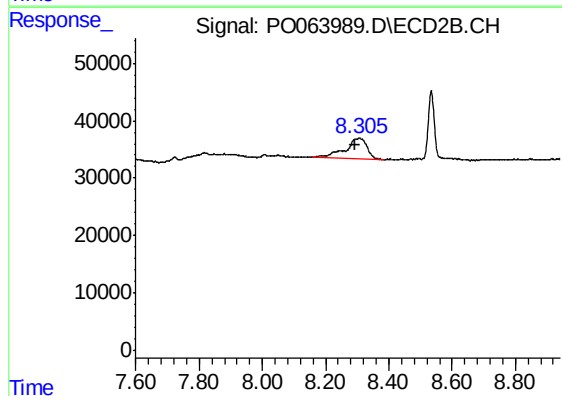

#45 AR-1268-5

R.T.: 8.306 min
Delta R.T.: 0.013 min
Response: 168715
Conc: 14.26 ng/ml