

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063991.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 3:22
 Operator : SM/AJ
 Sample : K5966-07 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110719-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 04:54:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.567	178765	133012	5.847	5.988
2)	SA Decachlor...	9.942	8.536	178365	158230	4.389	5.410
Target Compounds							
3)	L1 AR-1016-1	5.503	4.645	115253	90034	82.987	87.857
4)	L1 AR-1016-2	5.503	4.645	115253	90034	58.720	66.082
5)	L1 AR-1016-3	5.517	4.842	34915	69284	27.950	93.045 #
6)	L1 AR-1016-4	5.616	4.920	122684	70191	119.283	112.665
7)	L1 AR-1016-5	5.952	0.000	110793	0	104.121	N.D. #
9)	L2 AR-1221-2	4.619	3.871	27800	67396	88.631	320.526 #
10)	L2 AR-1221-3	4.619	3.906	27800	52935	29.310	79.411 #
11)	L3 AR-1232-1	4.619	3.906	27800	52935	20.901	56.157 #
12)	L3 AR-1232-2	5.213	4.689	19185	74082	26.902	73.517 #
13)	L3 AR-1232-3	5.503	4.842	115253	69284	80.553	130.899 #
14)	L3 AR-1232-4	5.616	4.920	122684	70191	165.261	149.502
15)	L3 AR-1232-5	5.747	0.000	242947	0	414.453	N.D. #
16)	L4 AR-1242-1	5.503	4.645	115253	90034	108.933	114.136
17)	L4 AR-1242-2	5.503	4.645	115253	90034	76.839	85.049
18)	L4 AR-1242-3	5.517	4.842	34915	69284	36.535	120.929 #
19)	L4 AR-1242-4	5.616	4.920	122684	70191	156.210	122.938
20)	L4 AR-1242-5	6.393	5.441	29129	28014	28.032	35.991 #
21)	L5 AR-1248-1	5.503	4.645	115253	90034	131.970	139.718
22)	L5 AR-1248-2	5.747	4.920	242947	70191	191.742	81.439 #
23)	L5 AR-1248-3	5.952	4.920	110793	70191	77.665	79.334
24)	L5 AR-1248-4	6.353	0.000	30281	0	17.494	N.D. #
25)	L5 AR-1248-5	6.393	5.441	29129	28014	17.270	25.117 #
26)	L6 AR-1254-1	6.326	5.441	73662	28014	42.164	15.811 #
27)	L6 AR-1254-2	6.544	5.587	65759	24585	23.589	15.592 #
28)	L6 AR-1254-3	6.909	5.989	69351	68823	22.091	25.667
29)	L6 AR-1254-4	7.193	6.216	39660	33036	16.040	18.629
30)	L6 AR-1254-5	7.610	6.633	48750	60045	17.985	24.030 #
31)	L7 AR-1260-1	7.071	6.118	34308	27171	17.000	17.302
32)	L7 AR-1260-2	7.323	6.305	64750	30037	25.701	15.269 #
33)	L7 AR-1260-3	7.637	6.458	45990	24778	22.698	13.893 #
34)	L7 AR-1260-4	7.899	6.935	32793	18478	13.770	11.736
35)	L7 AR-1260-5	8.225	7.168	35850	23657	7.637	6.102
36)	L8 AR-1262-1	7.637	0.000	45990	0	14.285	N.D. #
37)	L8 AR-1262-2	8.225	7.168	35850	23657	6.085	4.987
38)	L8 AR-1262-3	8.535	0.000	14244	0	3.476	N.D. #
39)	L8 AR-1262-4	8.535	7.537	14244	138418	4.555	39.207 #
40)	L8 AR-1262-5	9.234	0.000	122555	0	56.260	N.D. #
41)	L9 AR-1268-1	8.535	0.000	14244	0	2.107	N.D. #
42)	L9 AR-1268-2	8.535	7.537	14244	138418	2.270	27.776 #
43)	L9 AR-1268-3	0.000	7.773	0	29684	N.D.	7.478 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063991.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 3:22
 Operator : SM/AJ
 Sample : K5966-07 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110719-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 04:54:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
44) L9	AR-1268-4	9.234	0.000	122555	0	50.418	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063991.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 3:22
Operator : SM/AJ
Sample : K5966-07 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 04:54:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

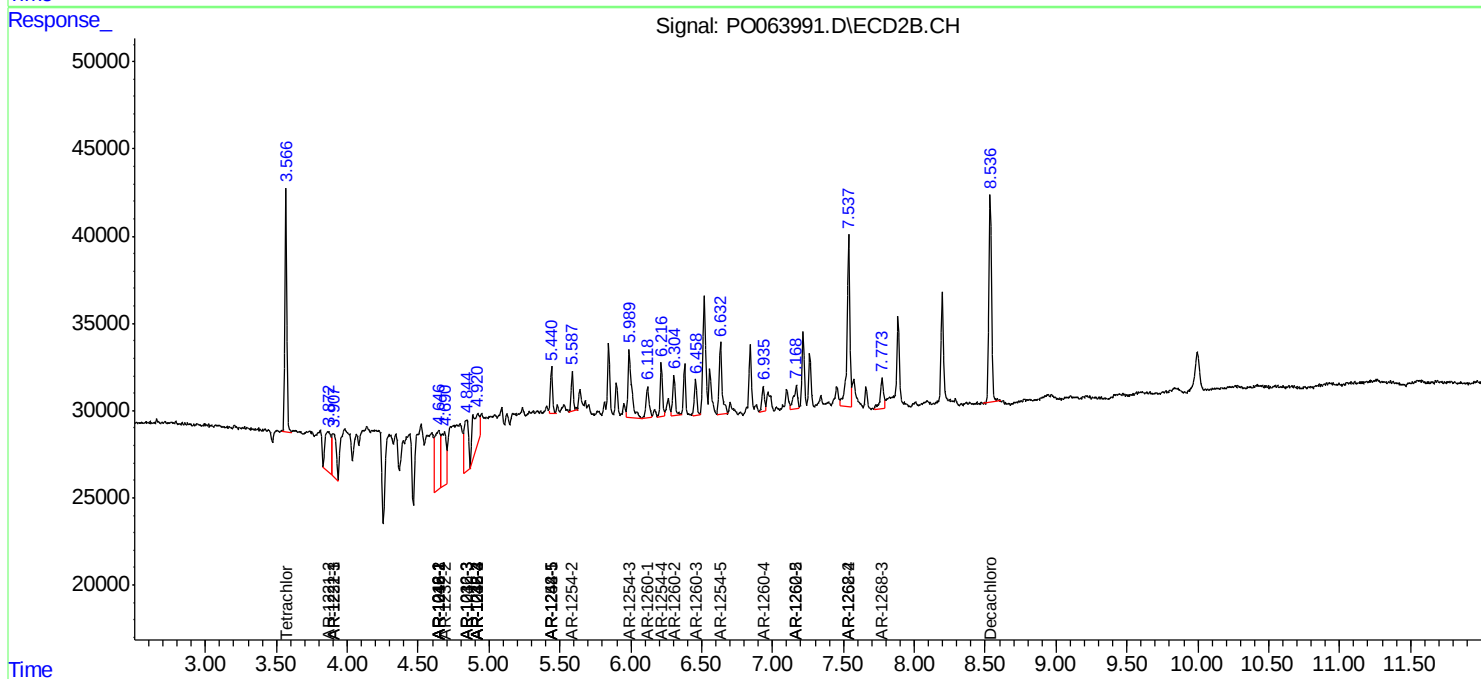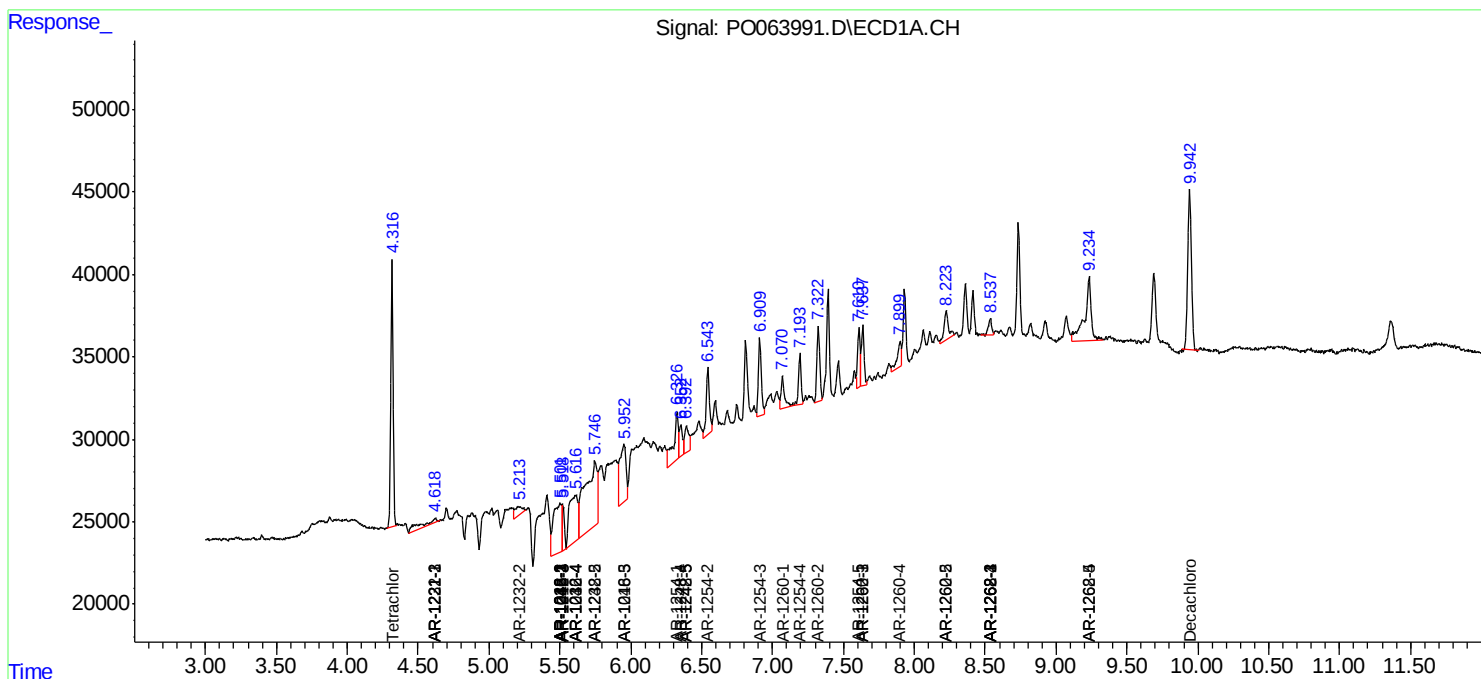


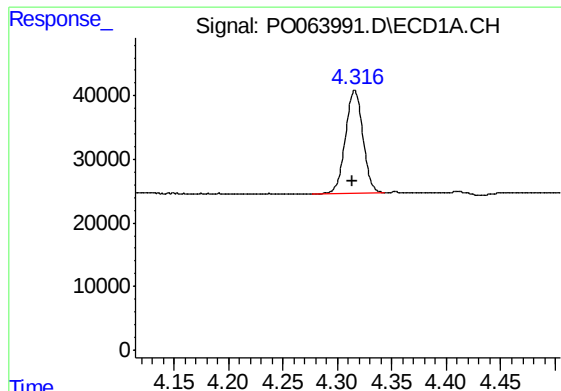

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 178765
Conc: 5.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

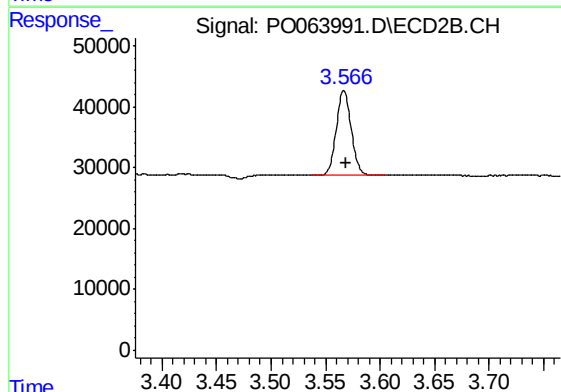


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.002 min
Response: 133012
Conc: 5.99 ng/ml

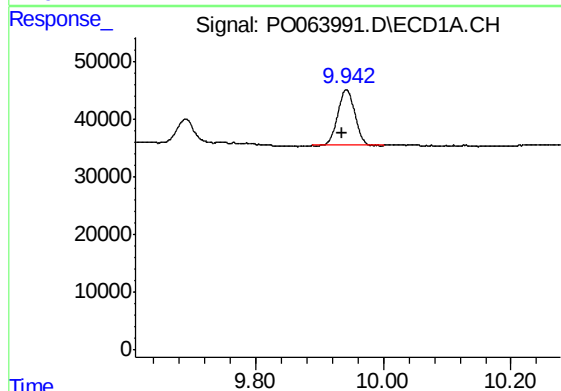


#2 Decachlorobiphenyl

R.T.: 9.942 min
Delta R.T.: 0.006 min
Response: 178365
Conc: 4.39 ng/ml

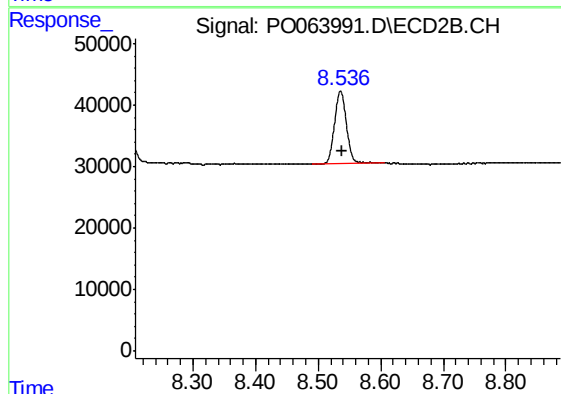

#2 Decachlorobiphenyl


R.T.: 8.536 min
Delta R.T.: -0.004 min
Response: 158230
Conc: 5.41 ng/ml

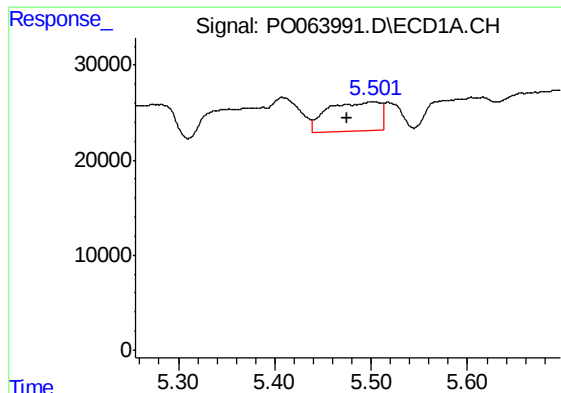

#3 AR-1016-1


R.T.: 5.503 min
Delta R.T.: 0.027 min
Response: 115253
Conc: 82.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

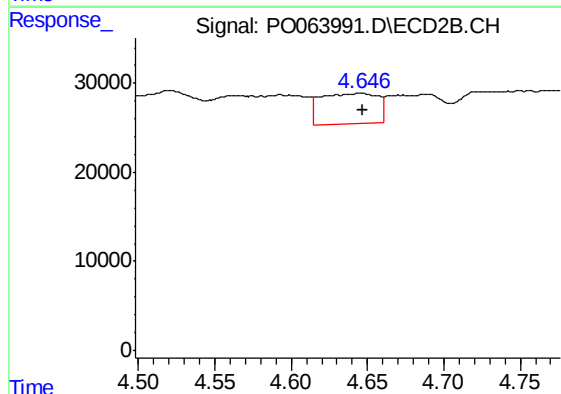


#3 AR-1016-1

R.T.: 4.645 min
Delta R.T.: -0.003 min
Response: 90034
Conc: 87.86 ng/ml

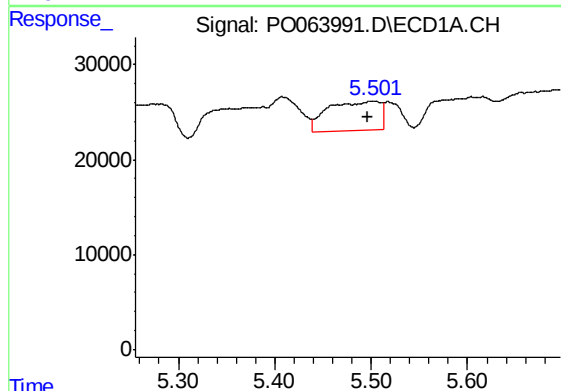


#4 AR-1016-2

R.T.: 5.503 min
Delta R.T.: 0.006 min
Response: 115253
Conc: 58.72 ng/ml

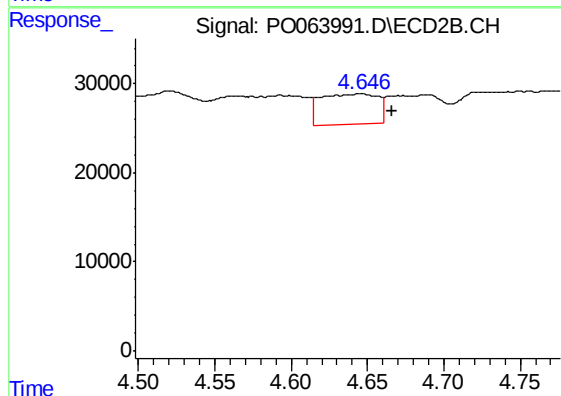

#4 AR-1016-2


R.T.: 4.645 min
Delta R.T.: -0.021 min
Response: 90034
Conc: 66.08 ng/ml

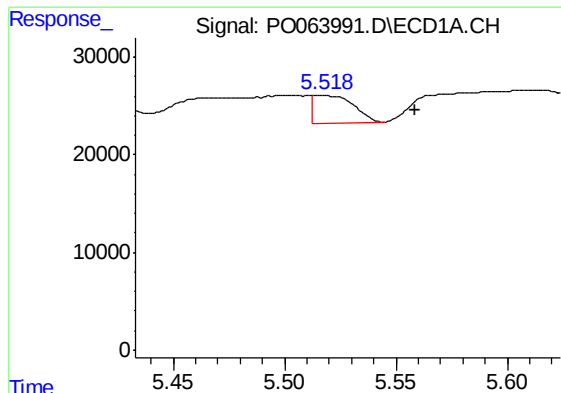

#5 AR-1016-3


R.T.: 5.517 min
Delta R.T.: -0.041 min
Response: 34915
Conc: 27.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

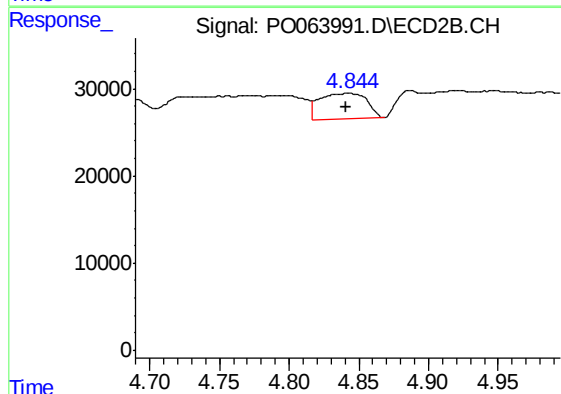


#5 AR-1016-3

R.T.: 4.842 min
Delta R.T.: 0.001 min
Response: 69284
Conc: 93.05 ng/ml

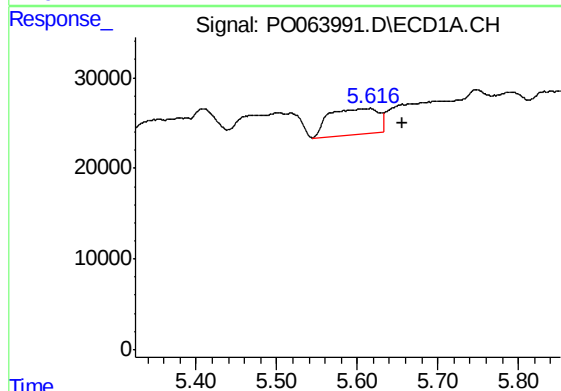


#6 AR-1016-4

R.T.: 5.616 min
Delta R.T.: -0.040 min
Response: 122684
Conc: 119.28 ng/ml

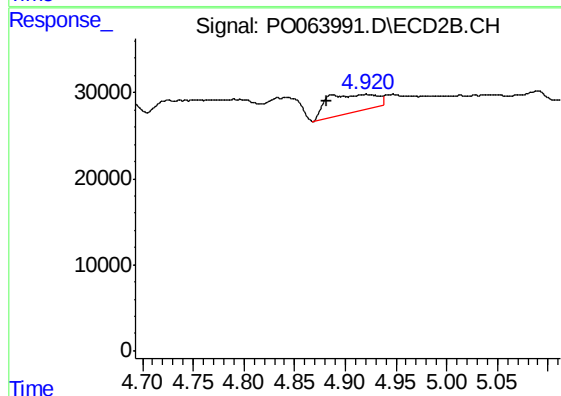

#6 AR-1016-4


R.T.: 4.920 min
Delta R.T.: 0.039 min
Response: 70191
Conc: 112.66 ng/ml



#7 AR-1016-5


R.T.: 5.952 min
Delta R.T.: 0.004 min
Response: 110793
Conc: 104.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.094 min
Response: 0
Conc: N.D.




#9 AR-1221-2

R.T.: 4.619 min
Delta R.T.: 0.009 min
Response: 27800
Conc: 88.63 ng/ml

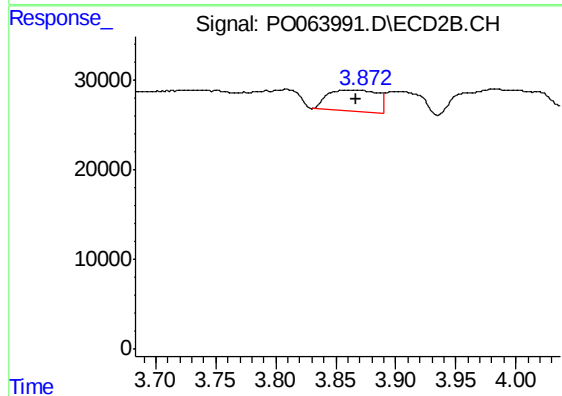

#9 AR-1221-2


R.T.: 3.871 min
Delta R.T.: 0.004 min
Response: 67396
Conc: 320.53 ng/ml



#10 AR-1221-3


R.T.: 4.619 min
Delta R.T.: -0.067 min
Response: 27800
Conc: 29.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#10 AR-1221-3

R.T.: 3.906 min
Delta R.T.: -0.038 min
Response: 52935
Conc: 79.41 ng/ml




#11 AR-1232-1

R.T.: 4.619 min
Delta R.T.: -0.067 min
Response: 27800
Conc: 20.90 ng/ml

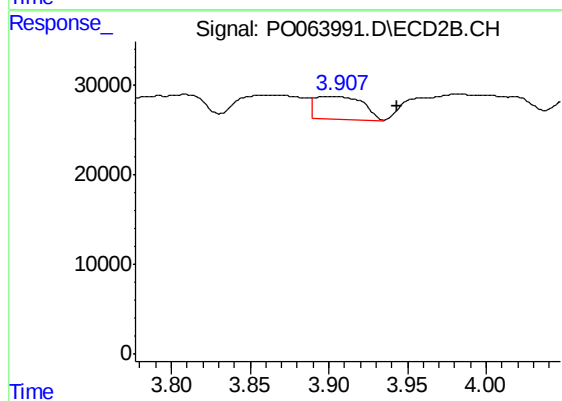

#11 AR-1232-1


R.T.: 3.906 min
Delta R.T.: -0.037 min
Response: 52935
Conc: 56.16 ng/ml

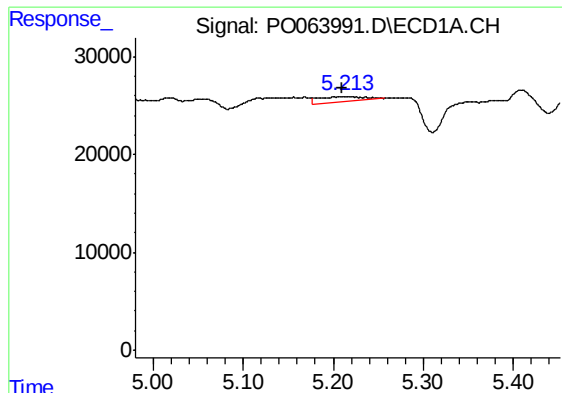

#12 AR-1232-2


R.T.: 5.213 min
Delta R.T.: 0.004 min
Response: 19185
Conc: 26.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

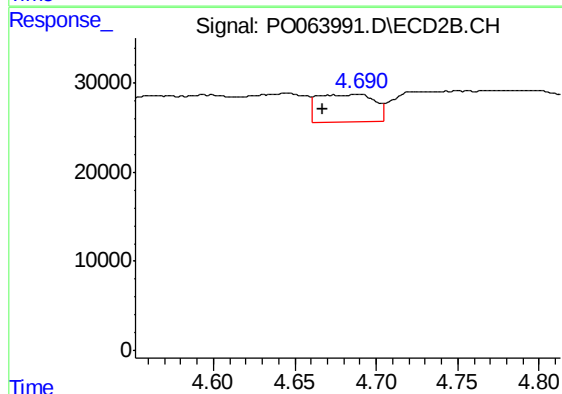


#12 AR-1232-2

R.T.: 4.689 min
Delta R.T.: 0.021 min
Response: 74082
Conc: 73.52 ng/ml




#13 AR-1232-3

R.T.: 5.503 min
Delta R.T.: 0.005 min
Response: 115253
Conc: 80.55 ng/ml

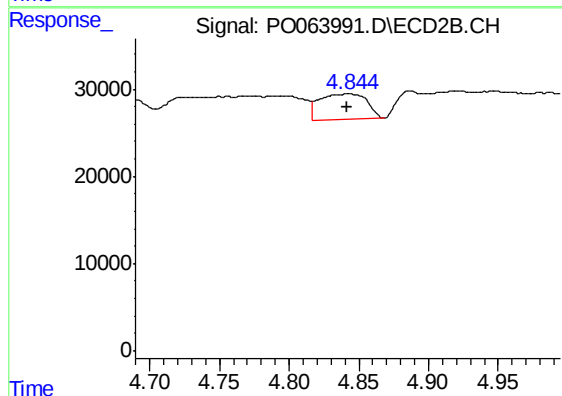

#13 AR-1232-3


R.T.: 4.842 min
Delta R.T.: 0.000 min
Response: 69284
Conc: 130.90 ng/ml



#14 AR-1232-4


R.T.: 5.616 min
Delta R.T.: -0.042 min
Response: 122684
Conc: 165.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#14 AR-1232-4

R.T.: 4.920 min
Delta R.T.: -0.004 min
Response: 70191
Conc: 149.50 ng/ml




#15 AR-1232-5

R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 242947
Conc: 414.45 ng/ml

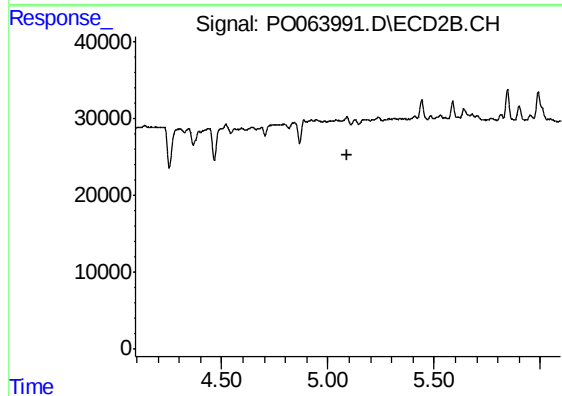

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.094 min
Response: 0
Conc: N.D.

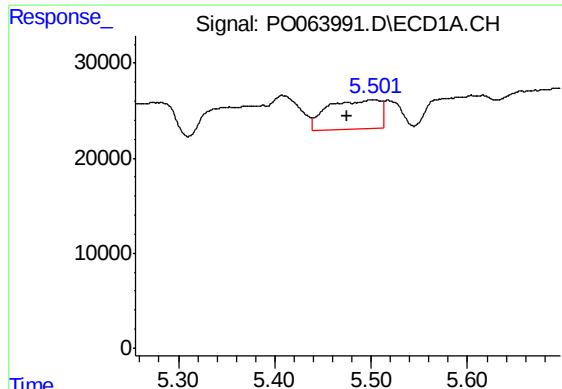

#16 AR-1242-1


R.T.: 5.503 min
Delta R.T.: 0.027 min
Response: 115253
Conc: 108.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#16 AR-1242-1

R.T.: 4.645 min
Delta R.T.: -0.003 min
Response: 90034
Conc: 114.14 ng/ml




#17 AR-1242-2

R.T.: 5.503 min
Delta R.T.: 0.005 min
Response: 115253
Conc: 76.84 ng/ml

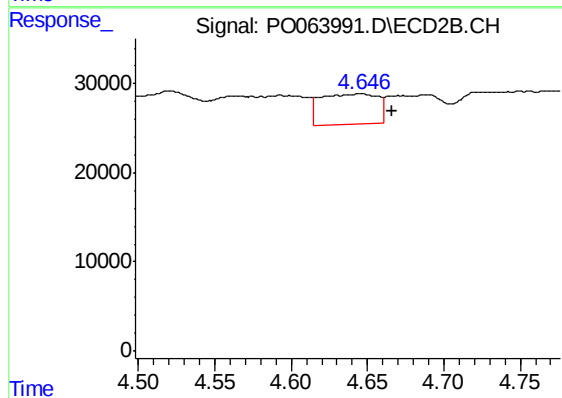

#17 AR-1242-2


R.T.: 4.645 min
Delta R.T.: -0.022 min
Response: 90034
Conc: 85.05 ng/ml

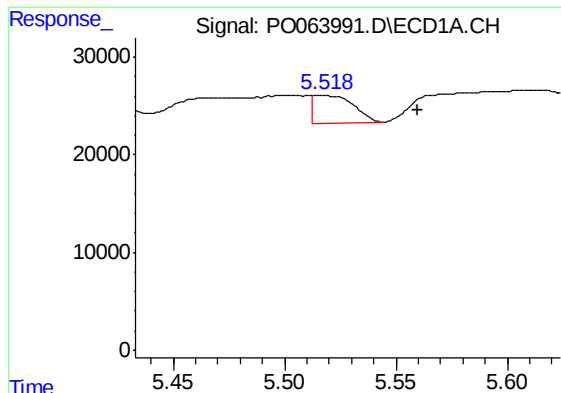

#18 AR-1242-3


R.T.: 5.517 min
Delta R.T.: -0.042 min
Response: 34915
Conc: 36.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

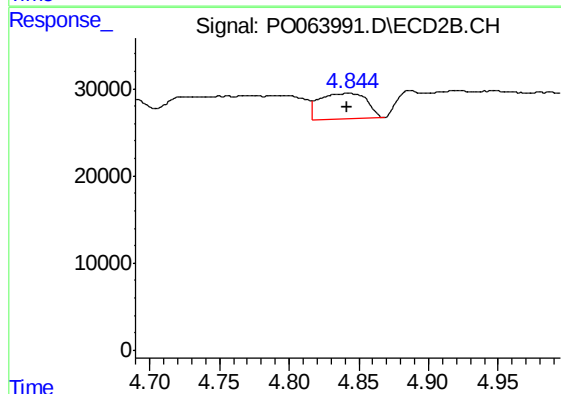


#18 AR-1242-3

R.T.: 4.842 min
Delta R.T.: 0.000 min
Response: 69284
Conc: 120.93 ng/ml

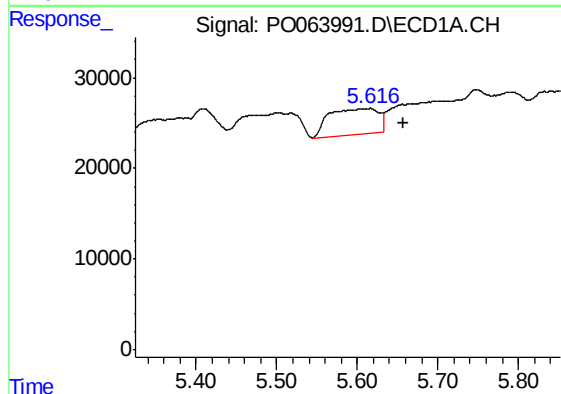


#19 AR-1242-4

R.T.: 5.616 min
Delta R.T.: -0.042 min
Response: 122684
Conc: 156.21 ng/ml

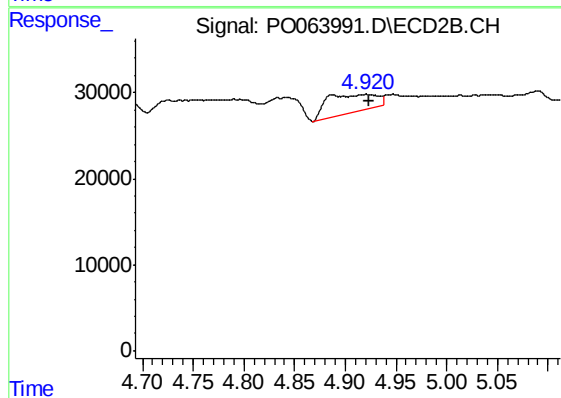

#19 AR-1242-4


R.T.: 4.920 min
Delta R.T.: -0.003 min
Response: 70191
Conc: 122.94 ng/ml



#20 AR-1242-5


R.T.: 6.393 min
Delta R.T.: 0.003 min
Response: 29129
Conc: 28.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#20 AR-1242-5

R.T.: 5.441 min
Delta R.T.: -0.002 min
Response: 28014
Conc: 35.99 ng/ml




#21 AR-1248-1

R.T.: 5.503 min
Delta R.T.: 0.027 min
Response: 115253
Conc: 131.97 ng/ml

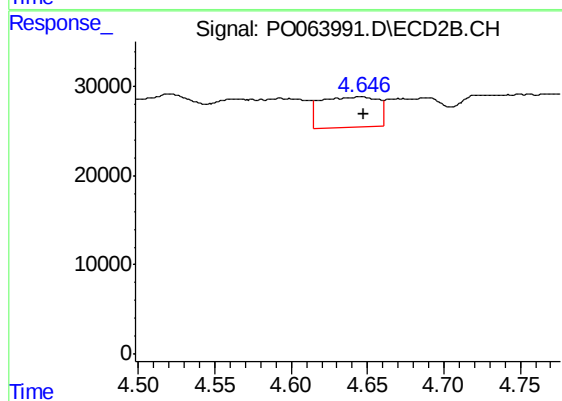

#21 AR-1248-1


R.T.: 4.645 min
Delta R.T.: -0.003 min
Response: 90034
Conc: 139.72 ng/ml

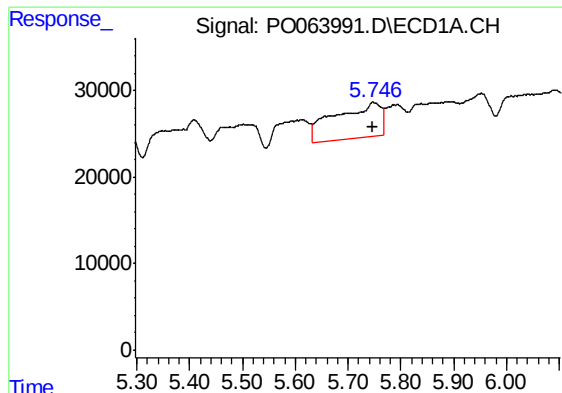

#22 AR-1248-2


R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 242947
Conc: 191.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

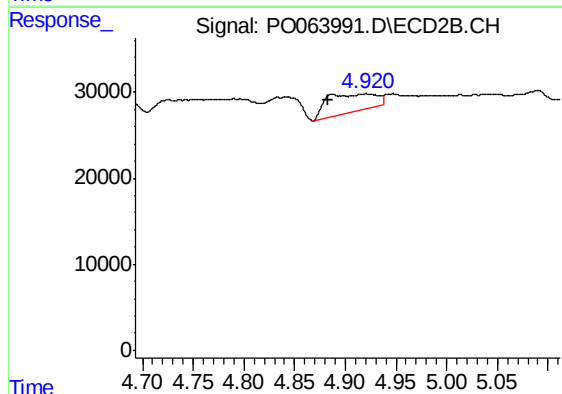


#22 AR-1248-2

R.T.: 4.920 min
Delta R.T.: 0.038 min
Response: 70191
Conc: 81.44 ng/ml

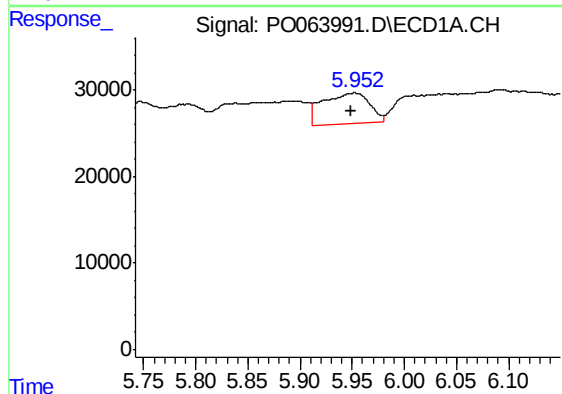


#23 AR-1248-3

R.T.: 5.952 min
Delta R.T.: 0.003 min
Response: 110793
Conc: 77.67 ng/ml

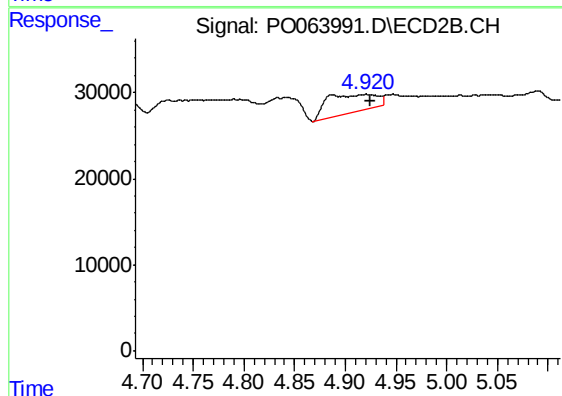

#23 AR-1248-3


R.T.: 4.920 min
Delta R.T.: -0.004 min
Response: 70191
Conc: 79.33 ng/ml

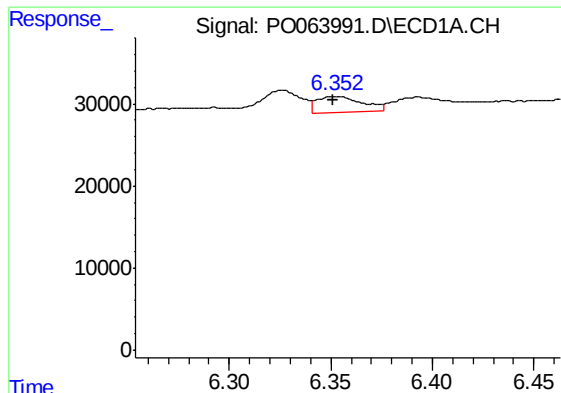

#24 AR-1248-4


R.T.: 6.353 min
Delta R.T.: 0.001 min
Response: 30281
Conc: 17.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

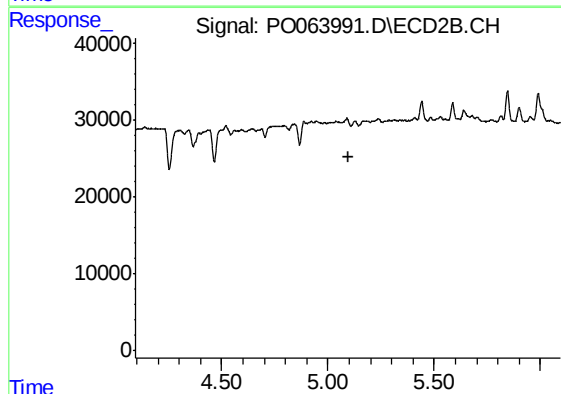


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.095 min
Response: 0
Conc: N.D.

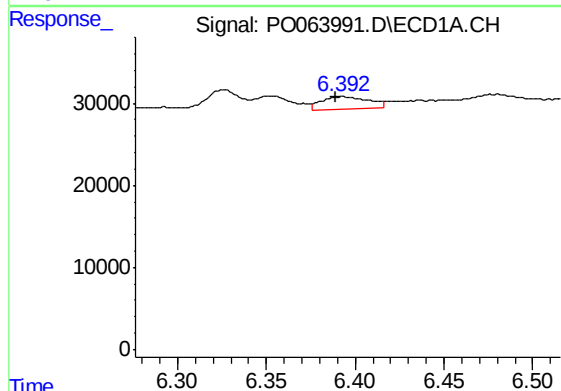


#25 AR-1248-5

R.T.: 6.393 min
Delta R.T.: 0.003 min
Response: 29129
Conc: 17.27 ng/ml

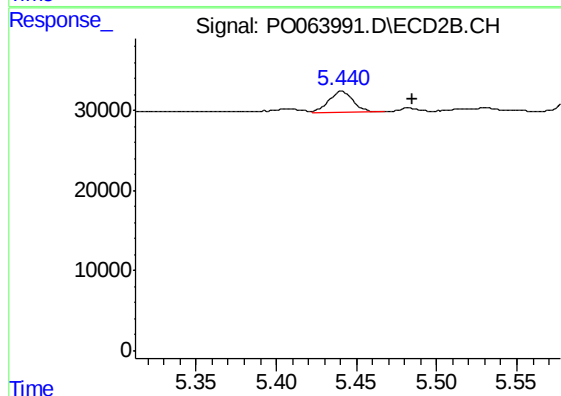

#25 AR-1248-5


R.T.: 5.441 min
Delta R.T.: -0.045 min
Response: 28014
Conc: 25.12 ng/ml

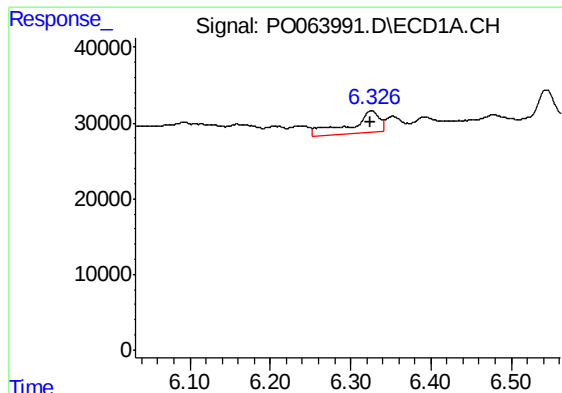

#26 AR-1254-1


R.T.: 6.326 min
Delta R.T.: 0.002 min
Response: 73662
Conc: 42.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

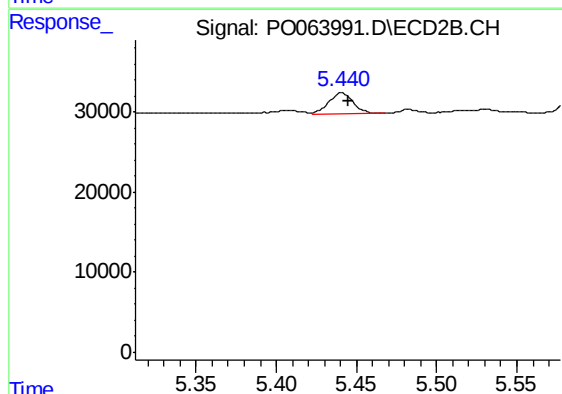


#26 AR-1254-1

R.T.: 5.441 min
Delta R.T.: -0.004 min
Response: 28014
Conc: 15.81 ng/ml

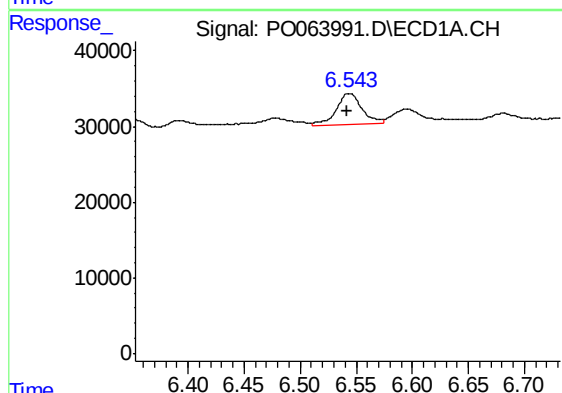


#27 AR-1254-2

R.T.: 6.544 min
Delta R.T.: 0.002 min
Response: 65759
Conc: 23.59 ng/ml

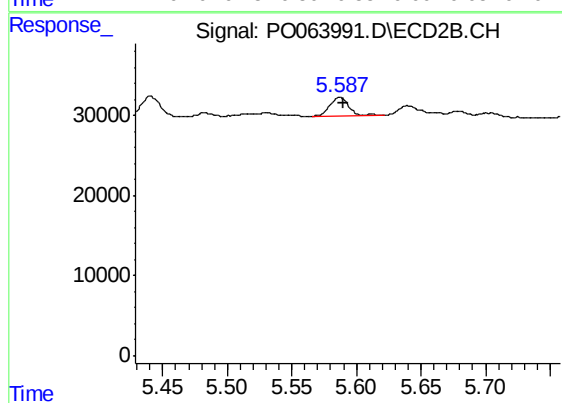

#27 AR-1254-2


R.T.: 5.587 min
Delta R.T.: -0.003 min
Response: 24585
Conc: 15.59 ng/ml



#28 AR-1254-3


R.T.: 6.909 min
Delta R.T.: 0.003 min
Response: 69351
Conc: 22.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

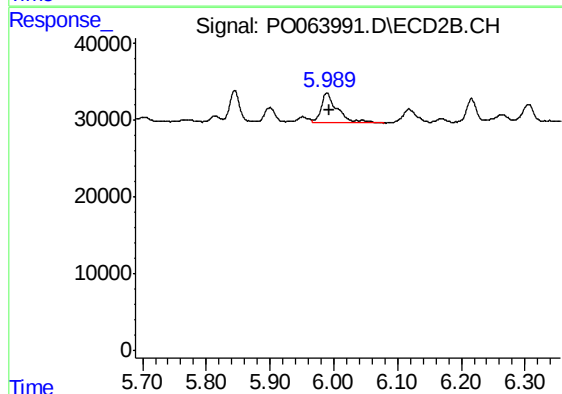


#28 AR-1254-3

R.T.: 5.989 min
Delta R.T.: -0.004 min
Response: 68823
Conc: 25.67 ng/ml




#29 AR-1254-4

R.T.: 7.193 min
Delta R.T.: 0.002 min
Response: 39660
Conc: 16.04 ng/ml

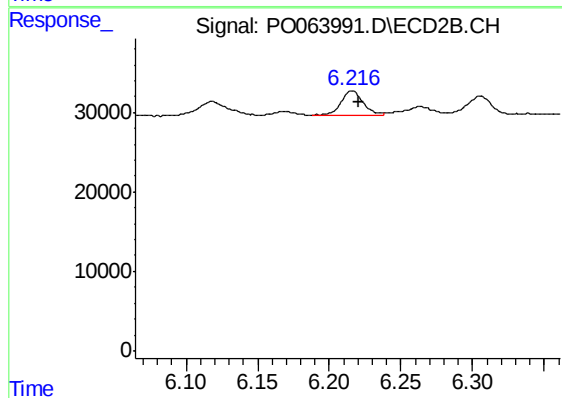

#29 AR-1254-4


R.T.: 6.216 min
Delta R.T.: -0.004 min
Response: 33036
Conc: 18.63 ng/ml



#30 AR-1254-5


R.T.: 7.610 min
Delta R.T.: 0.002 min
Response: 48750
Conc: 17.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

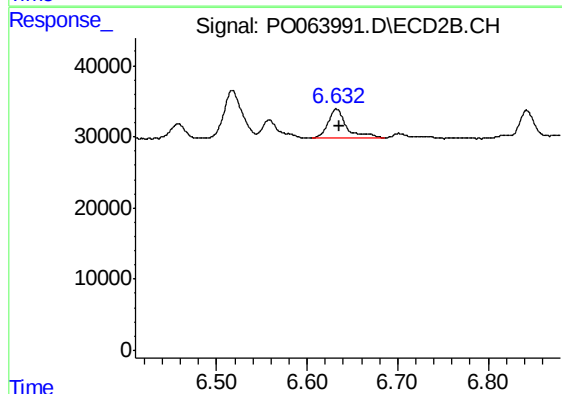


#30 AR-1254-5

R.T.: 6.633 min
Delta R.T.: -0.004 min
Response: 60045
Conc: 24.03 ng/ml




#31 AR-1260-1

R.T.: 7.071 min
Delta R.T.: 0.003 min
Response: 34308
Conc: 17.00 ng/ml

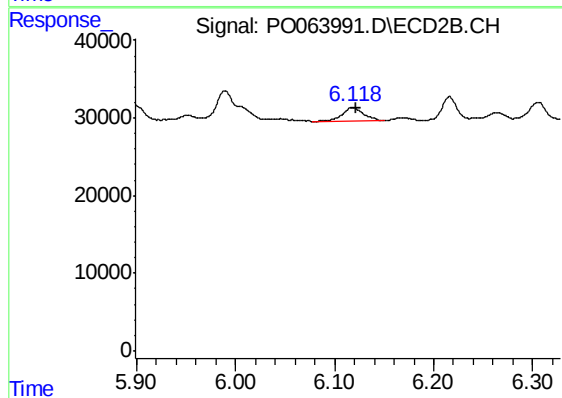

#31 AR-1260-1


R.T.: 6.118 min
Delta R.T.: -0.003 min
Response: 27171
Conc: 17.30 ng/ml

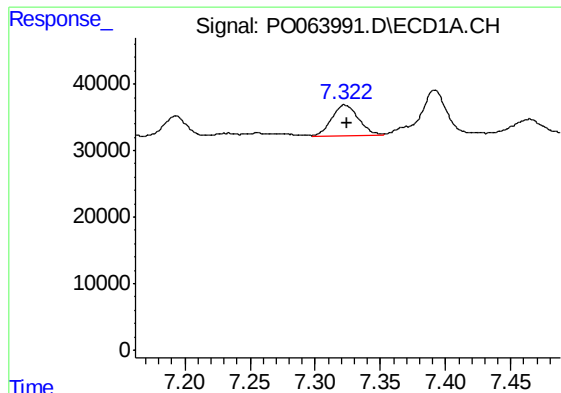

#32 AR-1260-2


R.T.: 7.323 min
Delta R.T.: -0.002 min
Response: 64750
Conc: 25.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

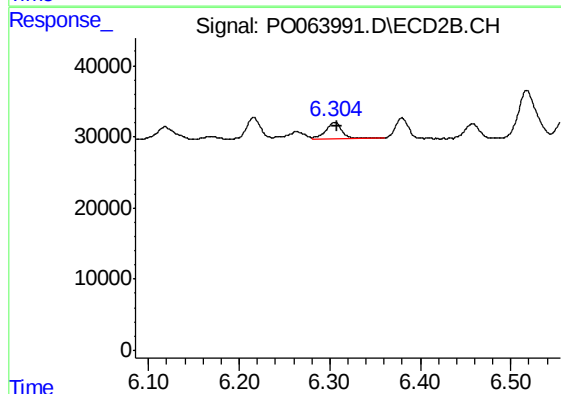


#32 AR-1260-2

R.T.: 6.305 min
Delta R.T.: -0.002 min
Response: 30037
Conc: 15.27 ng/ml

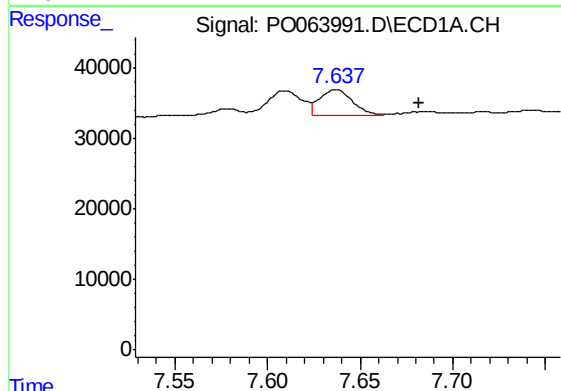


#33 AR-1260-3

R.T.: 7.637 min
Delta R.T.: -0.045 min
Response: 45990
Conc: 22.70 ng/ml

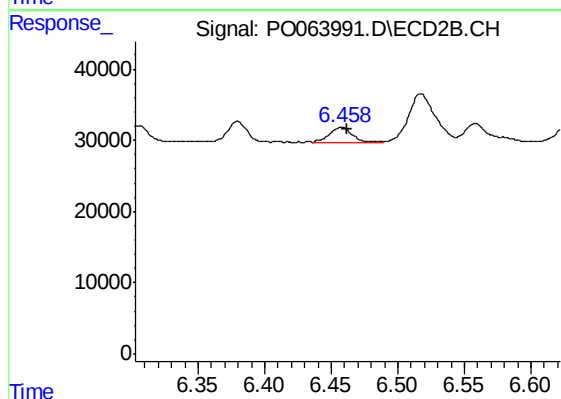

#33 AR-1260-3


R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 24778
Conc: 13.89 ng/ml

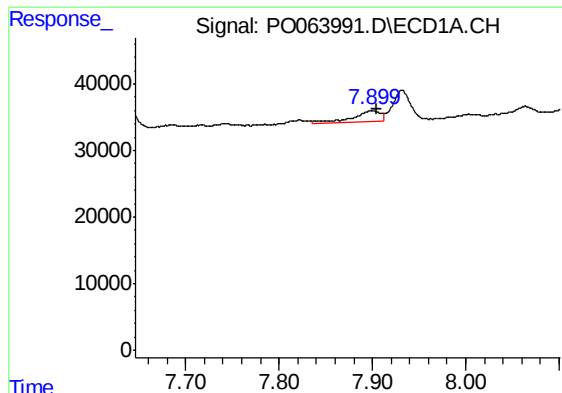

#34 AR-1260-4


R.T.: 7.899 min
Delta R.T.: -0.006 min
Response: 32793
Conc: 13.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

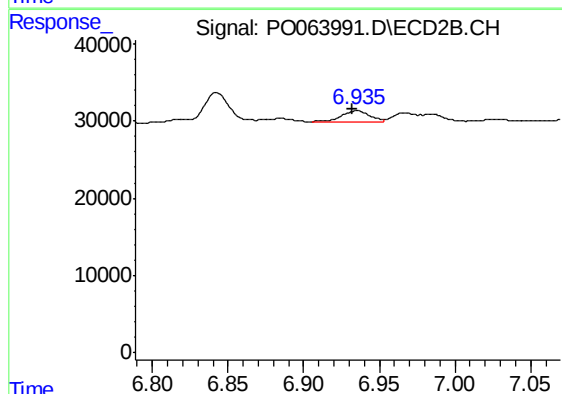


#34 AR-1260-4

R.T.: 6.935 min
Delta R.T.: 0.003 min
Response: 18478
Conc: 11.74 ng/ml

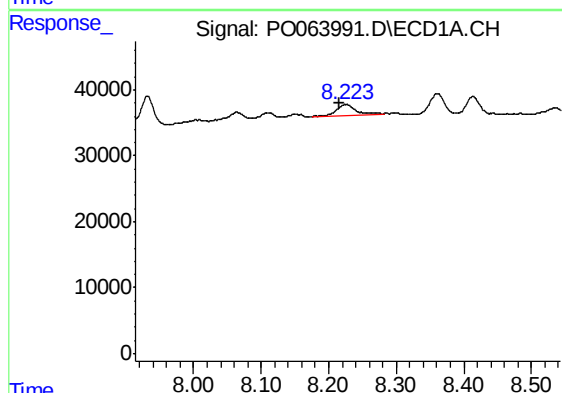


#35 AR-1260-5

R.T.: 8.225 min
Delta R.T.: 0.010 min
Response: 35850
Conc: 7.64 ng/ml

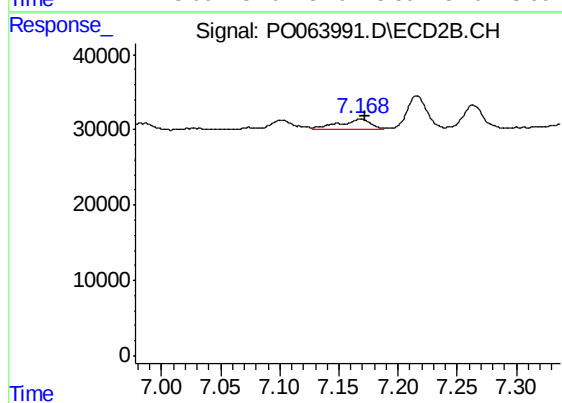

#35 AR-1260-5


R.T.: 7.168 min
Delta R.T.: -0.004 min
Response: 23657
Conc: 6.10 ng/ml

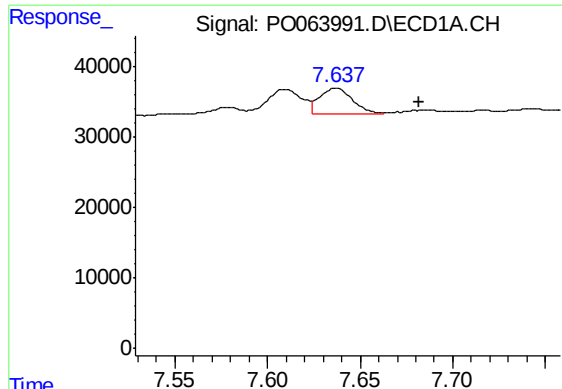

#36 AR-1262-1


R.T.: 7.637 min
Delta R.T.: -0.045 min
Response: 45990
Conc: 14.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.727 min
Response: 0
Conc: N.D.




#37 AR-1262-2

R.T.: 8.225 min
Delta R.T.: 0.008 min
Response: 35850
Conc: 6.09 ng/ml

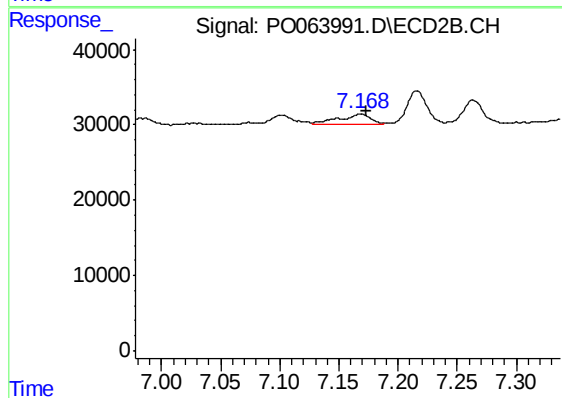

#37 AR-1262-2


R.T.: 7.168 min
Delta R.T.: -0.005 min
Response: 23657
Conc: 4.99 ng/ml



#38 AR-1262-3


R.T.: 8.535 min
Delta R.T.: 0.019 min
Response: 14244
Conc: 3.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.456 min
Response: 0
Conc: N.D.




#39 AR-1262-4

R.T.: 8.535 min
Delta R.T.: -0.067 min
Response: 14244
Conc: 4.55 ng/ml

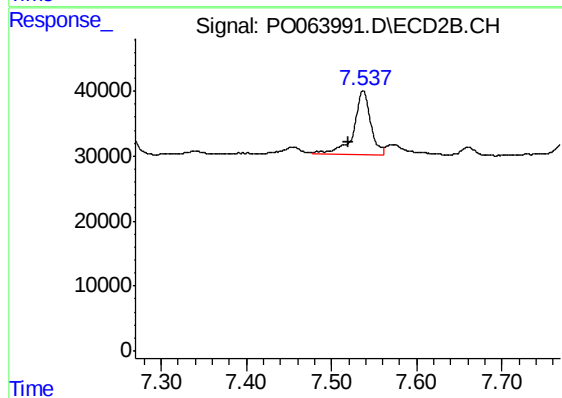

#39 AR-1262-4


R.T.: 7.537 min
Delta R.T.: 0.017 min
Response: 138418
Conc: 39.21 ng/ml



#40 AR-1262-5


R.T.: 9.234 min
Delta R.T.: 0.006 min
Response: 122555
Conc: 56.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07




#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.011 min
Response: 0
Conc: N.D.




#41 AR-1268-1

R.T.: 8.535 min
Delta R.T.: 0.022 min
Response: 14244
Conc: 2.11 ng/ml

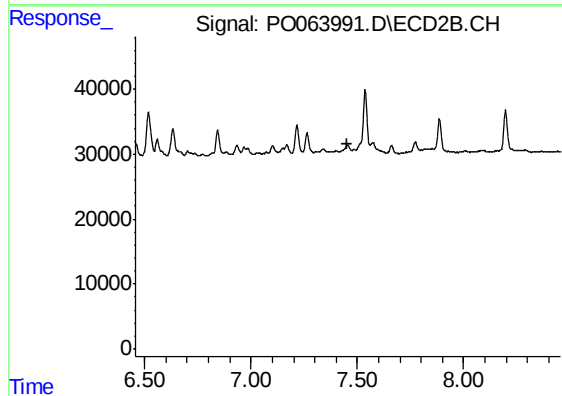

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 7.456 min
Response: 0
Conc: N.D.

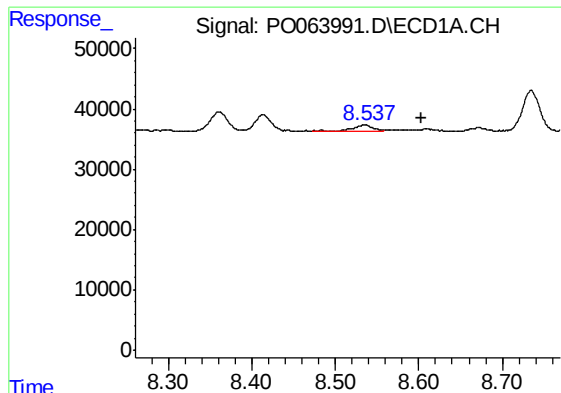

#42 AR-1268-2


R.T.: 8.535 min
Delta R.T.: -0.069 min
Response: 14244
Conc: 2.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

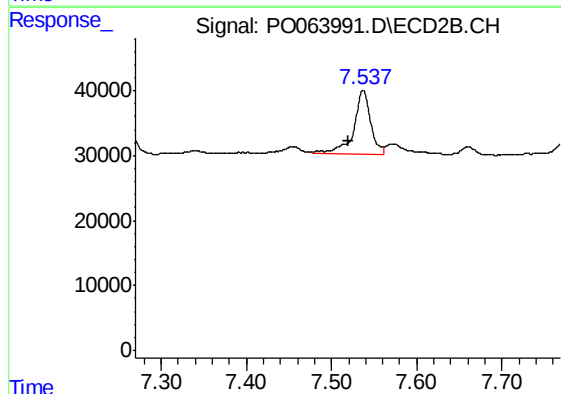


#42 AR-1268-2

R.T.: 7.537 min
Delta R.T.: 0.018 min
Response: 138418
Conc: 27.78 ng/ml

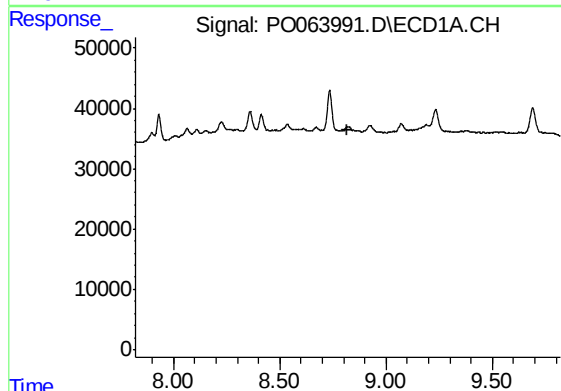


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

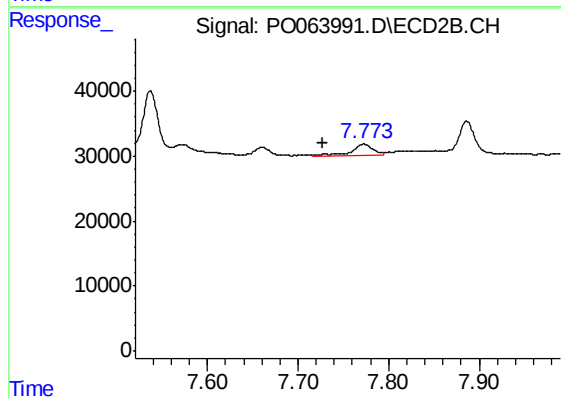

#43 AR-1268-3


R.T.: 7.773 min
Delta R.T.: 0.046 min
Response: 29684
Conc: 7.48 ng/ml

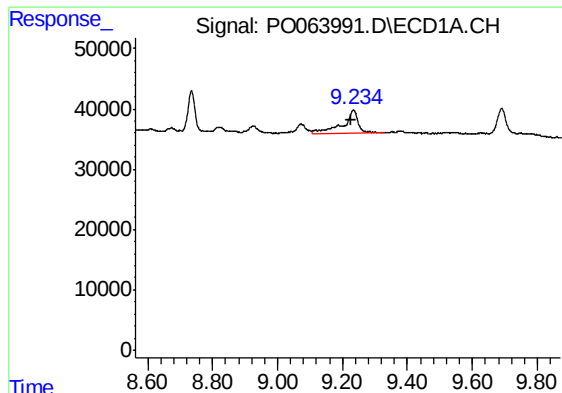

#44 AR-1268-4

R.T.: 9.234 min
Delta R.T.: 0.005 min
Response: 122555
Conc: 50.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110719-07

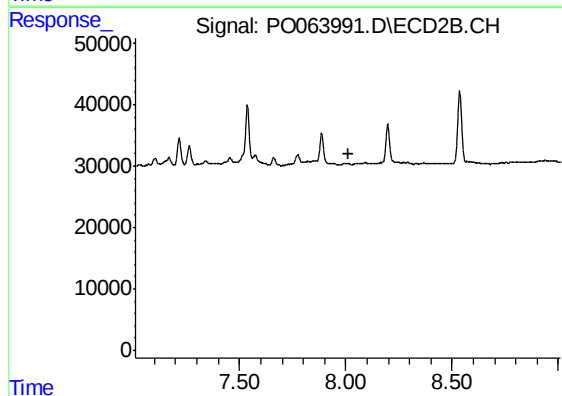

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.010 min
Response: 0
Conc: N.D.