

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063970.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2019 19:52
 Operator : SM/AJ
 Sample : K5951-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRONBOUND-8FT

Manual Integrations
 APPROVED

Ankita
 11/22/2019 1:24:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:46:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.567	723982	561005	23.679	25.258
2)	SA Decachlor...	9.938	8.533	774808	602276	19.068	20.593m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063970.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2019 19:52
Operator : SM/AJ
Sample : K5951-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRONBOUND-8FT


Manual Integrations
APPROVED

Ankita
11/22/2019 1:24:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:46:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

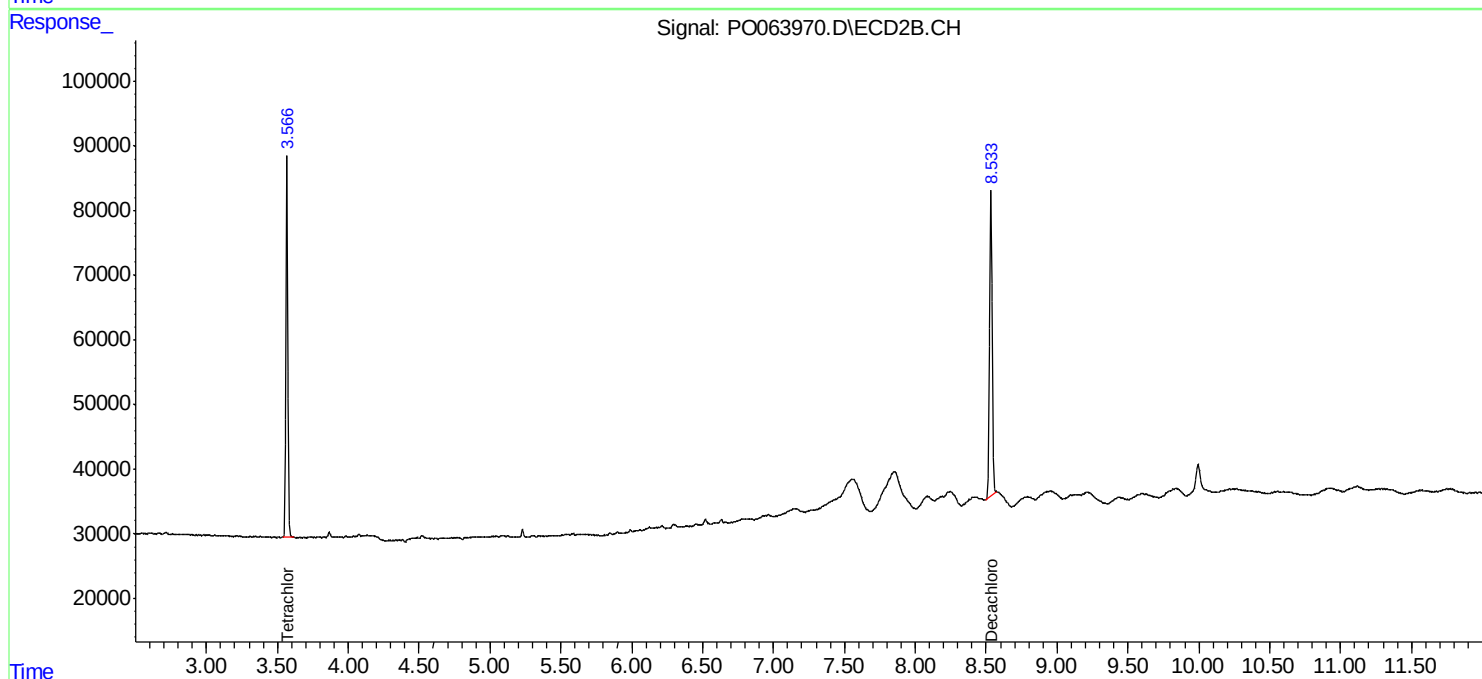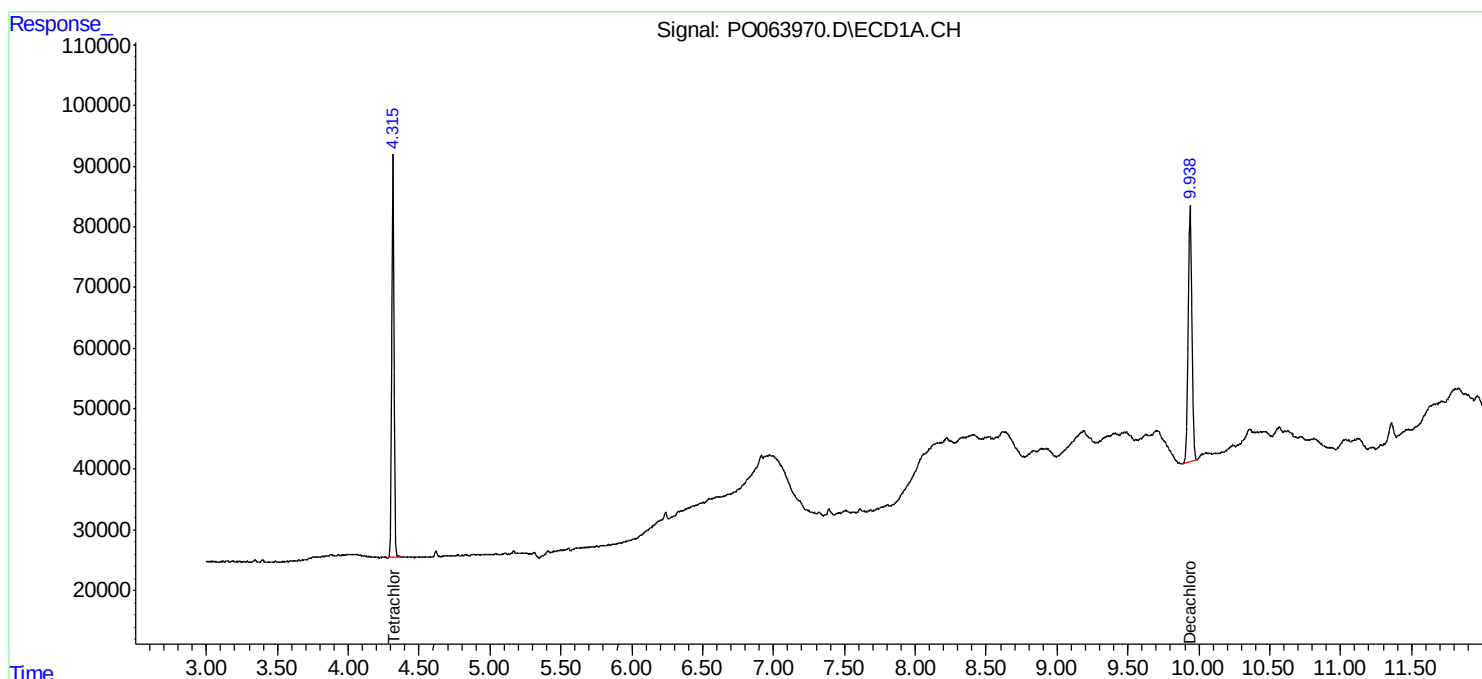

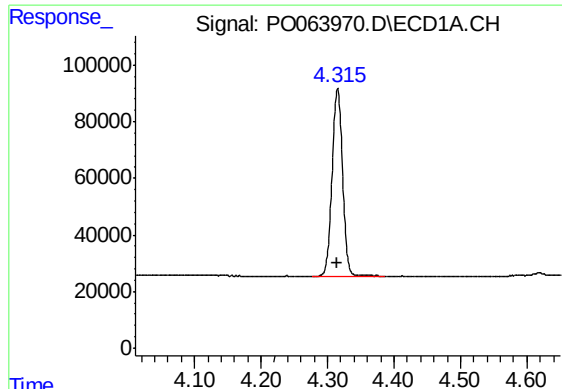


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: 0.001 min
Response: 723982
Conc: 23.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRONBOUND-8FT


Manual Integrations
APPROVED

Ankita
11/22/2019 1:24:26 PM

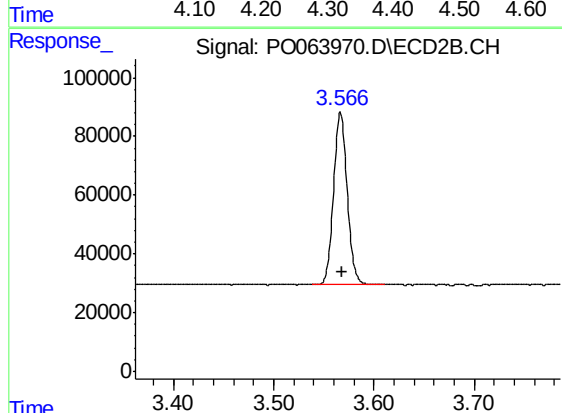


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.002 min
Response: 561005
Conc: 25.26 ng/ml

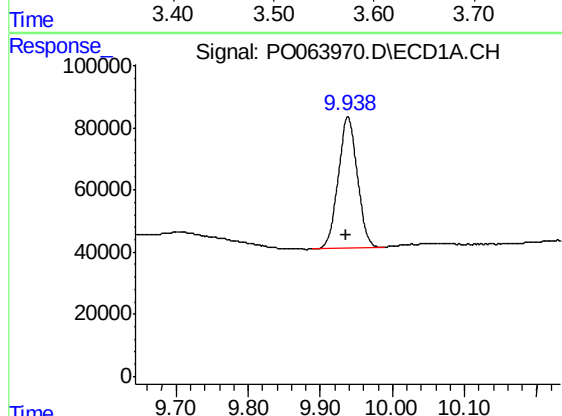

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.002 min
Response: 774808
Conc: 19.07 ng/ml

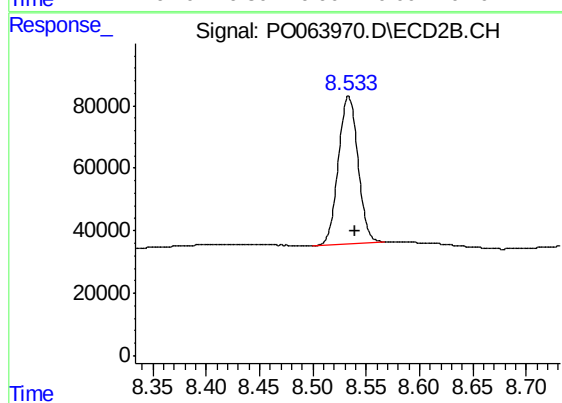

#2 Decachlorobiphenyl

R.T.: 8.533 min
Delta R.T.: -0.007 min
Response: 602276
Conc: 20.59 ng/ml m