

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063973.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2019 20:42
 Operator : SM/AJ
 Sample : K5955-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FOUNDATION-1

Manual Integrations
 APPROVED

Ankita
 11/22/2019 1:24:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:47:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.566	765909	596386	25.050	26.851
2)	SA Decachlor...	9.937	8.532	856262	675106	21.072	23.083m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
Data File : P0063973.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2019 20:42
Operator : SM/AJ
Sample : K5955-05
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FOUNDATION-1


Manual Integrations
APPROVED

Ankita
11/22/2019 1:24:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:47:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

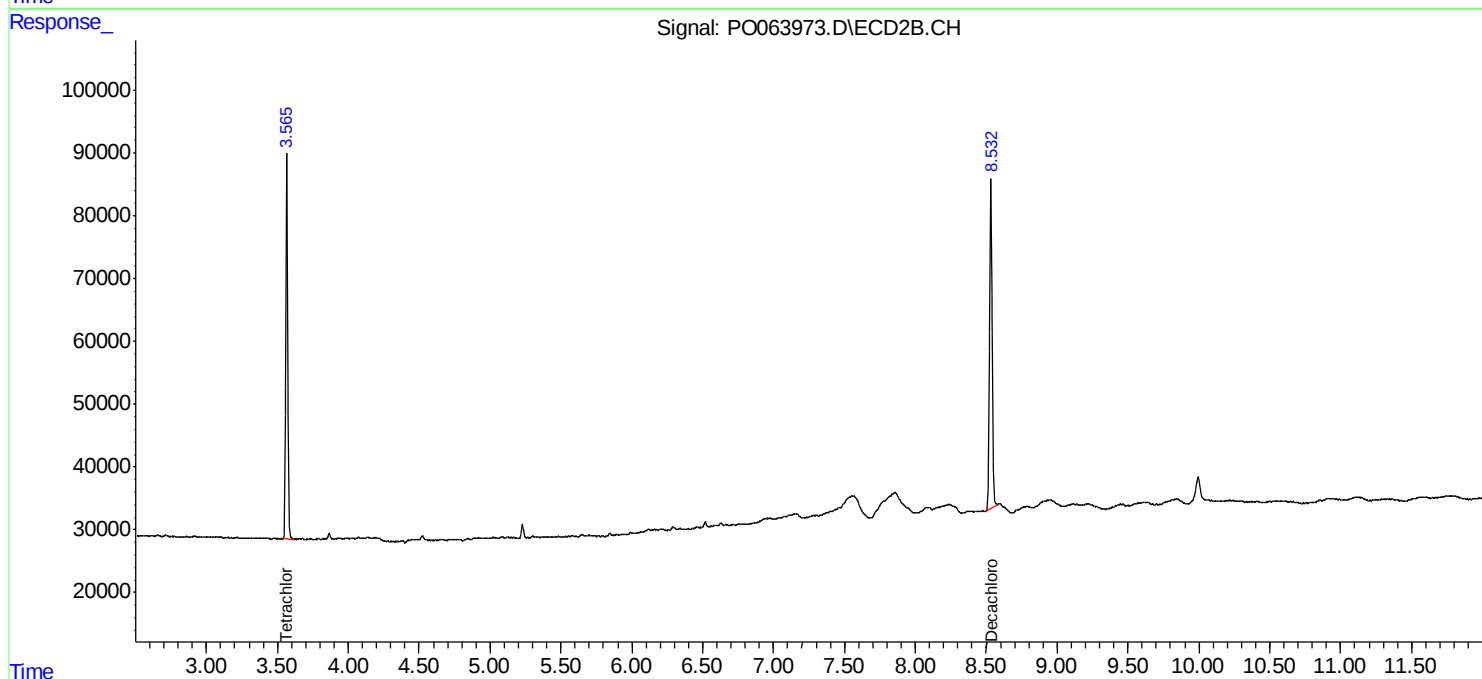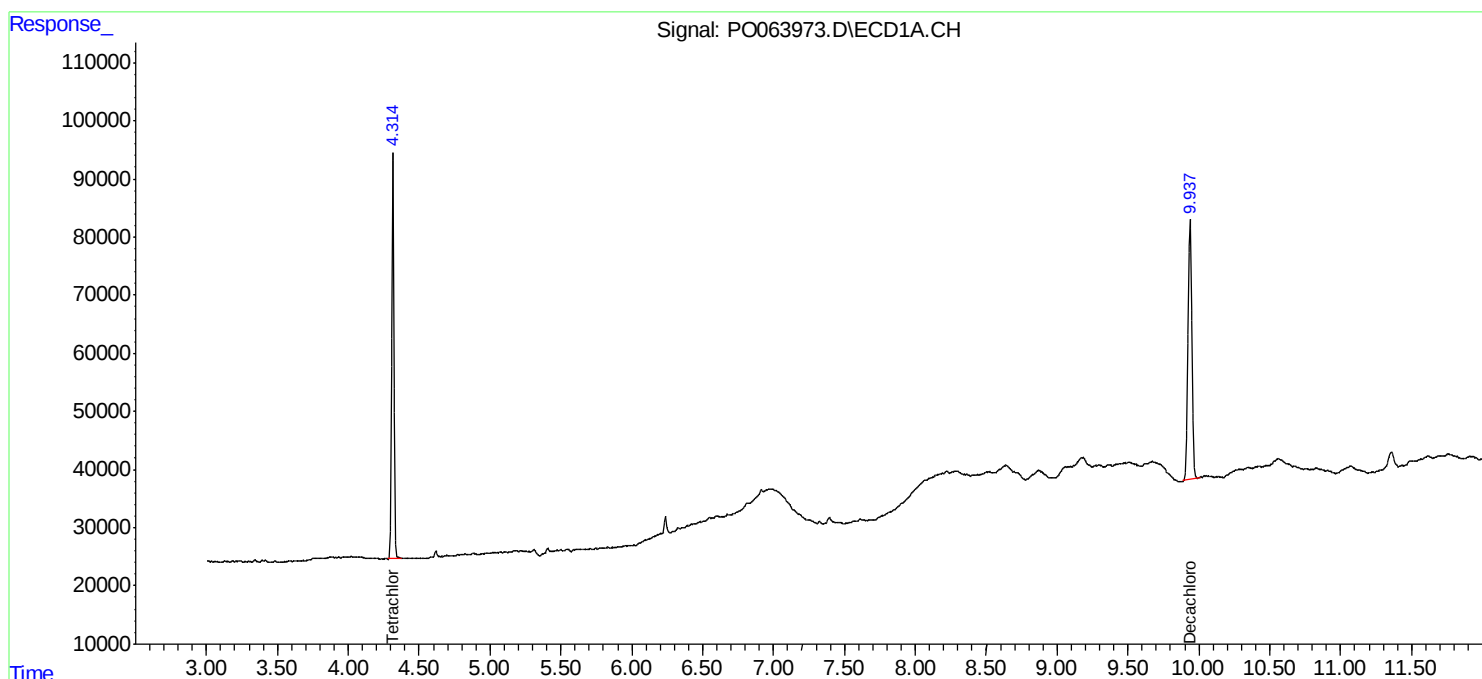

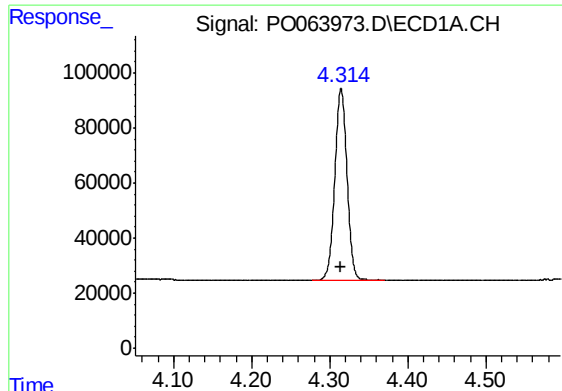


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: 0.000 min
Response: 765909
Conc: 25.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
FOUNDATION-1


Manual Integrations
APPROVED

Ankita
11/22/2019 1:24:35 PM

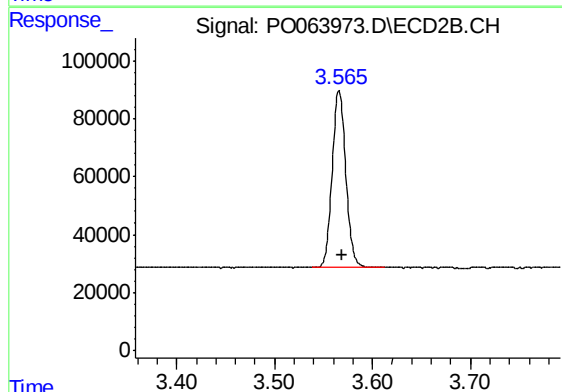


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 596386
Conc: 26.85 ng/ml

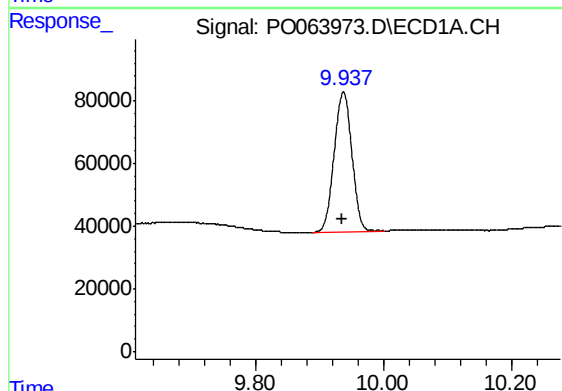

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: 0.002 min
Response: 856262
Conc: 21.07 ng/ml

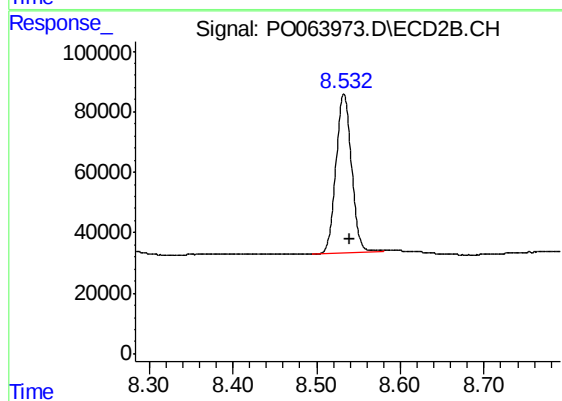

#2 Decachlorobiphenyl

R.T.: 8.532 min
Delta R.T.: -0.007 min
Response: 675106
Conc: 23.08 ng/ml m