

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
 Data File : P0063975.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2019 21:15
 Operator : SM/AJ
 Sample : K5959-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WS-112019-2-5-COMP-B2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:48:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.567	759218	631930	24.831	28.451
2)	SA Decachlor...	9.940	8.533	616366	481148	15.168	16.451

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063975.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2019 21:15
Operator : SM/AJ
Sample : K5959-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WS-112019-2-5-COMP-B2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:48:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

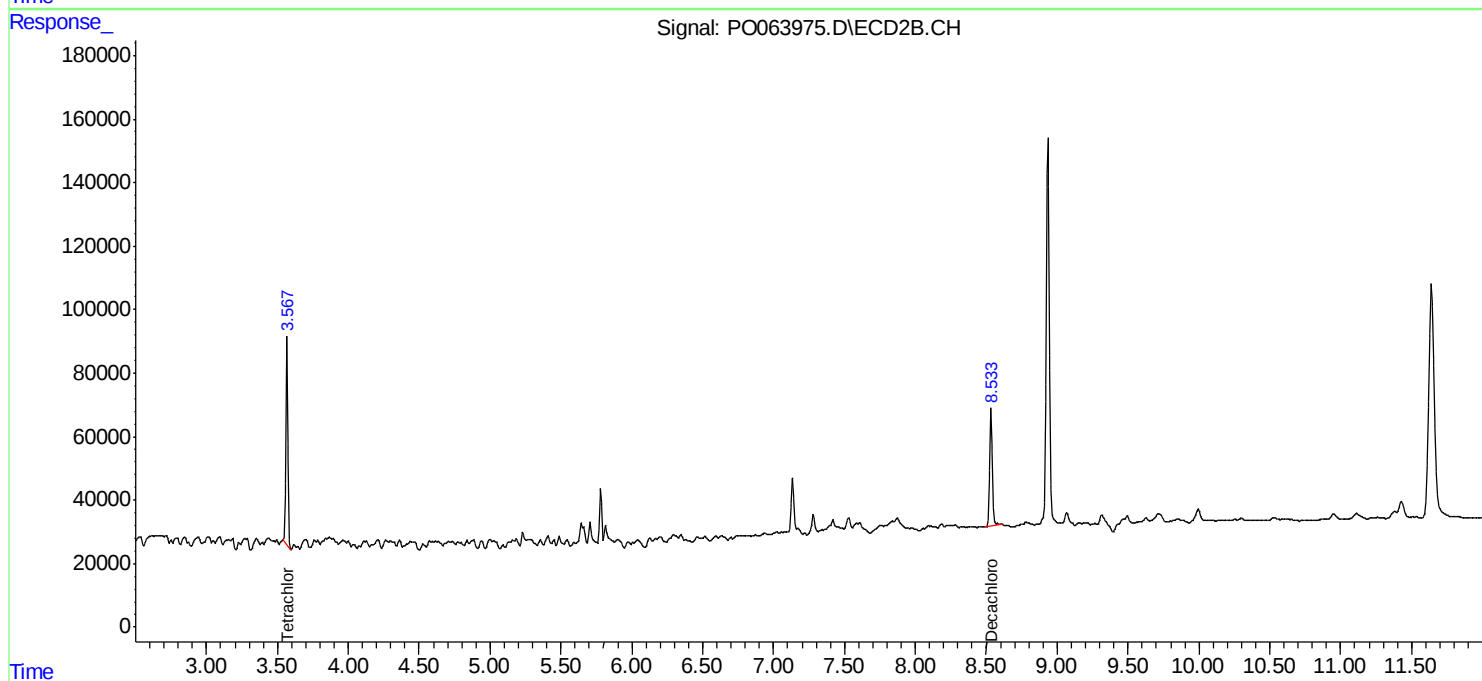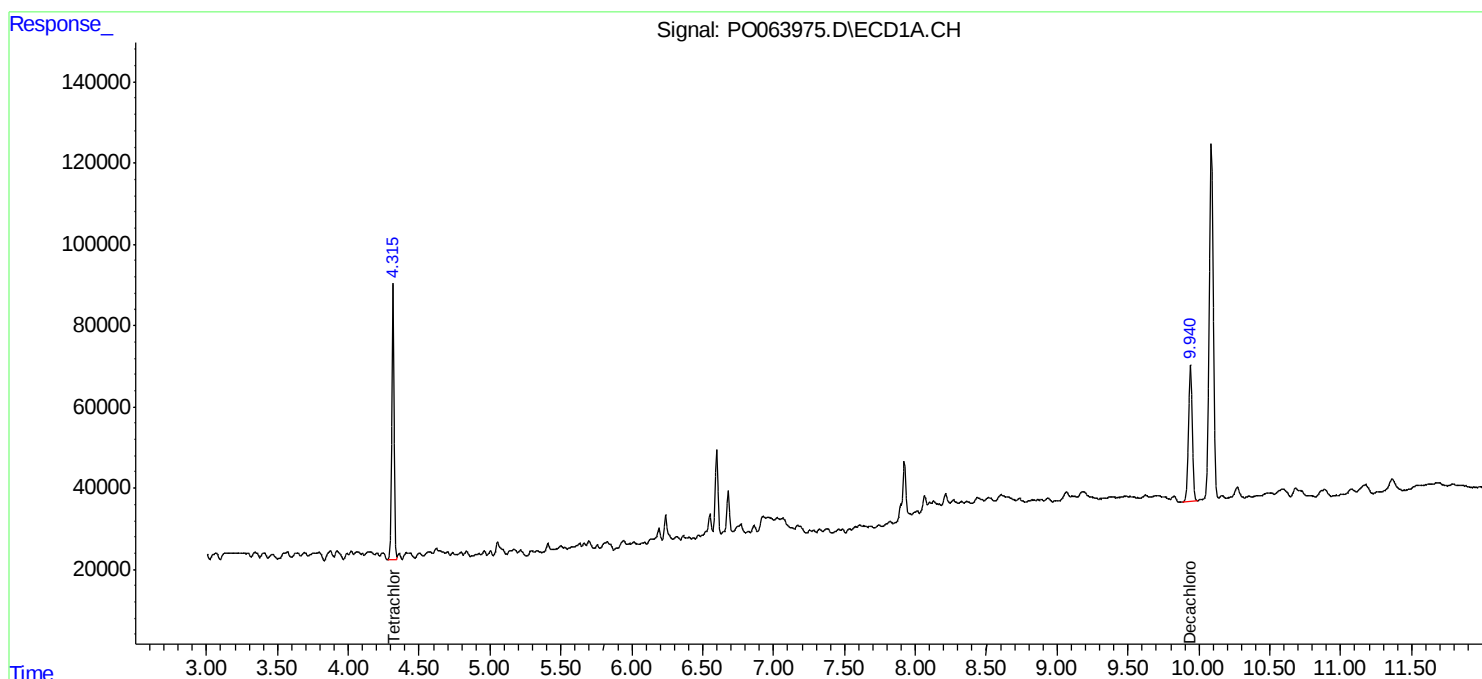


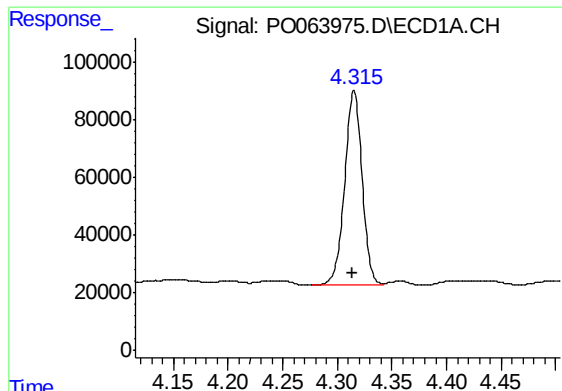

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.001 min
Response: 759218
Conc: 24.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
WS-112019-2-5-COMP-B2

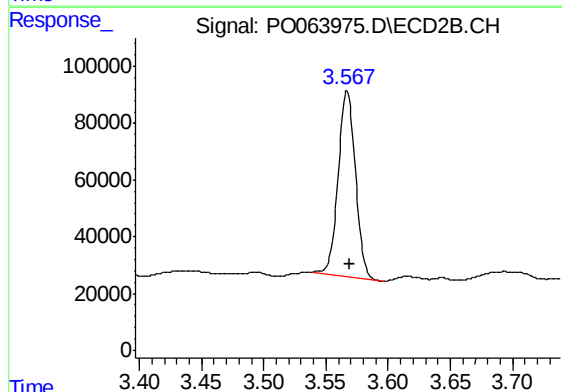


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.002 min
Response: 631930
Conc: 28.45 ng/ml

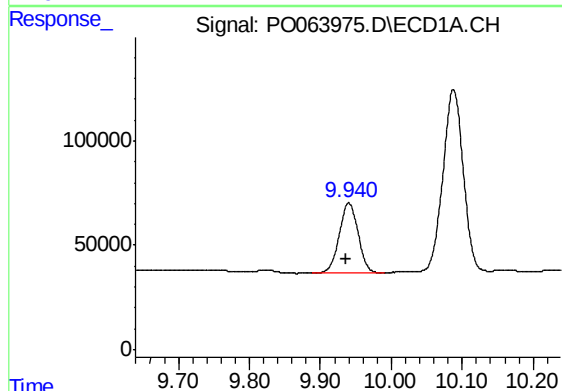

#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 616366
Conc: 15.17 ng/ml

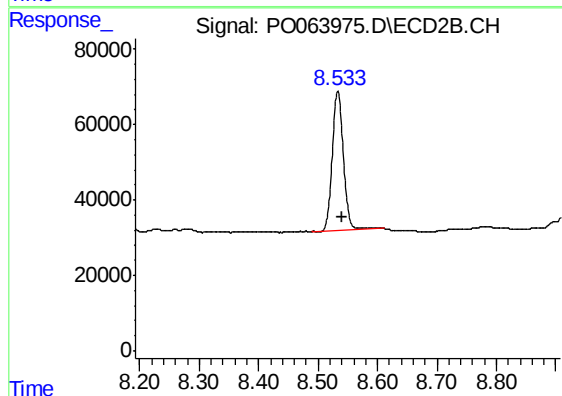

#2 Decachlorobiphenyl

R.T.: 8.533 min
Delta R.T.: -0.006 min
Response: 481148
Conc: 16.45 ng/ml