

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
Data File : P0063985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 1:42
Operator : SM/AJ
Sample : K5966-01 2X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-110419-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:54:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.566	263399	198137	8.615	8.921
2)	SA Decachlor...	9.940	8.534	283163	226317	6.969	7.738

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112119\
Data File : PO063985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 1:42
Operator : SM/AJ
Sample : K5966-01 2X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-110419-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:54:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

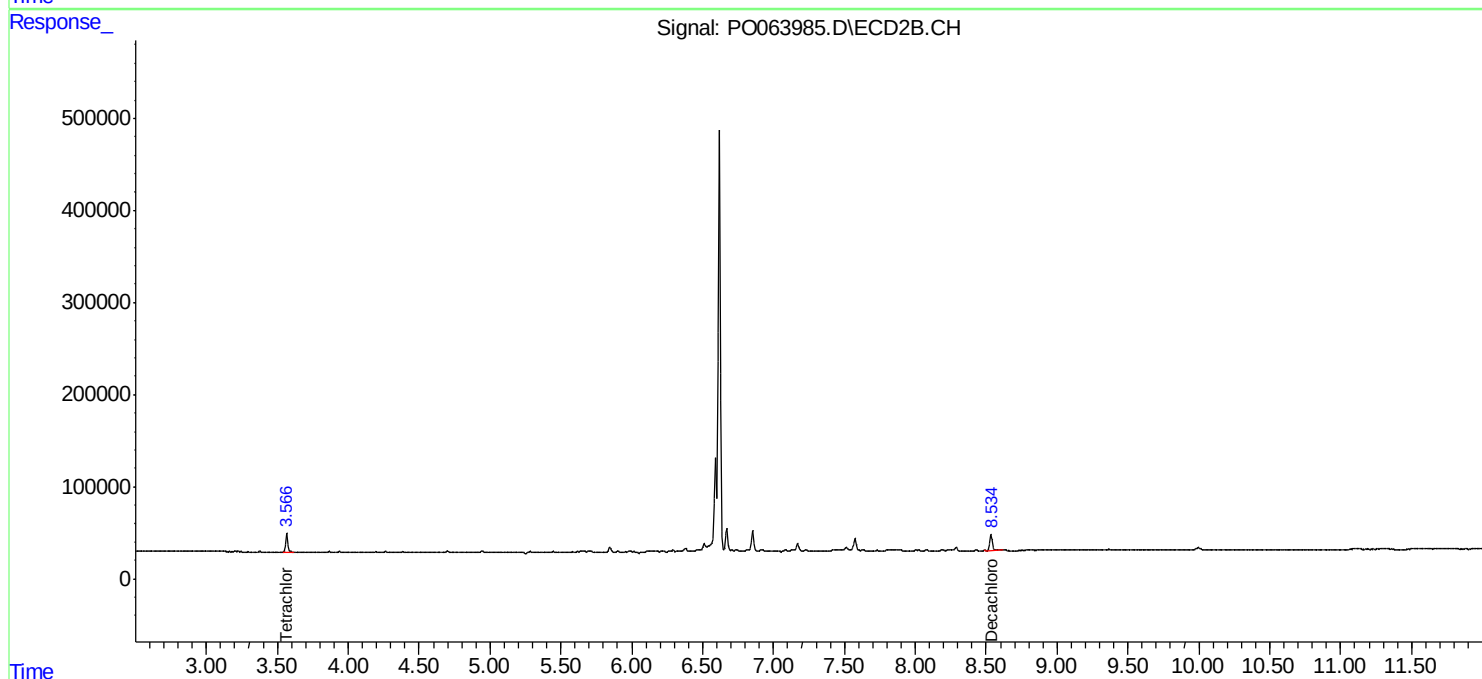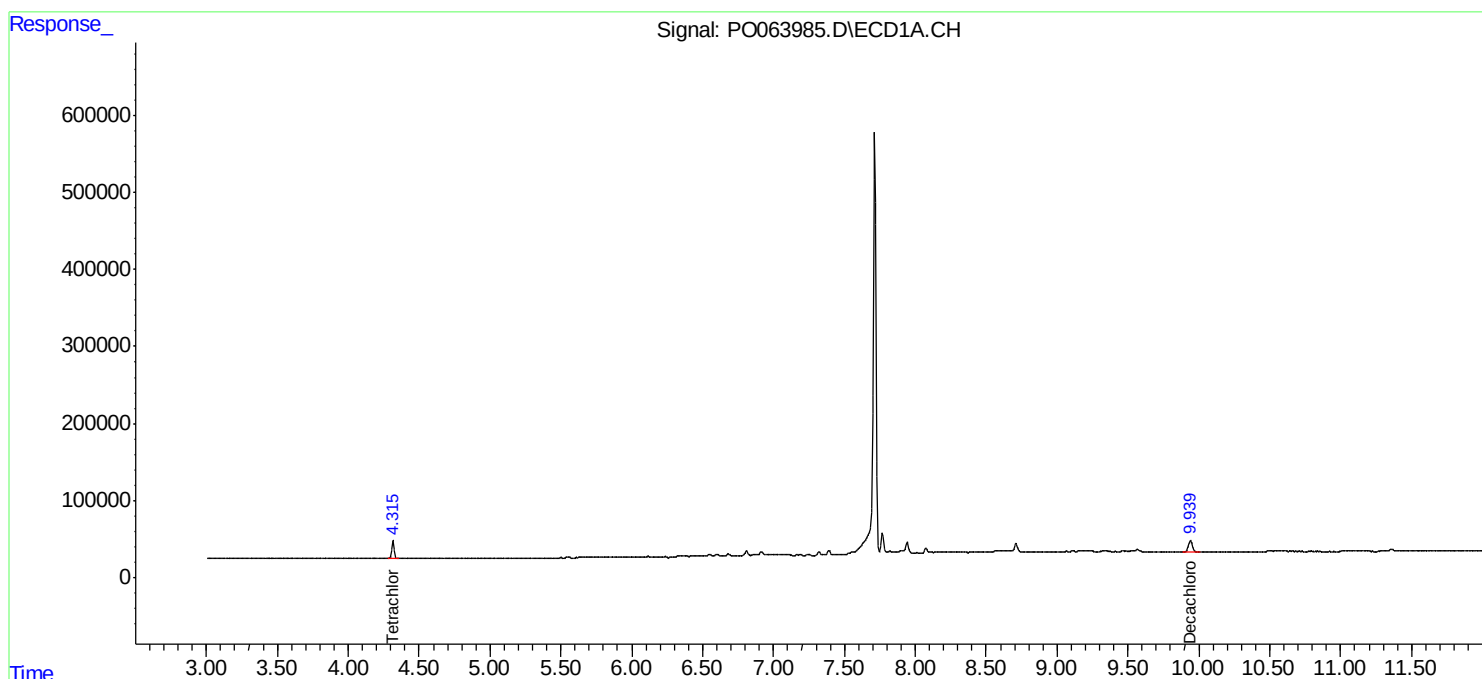


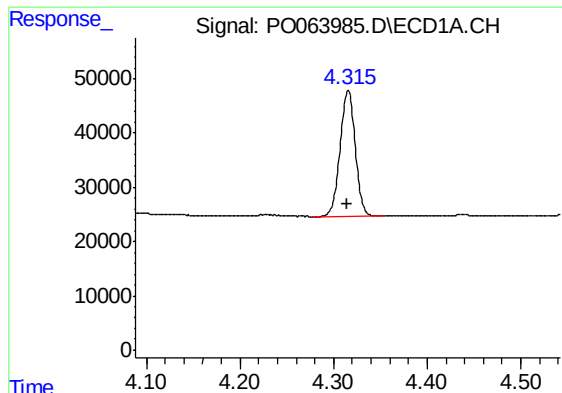

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 263399
Conc: 8.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110419-01

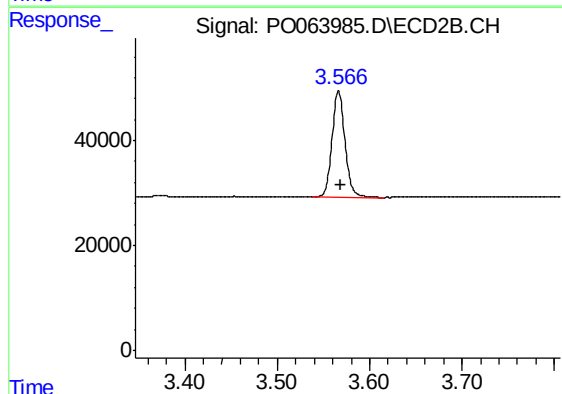


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.002 min
Response: 198137
Conc: 8.92 ng/ml

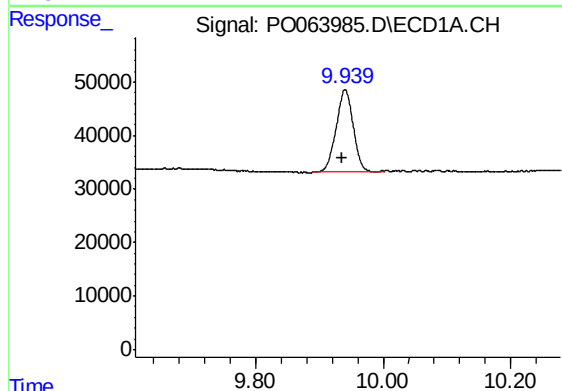

#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 283163
Conc: 6.97 ng/ml

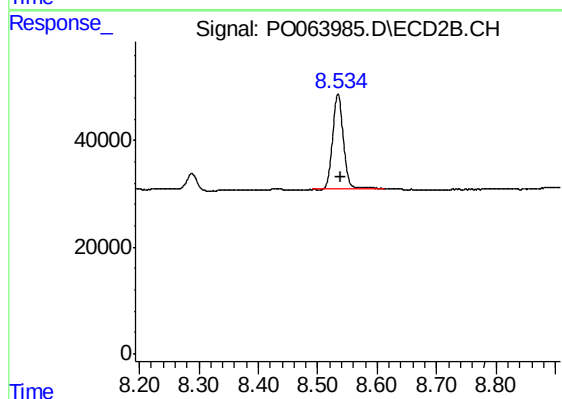

#2 Decachlorobiphenyl

R.T.: 8.534 min
Delta R.T.: -0.005 min
Response: 226317
Conc: 7.74 ng/ml