

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
 Data File : P0063989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 2:49
 Operator : SM/AJ
 Sample : K5966-05 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-110619-05

Manual Integrations
 APPROVED

Ankita
 11/22/2019 1:25:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 03:56:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.566	166995	128261	5.462	5.775
2)	SA Decachlor...	9.940	8.534	167574	150654	4.124	5.151
Target Compounds							
26)	L6 AR-1254-1	6.326	5.440	71538	57865	40.949m	32.659
27)	L6 AR-1254-2	6.543	5.586	107222	57554	38.462m	36.501
28)	L6 AR-1254-3	6.911	5.988	122439	63734	39.001m	23.769 #
29)	L6 AR-1254-4	7.191	6.215	67650	43399	27.360m	24.473
30)	L6 AR-1254-5	7.610	6.632	59542	137630	21.966m	55.080 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112119\
Data File : P0063989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 2:49
Operator : SM/AJ
Sample : K5966-05 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-110619-05


Manual Integrations
APPROVED

Ankita
11/22/2019 1:25:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 03:56:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

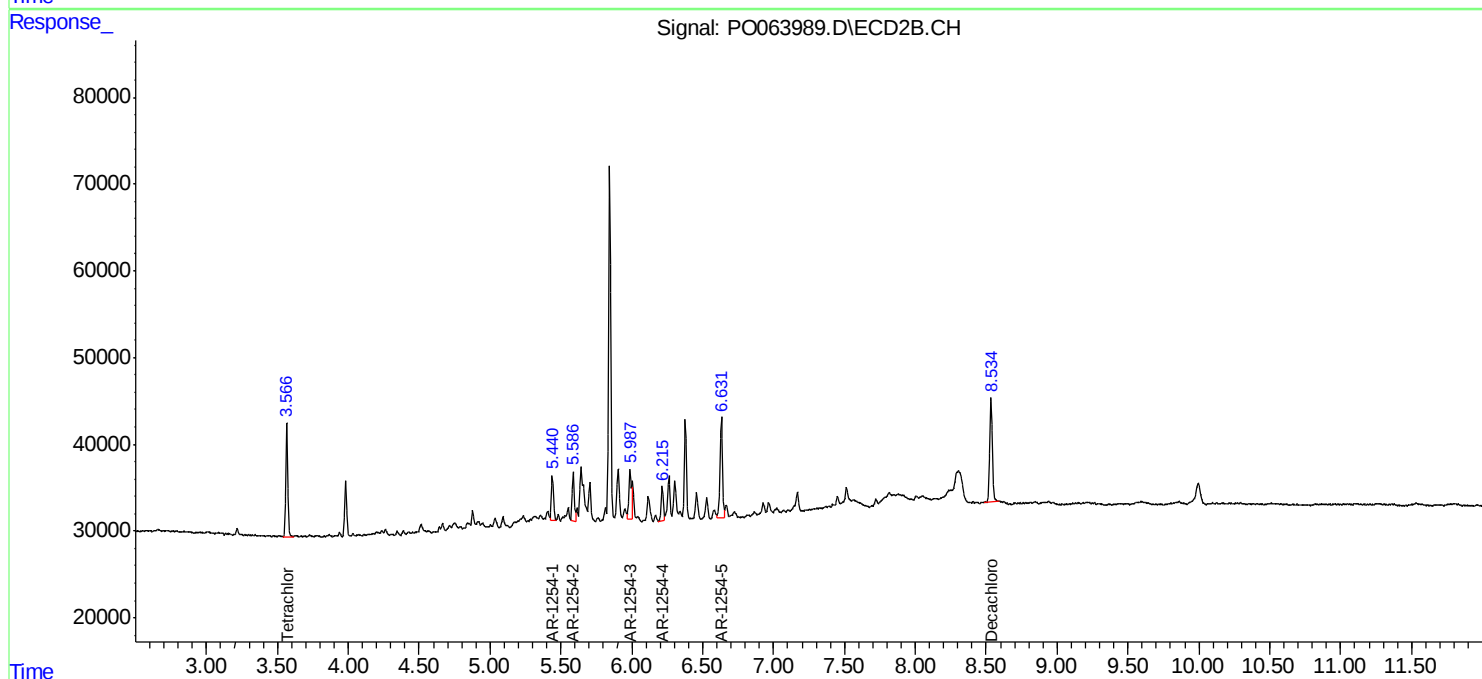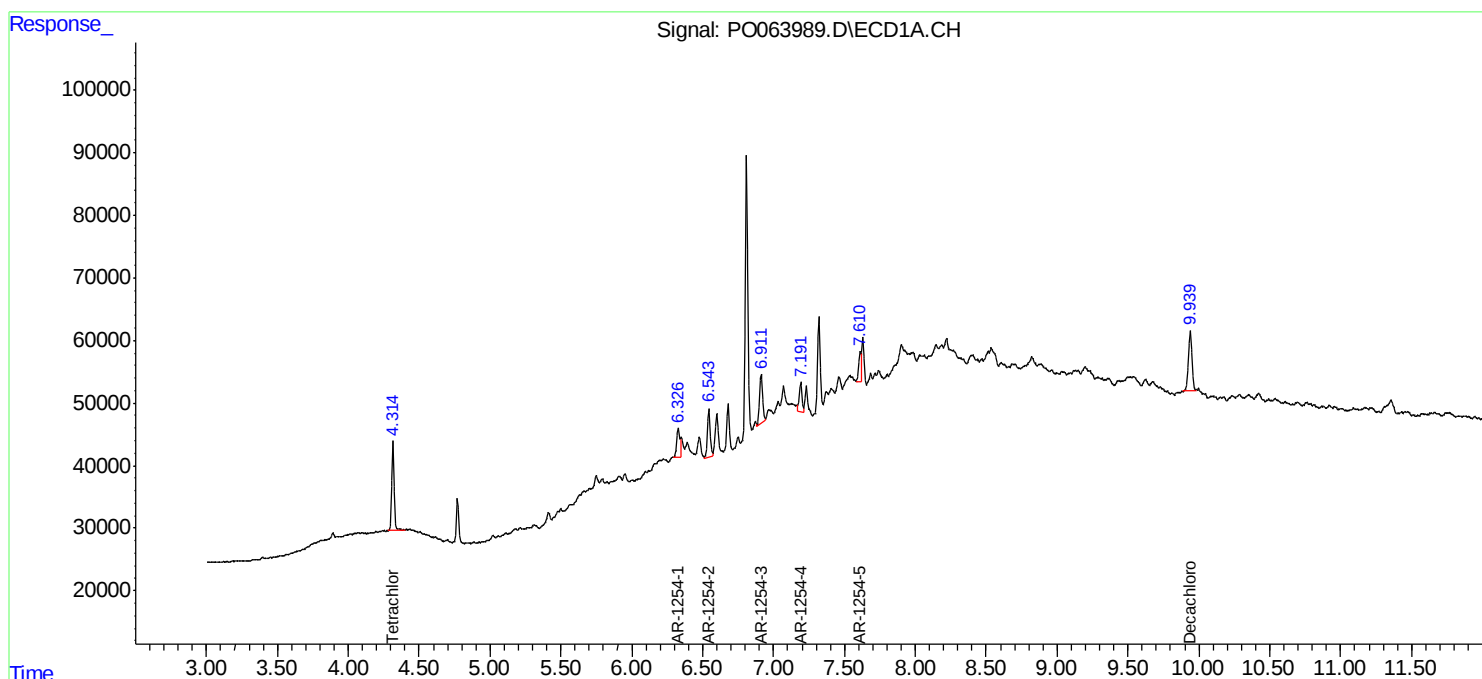

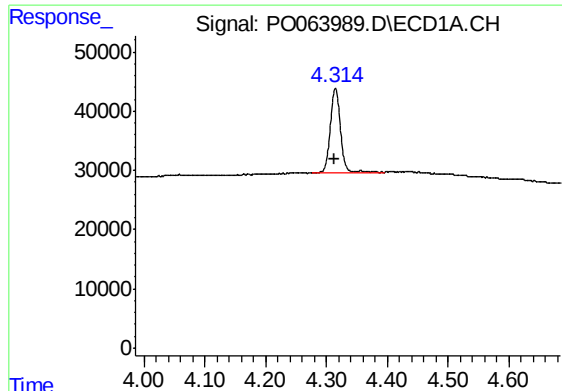


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: 0.001 min
Response: 166995
Conc: 5.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05


Manual Integrations
APPROVED

Ankita
11/22/2019 1:25:05 PM

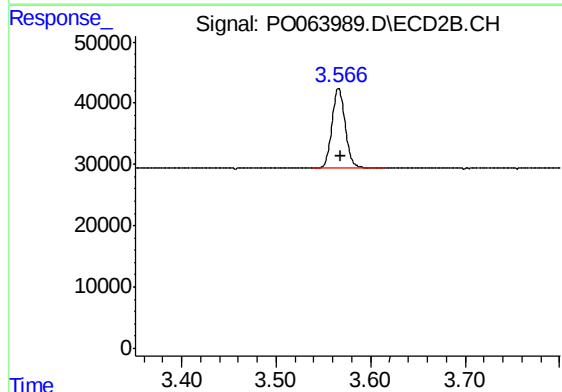


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 128261
Conc: 5.77 ng/ml

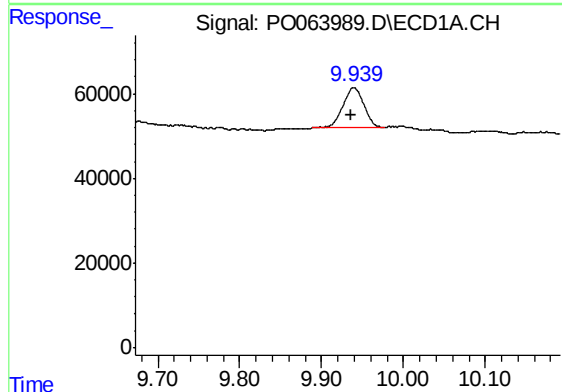


#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 167574
Conc: 4.12 ng/ml

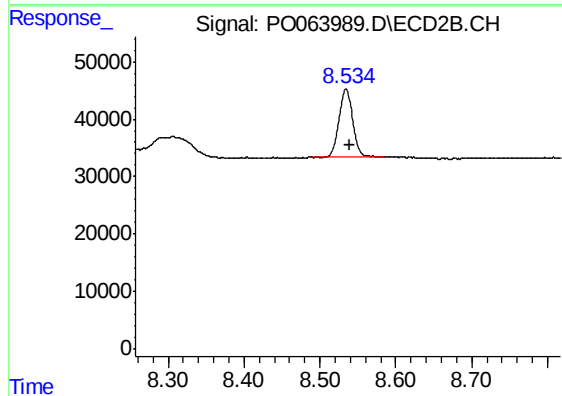

#2 Decachlorobiphenyl

R.T.: 8.534 min
Delta R.T.: -0.005 min
Response: 150654
Conc: 5.15 ng/ml

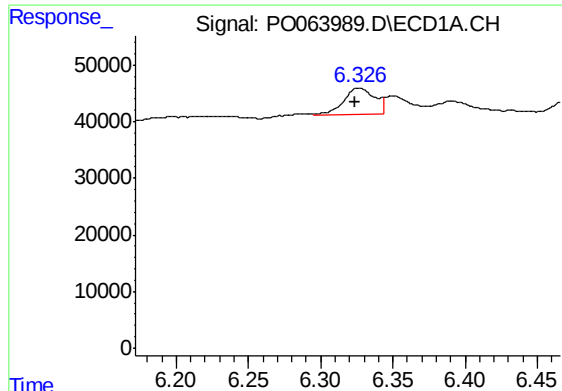


#26 AR-1254-1

R.T.: 6.326 min
Delta R.T.: 0.002 min
Response: 71538
Conc: 40.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05


Manual Integrations
APPROVED

Ankita
11/22/2019 1:25:05 PM

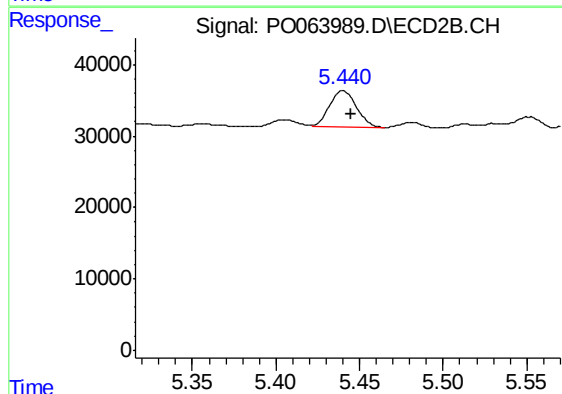


#26 AR-1254-1

R.T.: 5.440 min
Delta R.T.: -0.005 min
Response: 57865
Conc: 32.66 ng/ml

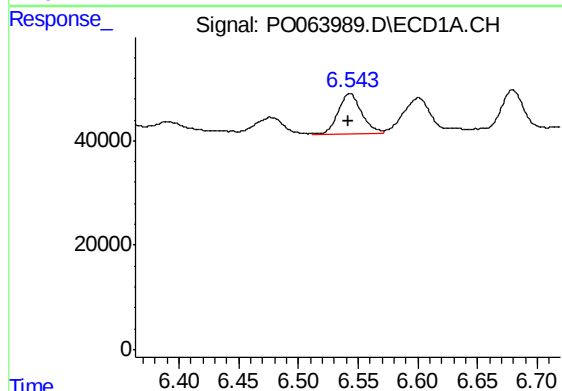


#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 107222
Conc: 38.46 ng/ml m

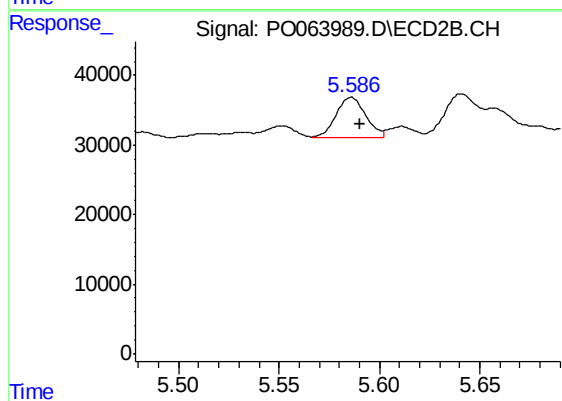

#27 AR-1254-2

R.T.: 5.586 min
Delta R.T.: -0.004 min
Response: 57554
Conc: 36.50 ng/ml

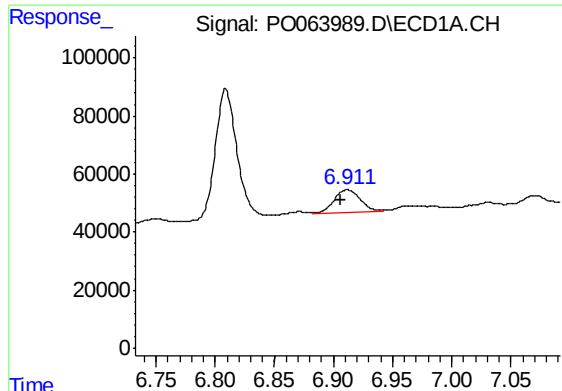


#28 AR-1254-3

R.T.: 6.911 min
Delta R.T.: 0.005 min
Response: 122439
Conc: 39.00 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05


Manual Integrations
APPROVED

Ankita
11/22/2019 1:25:05 PM

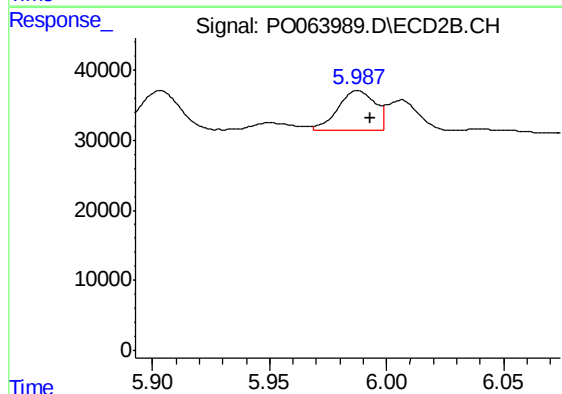


#28 AR-1254-3

R.T.: 5.988 min
Delta R.T.: -0.006 min
Response: 63734
Conc: 23.77 ng/ml

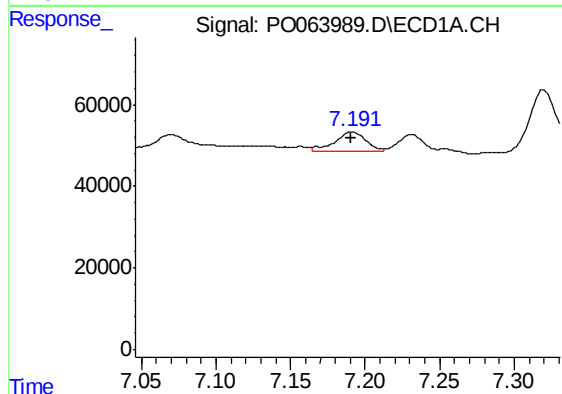


#29 AR-1254-4

R.T.: 7.191 min
Delta R.T.: 0.000 min
Response: 67650
Conc: 27.36 ng/ml m

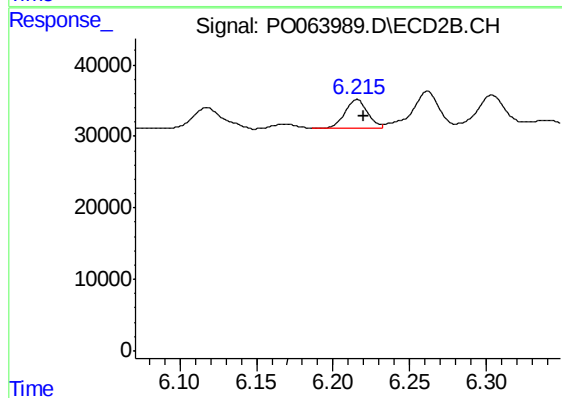

#29 AR-1254-4

R.T.: 6.215 min
Delta R.T.: -0.005 min
Response: 43399
Conc: 24.47 ng/ml

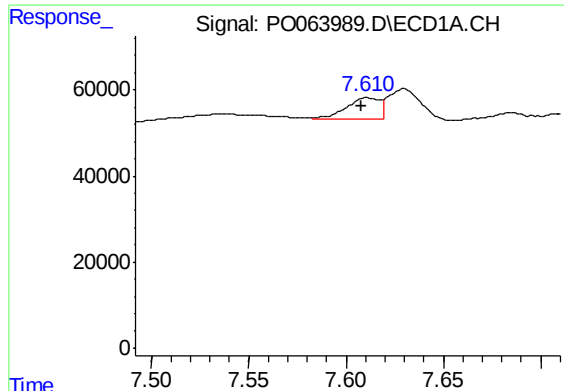


#30 AR-1254-5

R.T.: 7.610 min
Delta R.T.: 0.002 min
Response: 59542
Conc: 21.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-110619-05

Manual Integrations
APPROVED

Ankita
11/22/2019 1:25:05 PM

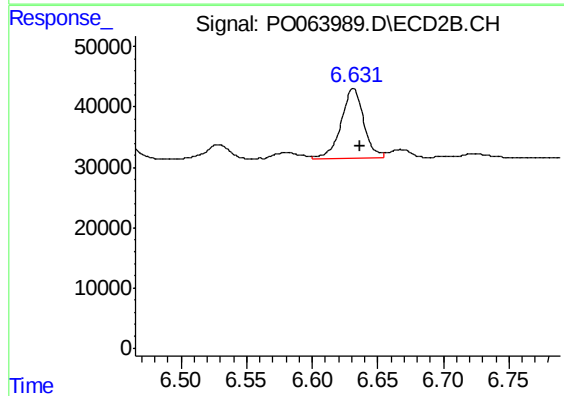

#30 AR-1254-5

R.T.: 6.632 min
Delta R.T.: -0.005 min
Response: 137630
Conc: 55.08 ng/ml