

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112122\
 Data File : P0090851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2022 22:45
 Operator : YP/AJ
 Sample : N5733-04 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC216342LOZ-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2022
 Supervised By :Ankita Jodhani 11/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 04:27:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.476	4260930	1573548	1.326	1.481
2) SA Decachlor...	10.045	8.481	3947592	1489229	1.611	1.446m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112122\
Data File : PO090851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2022 22:45
Operator : YP/AJ
Sample : N5733-04 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC216342LOZ-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2022
Supervised By :Ankita Jodhani 11/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 04:27:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

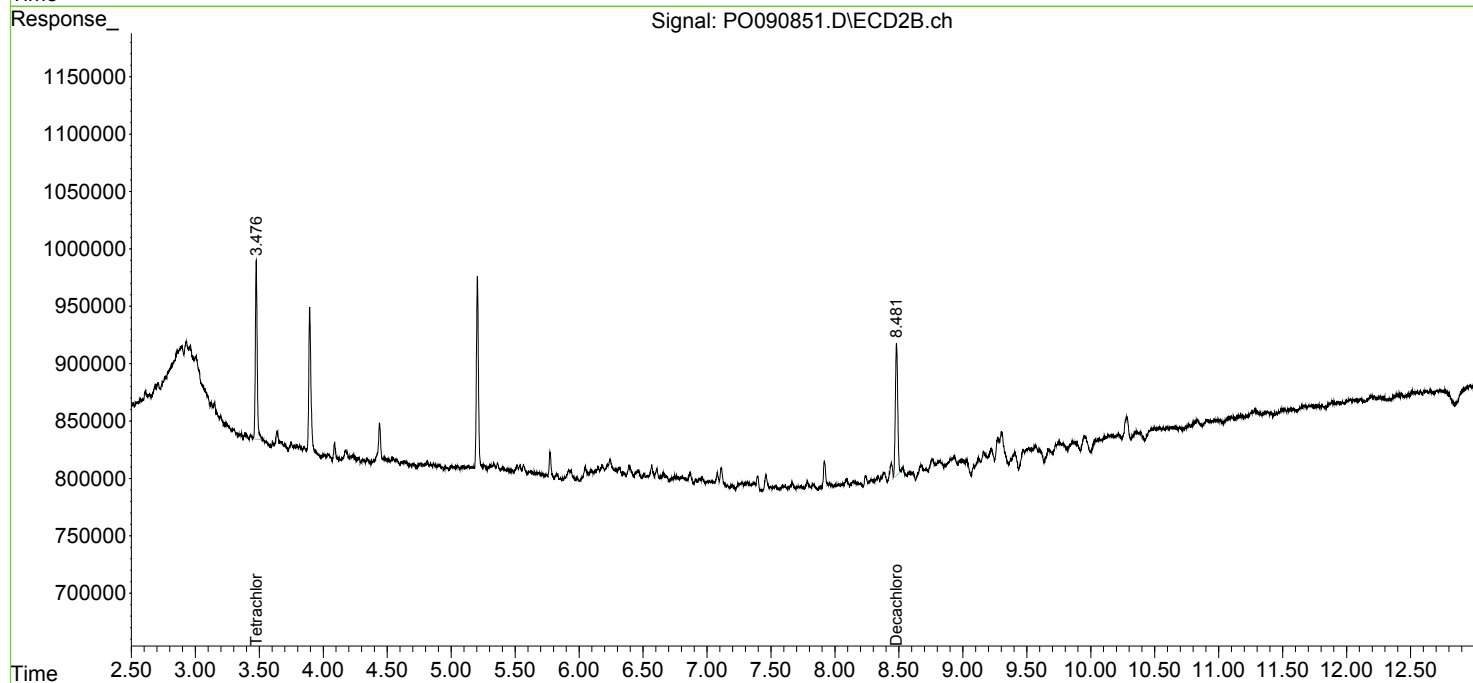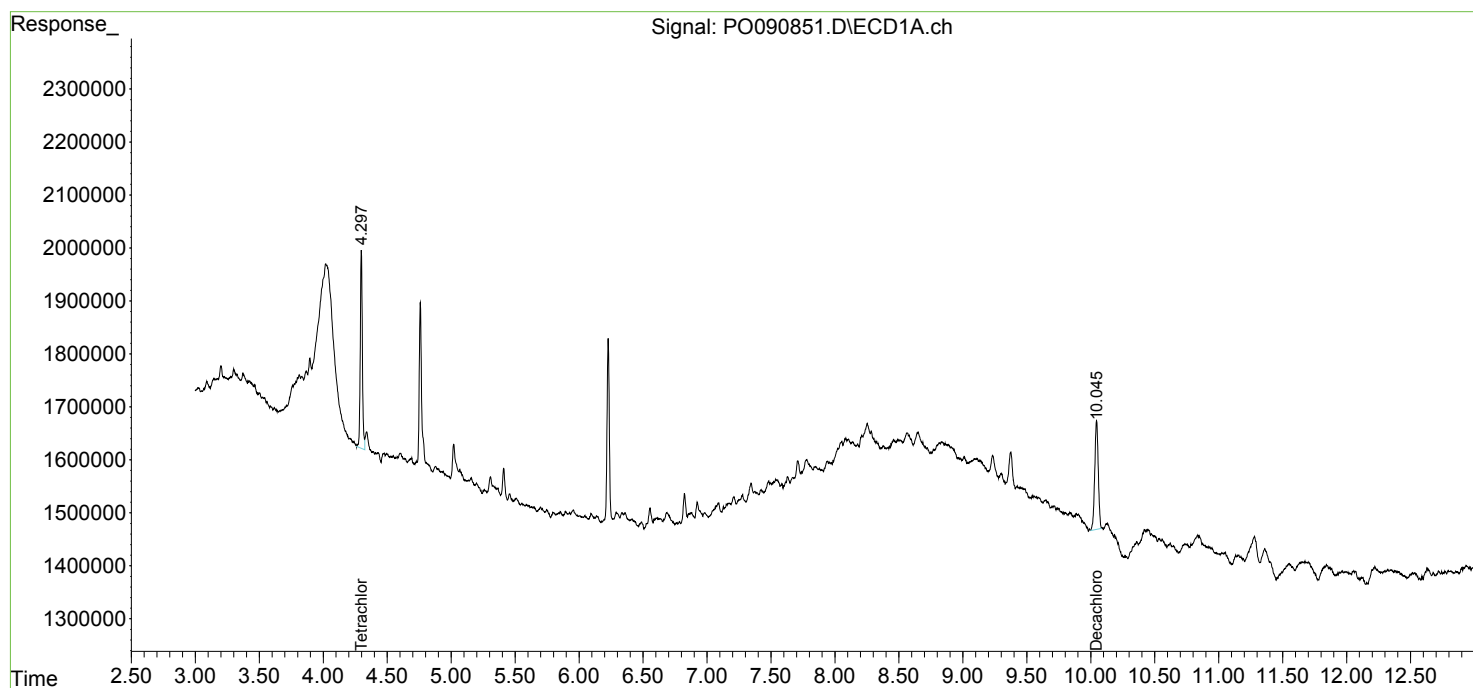

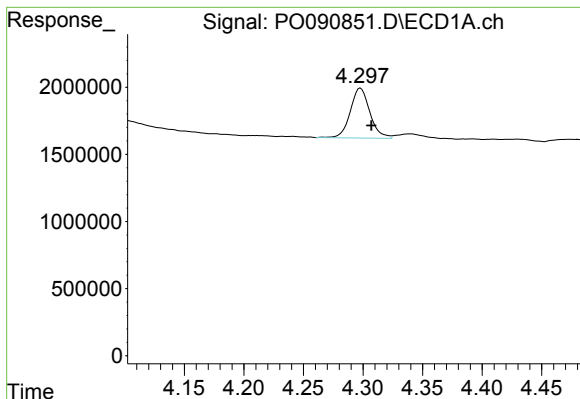


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: -0.009 min
Response: 4260930
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC216342LOZ-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2022
Supervised By :Ankita Jodhani 11/22/2022

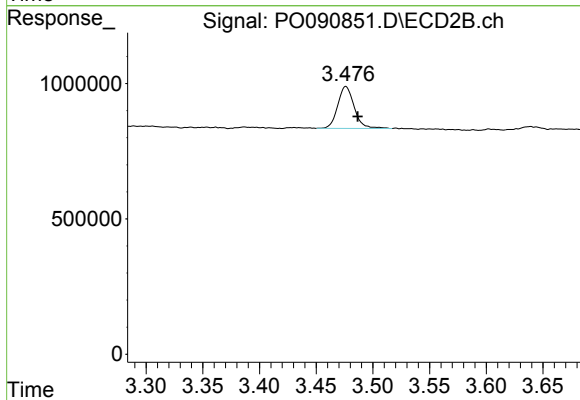


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.010 min
Response: 1573548
Conc: 1.48 ng/ml

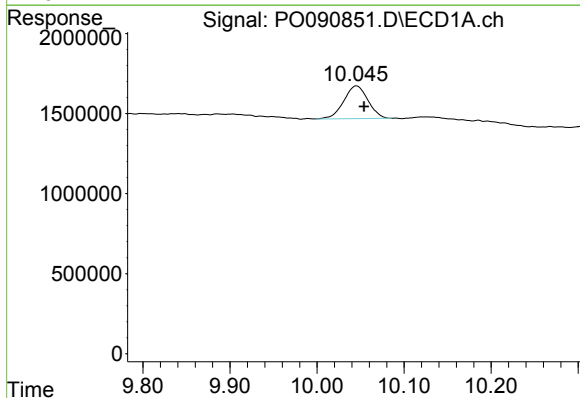

#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.008 min
Response: 3947592
Conc: 1.61 ng/ml

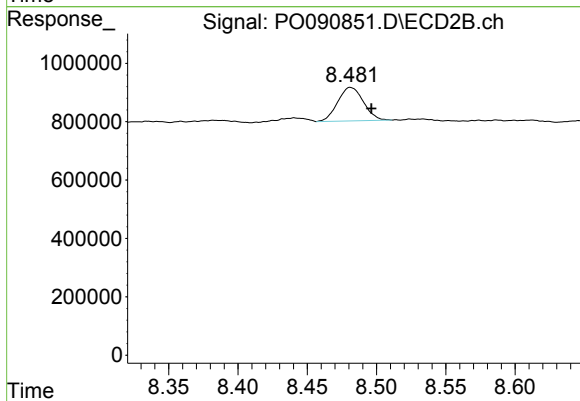

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.016 min
Response: 1489229
Conc: 1.45 ng/ml m