

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112122\
 Data File : P0090856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 00:10
 Operator : YP/AJ
 Sample : N5733-09 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LAW-2022-49B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2022
 Supervised By :Ankita Jodhani 11/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 04:29:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.476	3129867	1104785	0.974m	1.040
2) SA Decachlor...	10.044	8.479	3166213	1317040	1.292	1.279

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112122\
Data File : PO090856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 00:10
Operator : YP/AJ
Sample : N5733-09 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LAW-2022-49B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2022
Supervised By :Ankita Jodhani 11/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 04:29:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

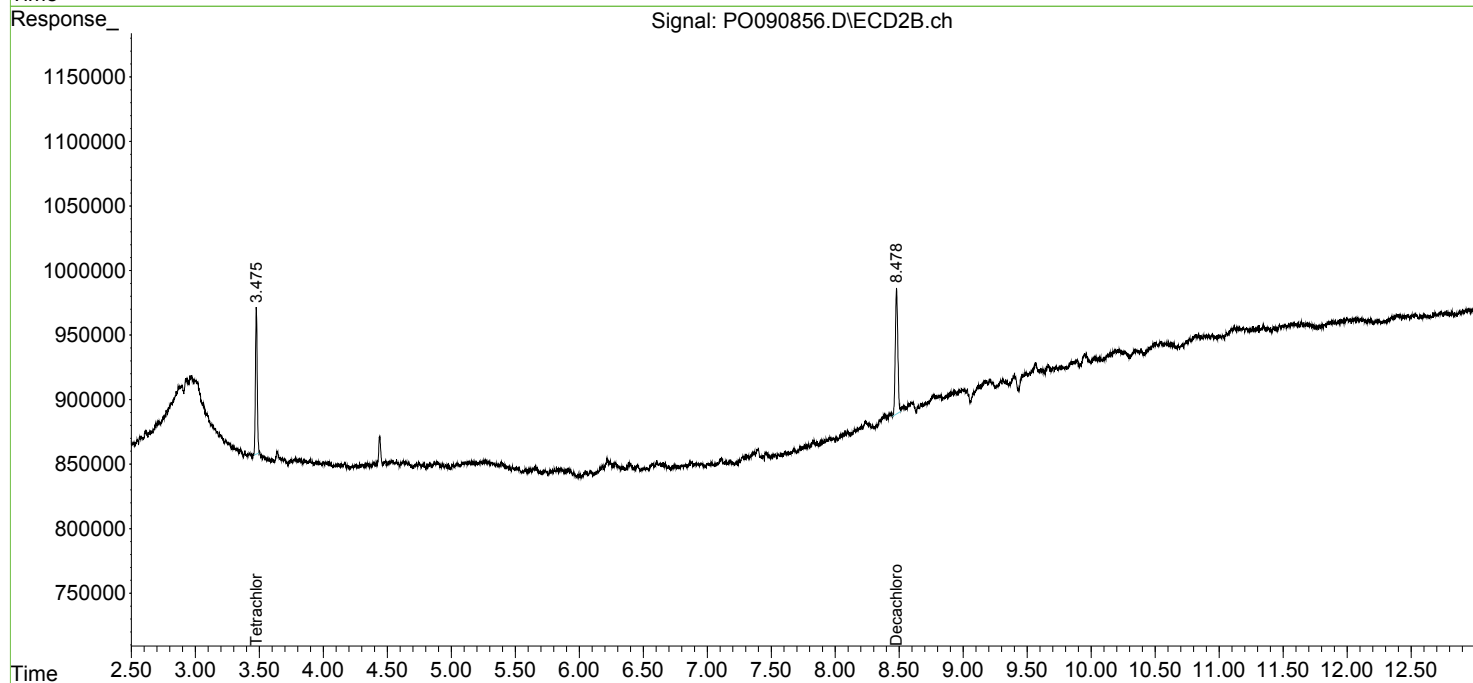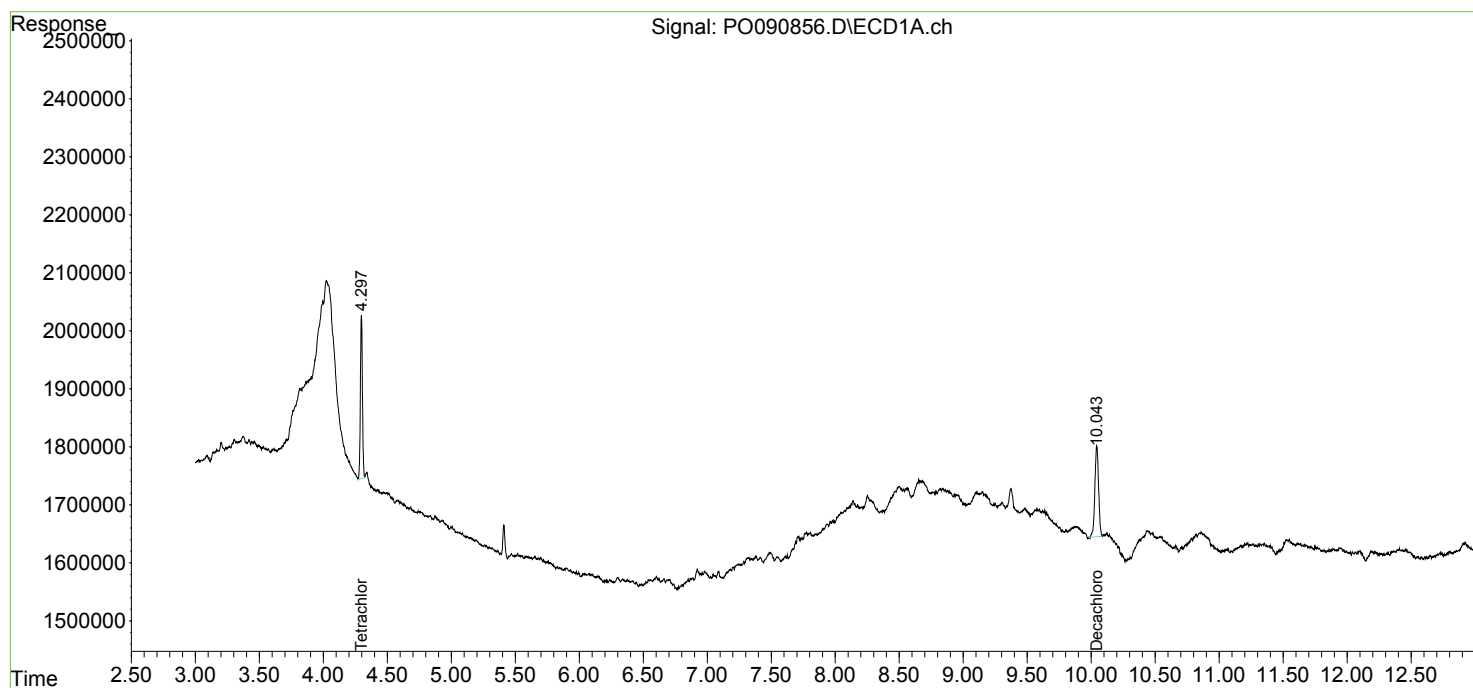

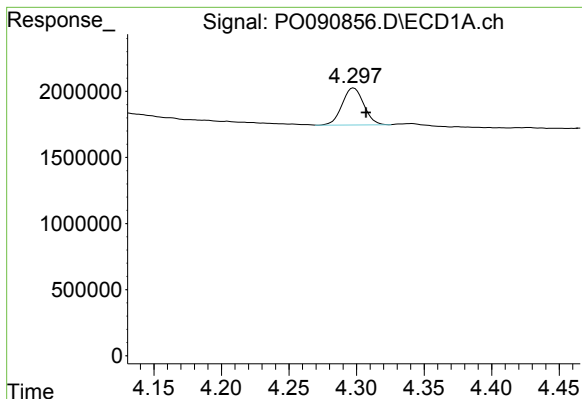

#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.010 min
Response: 3129867
Conc: 0.97 ng/ml

Instrument :

ECD_O


ClientSampleId :

LAW-2022-49B

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 11/22/2022
Supervised By :Ankita Jodhani 11/22/2022

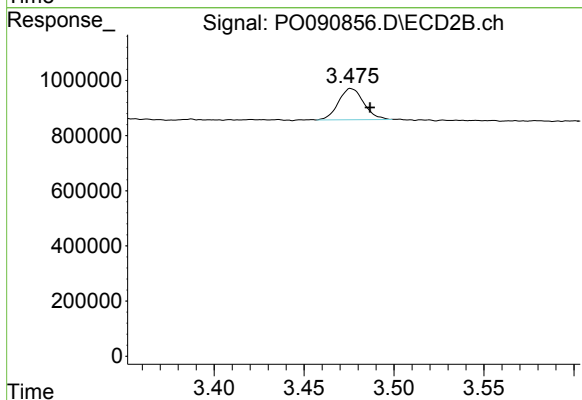


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.011 min
Response: 1104785
Conc: 1.04 ng/ml

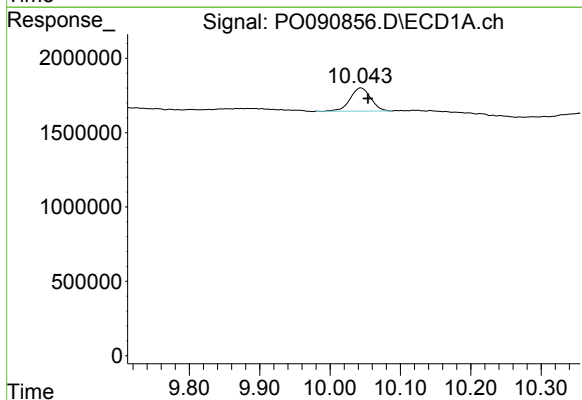

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.010 min
Response: 3166213
Conc: 1.29 ng/ml

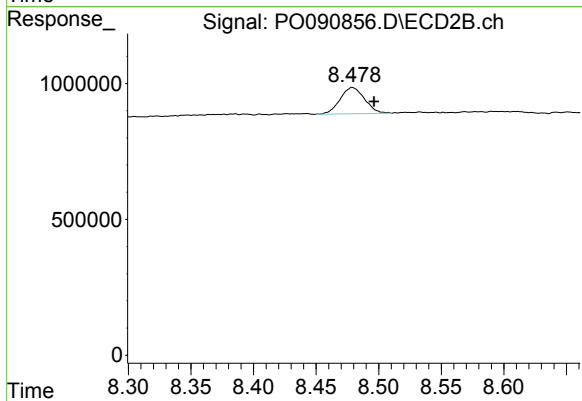

#2 Decachlorobiphenyl

R.T.: 8.479 min
Delta R.T.: -0.017 min
Response: 1317040
Conc: 1.28 ng/ml