

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112219\
 Data File : P0064021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2019 17:03
 Operator : SM/AJ
 Sample : K5959-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WS-112019-2-5-COMP-B4

Manual Integrations
 APPROVED

Ankita
 11/25/2019 11:46:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 18:04:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.566	847682	662258	27.725	29.816
2)	SA Decachlor...	9.943	8.534	1556105	1118519	38.295	38.244m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112219\
Data File : PO064021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2019 17:03
Operator : SM/AJ
Sample : K5959-07
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WS-112019-2-5-COMP-B4


Manual Integrations
APPROVED

Ankita
11/25/2019 11:46:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 18:04:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

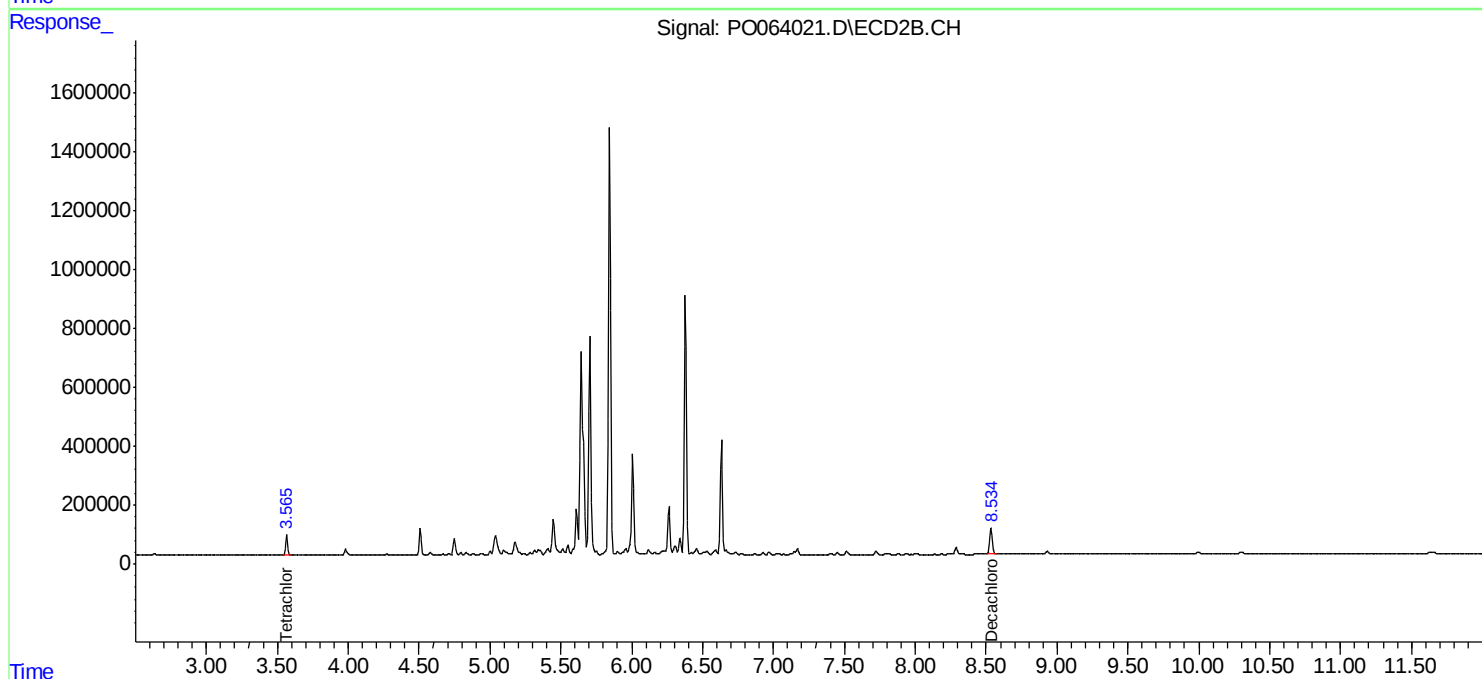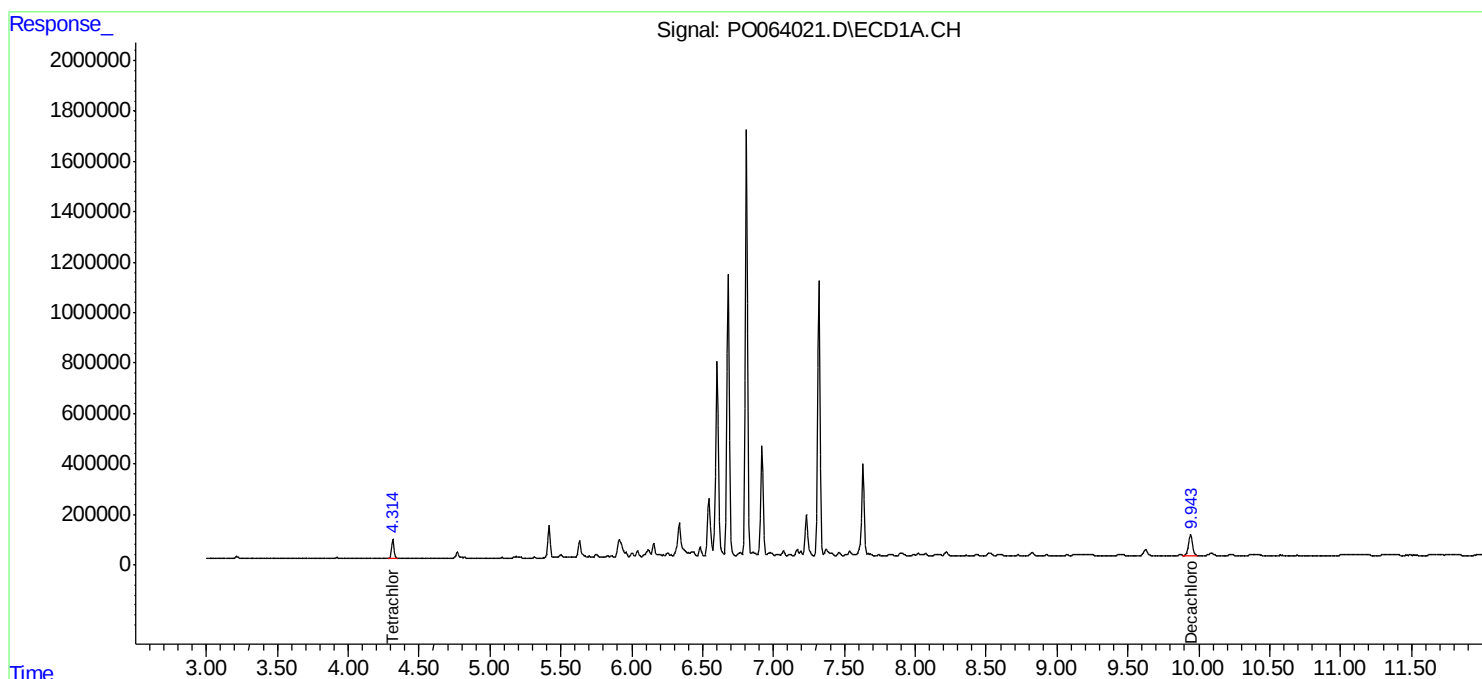

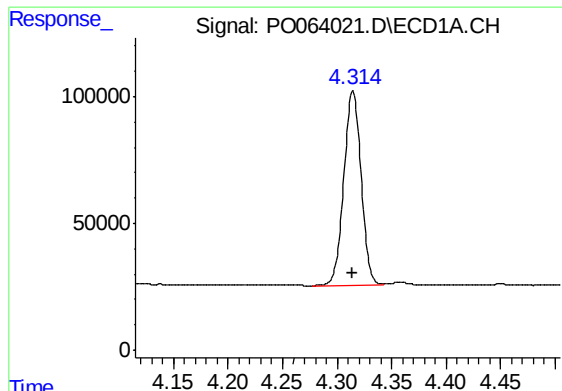


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: 0.000 min
Response: 847682
Conc: 27.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
WS-112019-2-5-COMP-B4


Manual Integrations
APPROVED

Ankita
11/25/2019 11:46:57 AM

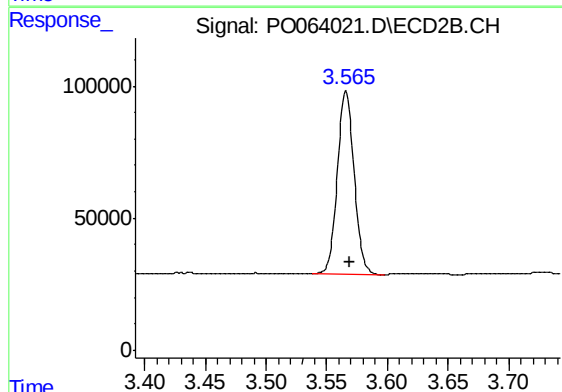


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.003 min
Response: 662258
Conc: 29.82 ng/ml

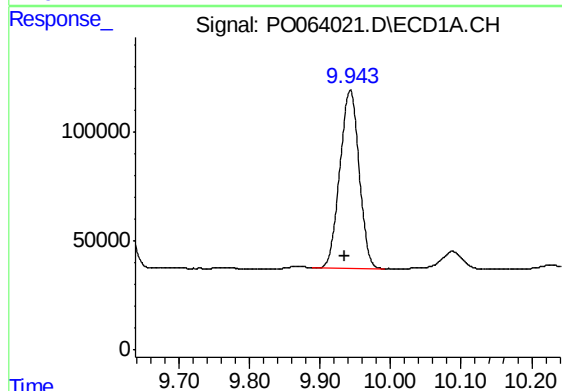

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.007 min
Response: 1556105
Conc: 38.30 ng/ml

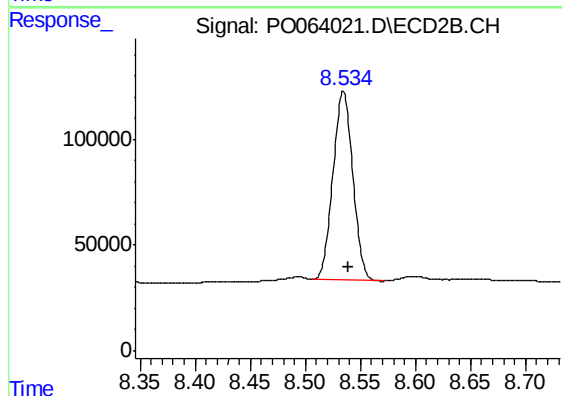

#2 Decachlorobiphenyl

R.T.: 8.534 min
Delta R.T.: -0.005 min
Response: 1118519
Conc: 38.24 ng/ml m