

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
 Data File : PO083145.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2021 9:28
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 22:52:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10)	L2	AR-1221-3	0.000	4.412	0	5455 N.D. 6.032 #
11)	L3	AR-1232-1	0.000	4.412	0	5455 N.D. 7.117 #
14)	L3	AR-1232-4	0.000	5.537f	0	10548 N.D. 30.000 #
19)	L4	AR-1242-4	0.000	5.537f	0	10548 N.D. 15.322 #
23)	L5	AR-1248-3	0.000	5.537	0	10548 N.D. 10.648 #
35)	L7	AR-1260-5	0.000	7.872	0	60396 N.D. 13.527 #
37)	L8	AR-1262-2	0.000	7.872	0	60396 N.D. 13.369 #
39)	L8	AR-1262-4	0.000	8.238	0	14380 N.D. 4.540 #
42)	L9	AR-1268-2	0.000	8.238	0	14380 N.D. 2.994 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
Data File : PO083145.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2021 9:28
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 22:52:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

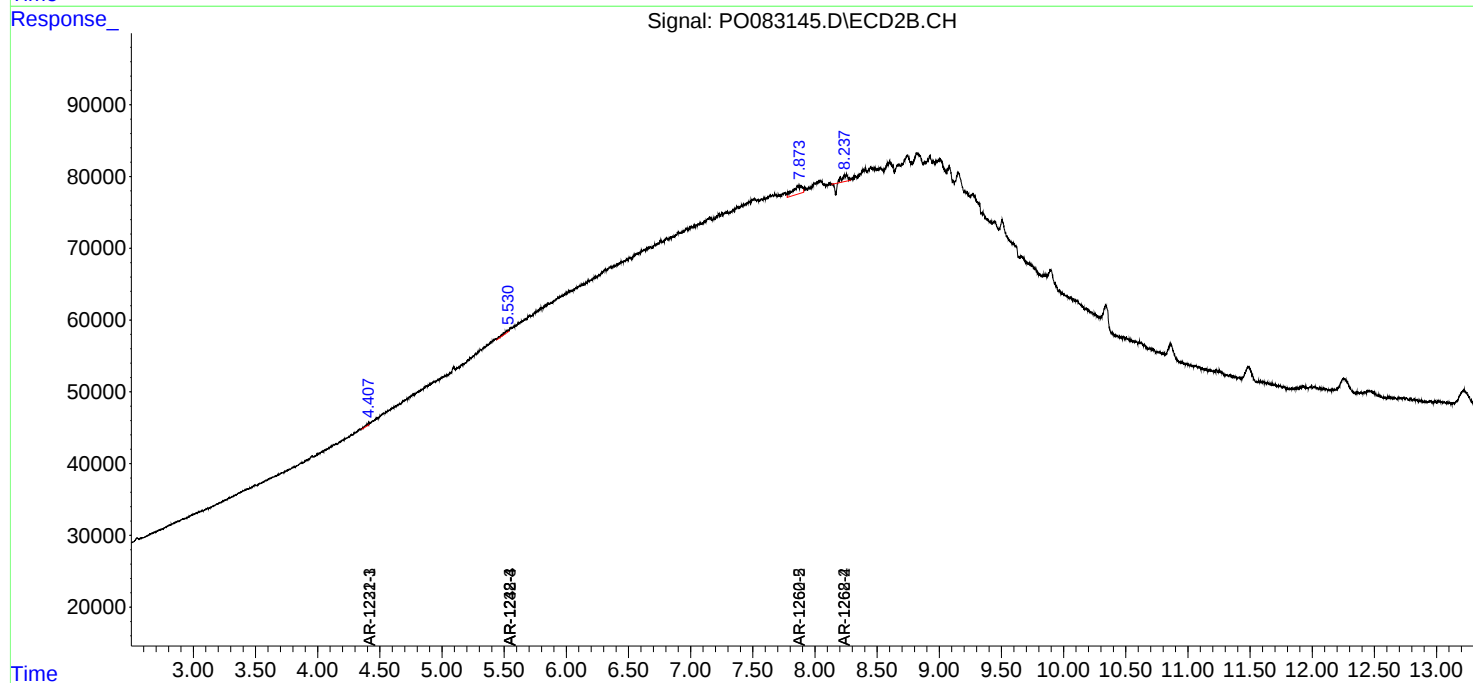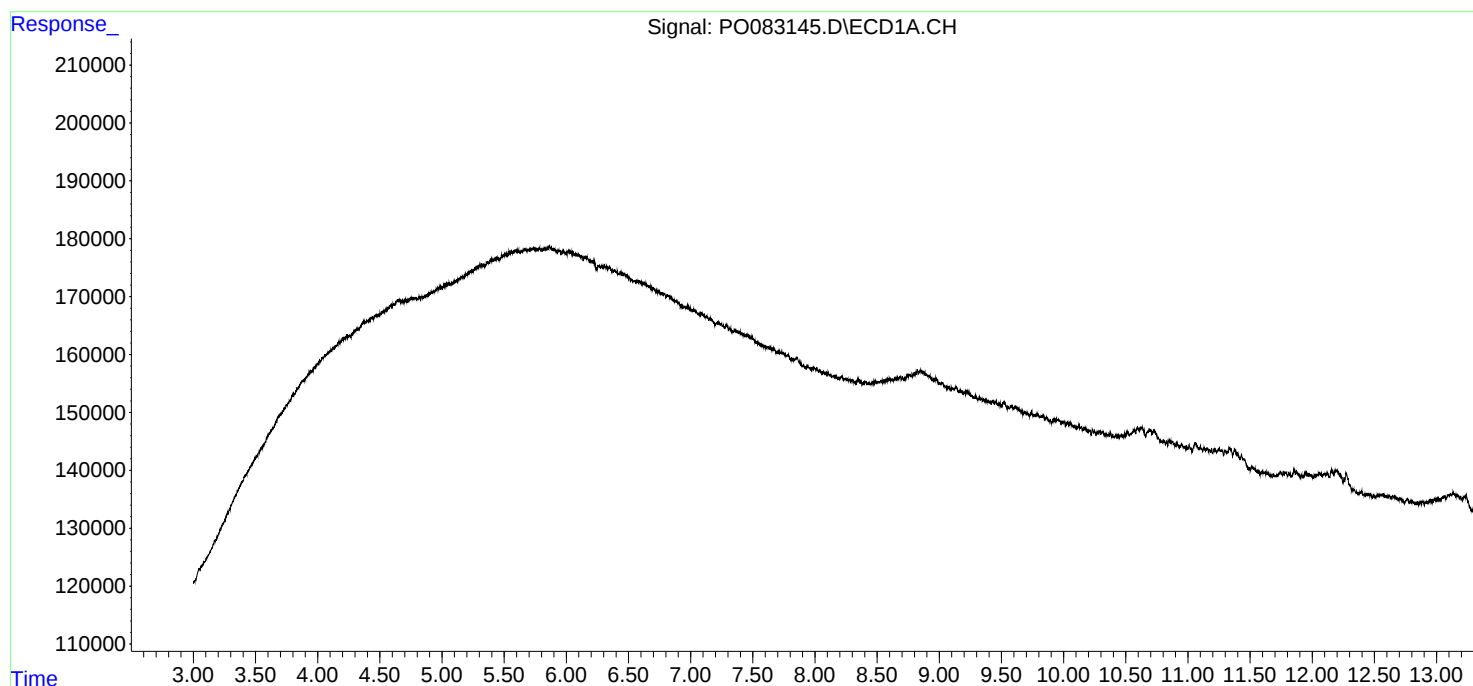


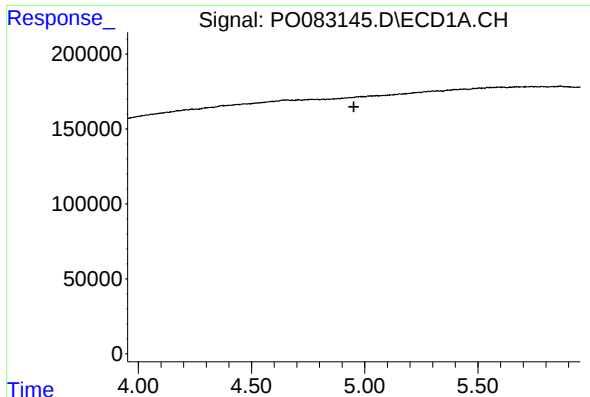

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

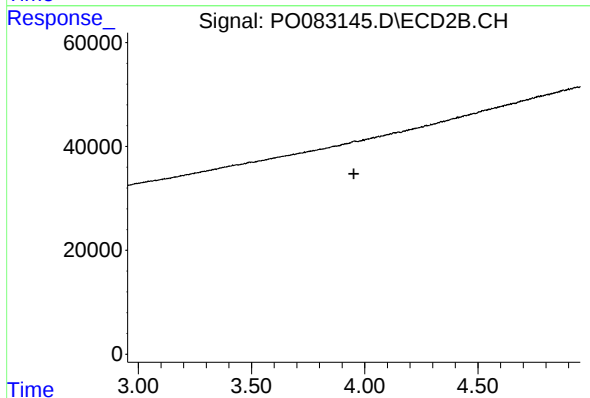


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

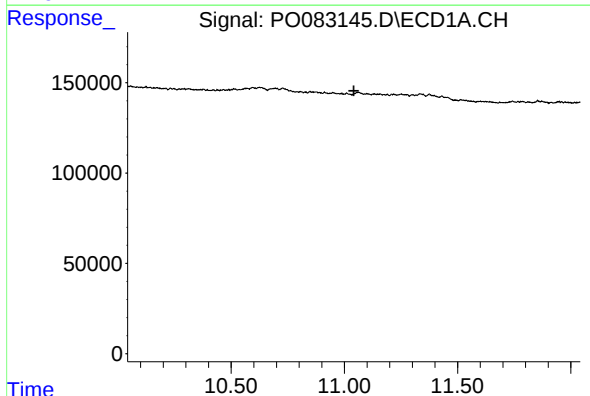


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.042 min
Response: 0
Conc: N.D.

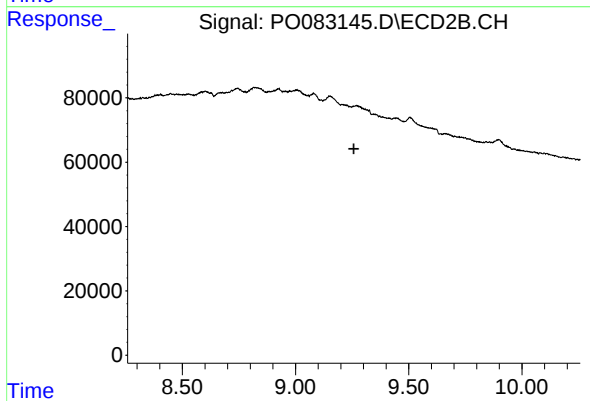

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.258 min
Response: 0
Conc: N.D.

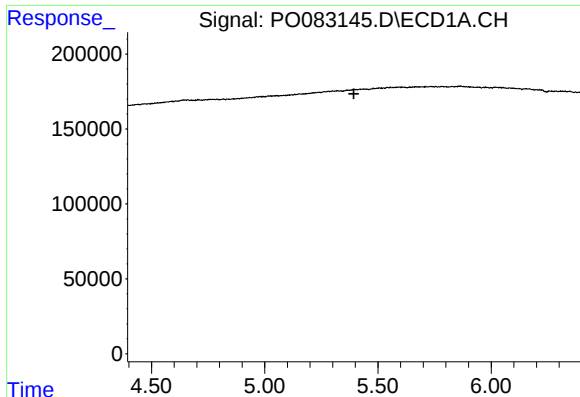

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

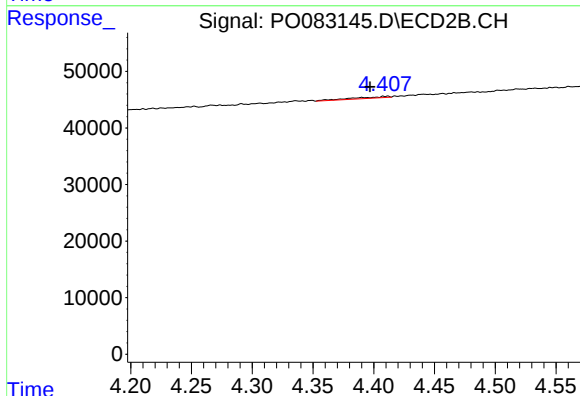


#10 AR-1221-3

R.T.: 4.412 min
Delta R.T.: 0.015 min
Response: 5455
Conc: 6.03 ng/ml

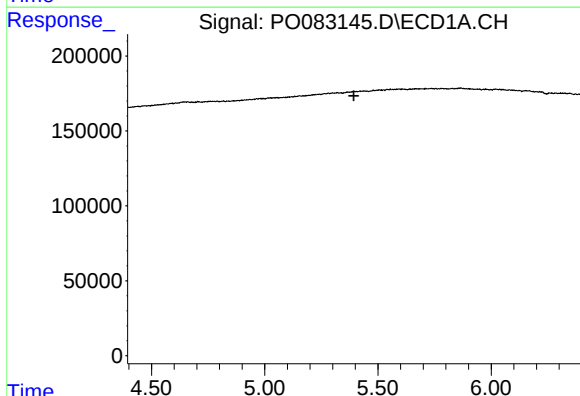


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.394 min
Response: 0
Conc: N.D.

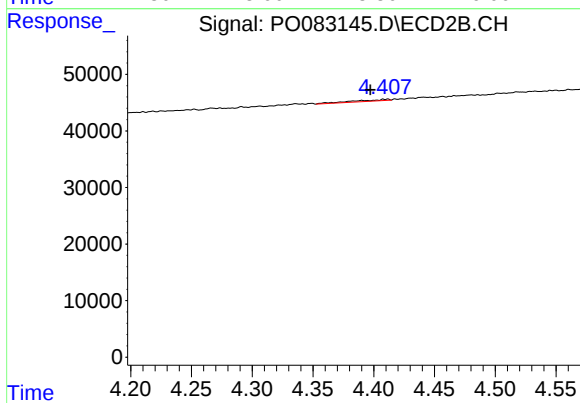

#11 AR-1232-1


R.T.: 4.412 min
Delta R.T.: 0.014 min
Response: 5455
Conc: 7.12 ng/ml

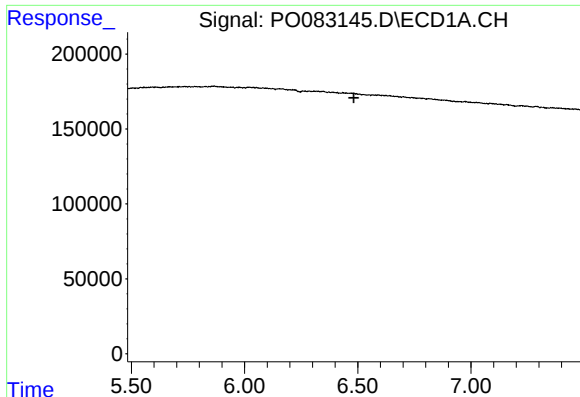

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

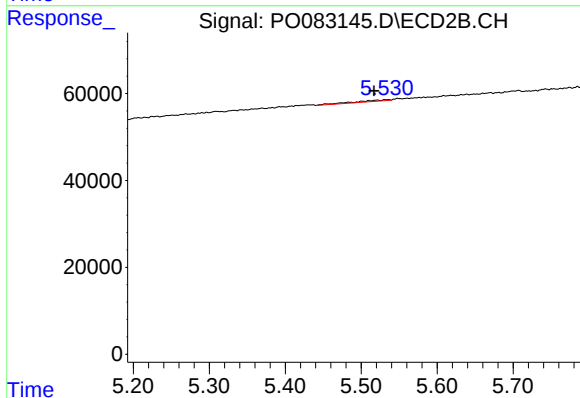


#14 AR-1232-4

R.T.: 5.537 min
Delta R.T.: 0.019 min
Response: 10548
Conc: 30.00 ng/ml

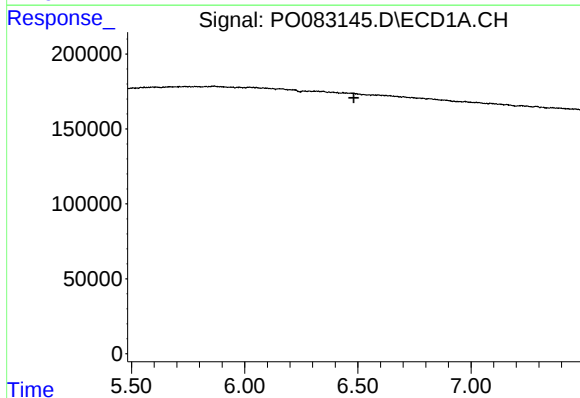


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.482 min
Response: 0
Conc: N.D.

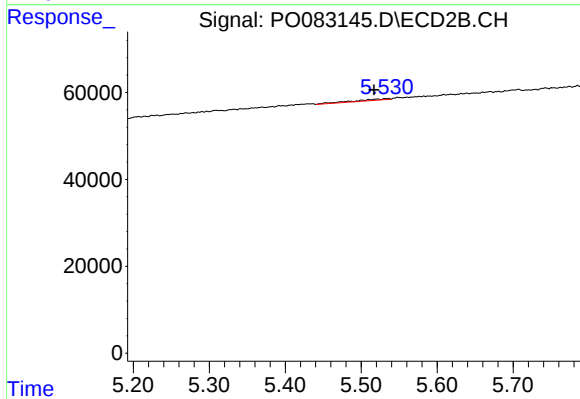

#19 AR-1242-4


R.T.: 5.537 min
Delta R.T.: 0.019 min
Response: 10548
Conc: 15.32 ng/ml

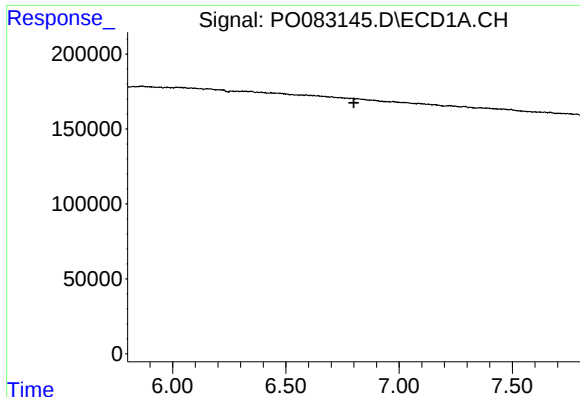

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

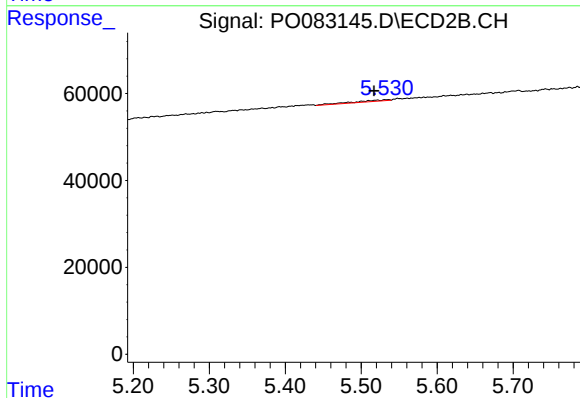


#23 AR-1248-3

R.T.: 5.537 min
Delta R.T.: 0.020 min
Response: 10548
Conc: 10.65 ng/ml

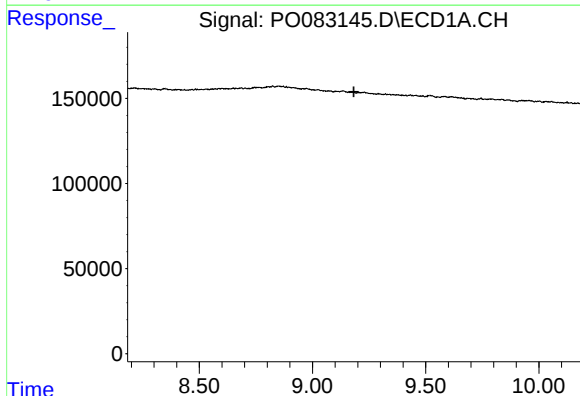


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 9.183 min
Response: 0
Conc: N.D.

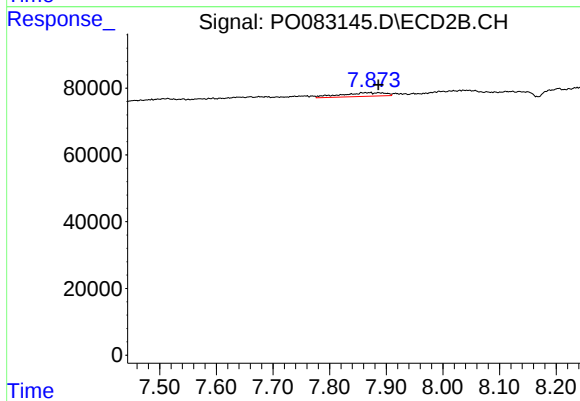

#35 AR-1260-5


R.T.: 7.872 min
Delta R.T.: -0.014 min
Response: 60396
Conc: 13.53 ng/ml

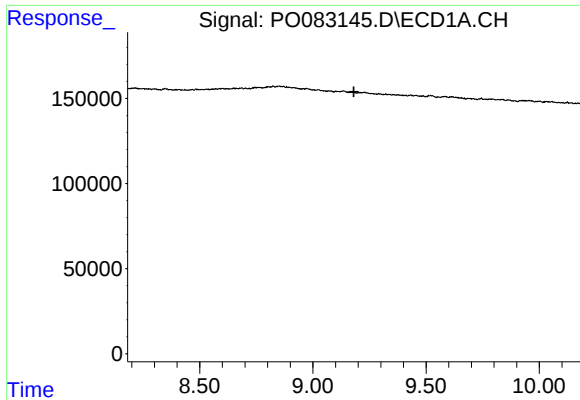

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

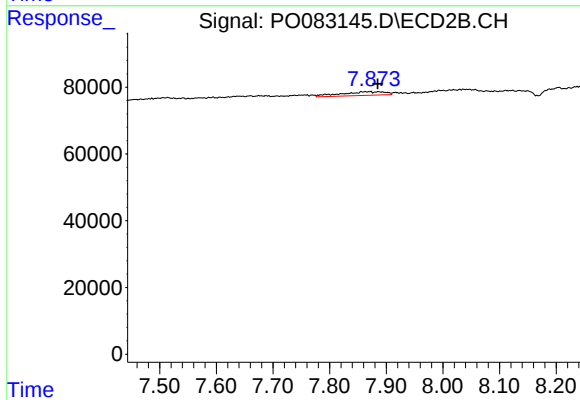


#37 AR-1262-2

R.T.: 7.872 min
Delta R.T.: -0.013 min
Response: 60396
Conc: 13.37 ng/ml

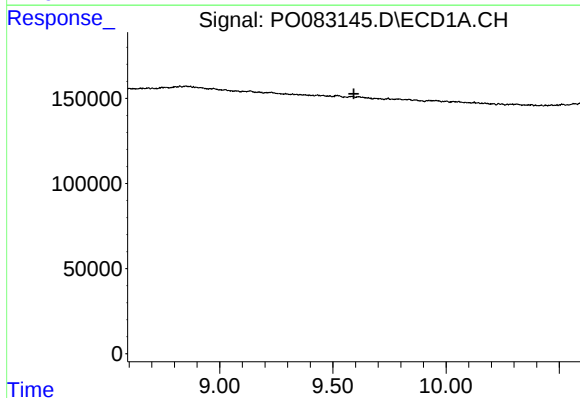


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.593 min
Response: 0
Conc: N.D.

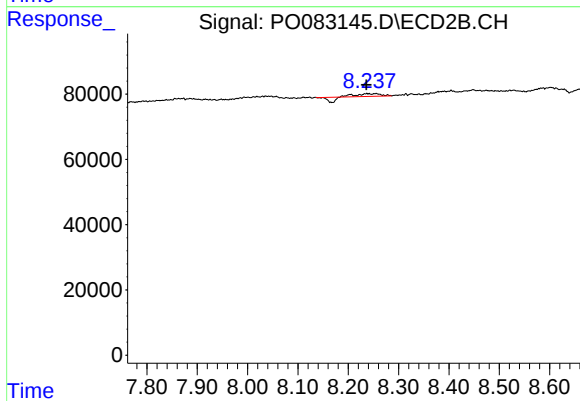

#39 AR-1262-4


R.T.: 8.238 min
Delta R.T.: 0.002 min
Response: 14380
Conc: 4.54 ng/ml

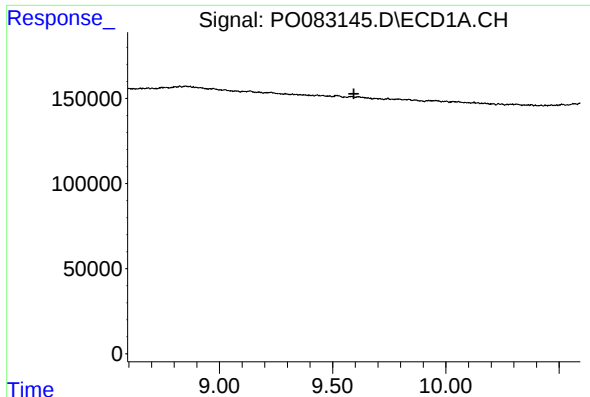

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.594 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

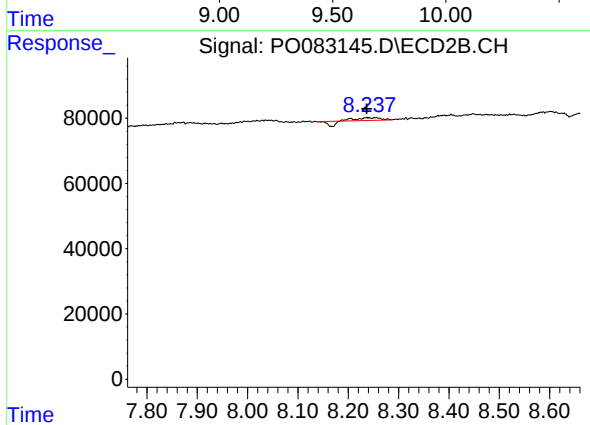

#42 AR-1268-2

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 14380
Conc: 2.99 ng/ml