

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
 Data File : PO083177.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2021 21:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 23:03:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.950	3.951	1868315	628416	21.289	20.616
2)	SA Decachlor...	11.042	9.258	1419848	596238	21.593	19.834
Target Compounds							
8)	L2 AR-1221-1	5.193	0.000	51161	0	53.989	N.D. #
9)	L2 AR-1221-2	5.306	0.000	23309	0	34.667	N.D. #
10)	L2 AR-1221-3	0.000	4.395	0	21842	N.D.	24.151 #
11)	L3 AR-1232-1	0.000	4.395	0	21842	N.D.	28.494 #
24)	L5 AR-1248-4	7.212	0.000	19428	0	7.415	N.D. #
26)	L6 AR-1254-1	7.212	0.000	19428	0	6.981	N.D. #
28)	L6 AR-1254-3	7.838f	0.000	19614	0	4.567	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
Data File : PO083177.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2021 21:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 23:03:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

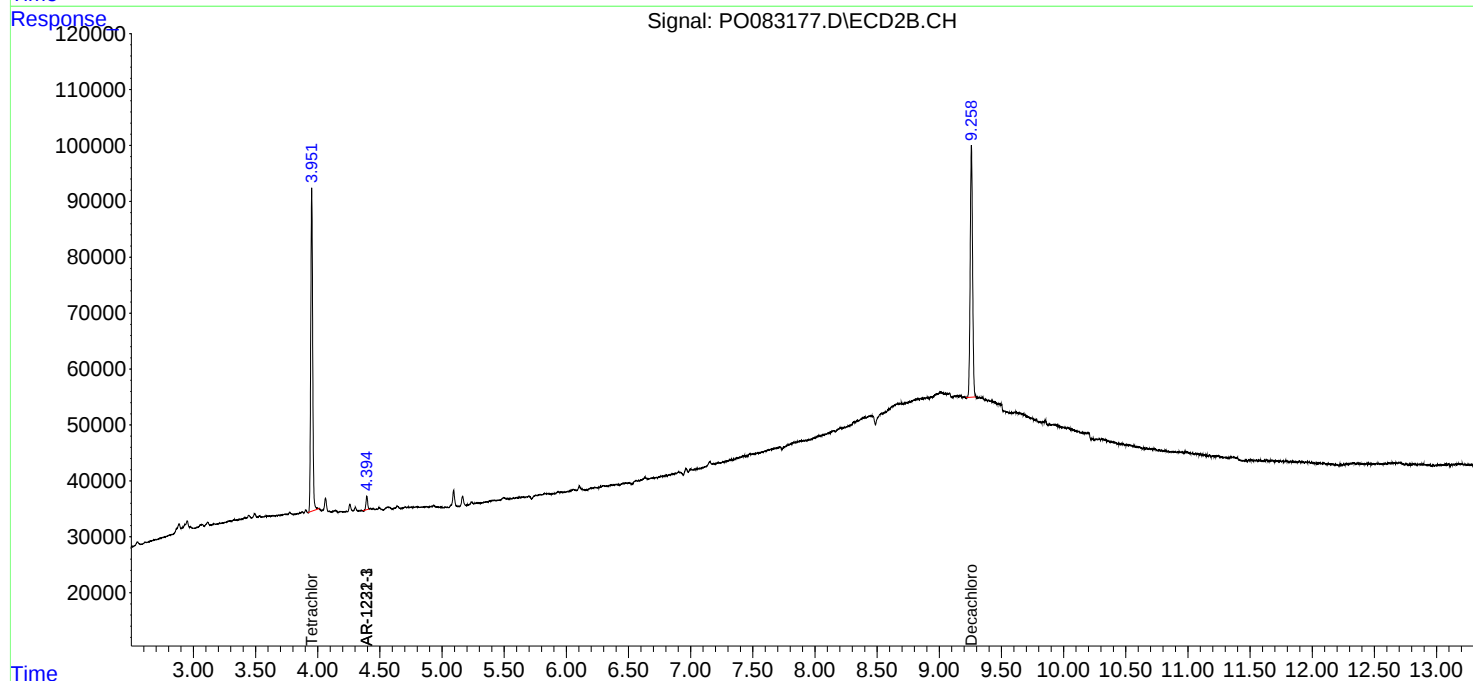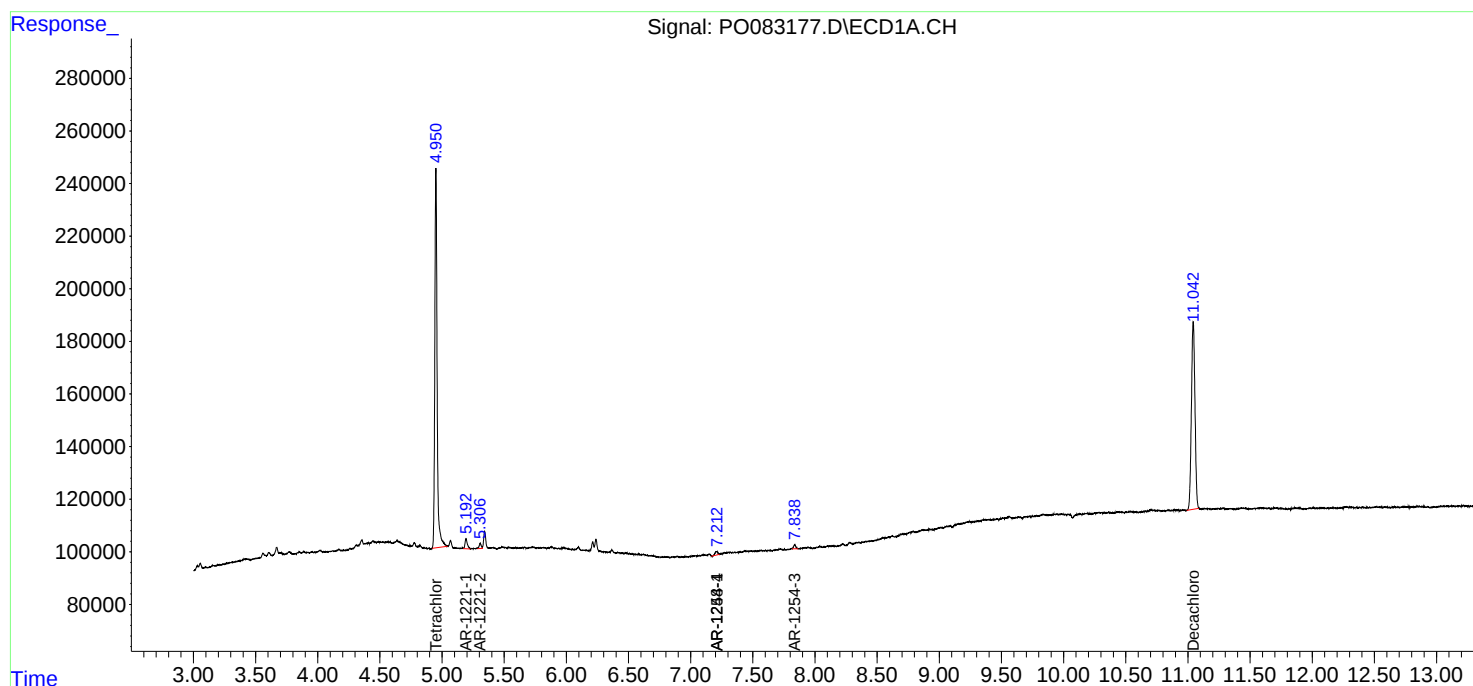


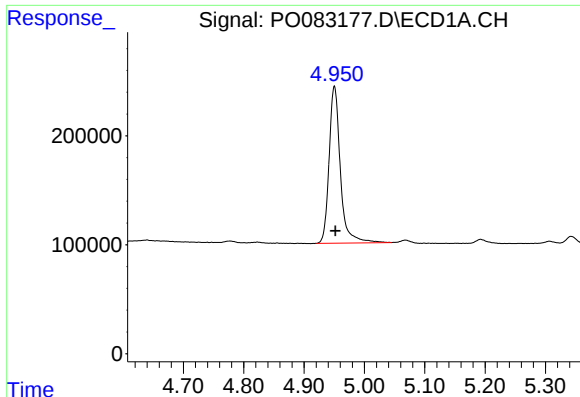

#1 Tetrachloro-m-xylene


R.T.: 4.950 min
Delta R.T.: -0.002 min
Response: 1868315
Conc: 21.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

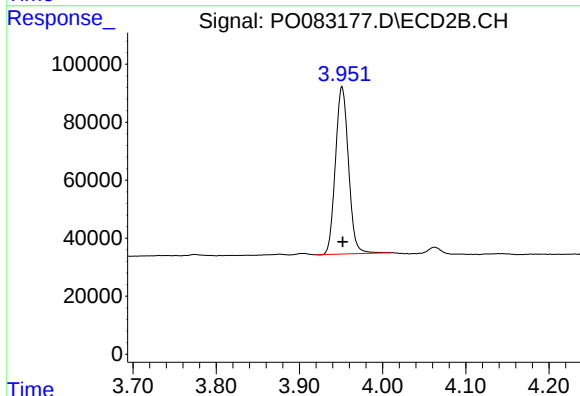


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 628416
Conc: 20.62 ng/ml

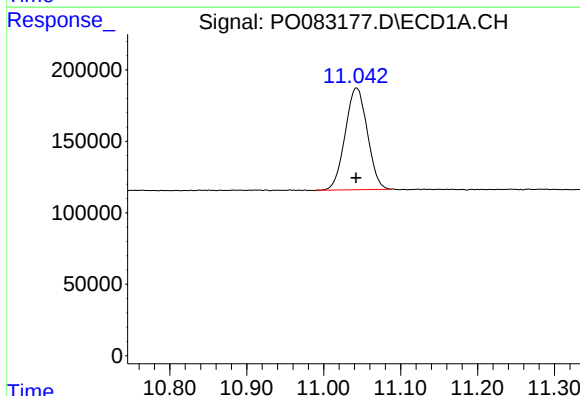


#2 Decachlorobiphenyl

R.T.: 11.042 min
Delta R.T.: 0.000 min
Response: 1419848
Conc: 21.59 ng/ml

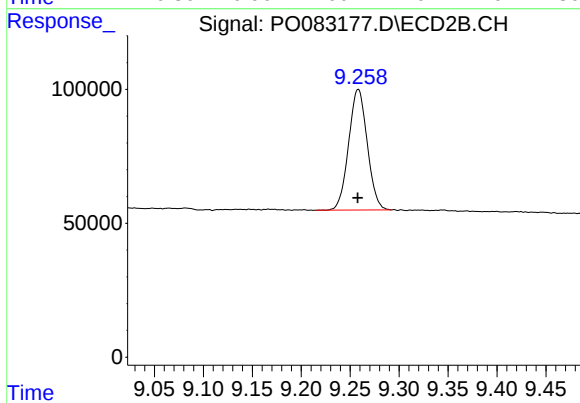

#2 Decachlorobiphenyl


R.T.: 9.258 min
Delta R.T.: 0.000 min
Response: 596238
Conc: 19.83 ng/ml

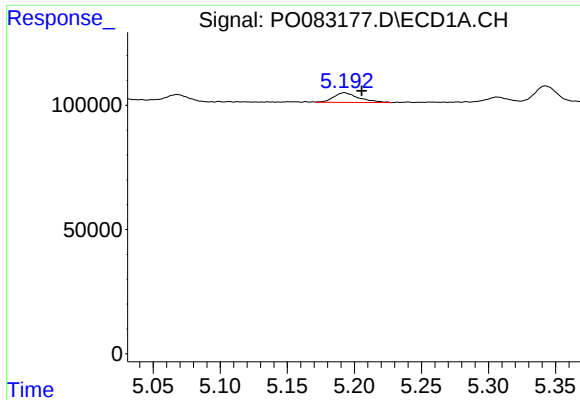

#8 AR-1221-1


R.T.: 5.193 min
Delta R.T.: -0.013 min
Response: 51161
Conc: 53.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

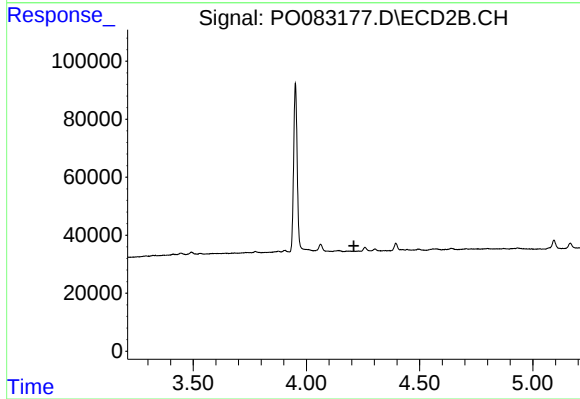


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.210 min
Response: 0
Conc: N.D.

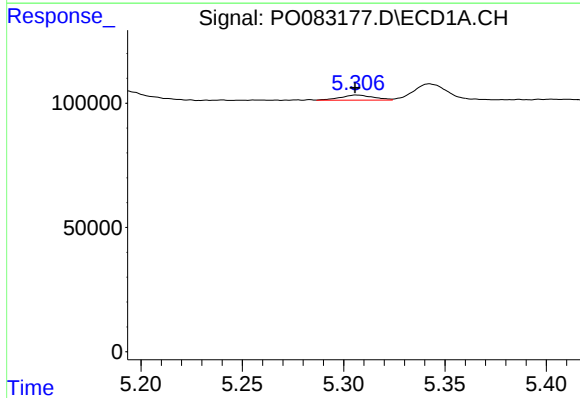


#9 AR-1221-2

R.T.: 5.306 min
Delta R.T.: 0.000 min
Response: 23309
Conc: 34.67 ng/ml

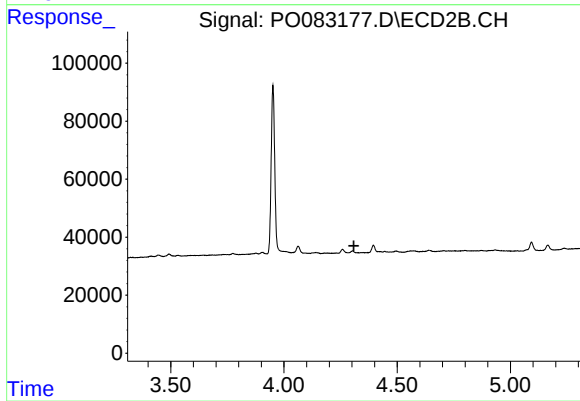

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.309 min
Response: 0
Conc: N.D.

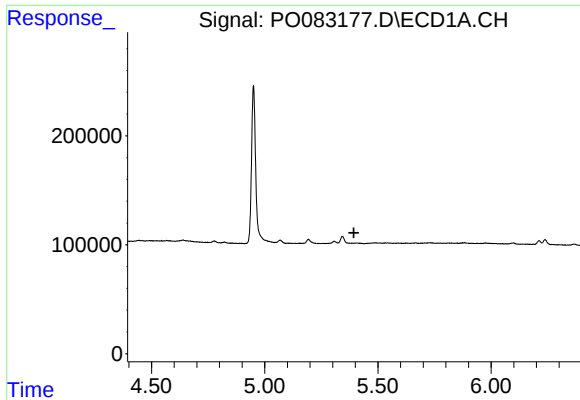

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

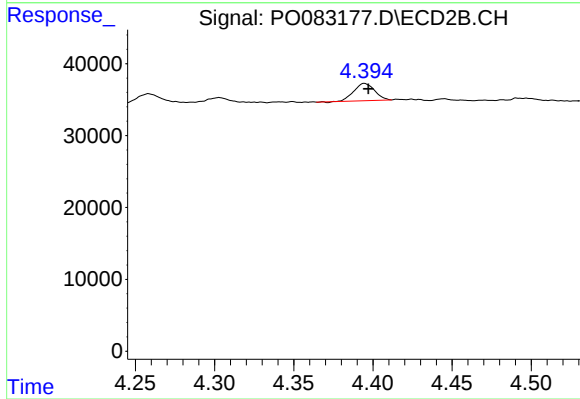


#10 AR-1221-3

R.T.: 4.395 min
Delta R.T.: -0.002 min
Response: 21842
Conc: 24.15 ng/ml

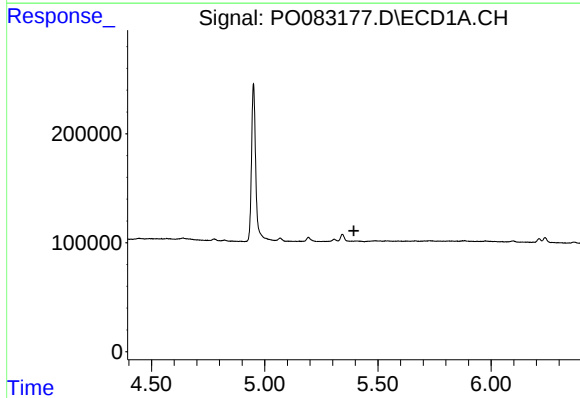


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

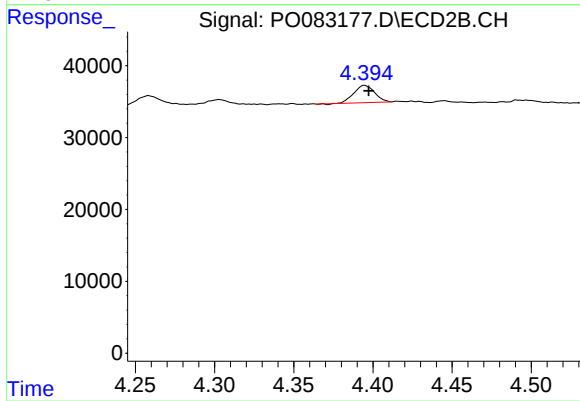

#11 AR-1232-1


R.T.: 4.395 min
Delta R.T.: -0.003 min
Response: 21842
Conc: 28.49 ng/ml

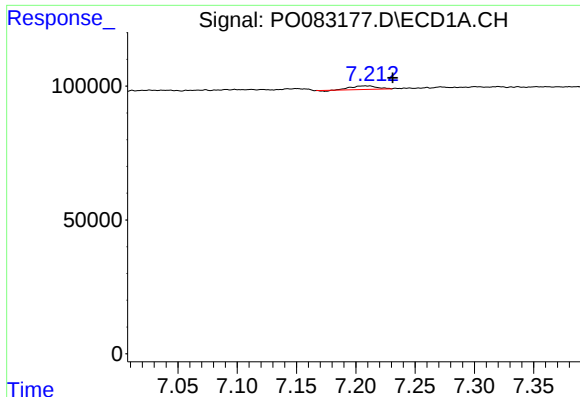

#24 AR-1248-4


R.T.: 7.212 min
Delta R.T.: -0.019 min
Response: 19428
Conc: 7.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

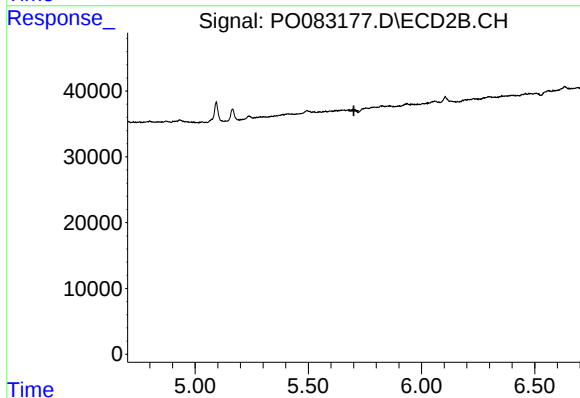


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.701 min
Response: 0
Conc: N.D.

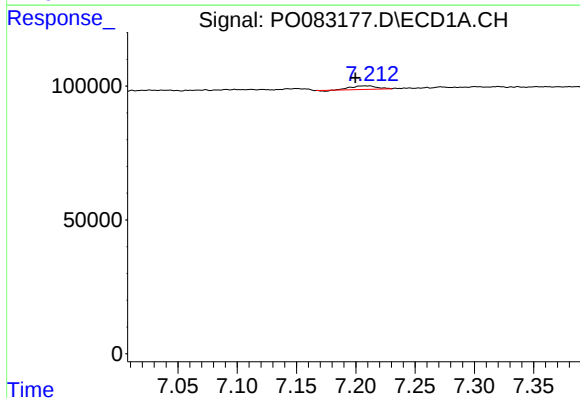


#26 AR-1254-1

R.T.: 7.212 min
Delta R.T.: 0.012 min
Response: 19428
Conc: 6.98 ng/ml

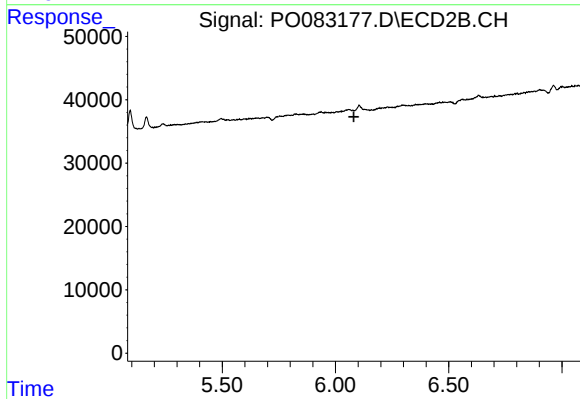

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

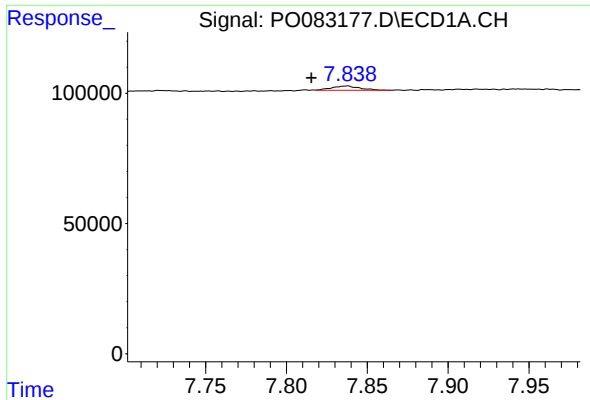

#28 AR-1254-3

R.T.: 7.838 min
Delta R.T.: 0.023 min
Response: 19614
Conc: 4.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

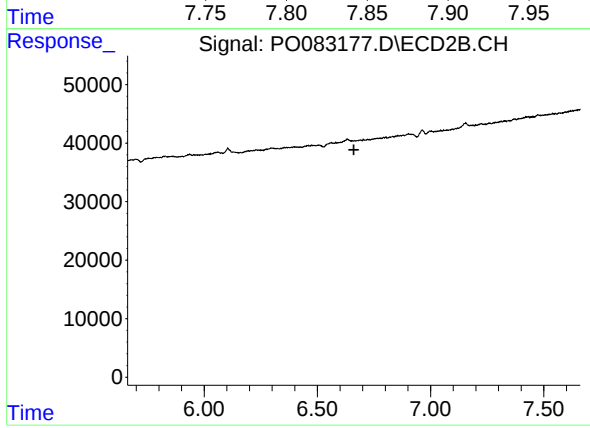

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.661 min
Response: 0
Conc: N.D.