

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
 Data File : PO083166.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2021 17:57
 Operator : AJ\MA
 Sample : M4782-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-111921

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 22:59:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.951	3.952	1650915	584963	18.812m	19.190
2) SA Decachlor...	11.045	9.259	1001085	456437	15.224	15.183

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
Data File : P0083166.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2021 17:57
Operator : AJ\MA
Sample : M4782-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-111921

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 22:59:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

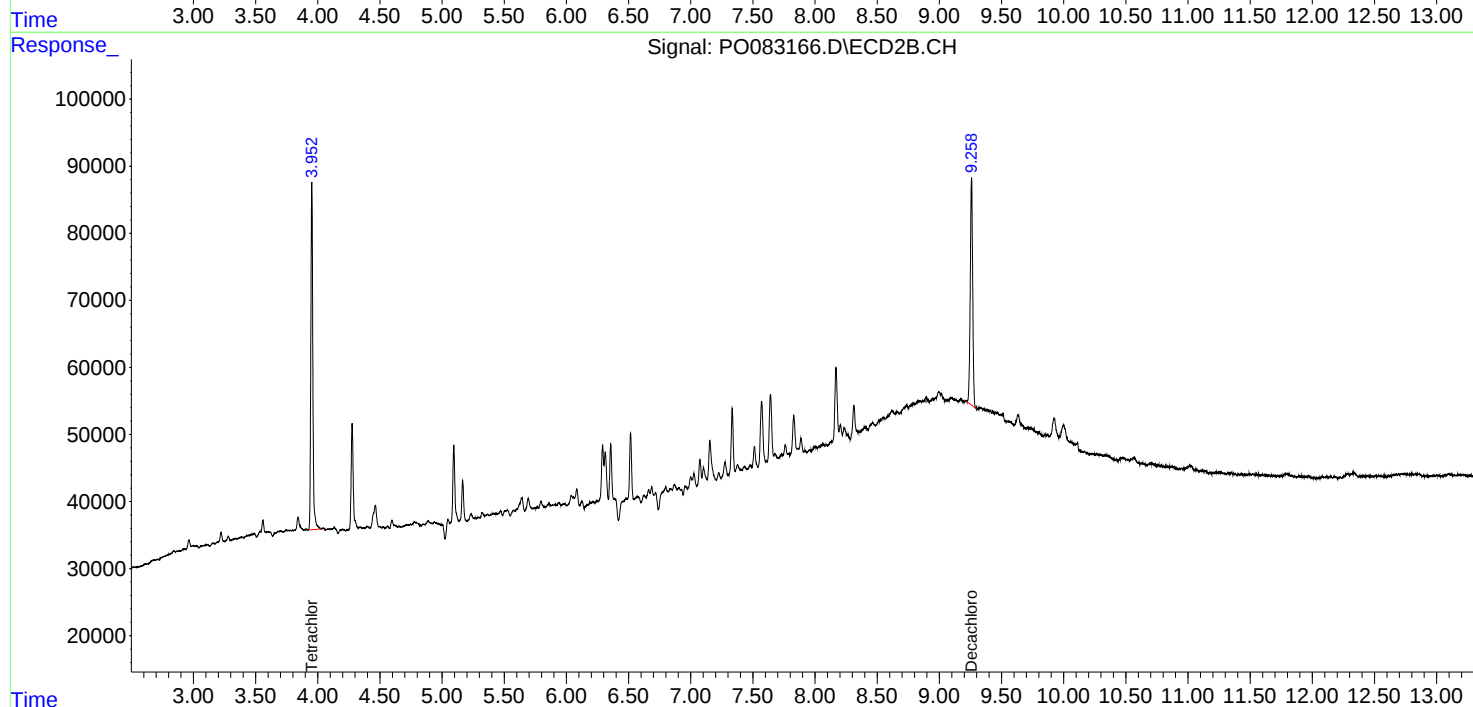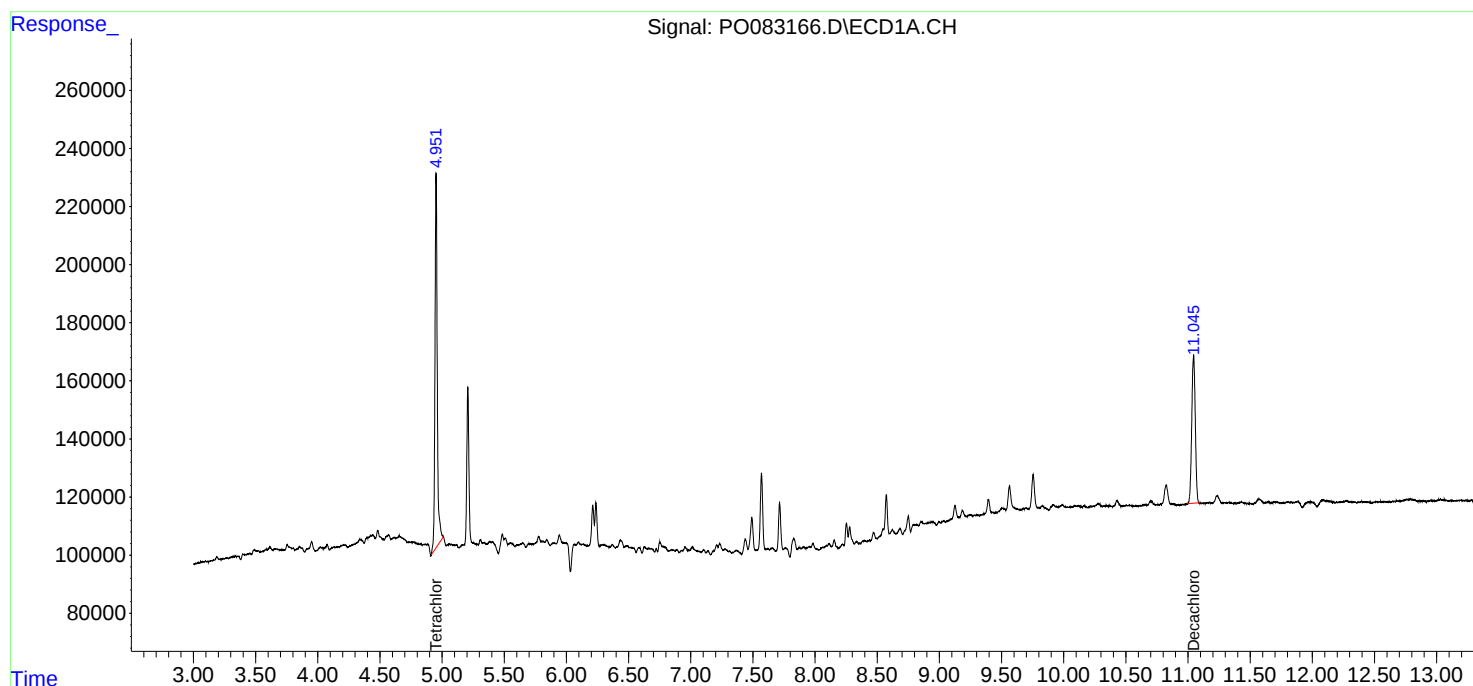


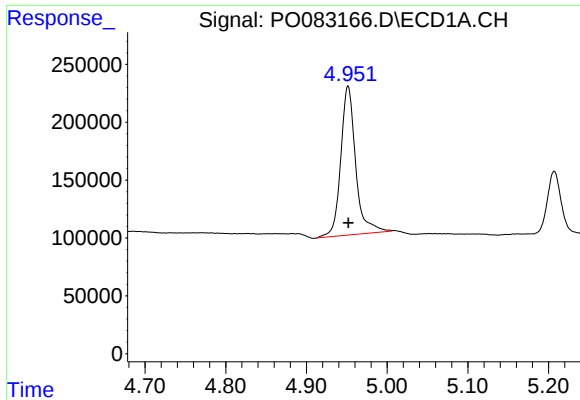

#1 Tetrachloro-m-xylene


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 1650915
Conc: 18.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-111921

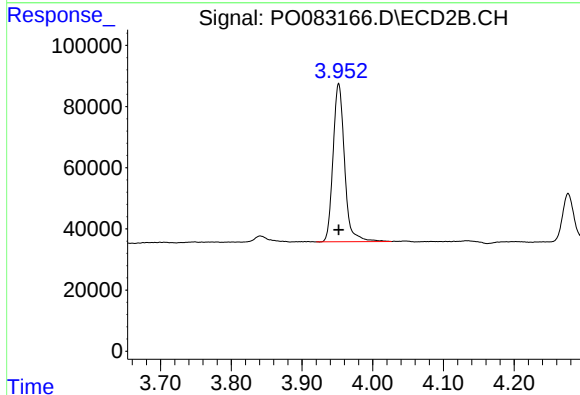


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 584963
Conc: 19.19 ng/ml

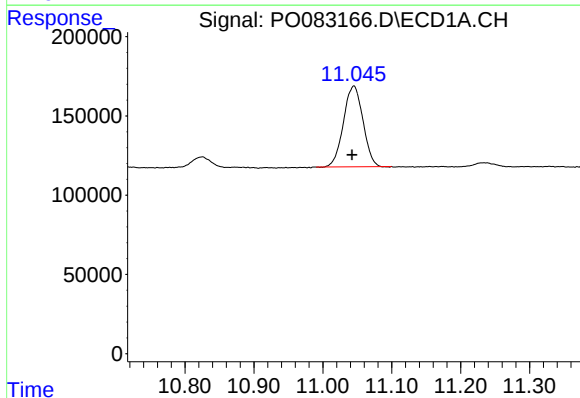

#2 Decachlorobiphenyl

R.T.: 11.045 min
Delta R.T.: 0.003 min
Response: 1001085
Conc: 15.22 ng/ml

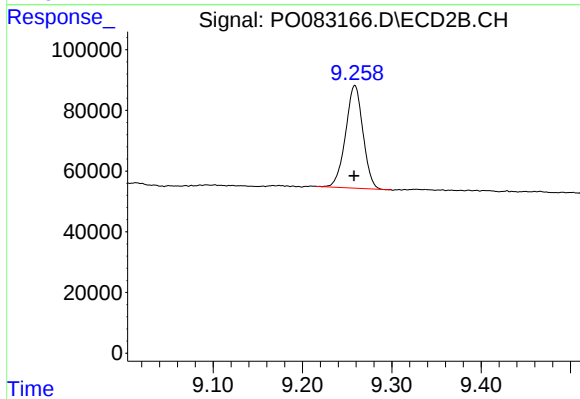

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: 0.000 min
Response: 456437
Conc: 15.18 ng/ml