

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112221\
 Data File : P0083171.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Nov 2021 19:23
 Operator : AJ\MA
 Sample : M4801-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SITE-1-DRILL-CUTTINGS-20211119

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 23:01:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.953	3.953	1906986	642359	21.730	21.073
2) SA Decachlor...	11.046	9.262	1431576	557214	21.771	18.536

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112221\
Data File : PO083171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Nov 2021 19:23
Operator : AJ\MA
Sample : M4801-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SITE-1-DRILL-CUTTINGS-20211119

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 23:01:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

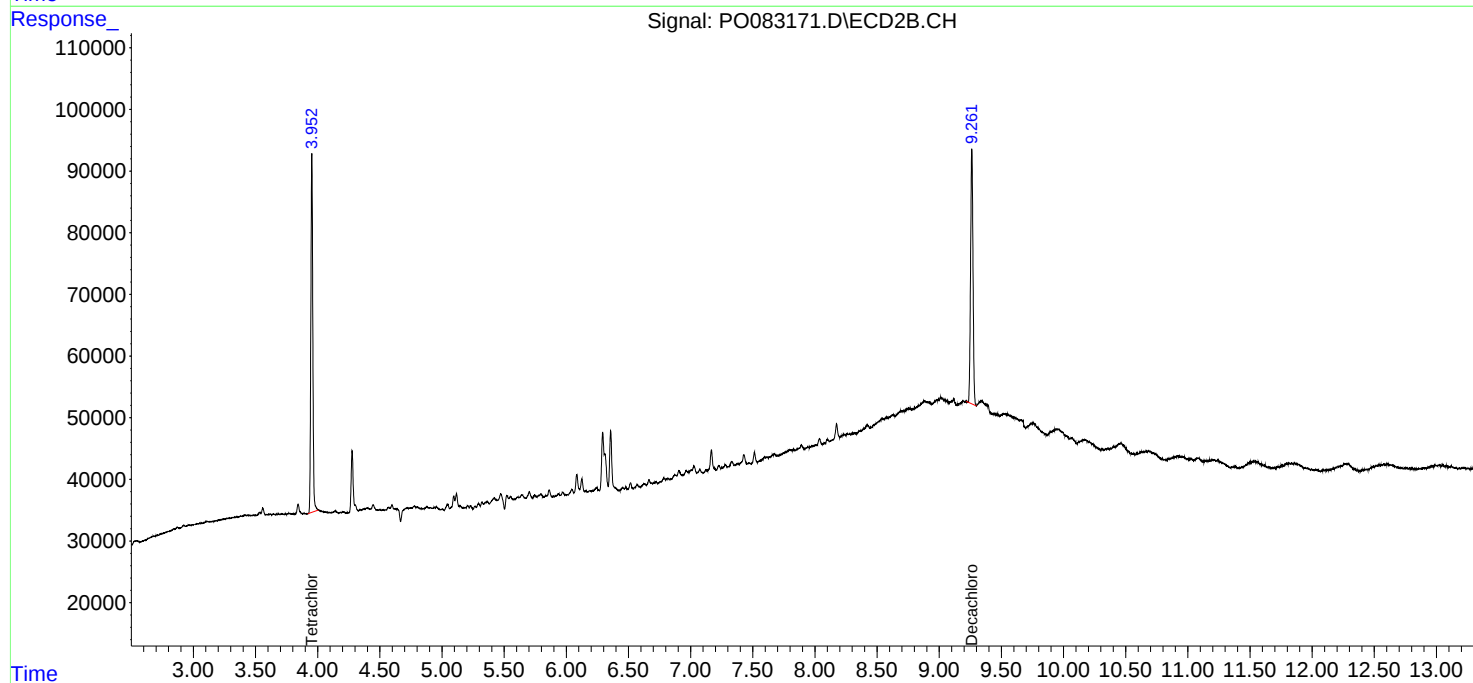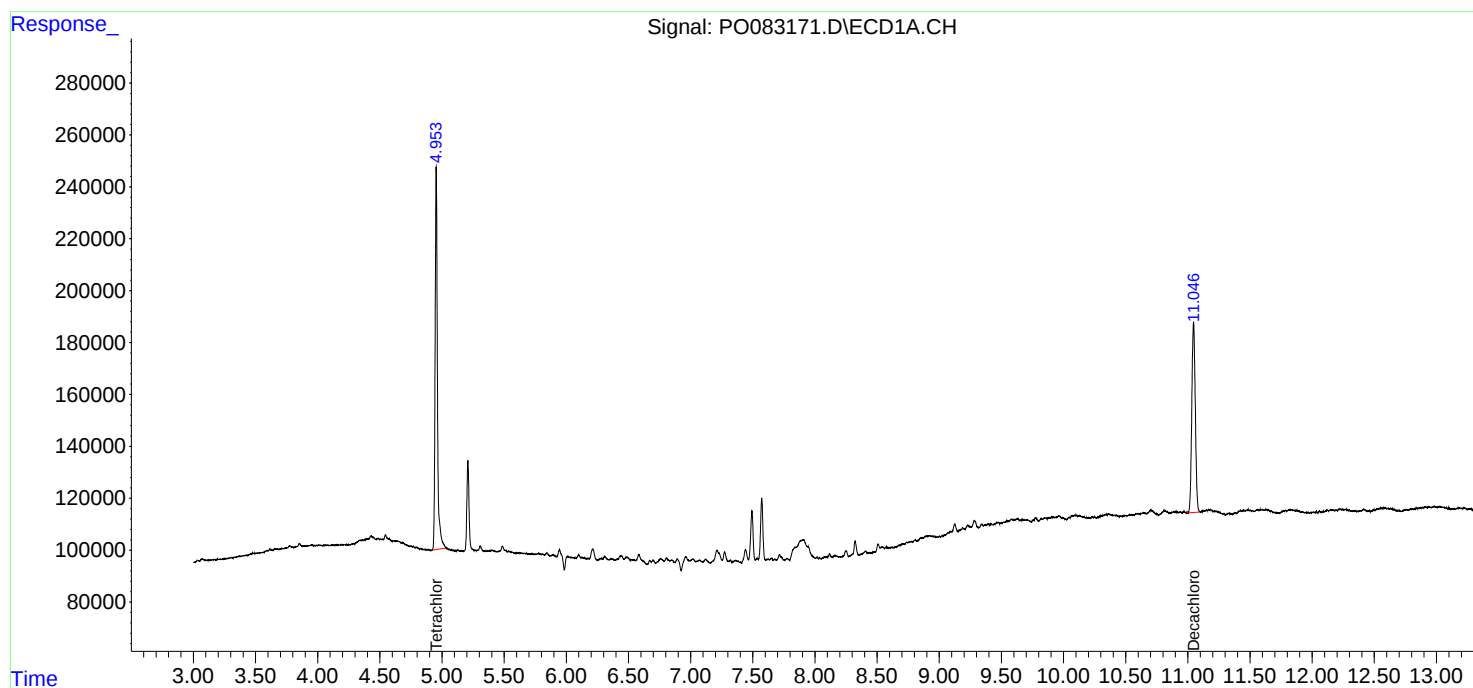


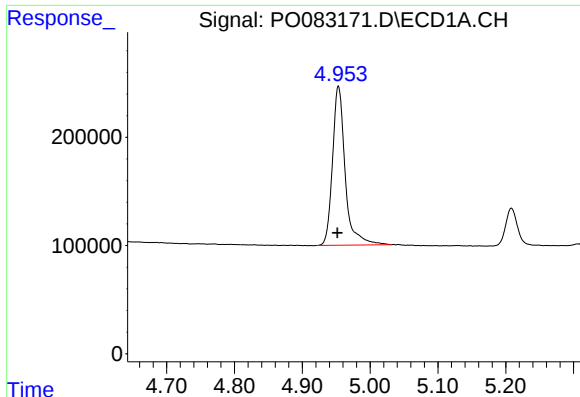

#1 Tetrachloro-m-xylene


R.T.: 4.953 min
Delta R.T.: 0.001 min
Response: 1906986
Conc: 21.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
SITE-1-DRILL-CUTTINGS-20211119

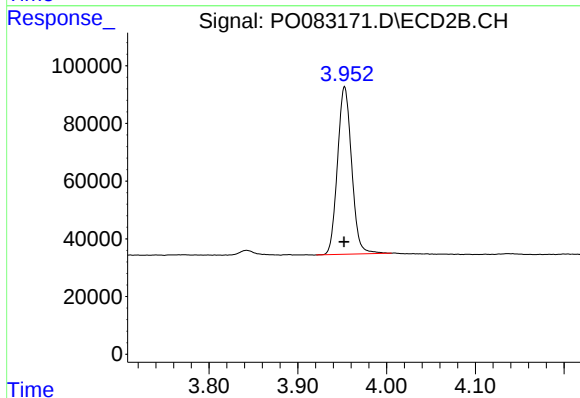


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: 0.000 min
Response: 642359
Conc: 21.07 ng/ml

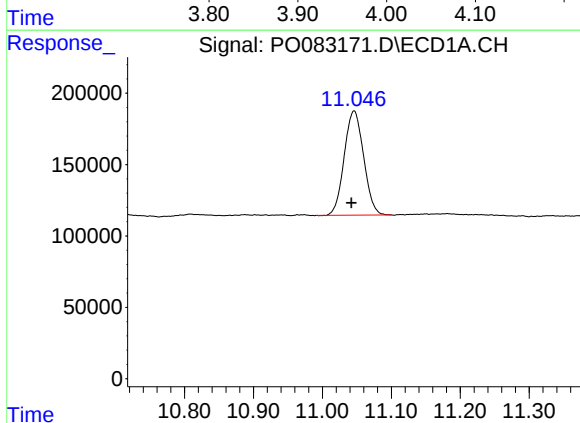

#2 Decachlorobiphenyl

R.T.: 11.046 min
Delta R.T.: 0.004 min
Response: 1431576
Conc: 21.77 ng/ml

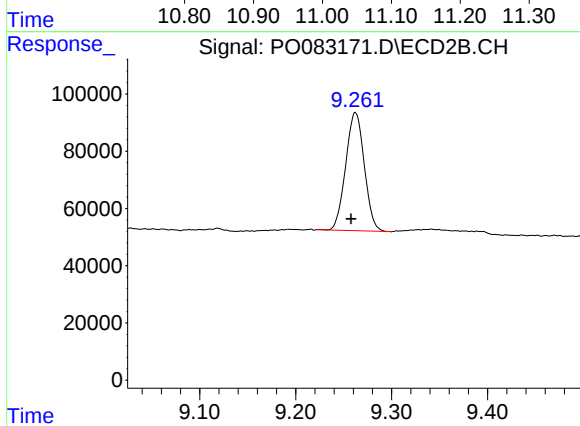

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: 0.004 min
Response: 557214
Conc: 18.54 ng/ml