

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112222\
 Data File : P0090889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 22:02
 Operator : YP/AJ
 Sample : N5733-22 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LAW-2022-56A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2022
 Supervised By :Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 04:49:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.477	4148643	1529414	1.291	1.439
2) SA Decachlor...	10.047	8.481	5026300	1530914	2.051	1.486m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112222\
Data File : PO090889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 22:02
Operator : YP/AJ
Sample : N5733-22 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LAW-2022-56A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 04:49:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

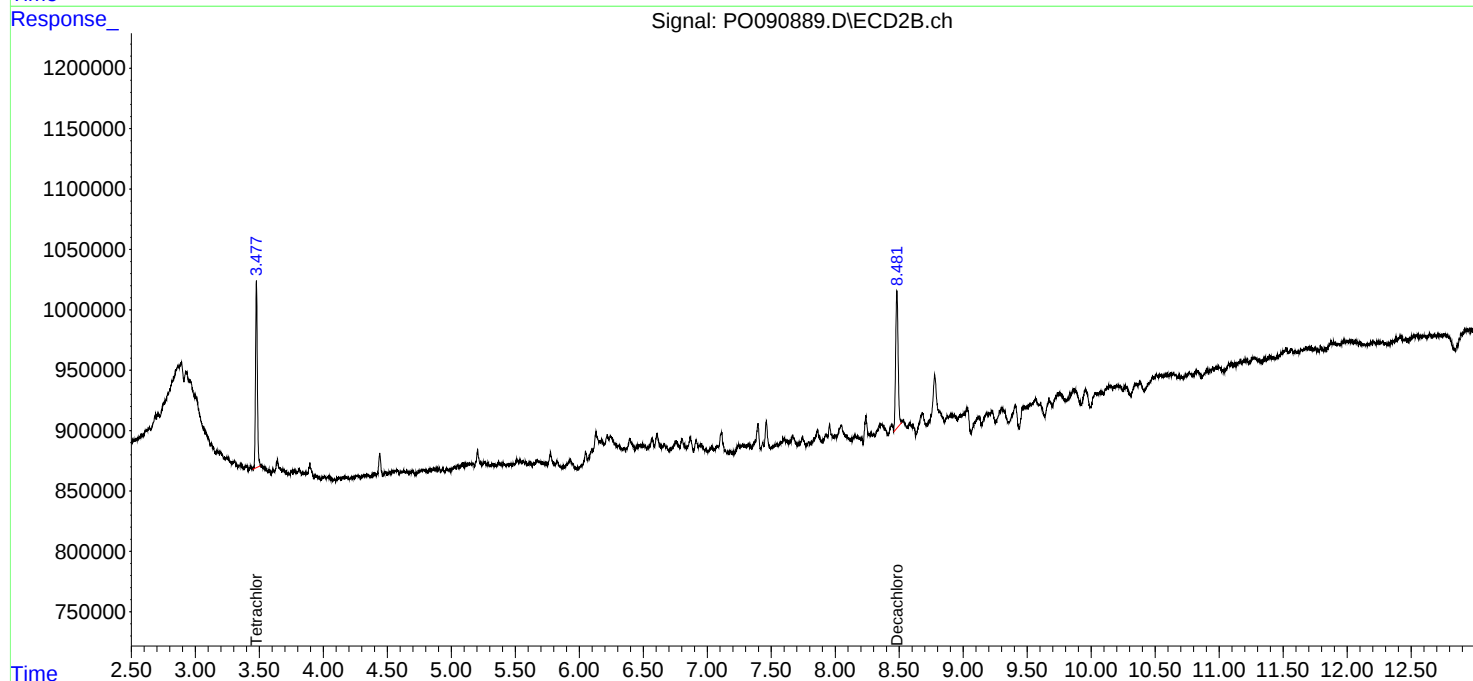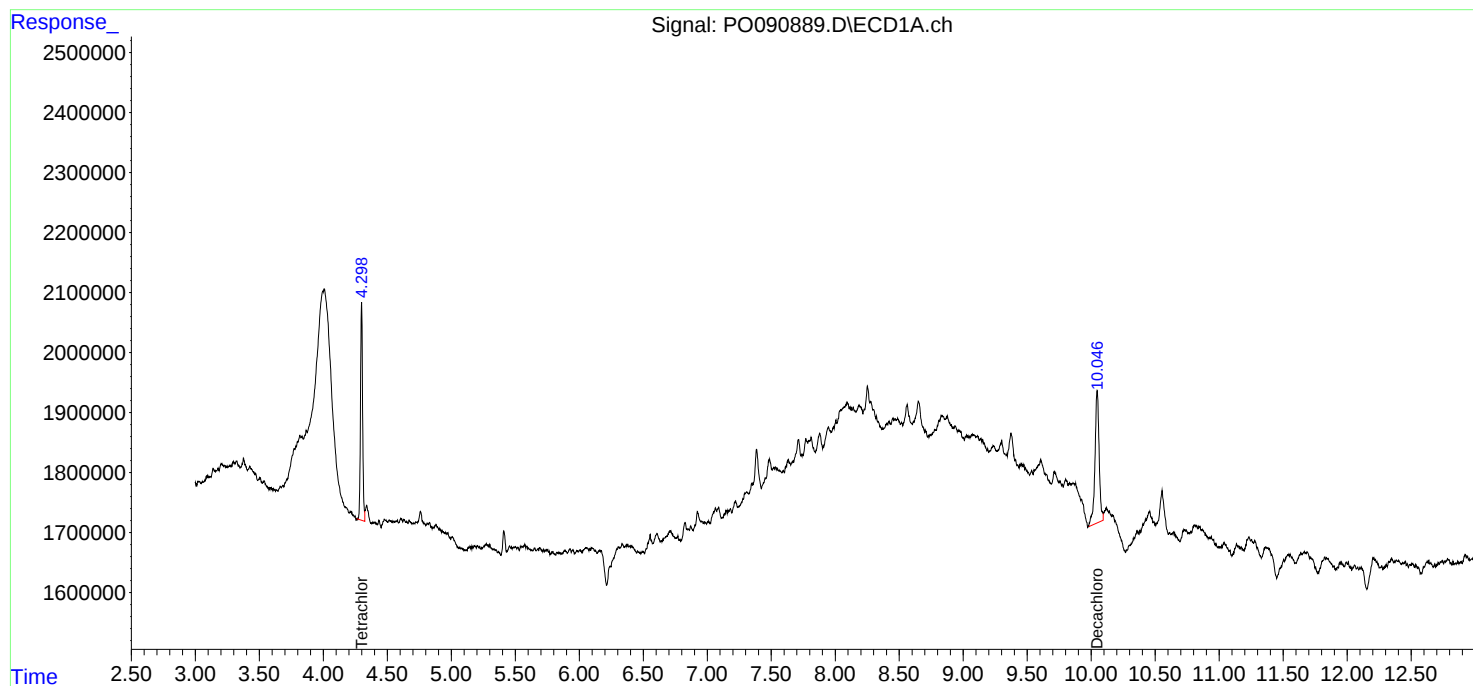

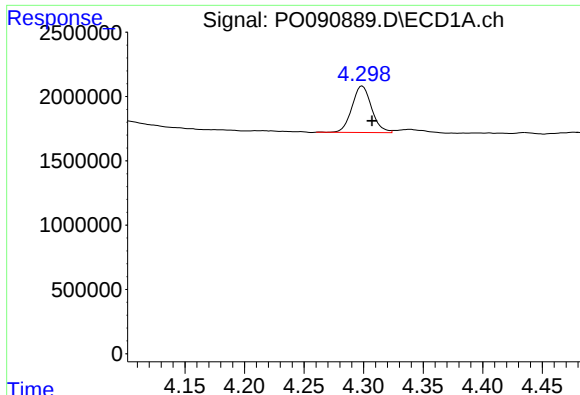


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.008 min
Response: 4148643
Conc: 1.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-56A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2022
Supervised By :Ankita Jodhani 11/23/2022

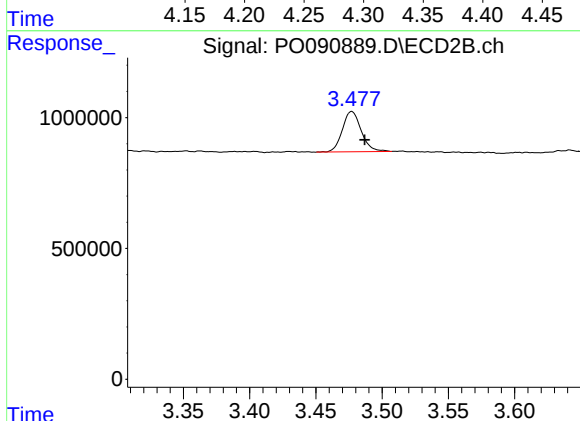


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.010 min
Response: 1529414
Conc: 1.44 ng/ml

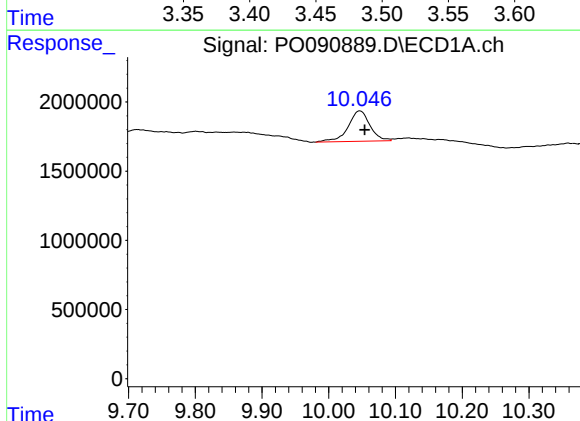

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: -0.007 min
Response: 5026300
Conc: 2.05 ng/ml

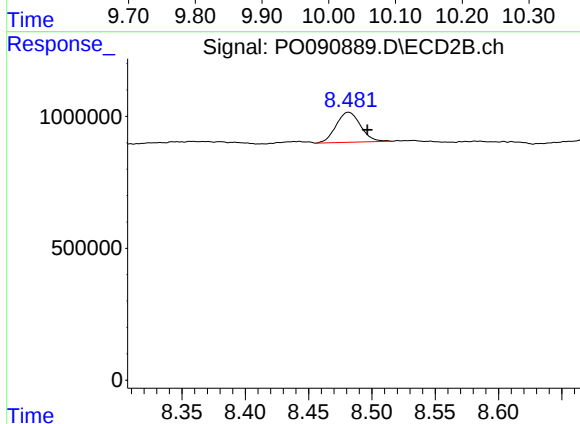

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.015 min
Response: 1530914
Conc: 1.49 ng/ml m