

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112224\
 Data File : PO108203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2024 19:44
 Operator : YP/AJ
 Sample : P4952-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GAS-BUR-1618

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/25/2024
 Supervised By :Ankita Jodhani 11/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 23:20:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.637	145.4E6	537.7E6	16.698m	158.591m#
2) SA Decachlor...	10.104	8.638	35438358	26315444	11.603	7.736 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112224\
Data File : PO108203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 19:44
Operator : YP/AJ
Sample : P4952-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GAS-BUR-1618


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 23:20:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

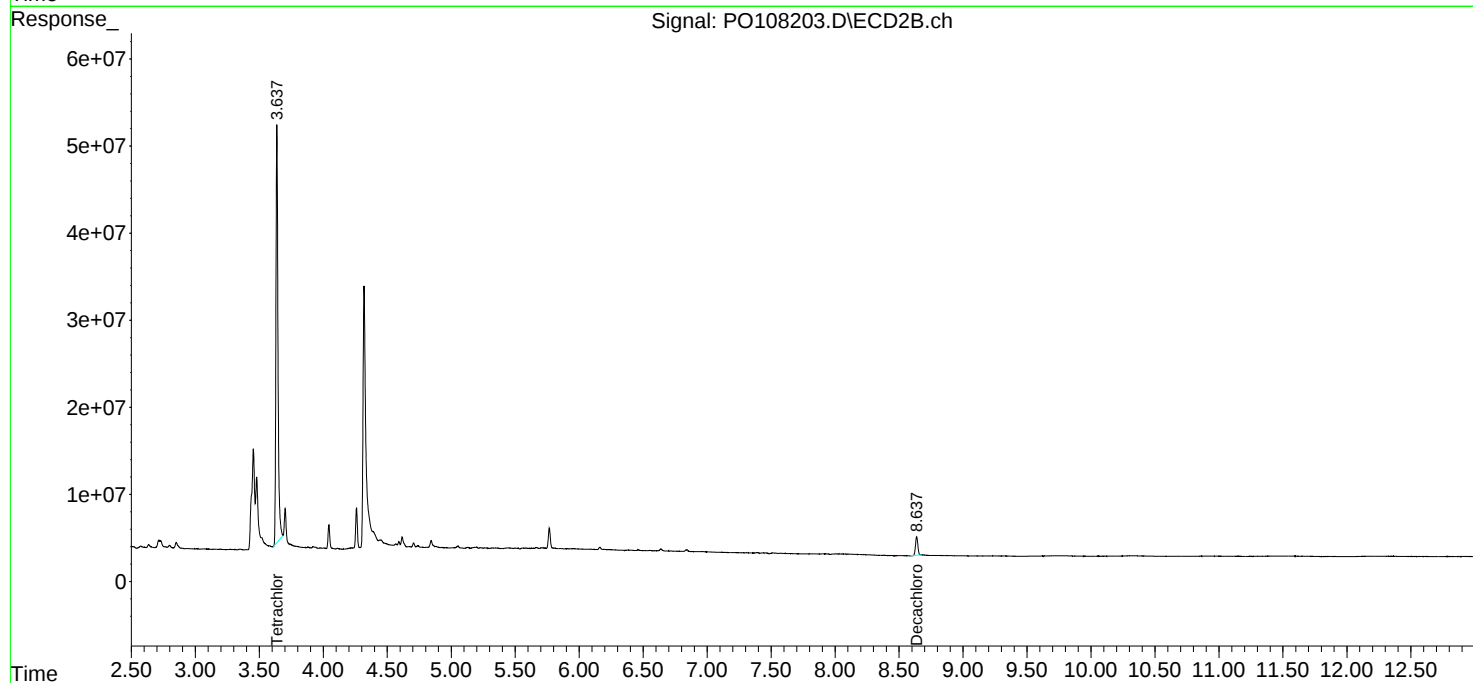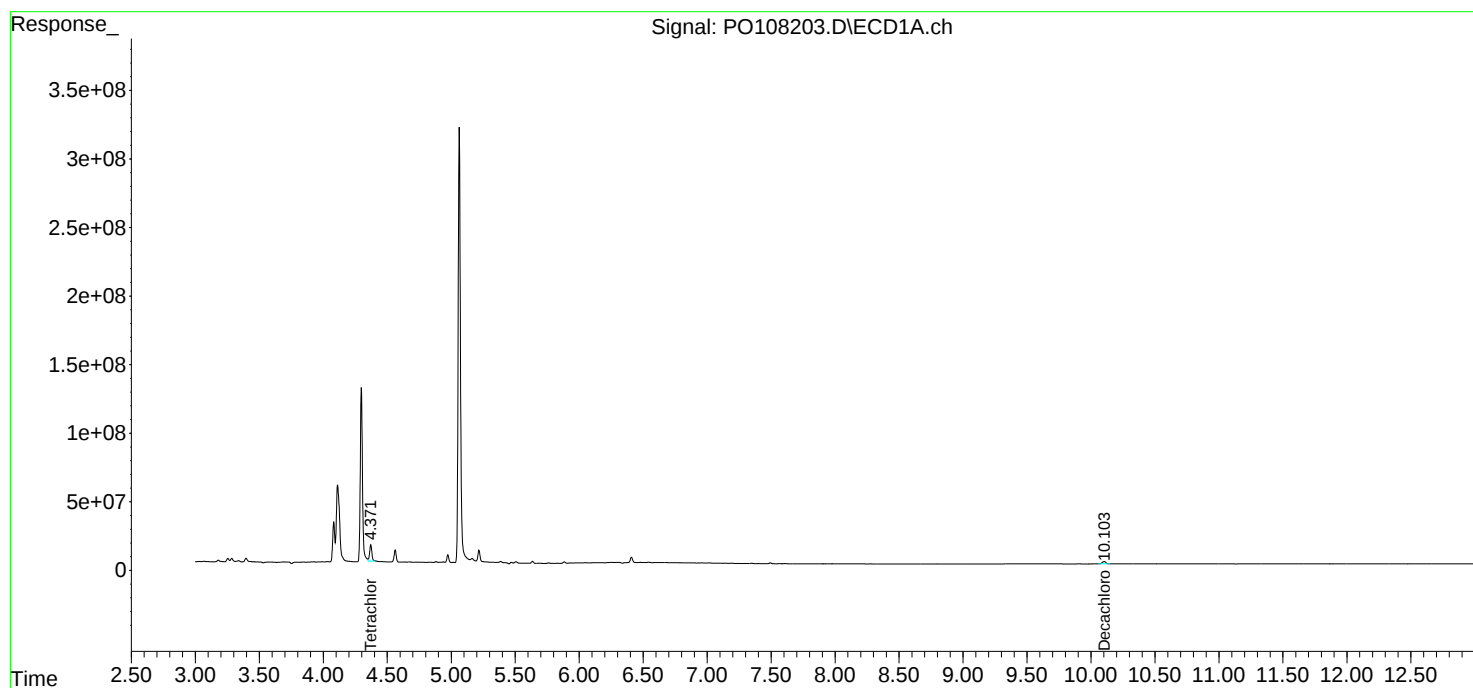

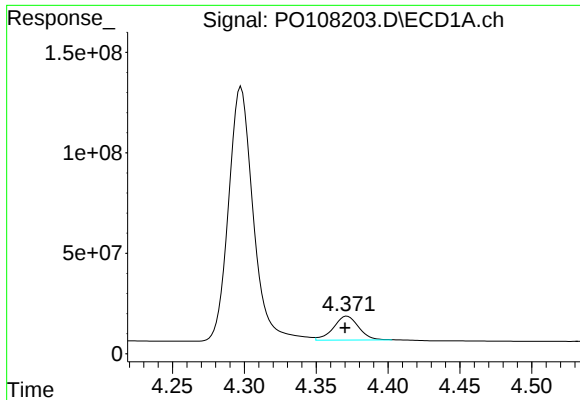


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 145370838
Conc: 16.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
GAS-BUR-1618


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

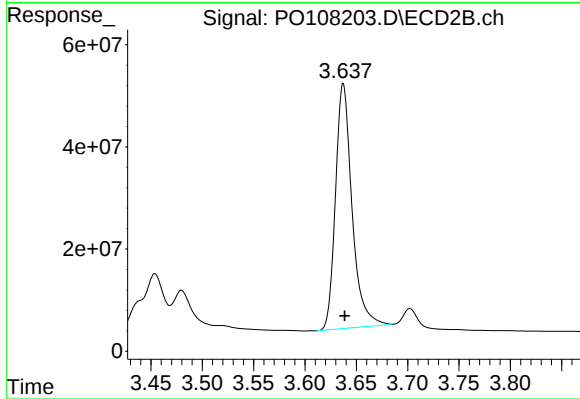


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 537689371
Conc: 158.59 ng/ml m

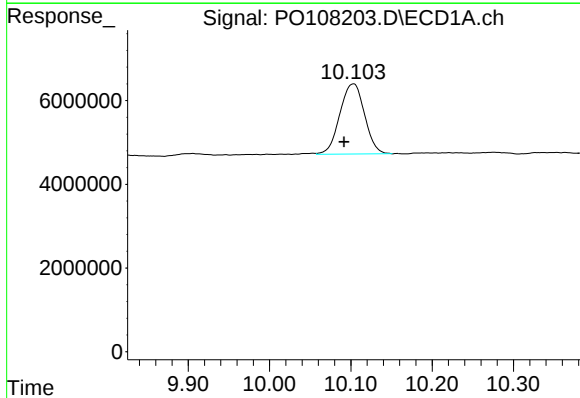

#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: 0.012 min
Response: 35438358
Conc: 11.60 ng/ml

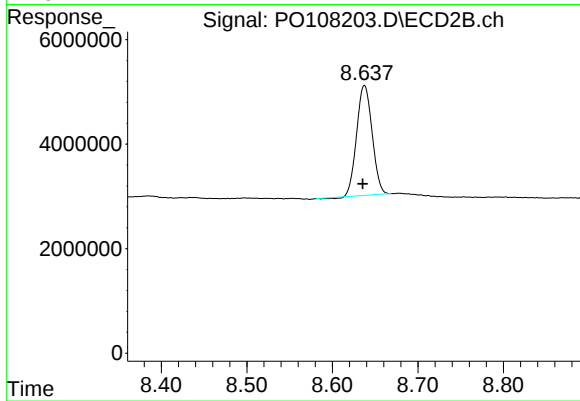

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.002 min
Response: 26315444
Conc: 7.74 ng/ml