

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112224\
 Data File : PO108211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2024 22:38
 Operator : YP/AJ
 Sample : P4953-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1297

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/25/2024
 Supervised By :Ankita Jodhani 11/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 00:19:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.639	123.5E6	59524187	14.184	17.557
2) SA Decachlor...	10.100	8.637	19630096	19894956	6.427m	5.849

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112224\
Data File : PO108211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 22:38
Operator : YP/AJ
Sample : P4953-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1297


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 00:19:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

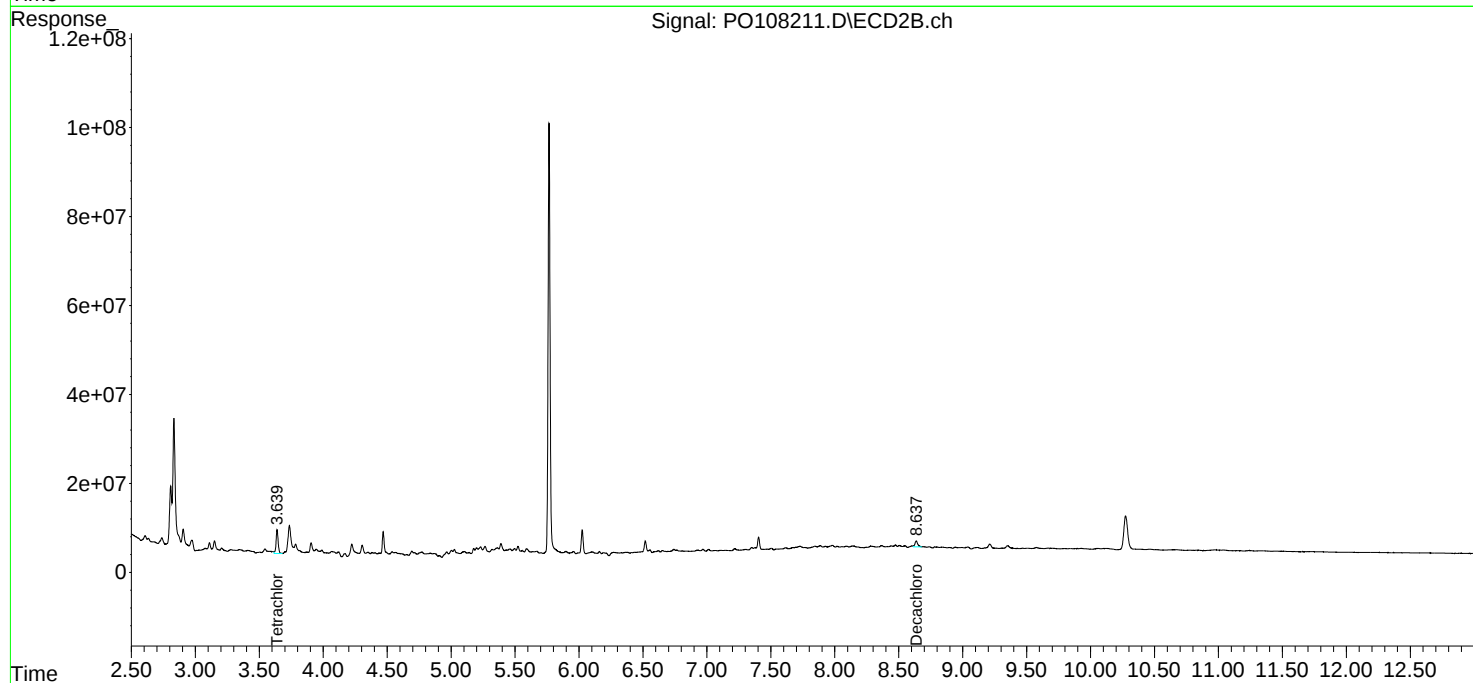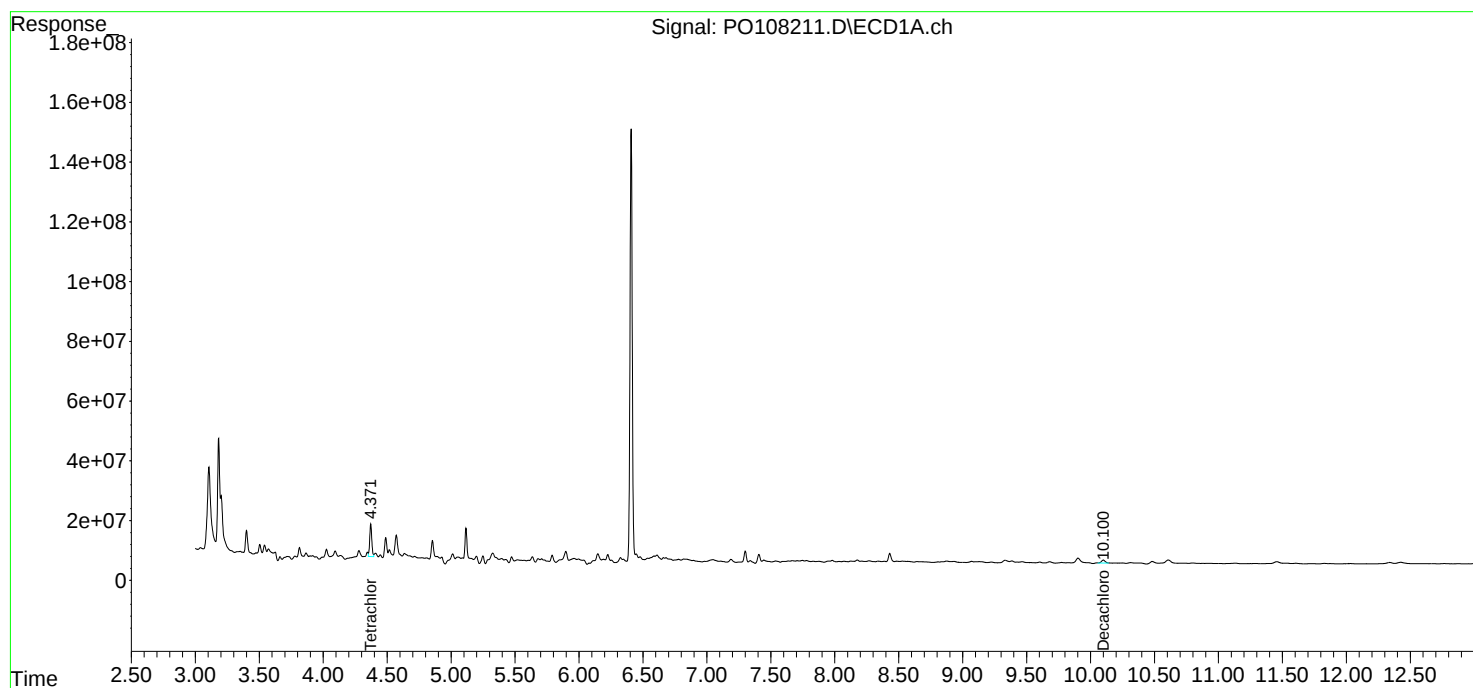

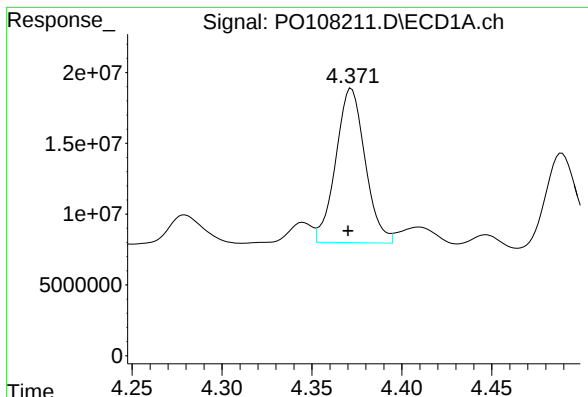


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: 0.002 min
Response: 123489976
Conc: 14.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
1297


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

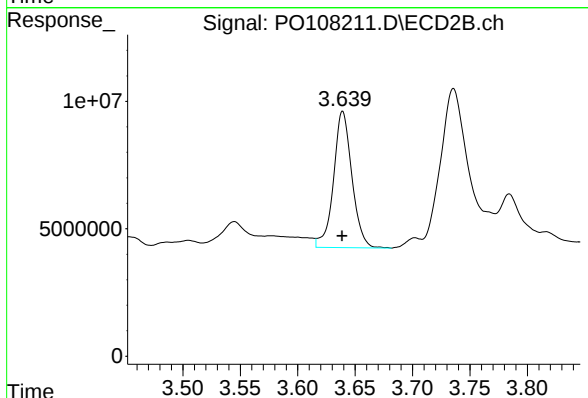


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 59524187
Conc: 17.56 ng/ml

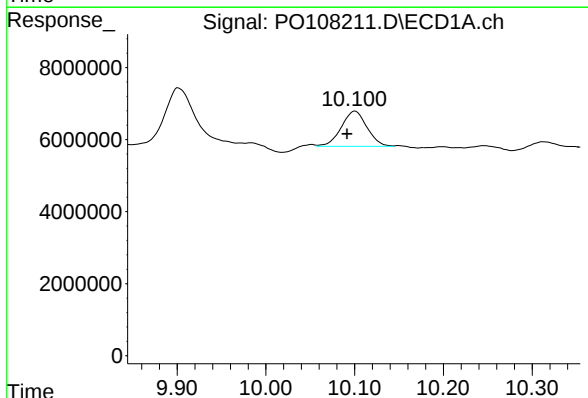

#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.008 min
Response: 19630096
Conc: 6.43 ng/ml m

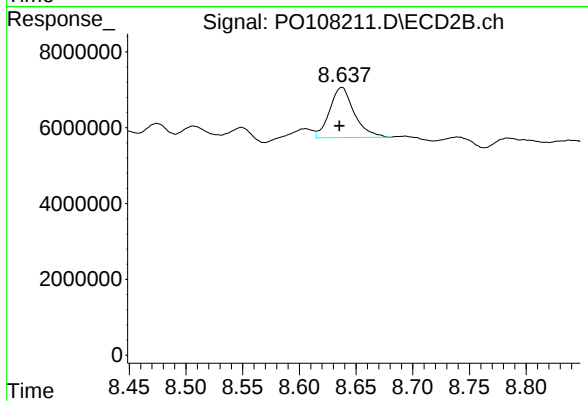

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: 0.002 min
Response: 19894956
Conc: 5.85 ng/ml