

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112320\
 Data File : P0073424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 9:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 14:37:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.943	4.011	1748025	1060341	20.897	21.627
2)	SA Decachlor...	10.972	9.283	1808969	1009620	21.940	22.020
Target Compounds							
9)	L2 AR-1221-2	5.298	0.000	24997	0	35.541	N.D. #
30)	L6 AR-1254-5	8.523	0.000	13818	0	2.903	N.D. #
32)	L7 AR-1260-2	8.241	0.000	19853	0	3.612	N.D. #
33)	L7 AR-1260-3	8.595	0.000	5523	0	1.245	N.D. #
35)	L7 AR-1260-5	9.153	0.000	45268	0	4.584	N.D. #
36)	L8 AR-1262-1	8.595	0.000	5523	0	0.885	N.D. #
37)	L8 AR-1262-2	9.153	0.000	45268	0	4.185	N.D. #
45)	L9 AR-1268-5	10.639	0.000	32124	0	1.009	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112320\
Data File : PO073424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 9:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 14:37:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

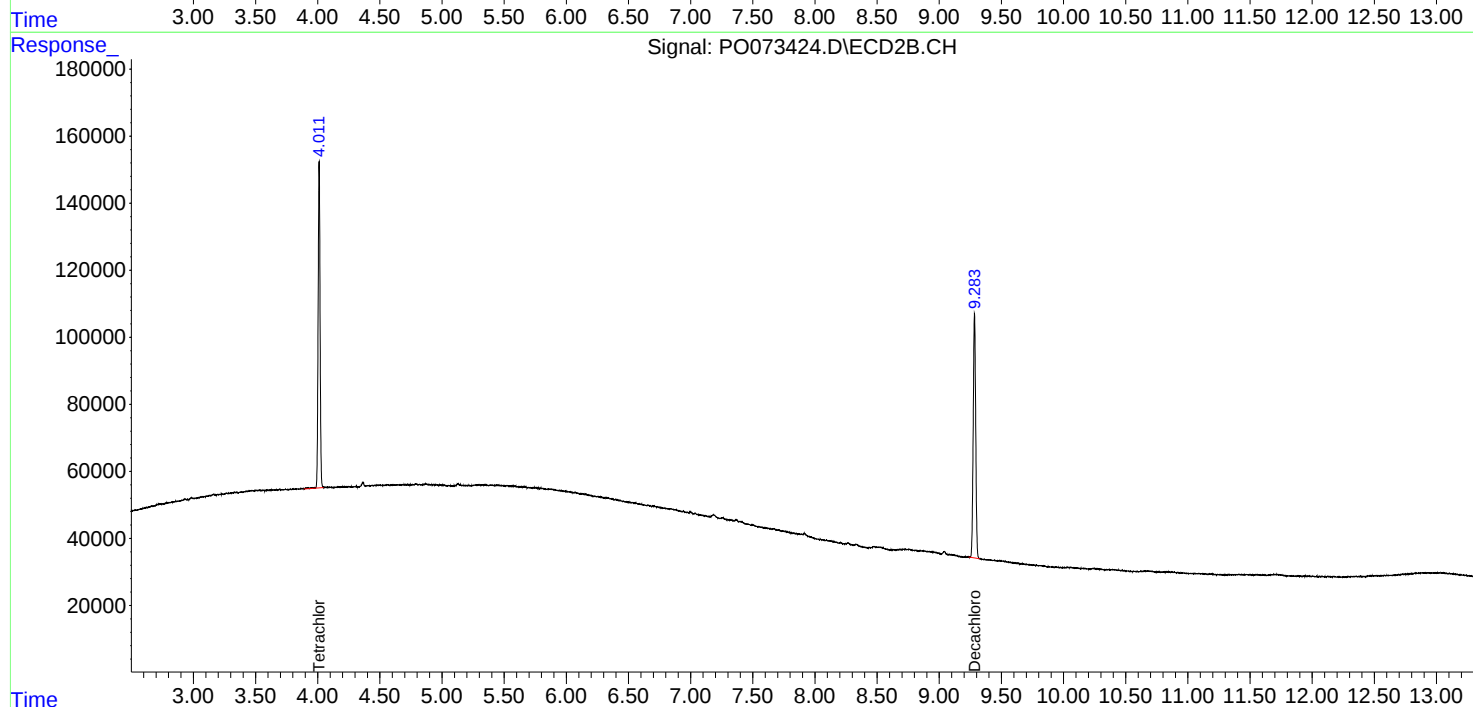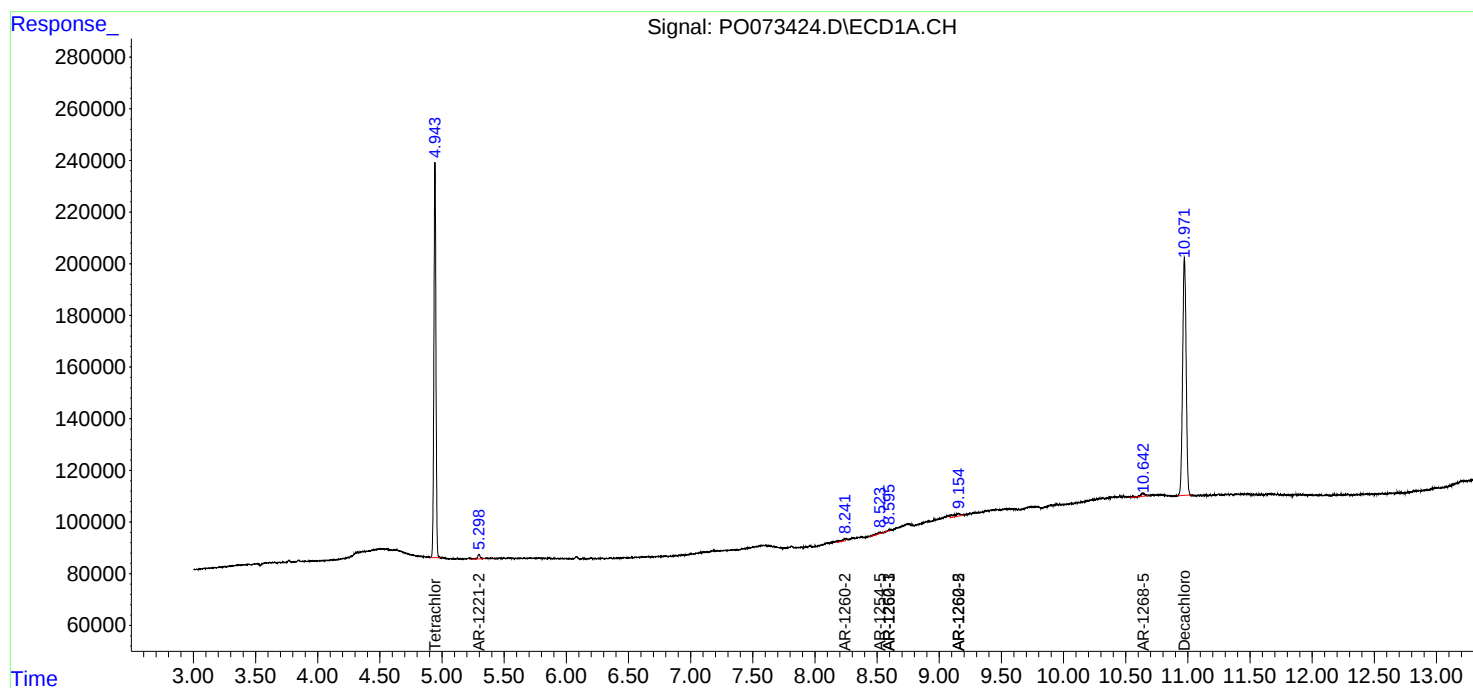


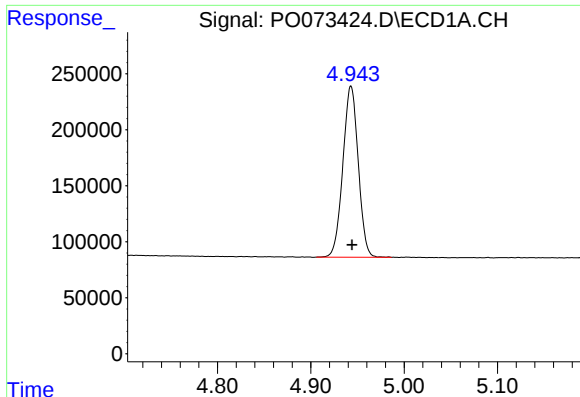

#1 Tetrachloro-m-xylene


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 1748025
Conc: 20.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

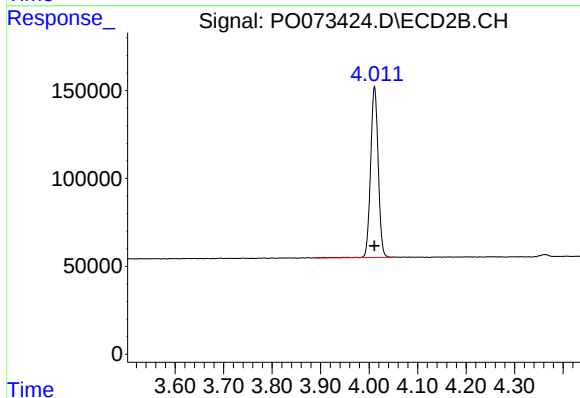


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 1060341
Conc: 21.63 ng/ml

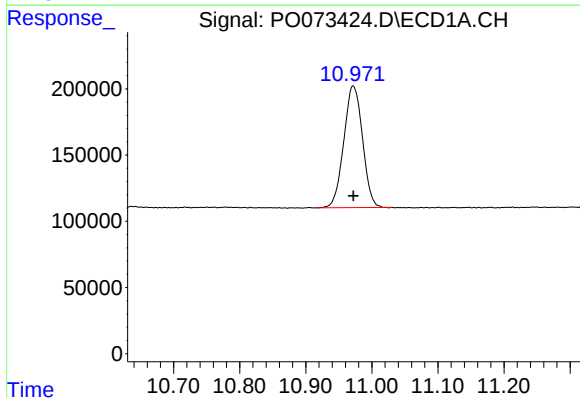


#2 Decachlorobiphenyl

R.T.: 10.972 min
Delta R.T.: 0.000 min
Response: 1808969
Conc: 21.94 ng/ml

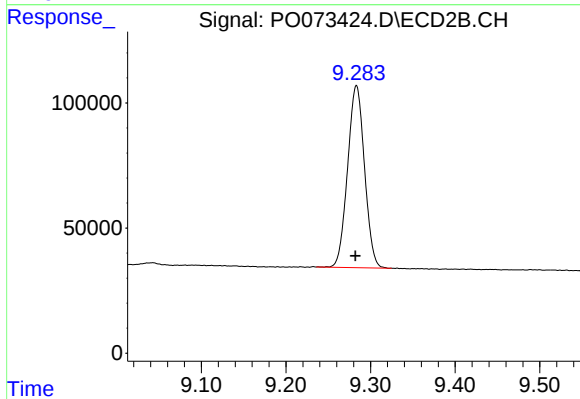

#2 Decachlorobiphenyl


R.T.: 9.283 min
Delta R.T.: 0.001 min
Response: 1009620
Conc: 22.02 ng/ml

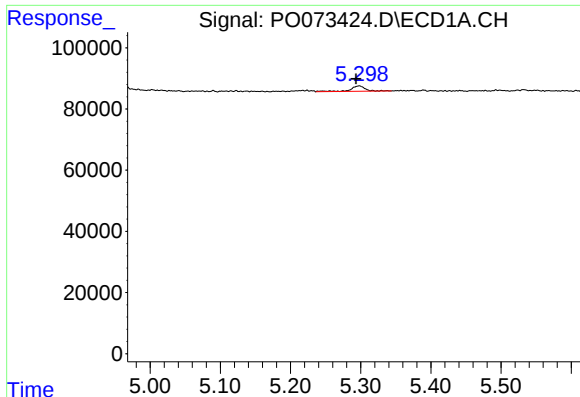

#9 AR-1221-2


R.T.: 5.298 min
Delta R.T.: 0.004 min
Response: 24997
Conc: 35.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

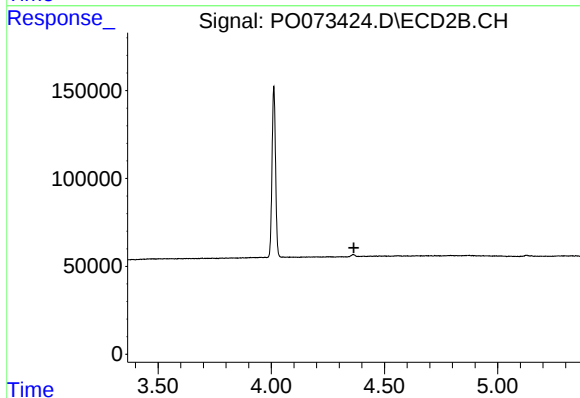


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.365 min
Response: 0
Conc: N.D.

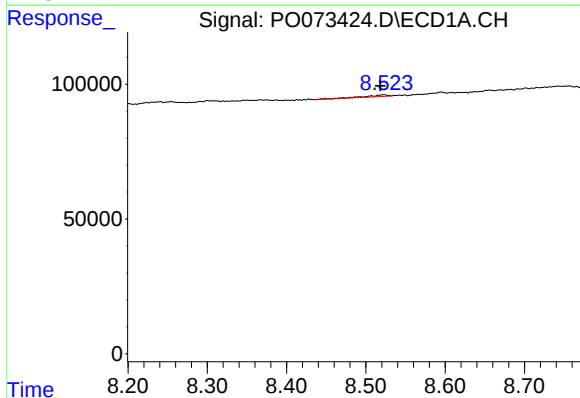


#30 AR-1254-5

R.T.: 8.523 min
Delta R.T.: 0.004 min
Response: 13818
Conc: 2.90 ng/ml

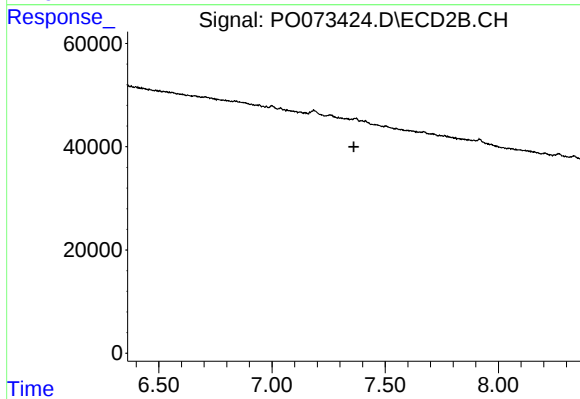

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

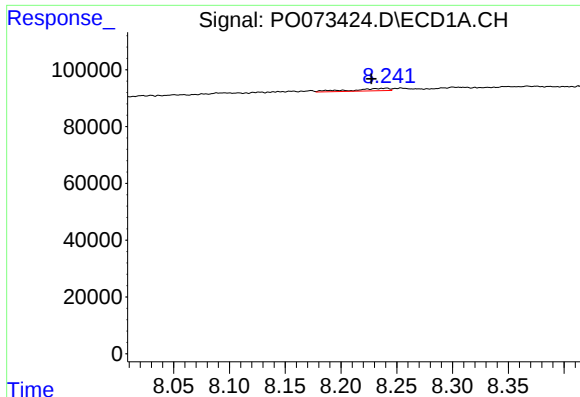

#32 AR-1260-2


R.T.: 8.241 min
Delta R.T.: 0.013 min
Response: 19853
Conc: 3.61 ng/ml

Instrument :
ECD_O
ClientSampleId :

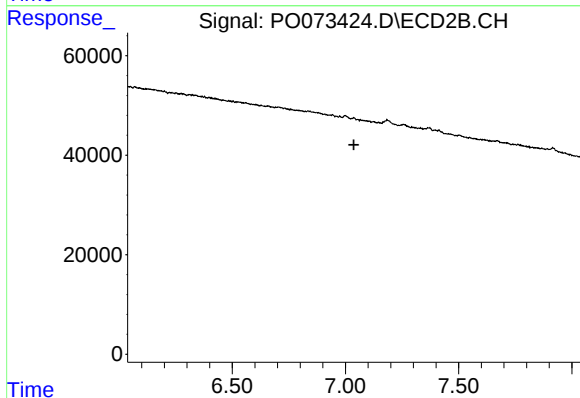


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

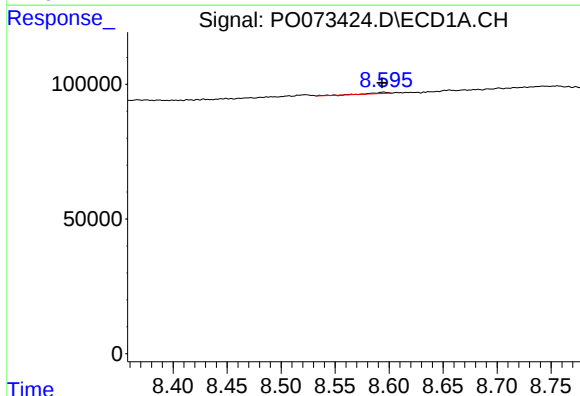


#33 AR-1260-3

R.T.: 8.595 min
Delta R.T.: 0.001 min
Response: 5523
Conc: 1.24 ng/ml

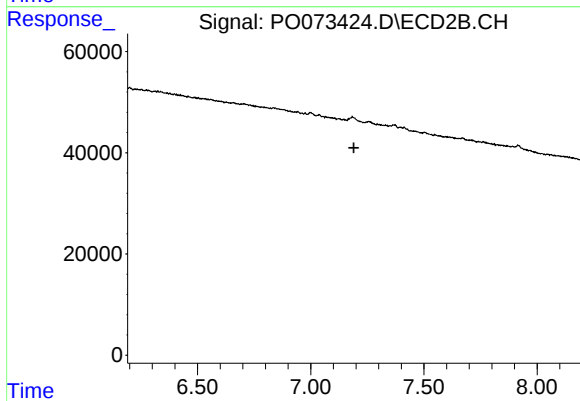

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.191 min
Response: 0
Conc: N.D.

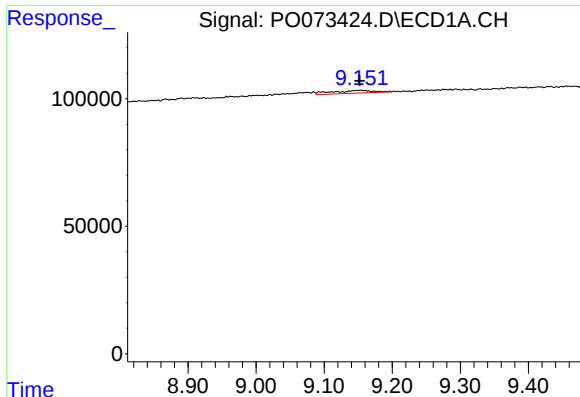

#35 AR-1260-5


R.T.: 9.153 min
Delta R.T.: 0.001 min
Response: 45268
Conc: 4.58 ng/ml

Instrument :
ECD_O
ClientSampleId :

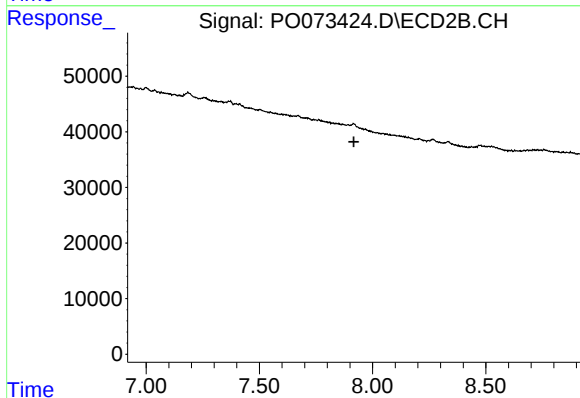


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.917 min
Response: 0
Conc: N.D.

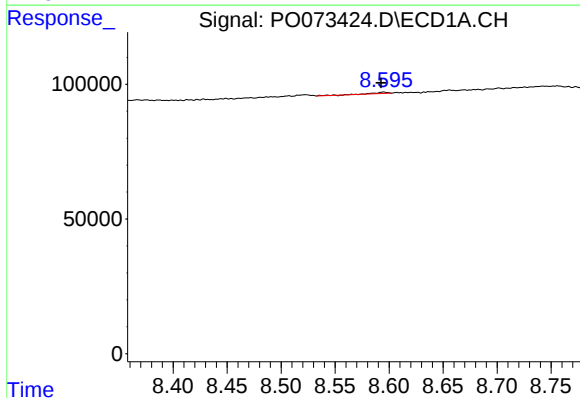


#36 AR-1262-1

R.T.: 8.595 min
Delta R.T.: 0.002 min
Response: 5523
Conc: 0.88 ng/ml

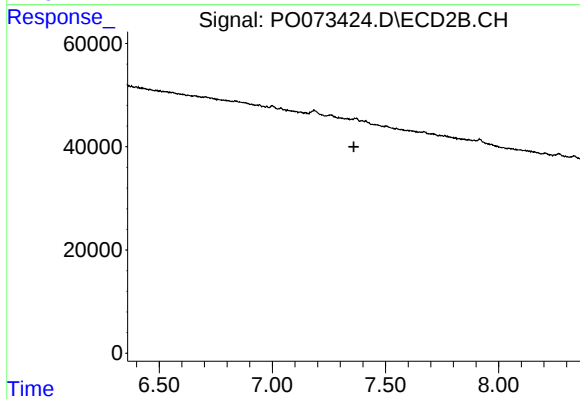

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.360 min
Response: 0
Conc: N.D.

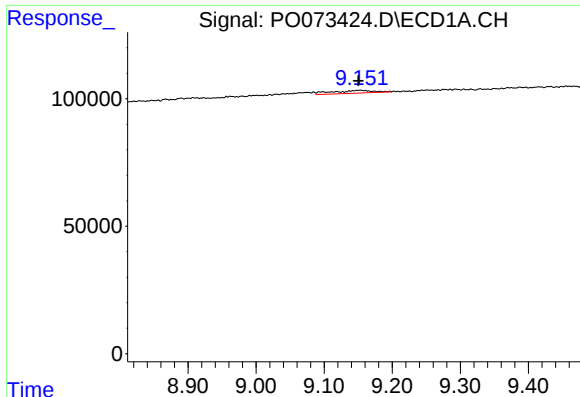

#37 AR-1262-2


R.T.: 9.153 min
Delta R.T.: 0.003 min
Response: 45268
Conc: 4.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

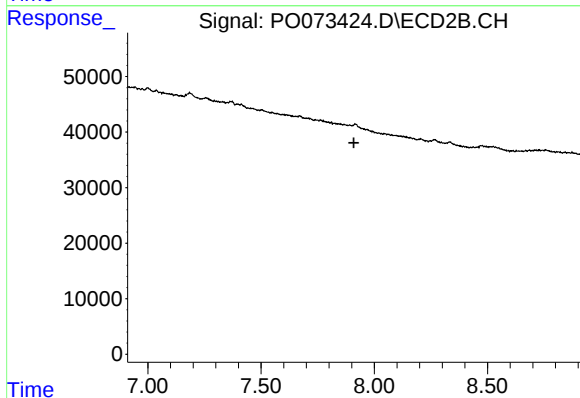


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.910 min
Response: 0
Conc: N.D.

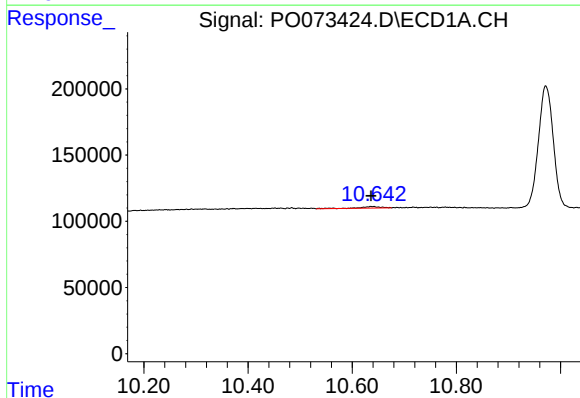

#45 AR-1268-5

R.T.: 10.639 min
Delta R.T.: 0.002 min
Response: 32124
Conc: 1.01 ng/ml

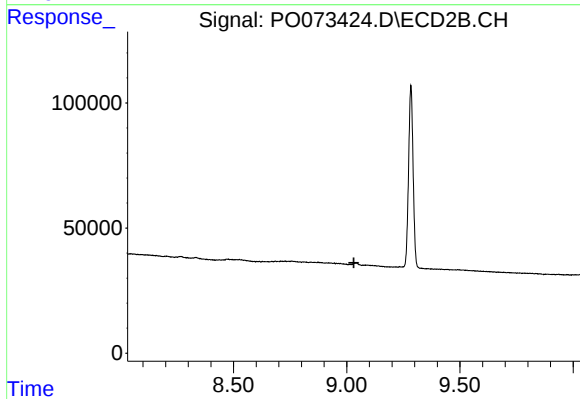

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.