

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112320\
 Data File : P0073459.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Nov 2020 20:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 12:08:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.942	4.003	1735179	1070763	20.743	21.840
2)	SA Decachlor...	10.969	9.274	1815426	1056571	22.018	23.044
Target Compounds							
9)	L2 AR-1221-2	5.295	0.000	23724	0	33.731	N.D. #
29)	L6 AR-1254-4	8.118f	0.000	86742	0	17.929	N.D. #
32)	L7 AR-1260-2	0.000	7.036	0	47050	N.D.	14.106 #
33)	L7 AR-1260-3	8.593	0.000	7014	0	1.581	N.D. #
34)	L7 AR-1260-4	8.824	0.000	13247	0	3.069	N.D. #
35)	L7 AR-1260-5	9.150	0.000	17523	0	1.774	N.D. #
36)	L8 AR-1262-1	8.593	0.000	7014	0	1.123	N.D. #
37)	L8 AR-1262-2	9.150	0.000	17523	0	1.620	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112320\
Data File : PO073459.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Nov 2020 20:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 12:08:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

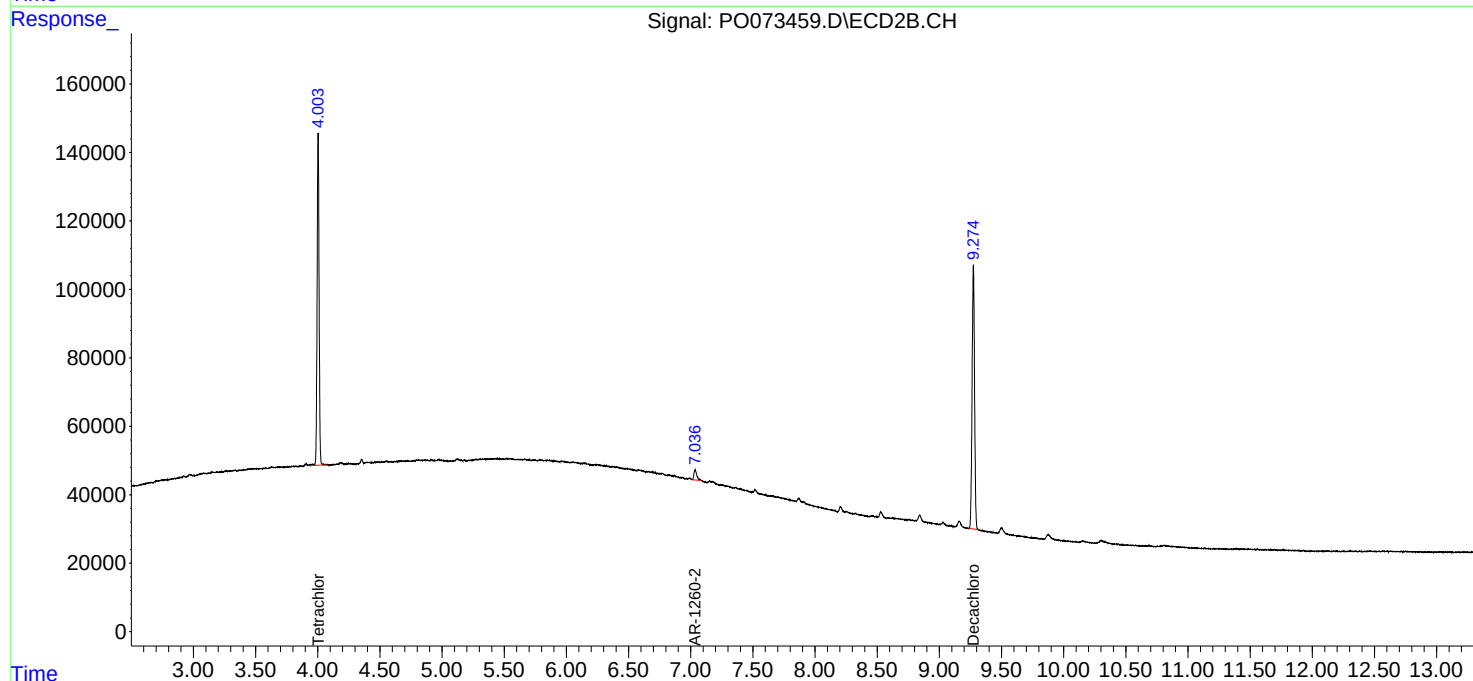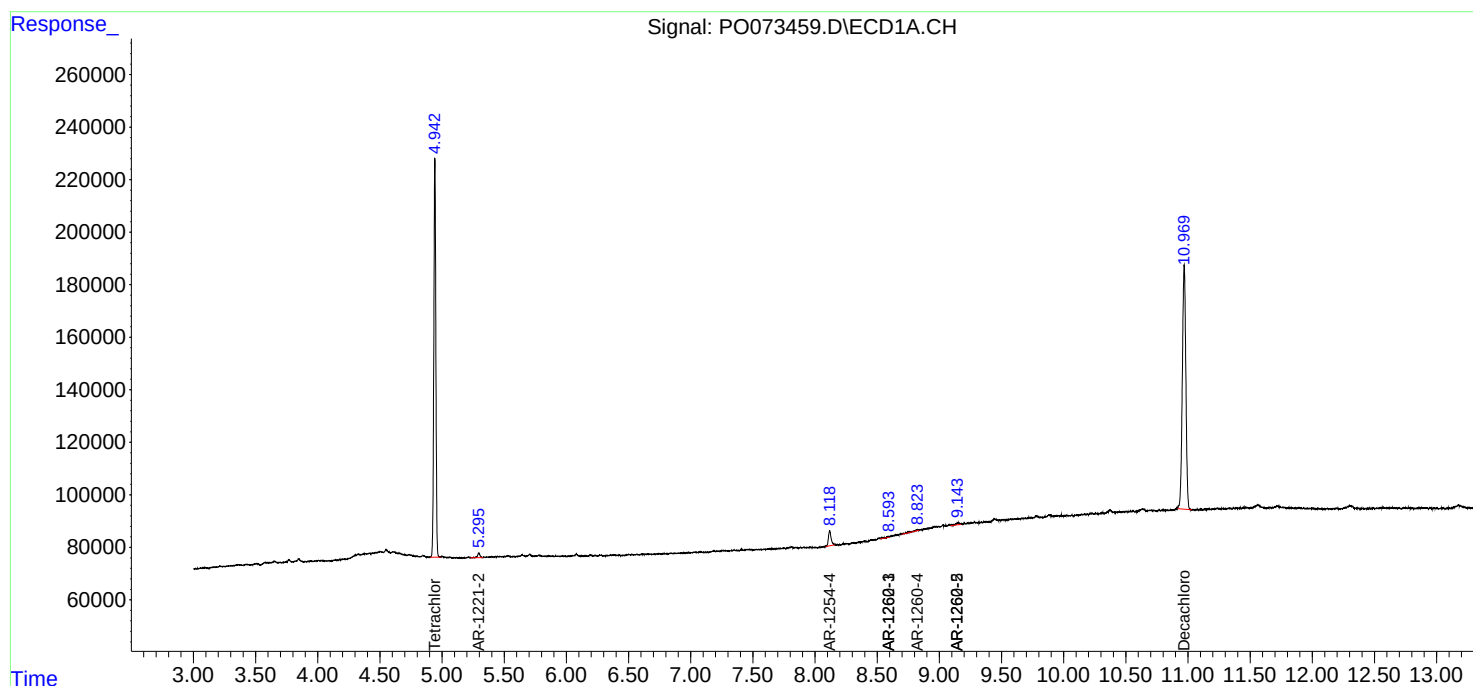


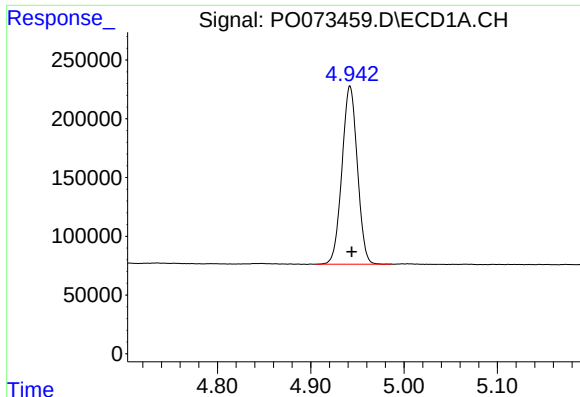

#1 Tetrachloro-m-xylene


R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 1735179
Conc: 20.74 ng/ml

Instrument :
ECD_O
ClientSampleId :

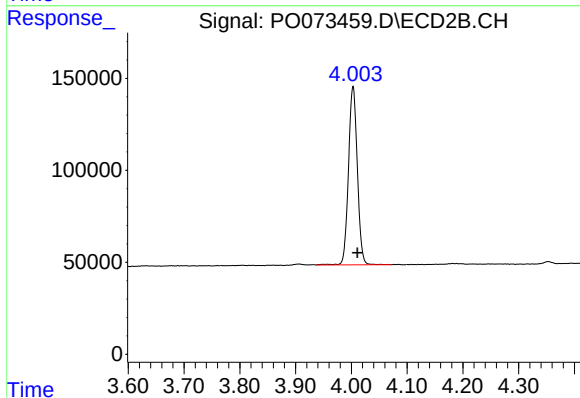


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.008 min
Response: 1070763
Conc: 21.84 ng/ml

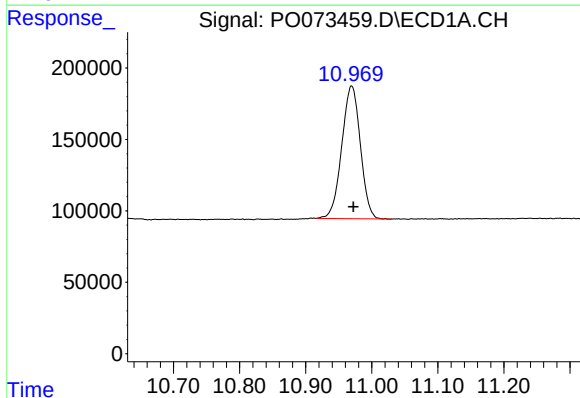


#2 Decachlorobiphenyl

R.T.: 10.969 min
Delta R.T.: -0.002 min
Response: 1815426
Conc: 22.02 ng/ml

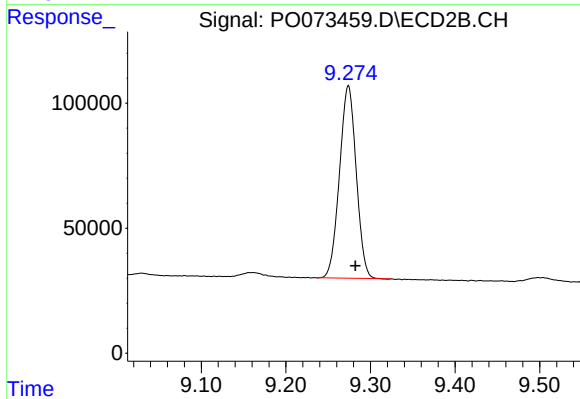

#2 Decachlorobiphenyl


R.T.: 9.274 min
Delta R.T.: -0.008 min
Response: 1056571
Conc: 23.04 ng/ml

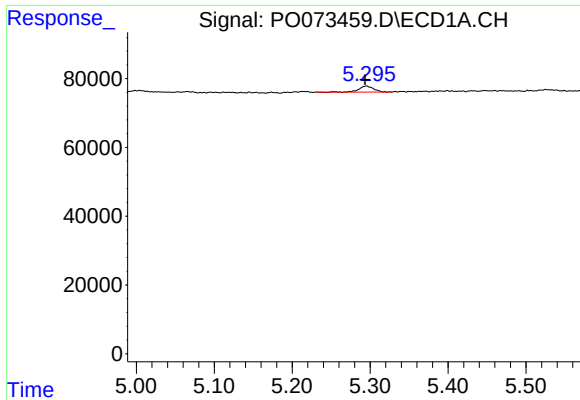

#9 AR-1221-2


R.T.: 5.295 min
Delta R.T.: 0.002 min
Response: 23724
Conc: 33.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

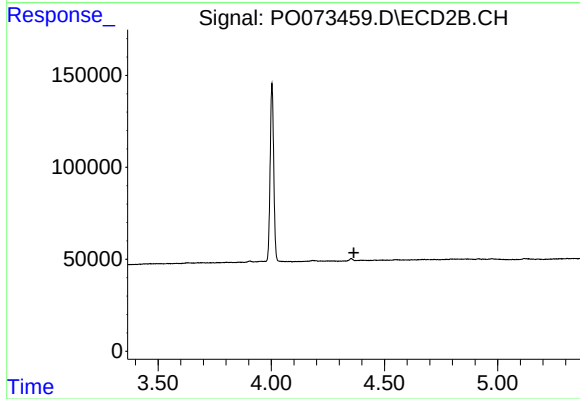


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.365 min
Response: 0
Conc: N.D.

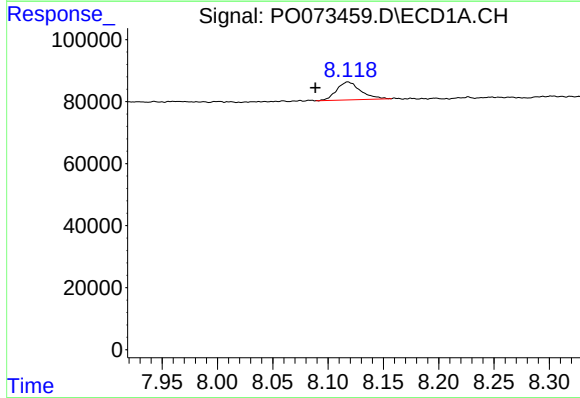


#29 AR-1254-4

R.T.: 8.118 min
Delta R.T.: 0.029 min
Response: 86742
Conc: 17.93 ng/ml

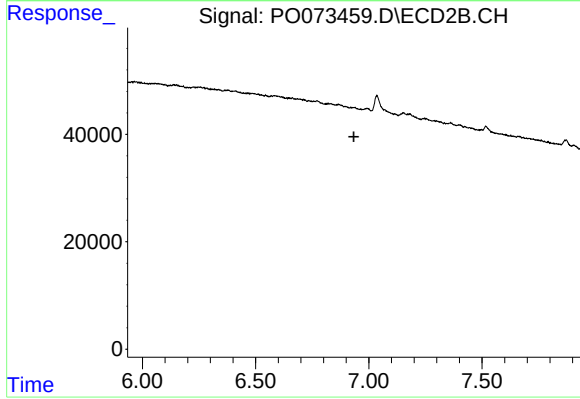

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.934 min
Response: 0
Conc: N.D.

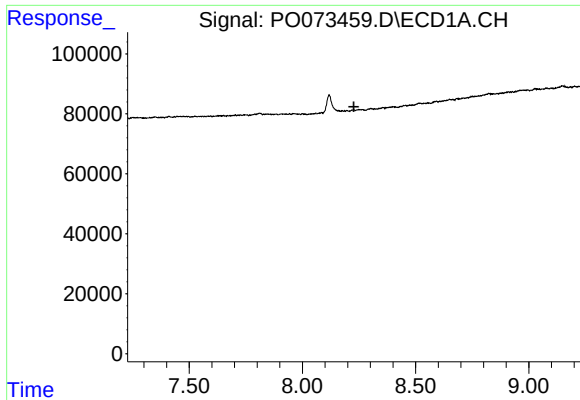

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

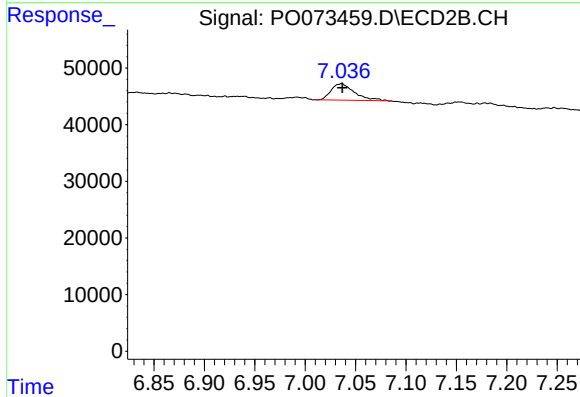


#32 AR-1260-2

R.T.: 7.036 min
Delta R.T.: -0.001 min
Response: 47050
Conc: 14.11 ng/ml

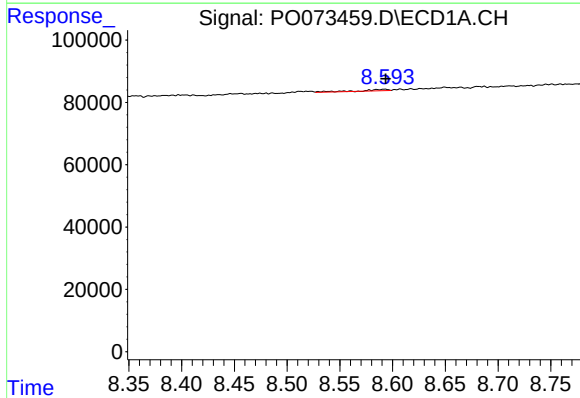


#33 AR-1260-3

R.T.: 8.593 min
Delta R.T.: 0.000 min
Response: 7014
Conc: 1.58 ng/ml

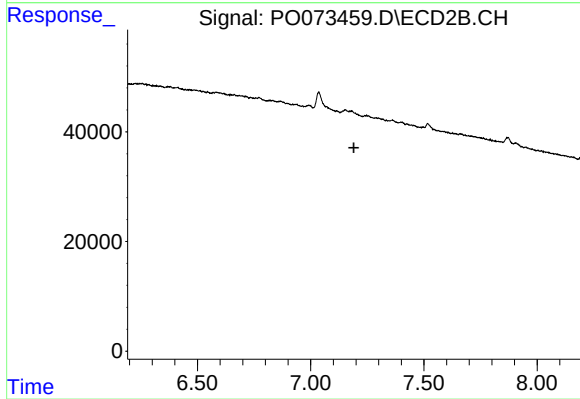

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.191 min
Response: 0
Conc: N.D.

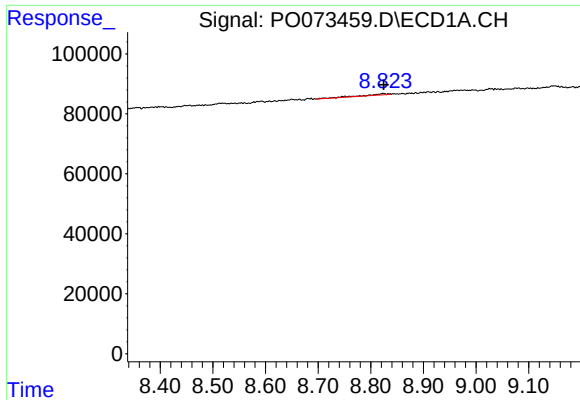

#34 AR-1260-4


R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 13247
Conc: 3.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

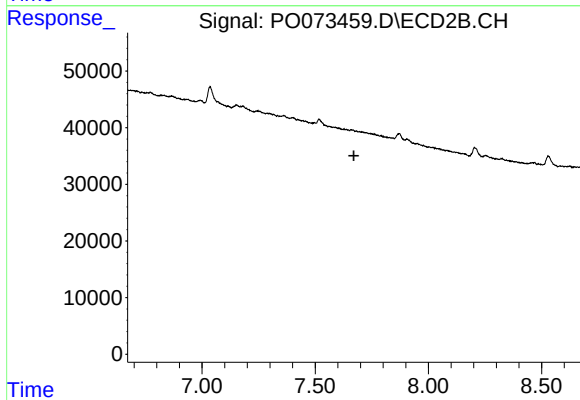


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.671 min
Response: 0
Conc: N.D.

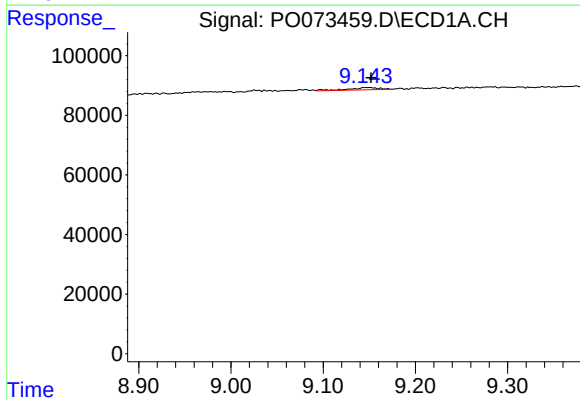


#35 AR-1260-5

R.T.: 9.150 min
Delta R.T.: -0.002 min
Response: 17523
Conc: 1.77 ng/ml

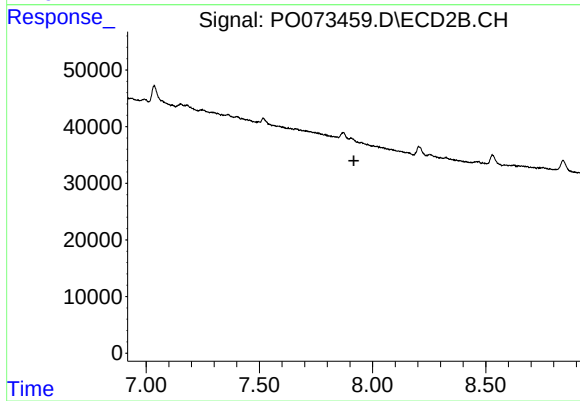

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.917 min
Response: 0
Conc: N.D.

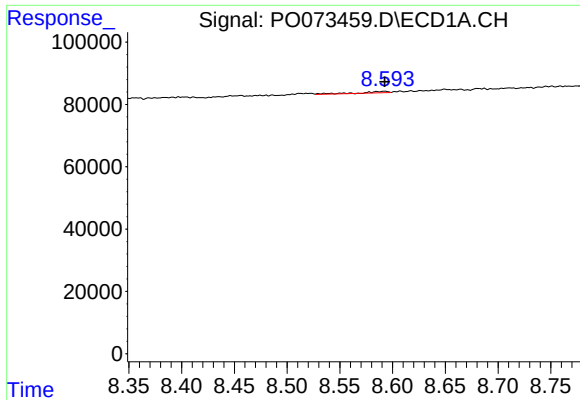

#36 AR-1262-1


R.T.: 8.593 min
Delta R.T.: 0.000 min
Response: 7014
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

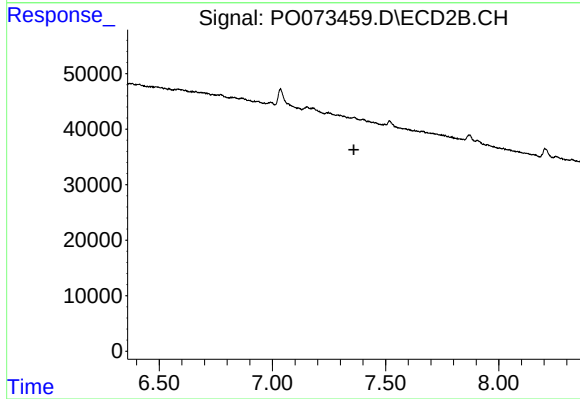


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.360 min
Response: 0
Conc: N.D.

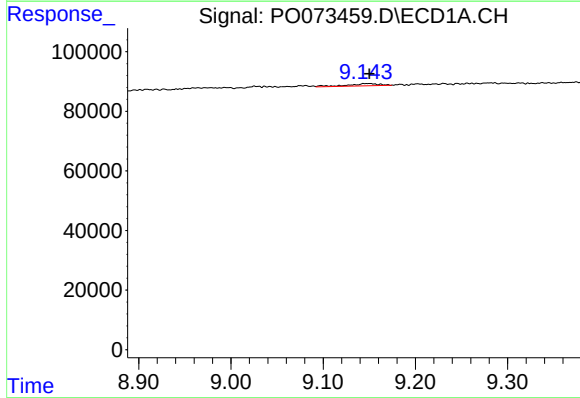

#37 AR-1262-2

R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 17523
Conc: 1.62 ng/ml

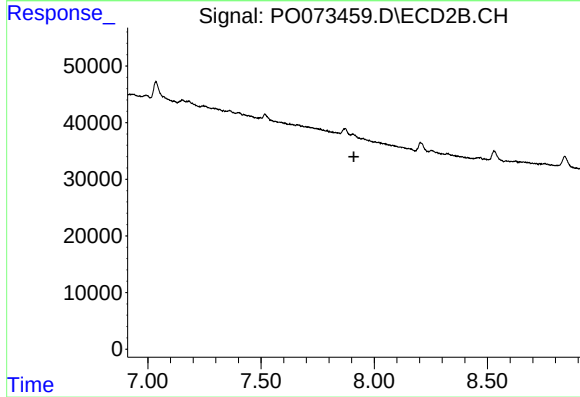

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.910 min
Response: 0
Conc: N.D.