

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112320\
 Data File : P0073484.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 6:05
 Operator : DD\AJ
 Sample : L4844-01
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-112020

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:33:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 12:20:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.943	4.007	1525929	1156656	18.242m	23.592m#
2) SA Decachlor...	10.968	9.274	1506825	807424	18.275	17.610

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112320\
Data File : PO073484.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 6:05
Operator : DD\AJ
Sample : L4844-01
Misc :
ALS Vial : 66 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-112020


Manual Integrations
APPROVED

Ankita
11/25/2020 5:33:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 12:20:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

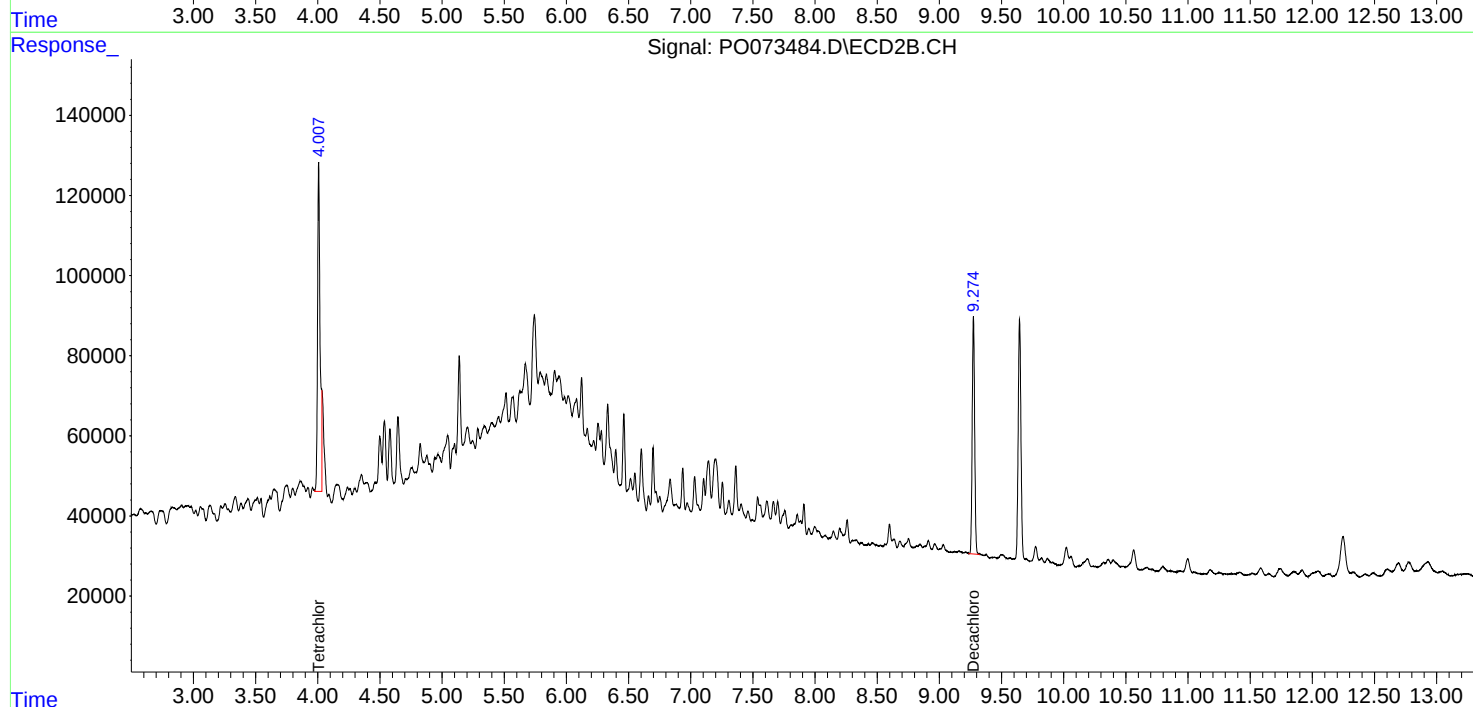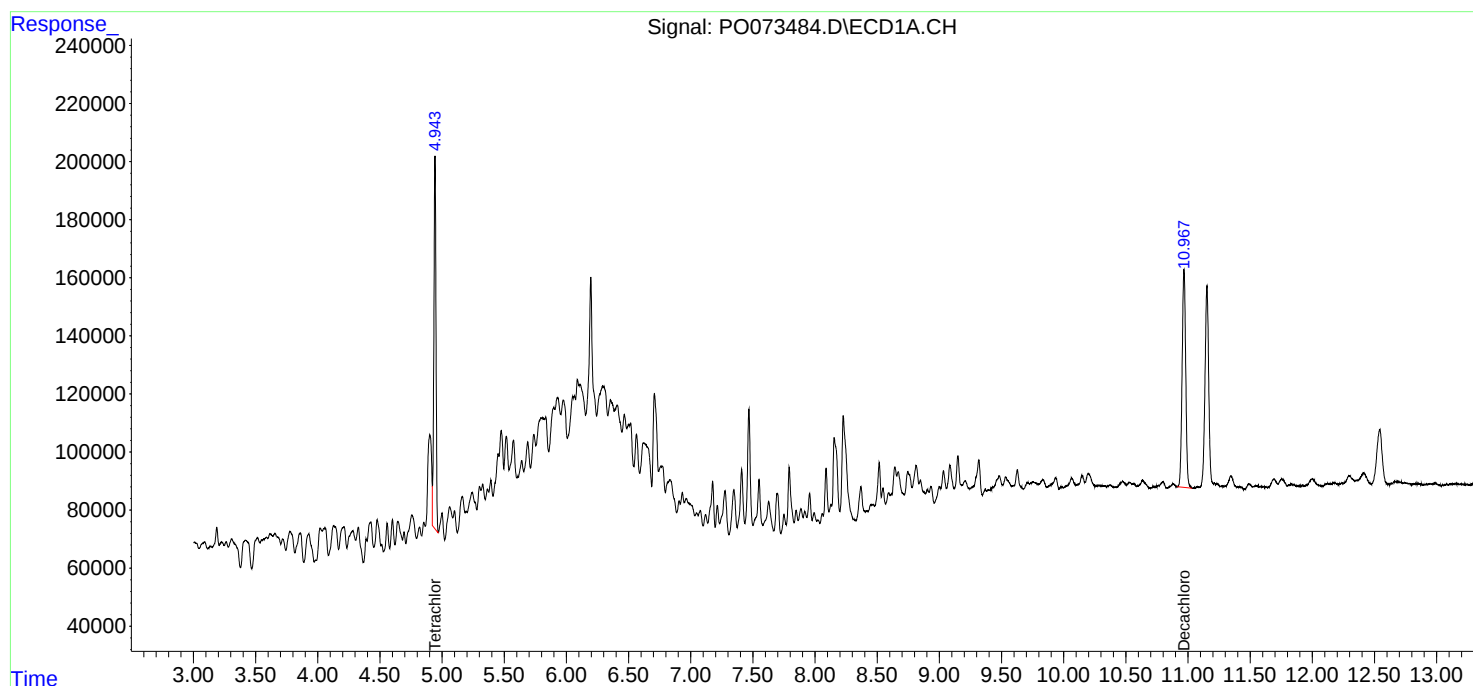

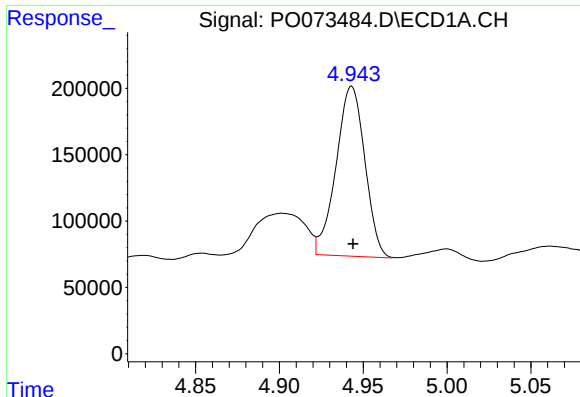


#1 Tetrachloro-m-xylene

R.T.: 4.943 min
Delta R.T.: -0.001 min
Response: 1525929
Conc: 18.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-02-112020


Manual Integrations
APPROVED

Ankita
11/25/2020 5:33:28 PM

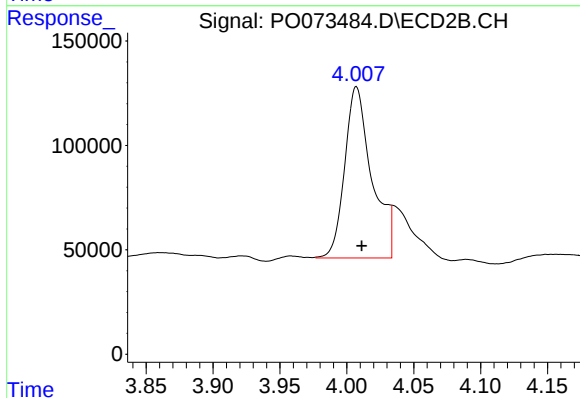


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.004 min
Response: 1156656
Conc: 23.59 ng/ml m

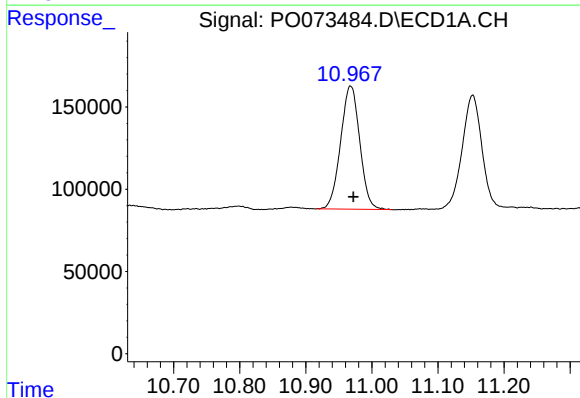

#2 Decachlorobiphenyl

R.T.: 10.968 min
Delta R.T.: -0.004 min
Response: 1506825
Conc: 18.28 ng/ml

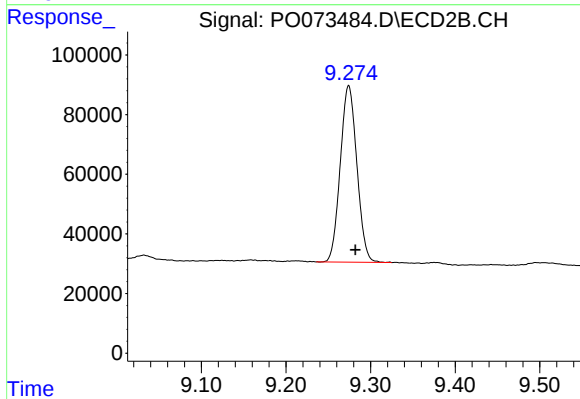

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.008 min
Response: 807424
Conc: 17.61 ng/ml