

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
 Data File : PO073497.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 9:48
 Operator : DD\AJ
 Sample : L4842-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40642

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:39:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 10:26:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.944	4.010	1372958	1019025	16.413	20.785 #
2) SA Decachlor...	10.968	9.277	1420012	731021	17.223	15.944m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
Data File : PO073497.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 9:48
Operator : DD\AJ
Sample : L4842-04
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40642


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 10:26:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

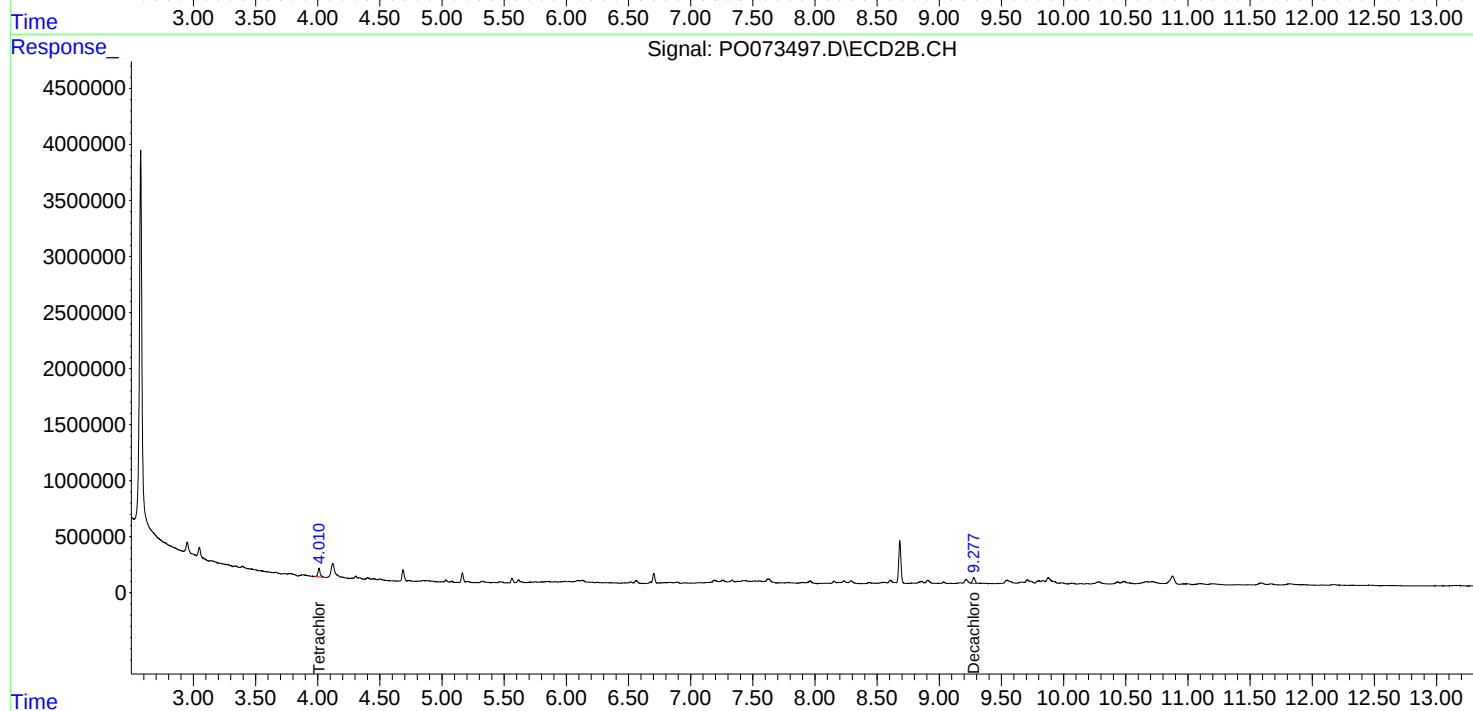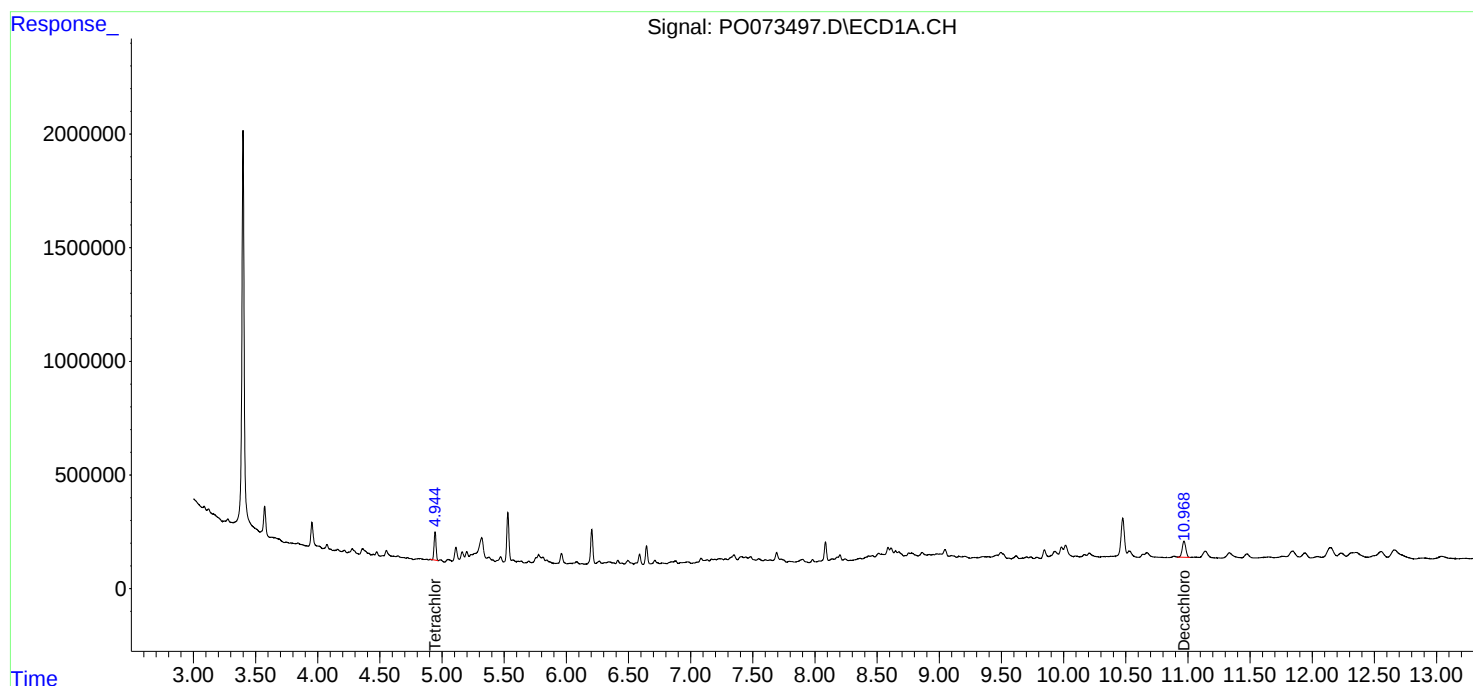

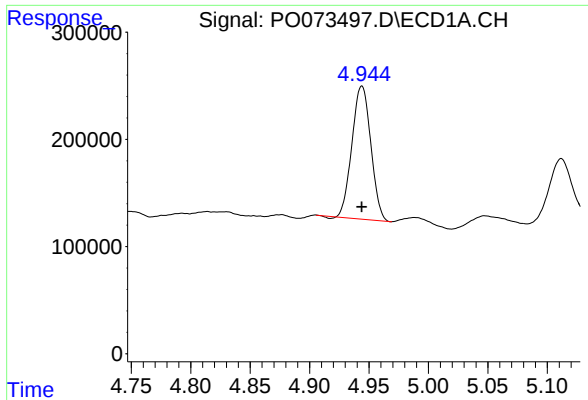


#1 Tetrachloro-m-xylene

R.T.: 4.944 min
 Delta R.T.: 0.000 min
 Response: 1372958
 Conc: 16.41 ng/ml

Instrument :
 ECD_O
 ClientSampleId :
 40642


Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:39:06 PM

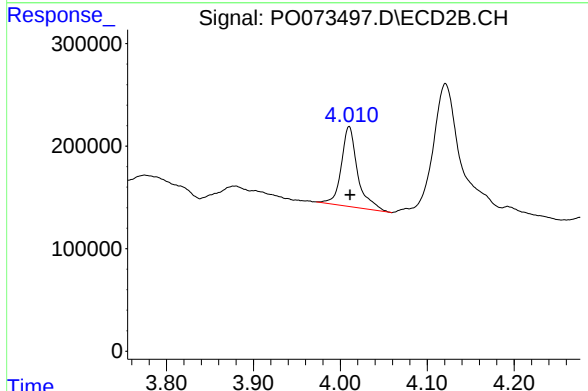


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
 Delta R.T.: 0.000 min
 Response: 1019025
 Conc: 20.78 ng/ml

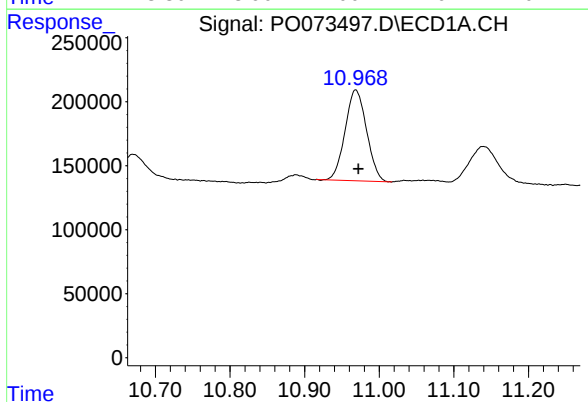

#2 Decachlorobiphenyl

R.T.: 10.968 min
 Delta R.T.: -0.004 min
 Response: 1420012
 Conc: 17.22 ng/ml

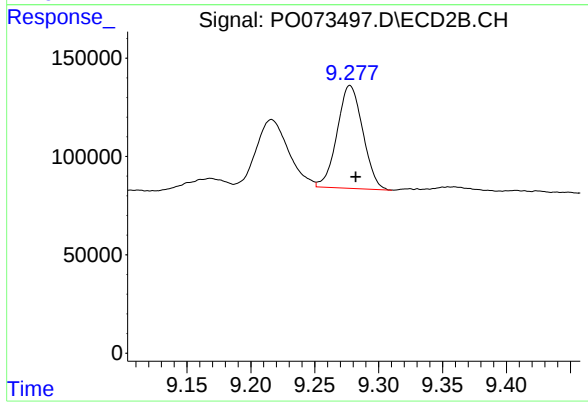

#2 Decachlorobiphenyl

R.T.: 9.277 min
 Delta R.T.: -0.005 min
 Response: 731021
 Conc: 15.94 ng/ml m