

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
 Data File : PO073501.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 10:56
 Operator : DD\AJ
 Sample : L4836-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-01

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:39:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 10:27:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.942	4.007	1726641	1191523	20.641m	24.303
2)	SA Decachlor...	10.964	9.273	1747678	915307	21.197	19.963
Target Compounds							
31)	L7 AR-1260-1	7.957	6.833	715338	442749	177.273m	164.788
32)	L7 AR-1260-2	8.221	7.037	829740	538957	150.975	161.583
33)	L7 AR-1260-3	8.590	7.184	597526	395925	134.653	128.166
34)	L7 AR-1260-4	8.820	7.664	633221	293198	146.709	119.148
35)	L7 AR-1260-5	9.148	7.910	1289019	755914	130.535	122.019

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
Data File : PO073501.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 10:56
Operator : DD\AJ
Sample : L4836-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-01


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 10:27:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

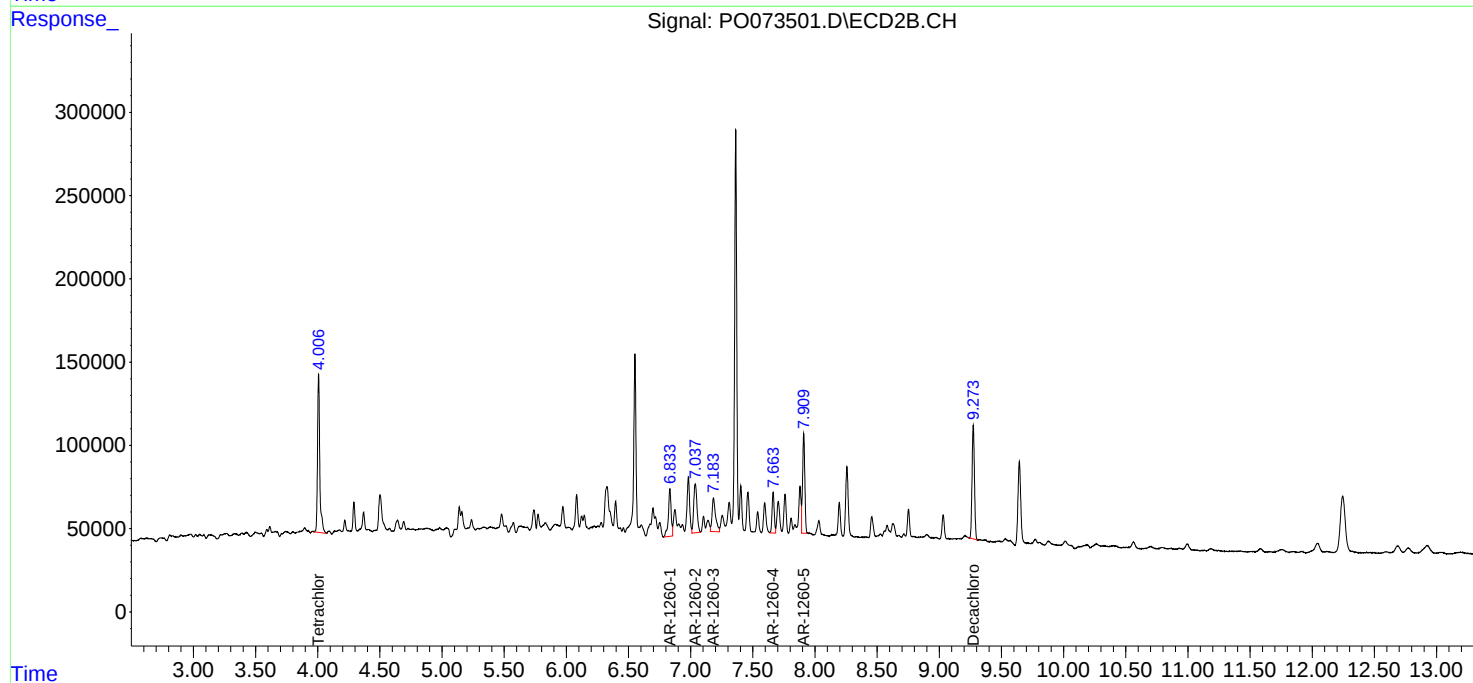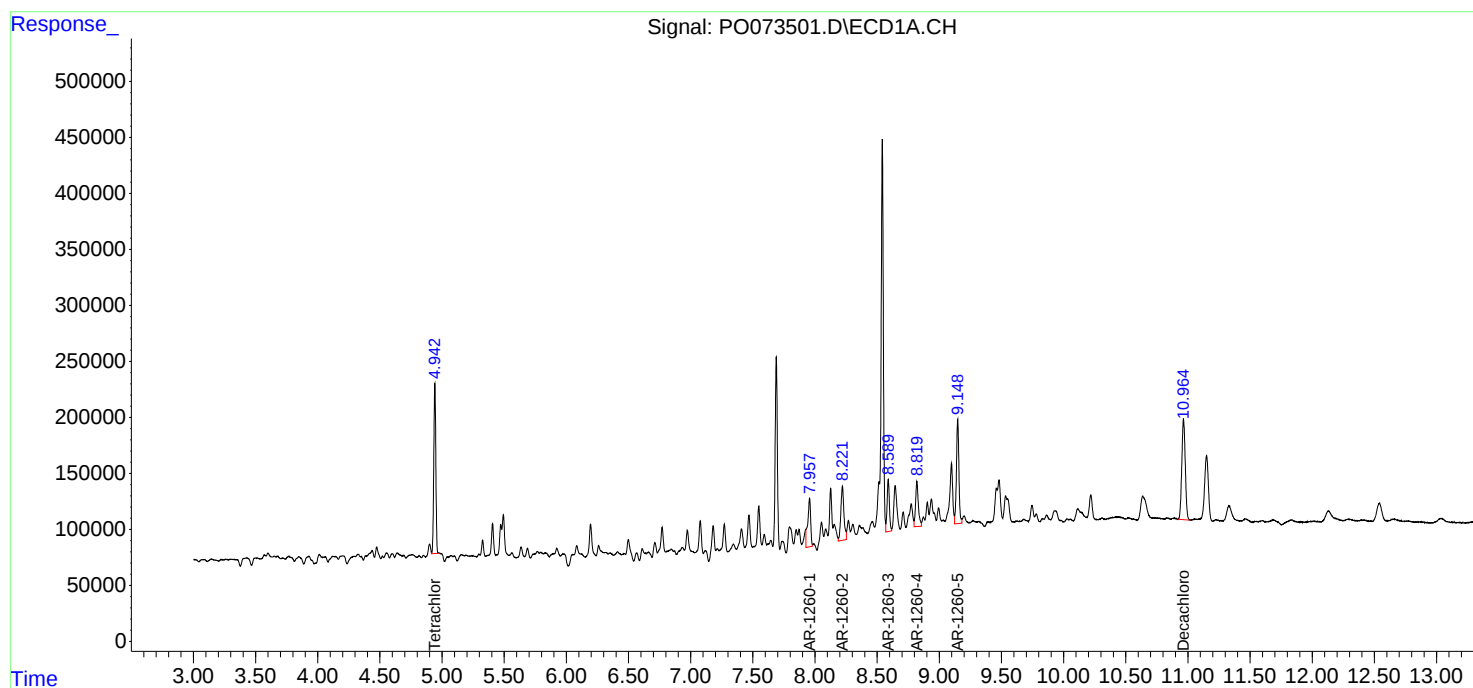

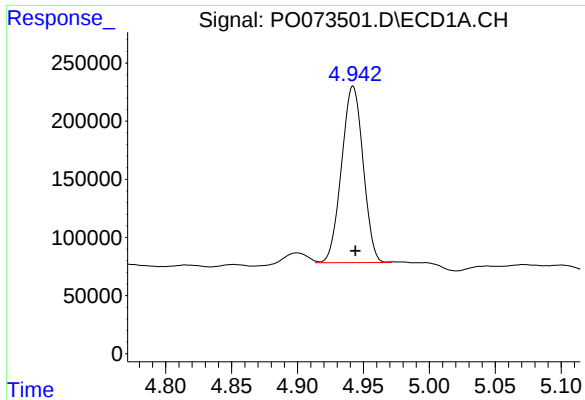


#1 Tetrachloro-m-xylene

R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 1726641
Conc: 20.64 ng/ml m

Instrument :
ECD_O
ClientSampled :
SB-01


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:11 PM

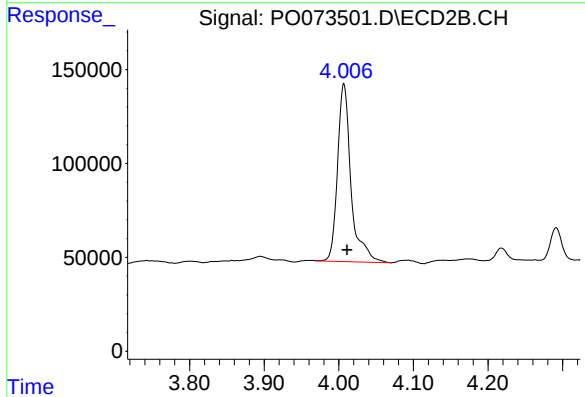


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.004 min
Response: 1191523
Conc: 24.30 ng/ml

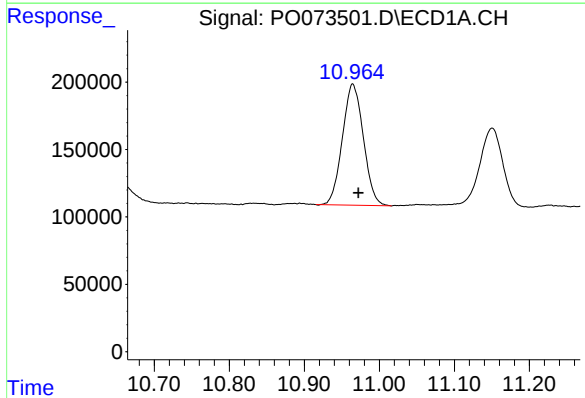


#2 Decachlorobiphenyl

R.T.: 10.964 min
Delta R.T.: -0.007 min
Response: 1747678
Conc: 21.20 ng/ml

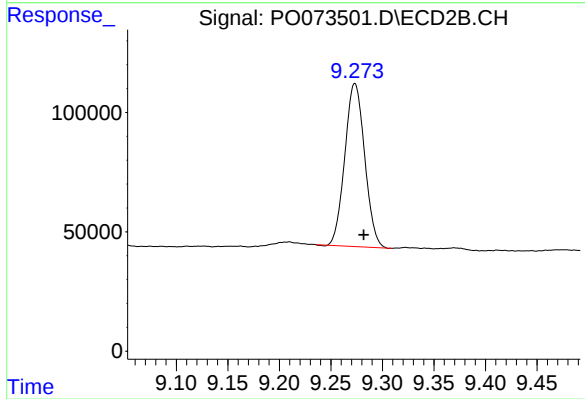

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.009 min
Response: 915307
Conc: 19.96 ng/ml

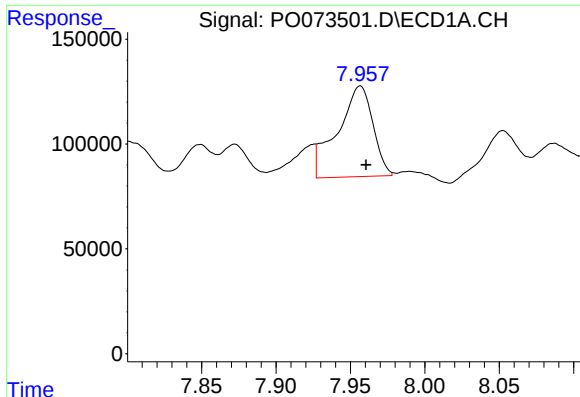


#31 AR-1260-1

R.T.: 7.957 min
Delta R.T.: -0.004 min
Response: 715338
Conc: 177.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-01


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:11 PM

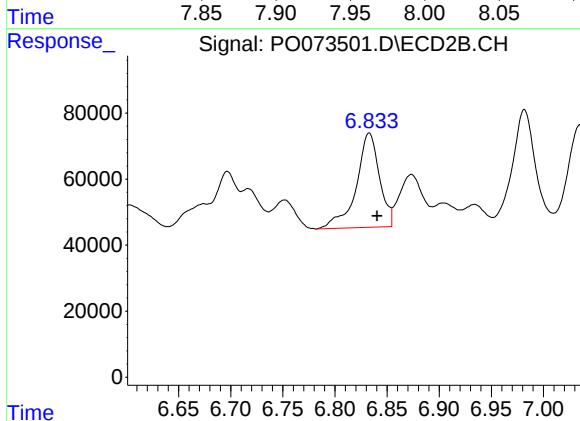


#31 AR-1260-1

R.T.: 6.833 min
Delta R.T.: -0.007 min
Response: 442749
Conc: 164.79 ng/ml

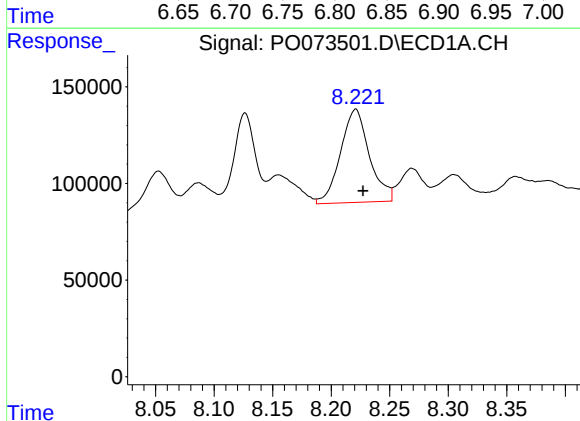


#32 AR-1260-2

R.T.: 8.221 min
Delta R.T.: -0.006 min
Response: 829740
Conc: 150.98 ng/ml

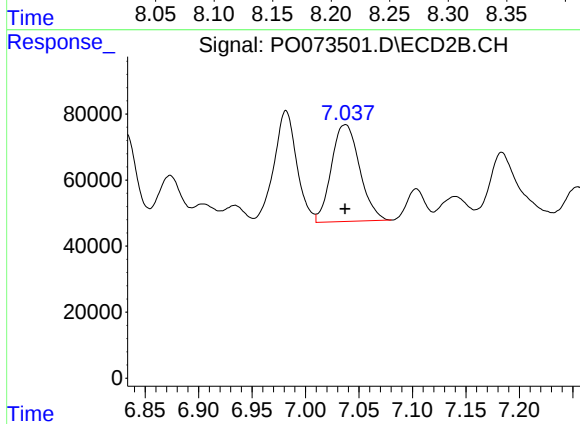

#32 AR-1260-2

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 538957
Conc: 161.58 ng/ml

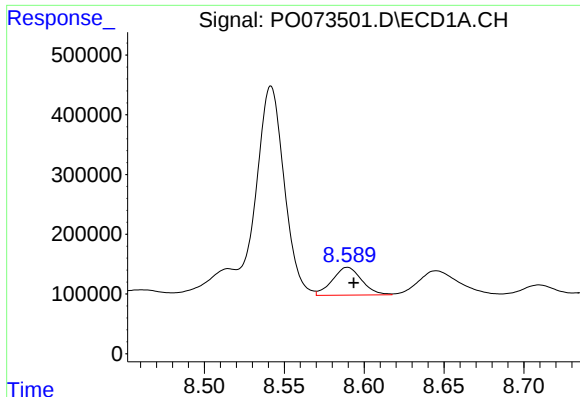


#33 AR-1260-3

R.T.: 8.590 min
Delta R.T.: -0.004 min
Response: 597526
Conc: 134.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:11 PM

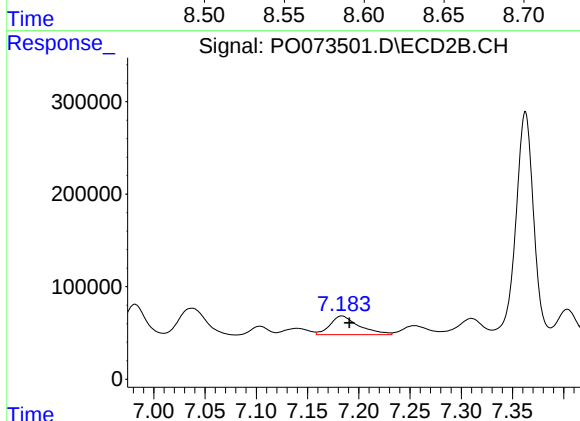


#33 AR-1260-3

R.T.: 7.184 min
Delta R.T.: -0.007 min
Response: 395925
Conc: 128.17 ng/ml

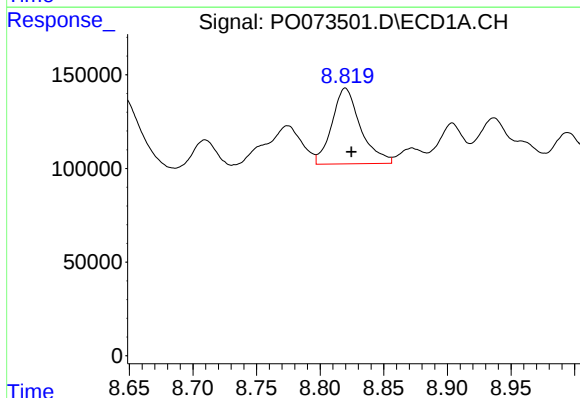


#34 AR-1260-4

R.T.: 8.820 min
Delta R.T.: -0.005 min
Response: 633221
Conc: 146.71 ng/ml

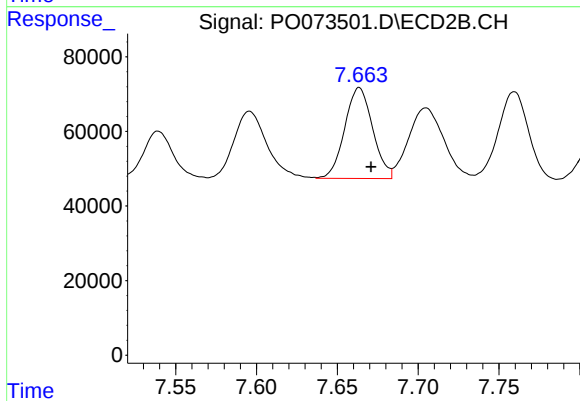

#34 AR-1260-4

R.T.: 7.664 min
Delta R.T.: -0.007 min
Response: 293198
Conc: 119.15 ng/ml

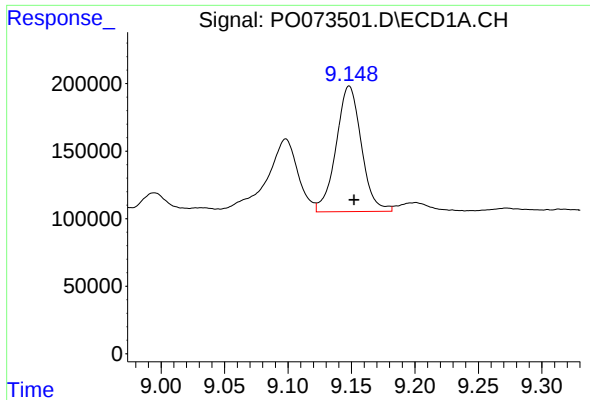


#35 AR-1260-5

R.T.: 9.148 min
Delta R.T.: -0.004 min
Response: 1289019
Conc: 130.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01

Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:11 PM

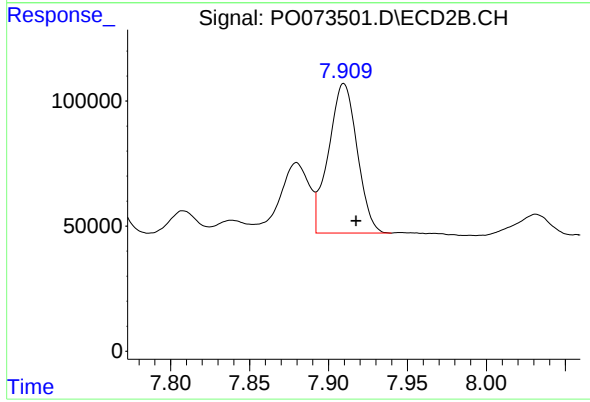

#35 AR-1260-5

R.T.: 7.910 min
Delta R.T.: -0.008 min
Response: 755914
Conc: 122.02 ng/ml