

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
 Data File : PO073516.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 15:30
 Operator : DD\AJ
 Sample : L4592-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-112020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 10:33:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.942	4.007	1322439	930945	15.809	18.988
2)	SA Decachlor...	10.966	9.273	1234198	708957	14.969	15.462

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
Data File : PO073516.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 15:30
Operator : DD\AJ
Sample : L4592-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EO-01-112020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 10:33:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

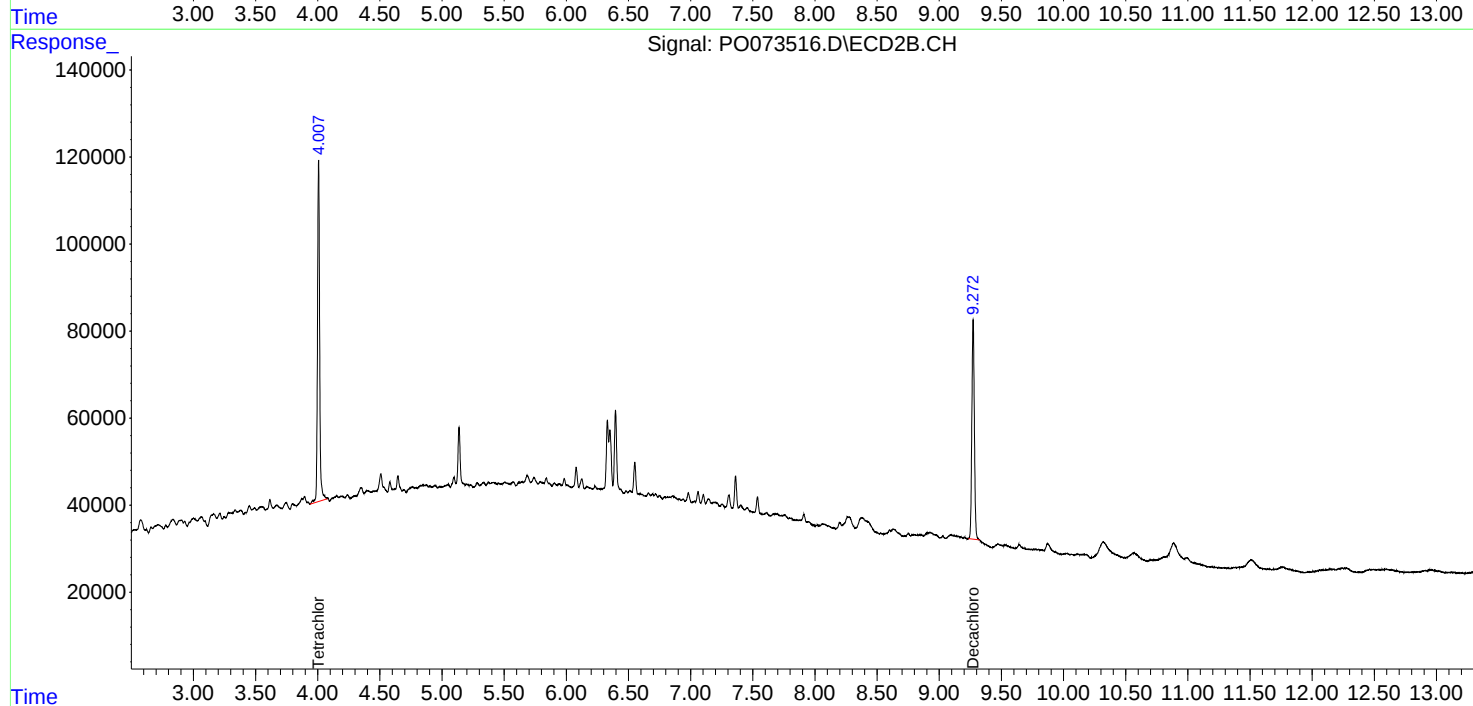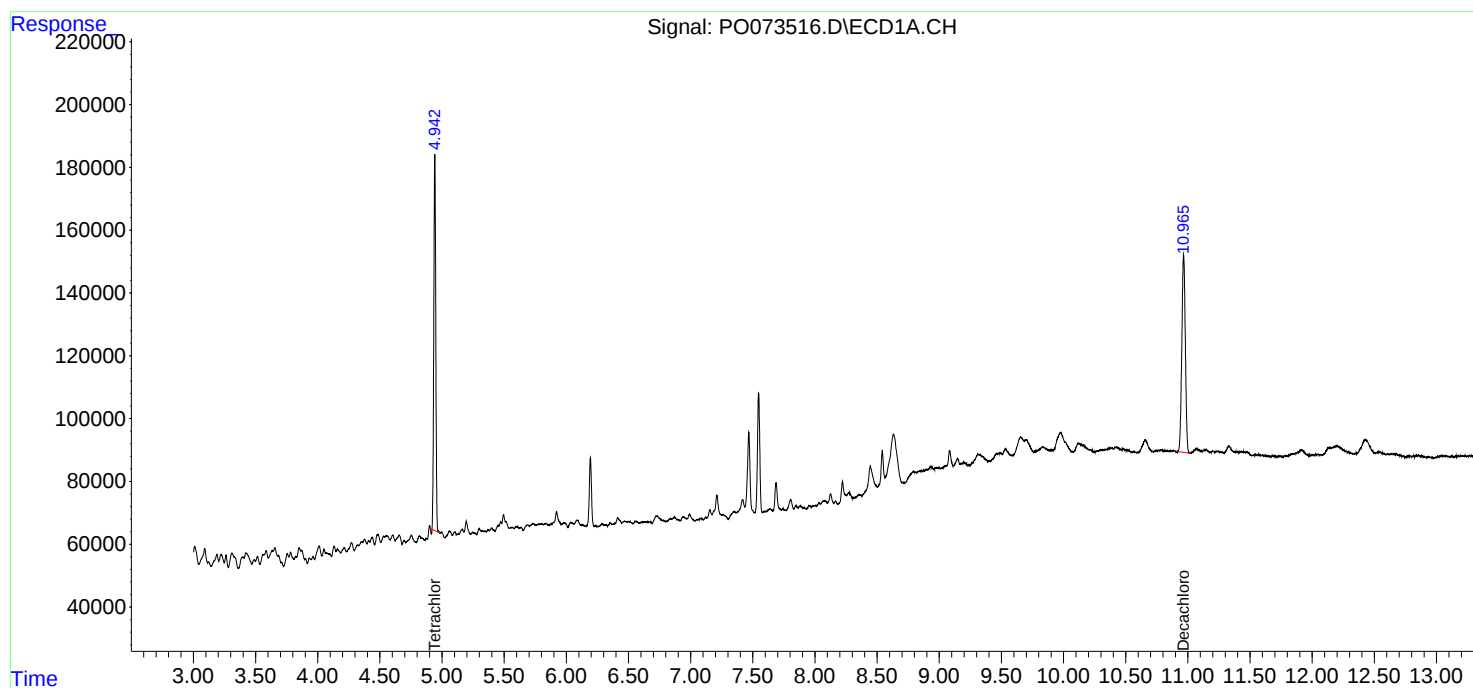


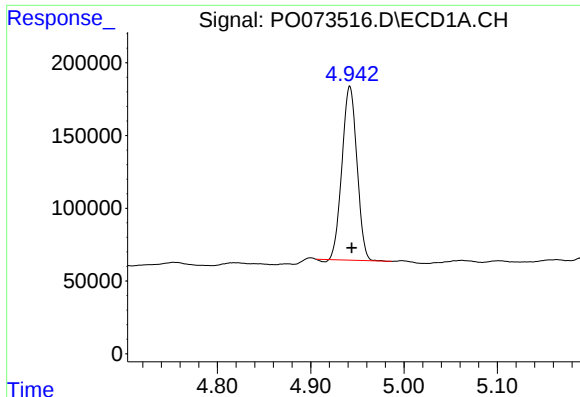

#1 Tetrachloro-m-xylene


R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 1322439
Conc: 15.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-01-112020

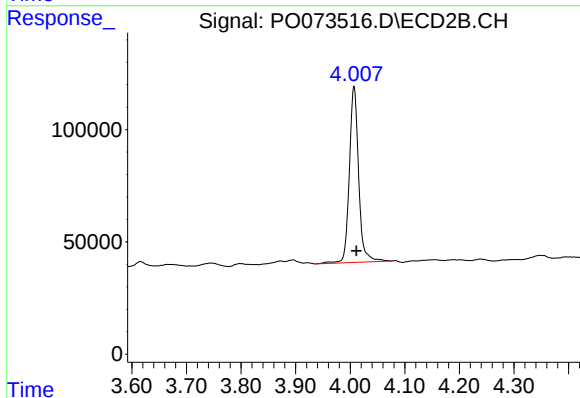


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.004 min
Response: 930945
Conc: 18.99 ng/ml

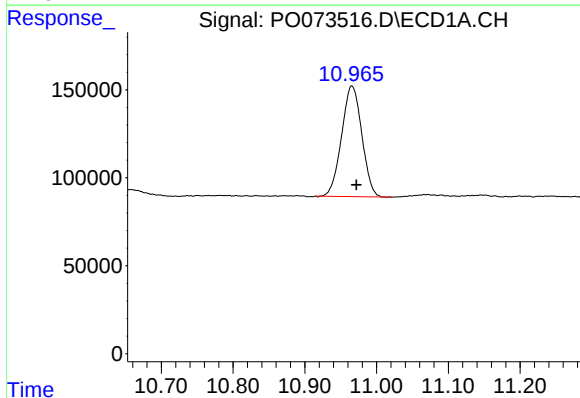

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: -0.006 min
Response: 1234198
Conc: 14.97 ng/ml

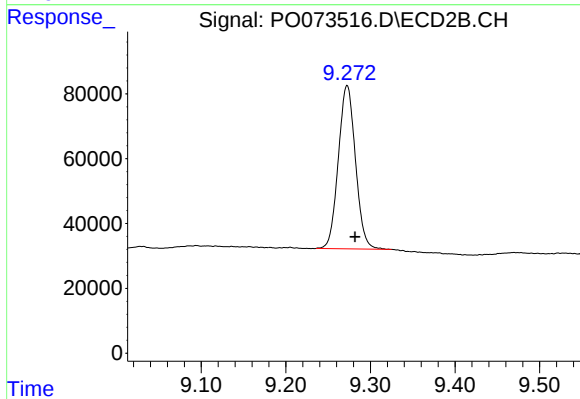

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.010 min
Response: 708957
Conc: 15.46 ng/ml