

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
 Data File : PO073536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Nov 2020 21:12
 Operator : DD\AJ
 Sample : L4875-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-08-112320

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:39:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 10:39:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	4.006	1615924	1036658	19.318	21.144m
2) SA Decachlor...	10.964	9.272	1280999	726906	15.536	15.854

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112420\
Data File : PO073536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Nov 2020 21:12
Operator : DD\AJ
Sample : L4875-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-08-112320


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 10:39:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

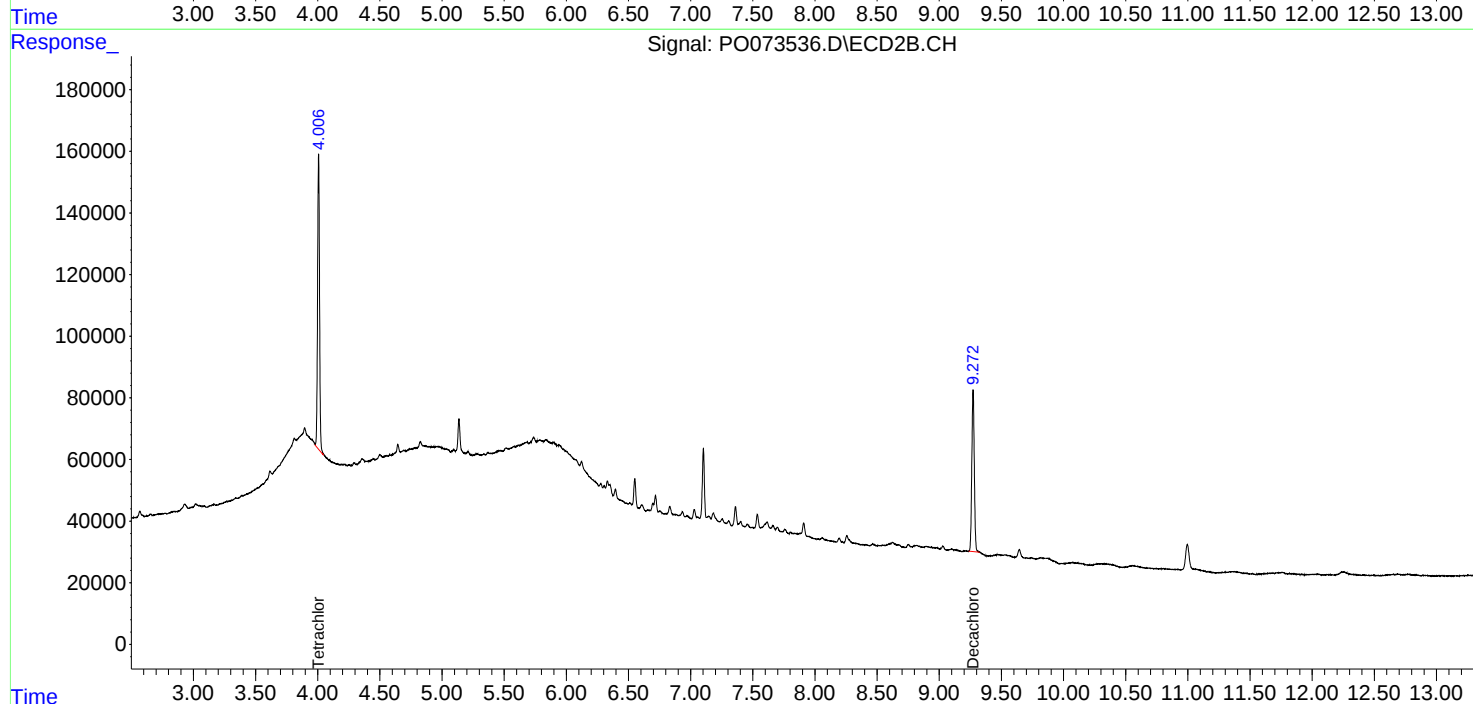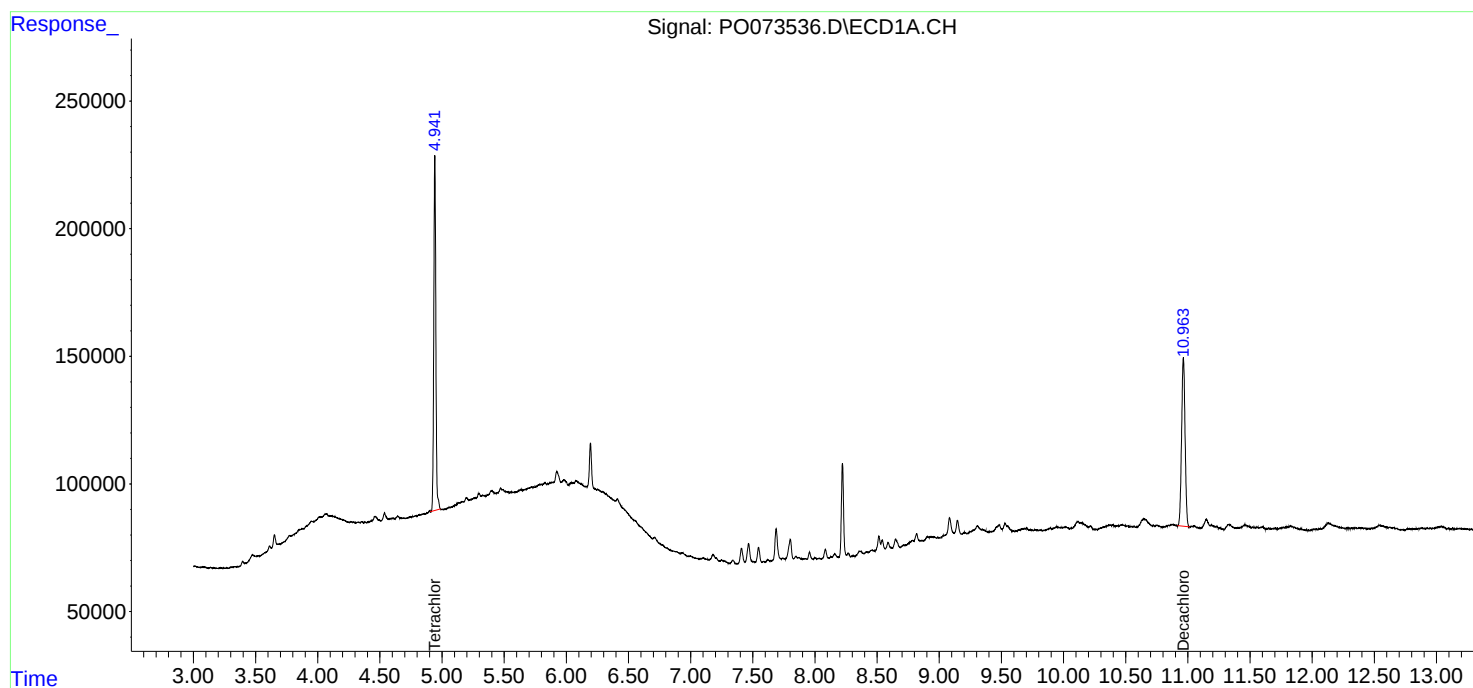

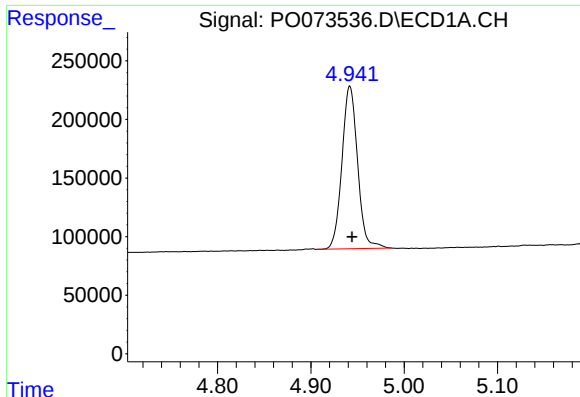


#1 Tetrachloro-m-xylene

R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 1615924
Conc: 19.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-08-112320


Manual Integrations
APPROVED

Ankita
11/25/2020 5:39:26 PM

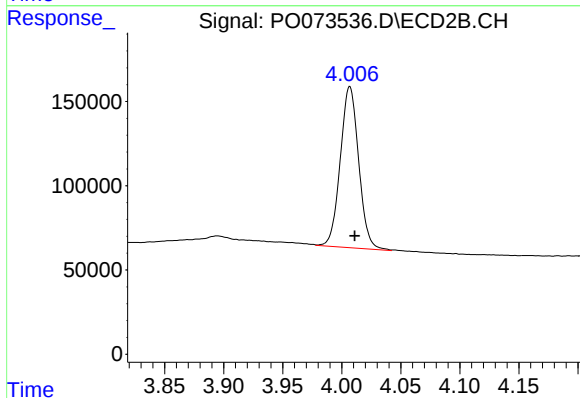


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.005 min
Response: 1036658
Conc: 21.14 ng/ml m

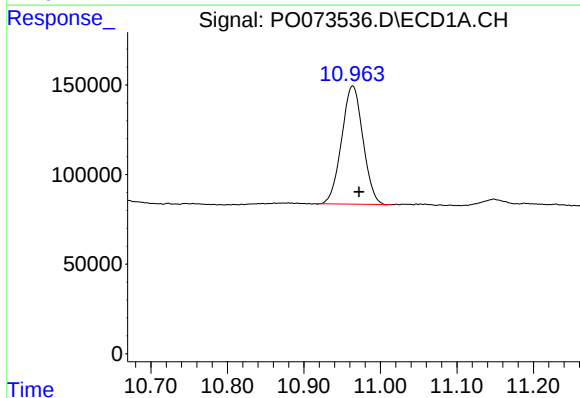

#2 Decachlorobiphenyl

R.T.: 10.964 min
Delta R.T.: -0.008 min
Response: 1280999
Conc: 15.54 ng/ml

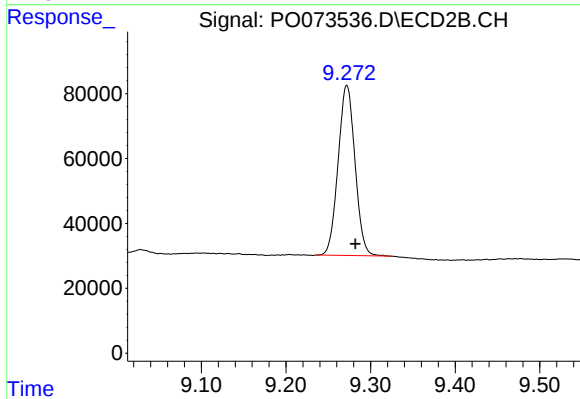

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: -0.010 min
Response: 726906
Conc: 15.85 ng/ml