

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112423\
 Data File : PO100040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2023 14:43
 Operator : YP/AJ
 Sample : 05540-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-06-11222023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 23:57:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.481	3.705	29048570	25375013	17.019	16.918
2) SA Decachlor...	10.363	8.802	9874081	13744826	13.594	12.283

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112423\
Data File : PO100040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2023 14:43
Operator : YP/AJ
Sample : 05540-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TR-06-11222023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 23:57:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

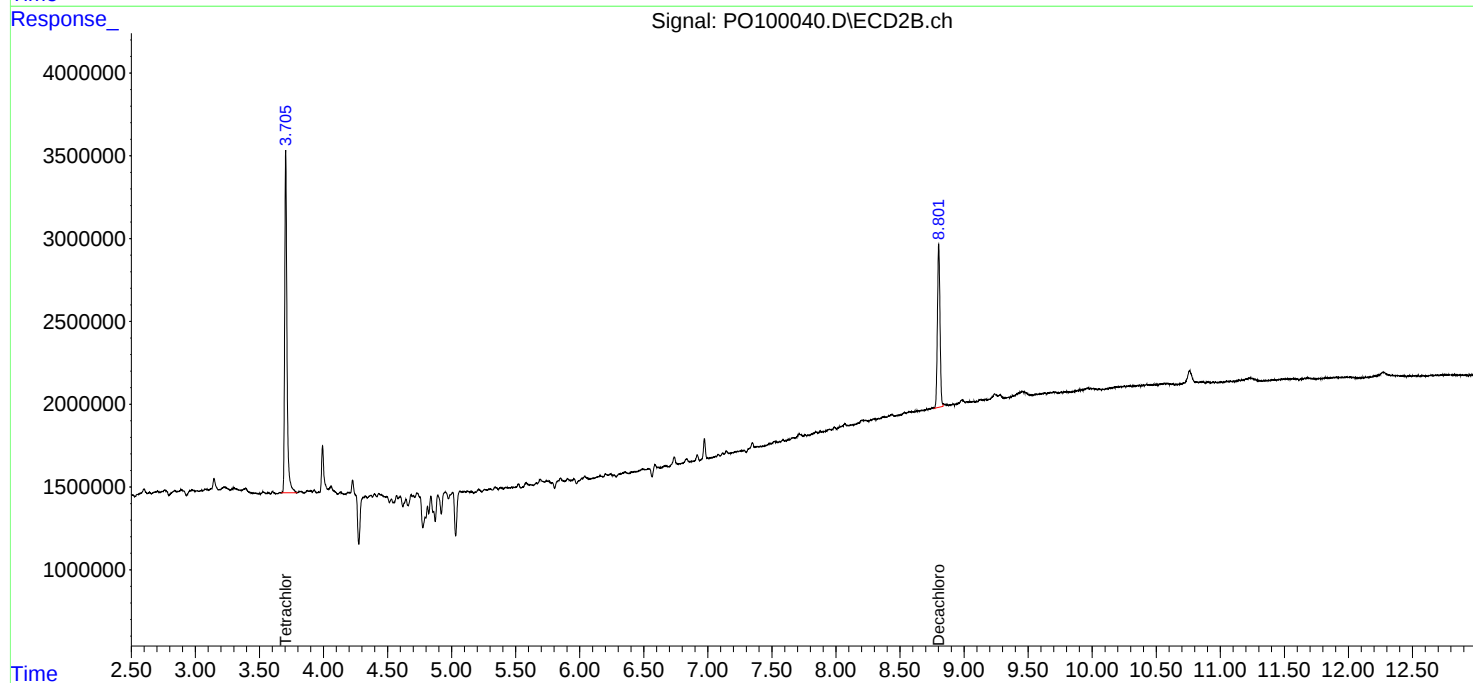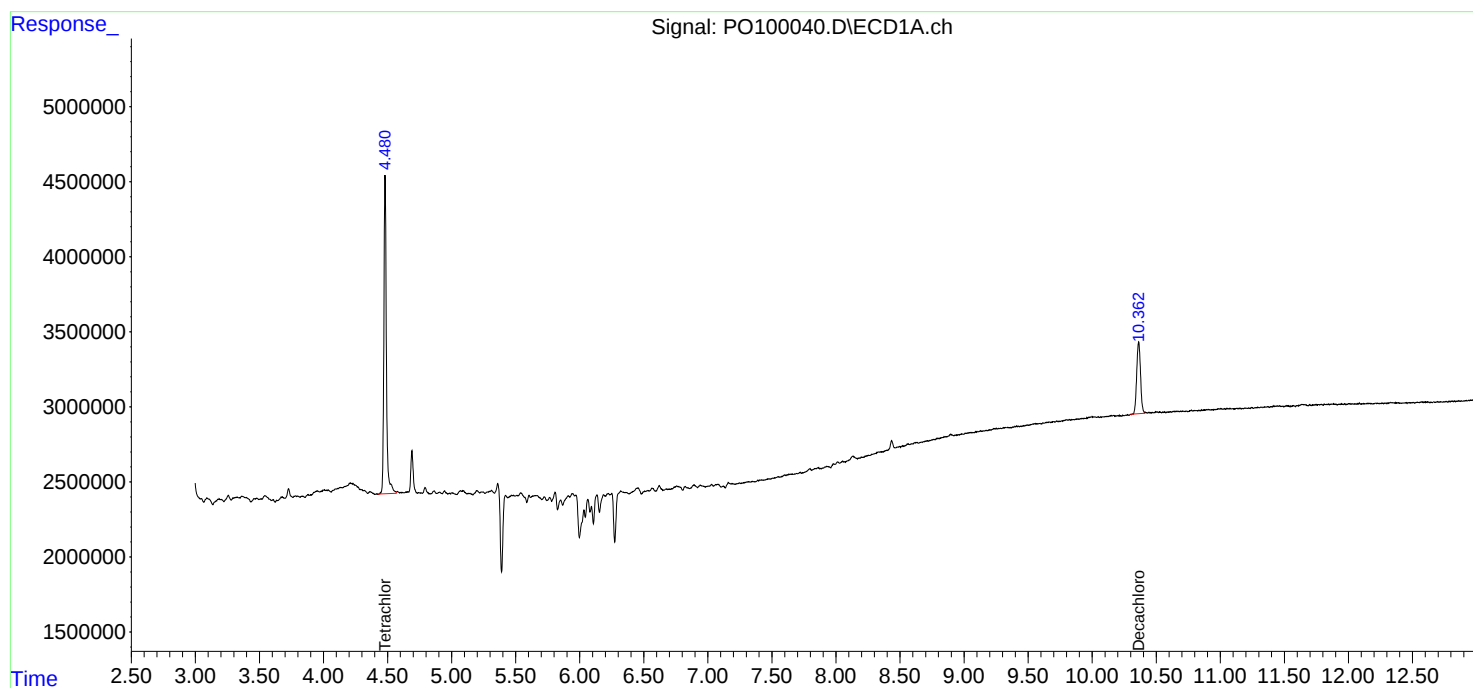


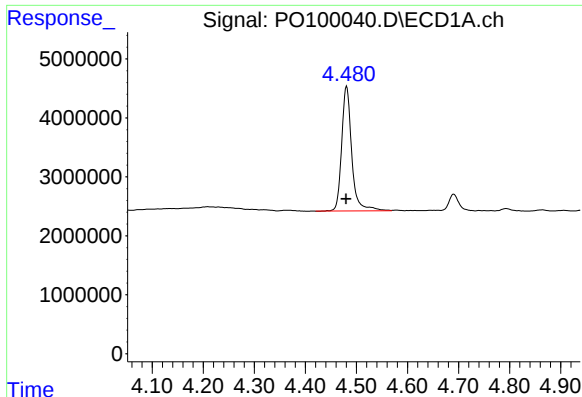

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 29048570
Conc: 17.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-06-11222023

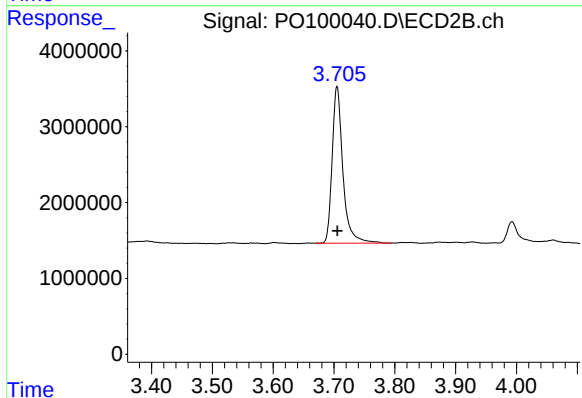


#1 Tetrachloro-m-xylene

R.T.: 3.705 min
Delta R.T.: 0.000 min
Response: 25375013
Conc: 16.92 ng/ml

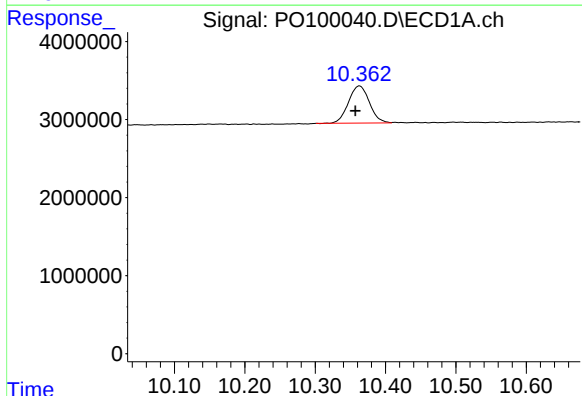

#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: 0.006 min
Response: 9874081
Conc: 13.59 ng/ml

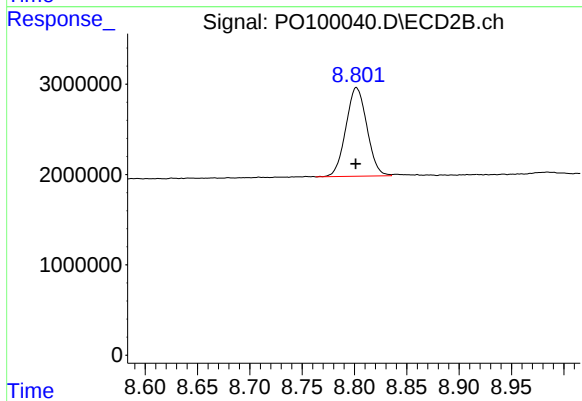

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 13744826
Conc: 12.28 ng/ml