

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112519\
 Data File : P0064072.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2019 15:34
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 16:02:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.313	3.564	652436	484029	21.339	21.792
2)	SA Decachlor...	9.940	8.531	787644	649332	19.384	22.202
Target Compounds							
9)	L2 AR-1221-2	4.617	0.000	10659	0	33.981	N.D. #
10)	L2 AR-1221-3	4.617	0.000	10659	0	11.238	N.D. #
11)	L3 AR-1232-1	4.617	0.000	10659	0	8.013	N.D. #
15)	L3 AR-1232-5	5.790	0.000	2879	0	4.911	N.D. #
22)	L5 AR-1248-2	5.790	0.000	2879	0	2.272	N.D. #
32)	L7 AR-1260-2	7.390	0.000	17516	0	6.953	N.D. #
40)	L8 AR-1262-5	9.188	0.000	11733	0	5.386	N.D. #
44)	L9 AR-1268-4	9.188	0.000	11733	0	4.827	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112519\
Data File : PO064072.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2019 15:34
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 16:02:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

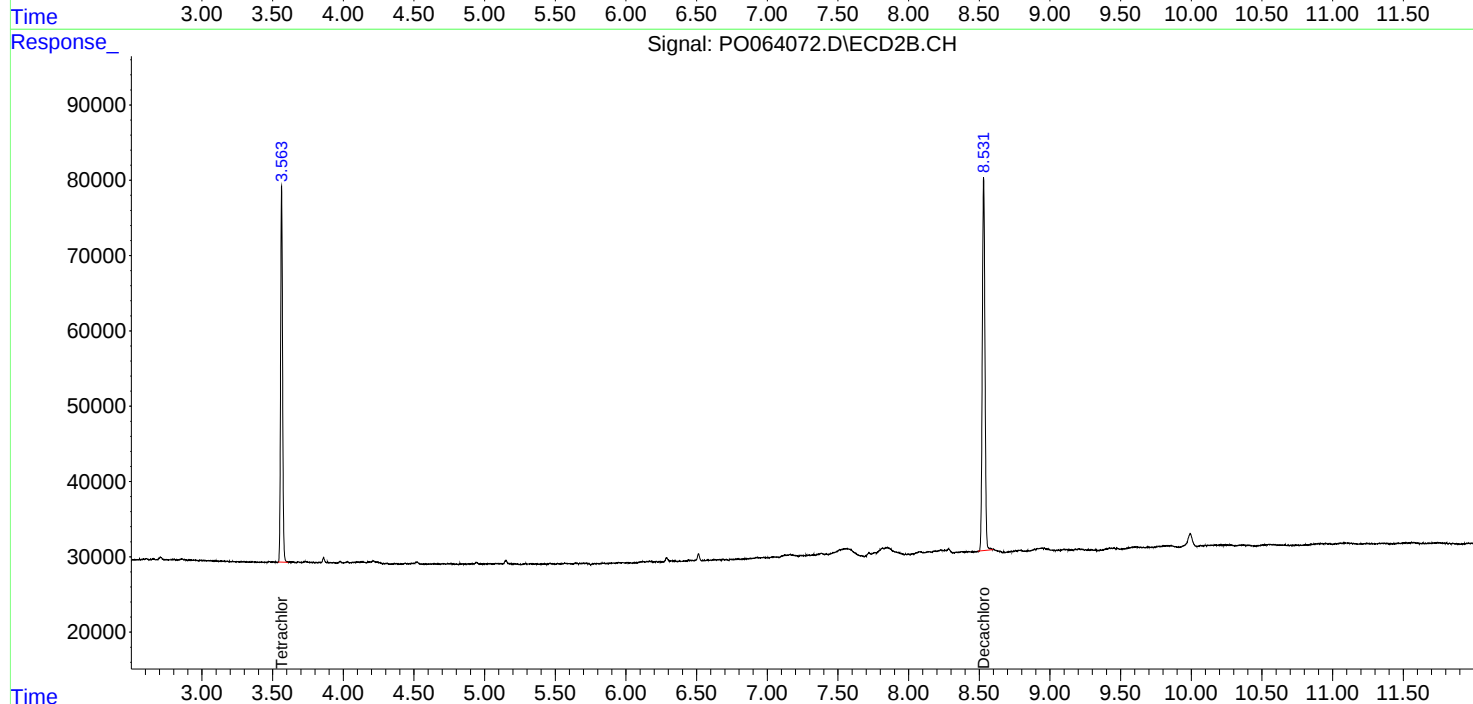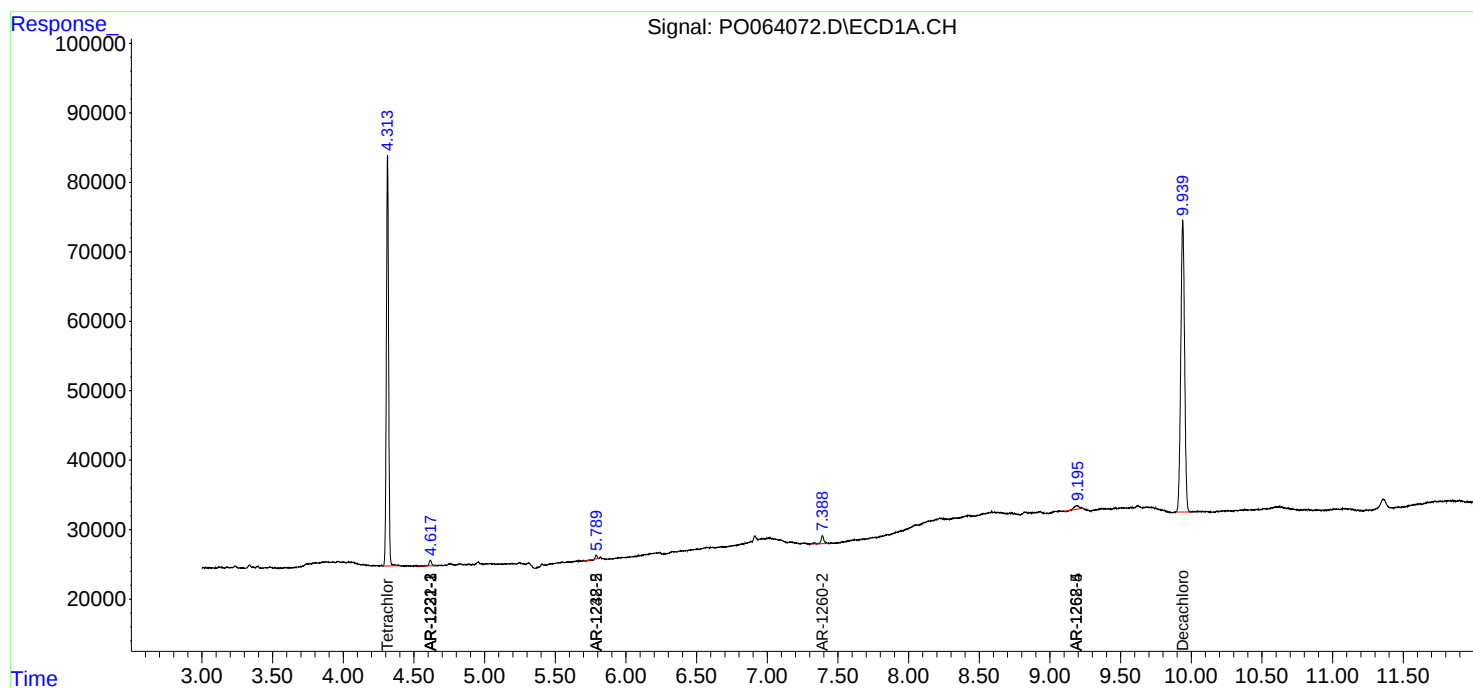


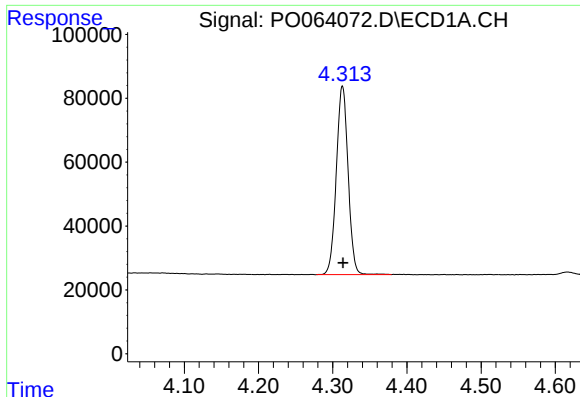

#1 Tetrachloro-m-xylene


R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 652436
Conc: 21.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

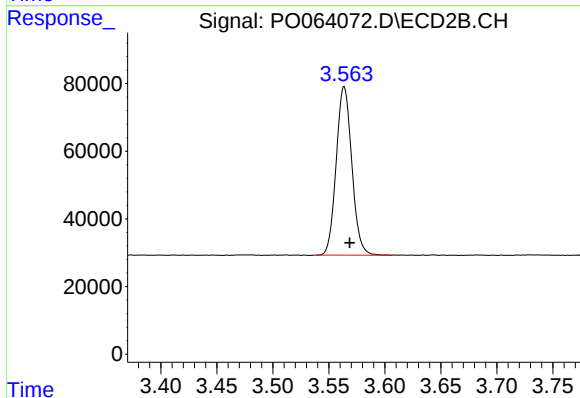


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.005 min
Response: 484029
Conc: 21.79 ng/ml

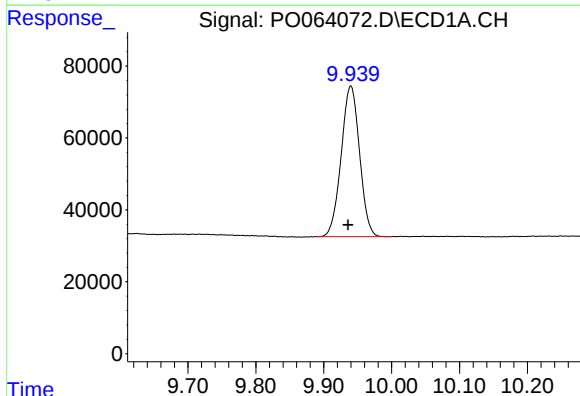


#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 787644
Conc: 19.38 ng/ml

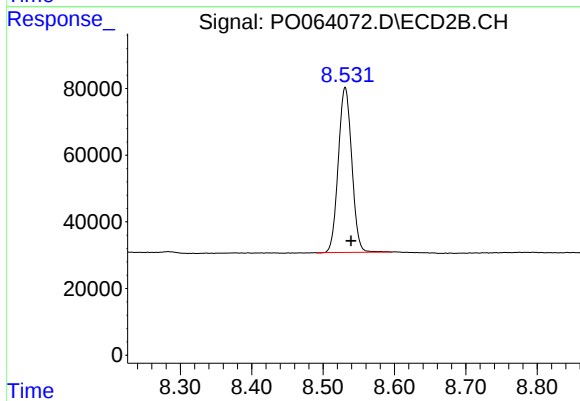

#2 Decachlorobiphenyl


R.T.: 8.531 min
Delta R.T.: -0.008 min
Response: 649332
Conc: 22.20 ng/ml

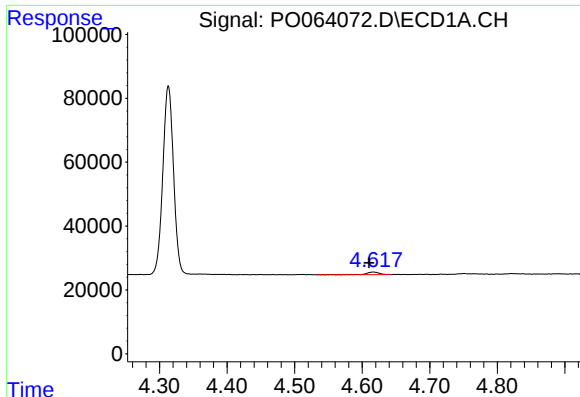

#9 AR-1221-2


R.T.: 4.617 min
Delta R.T.: 0.007 min
Response: 10659
Conc: 33.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

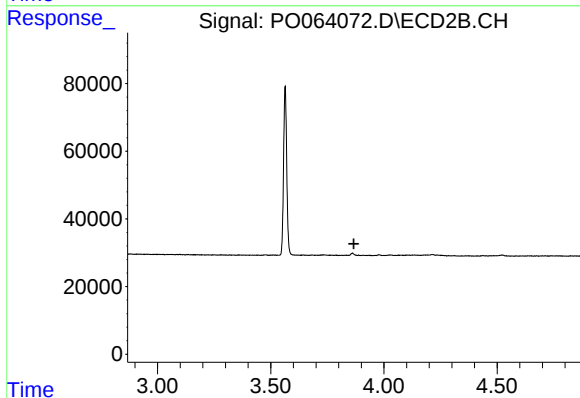


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.868 min
Response: 0
Conc: N.D.

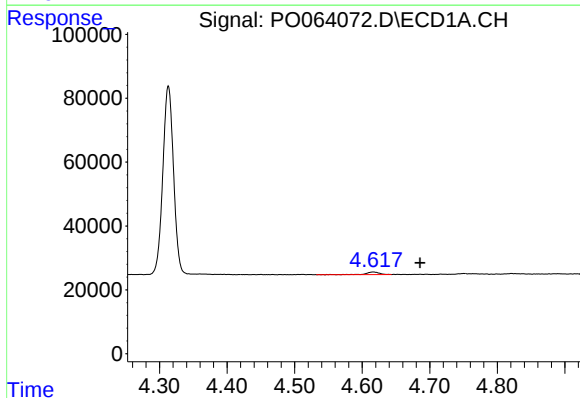


#10 AR-1221-3

R.T.: 4.617 min
Delta R.T.: -0.069 min
Response: 10659
Conc: 11.24 ng/ml

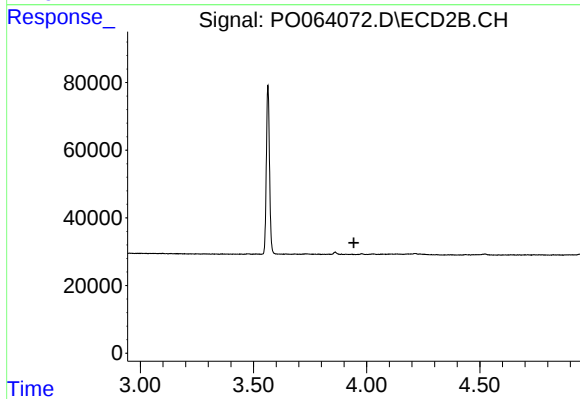

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.944 min
Response: 0
Conc: N.D.

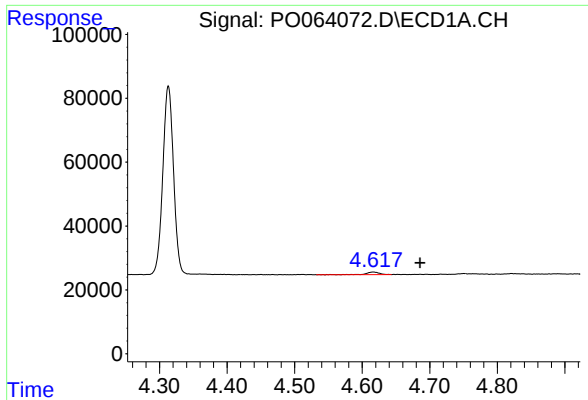

#11 AR-1232-1


R.T.: 4.617 min
Delta R.T.: -0.069 min
Response: 10659
Conc: 8.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

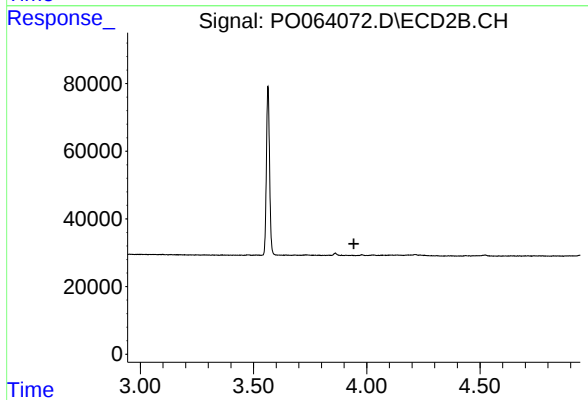


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.943 min
Response: 0
Conc: N.D.

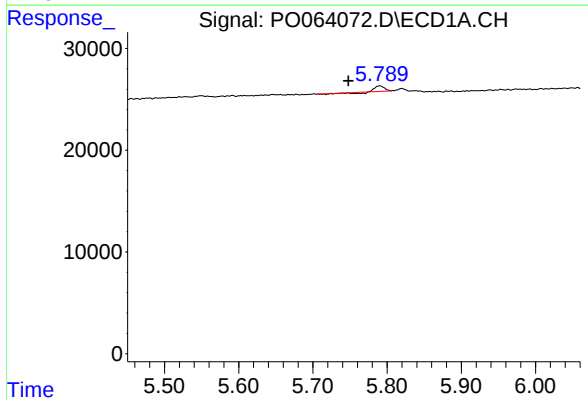


#15 AR-1232-5

R.T.: 5.790 min
Delta R.T.: 0.042 min
Response: 2879
Conc: 4.91 ng/ml

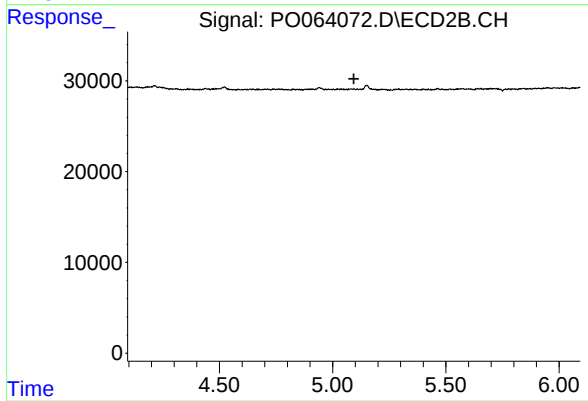

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.094 min
Response: 0
Conc: N.D.

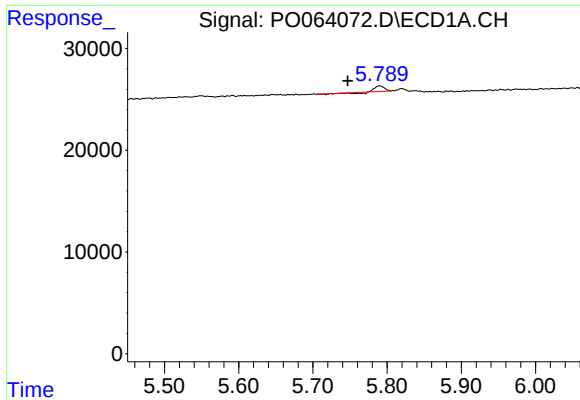

#22 AR-1248-2


R.T.: 5.790 min
Delta R.T.: 0.043 min
Response: 2879
Conc: 2.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

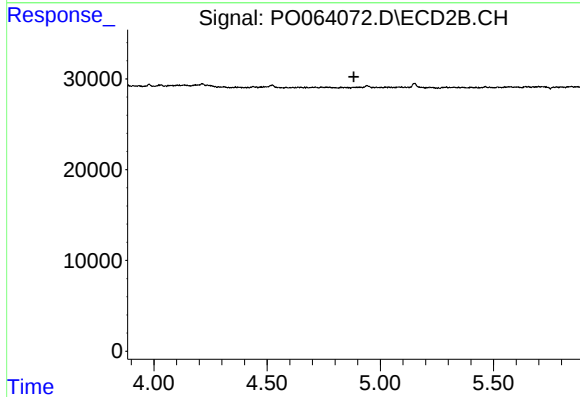


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 4.883 min
Response: 0
Conc: N.D.

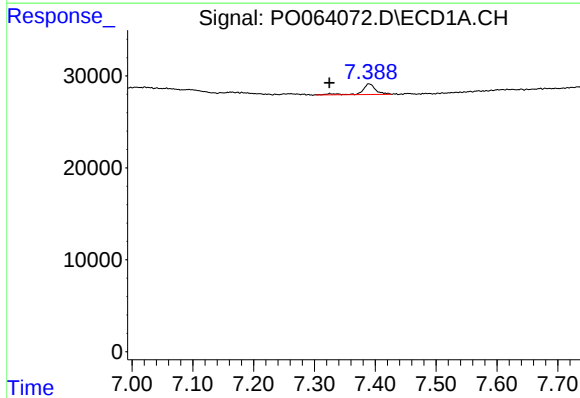


#32 AR-1260-2

R.T.: 7.390 min
Delta R.T.: 0.065 min
Response: 17516
Conc: 6.95 ng/ml

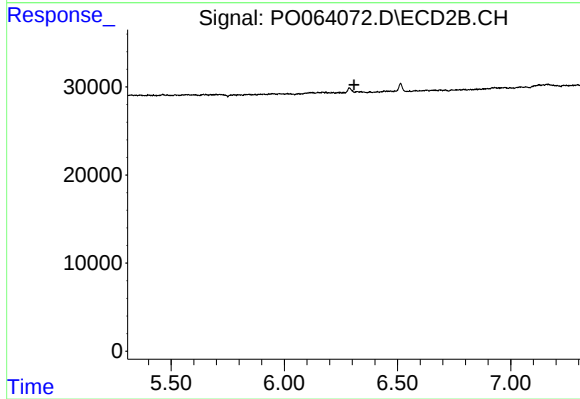

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

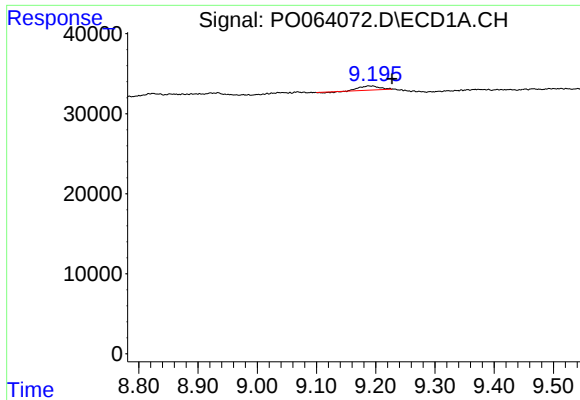

#40 AR-1262-5


R.T.: 9.188 min
Delta R.T.: -0.040 min
Response: 11733
Conc: 5.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

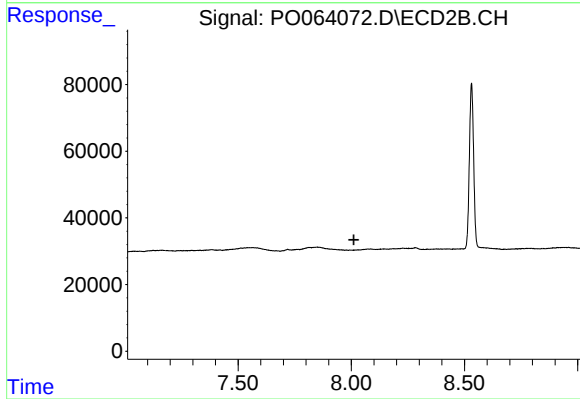


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.011 min
Response: 0
Conc: N.D.

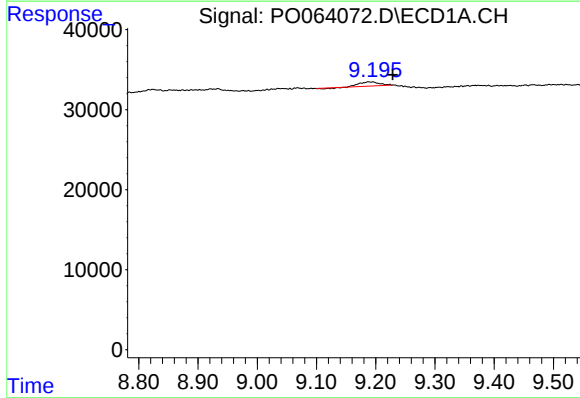

#44 AR-1268-4

R.T.: 9.188 min
Delta R.T.: -0.041 min
Response: 11733
Conc: 4.83 ng/ml

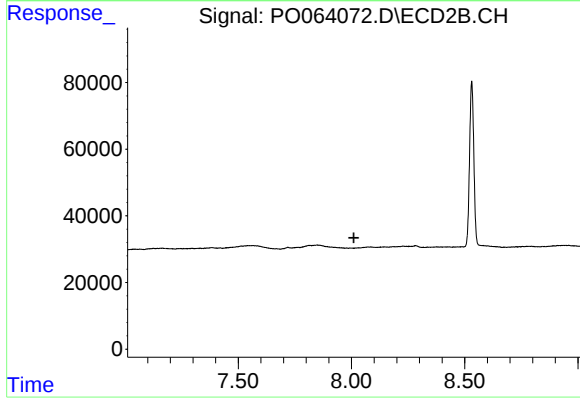

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.010 min
Response: 0
Conc: N.D.