

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112519\
 Data File : P0064092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2019 21:12
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 03:11:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.566	921114	798039	30.126	35.929
2)	SA Decachlor...	9.941	8.532	548419	434021	13.496	14.840
Target Compounds							
9)	L2 AR-1221-2	4.618	0.000	13295	0	42.387	N.D. #
10)	L2 AR-1221-3	4.618	0.000	13295	0	14.017	N.D. #
11)	L3 AR-1232-1	4.618	0.000	13295	0	9.996	N.D. #
15)	L3 AR-1232-5	5.791	0.000	7013	0	11.964	N.D. #
22)	L5 AR-1248-2	5.791	0.000	7013	0	5.535	N.D. #
28)	L6 AR-1254-3	6.913	0.000	13115	0	4.178	N.D. #
35)	L7 AR-1260-5	8.231	0.000	13524	0	2.881	N.D. #
37)	L8 AR-1262-2	8.231	0.000	13524	0	2.296	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112519\
Data File : PO064092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2019 21:12
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 03:11:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

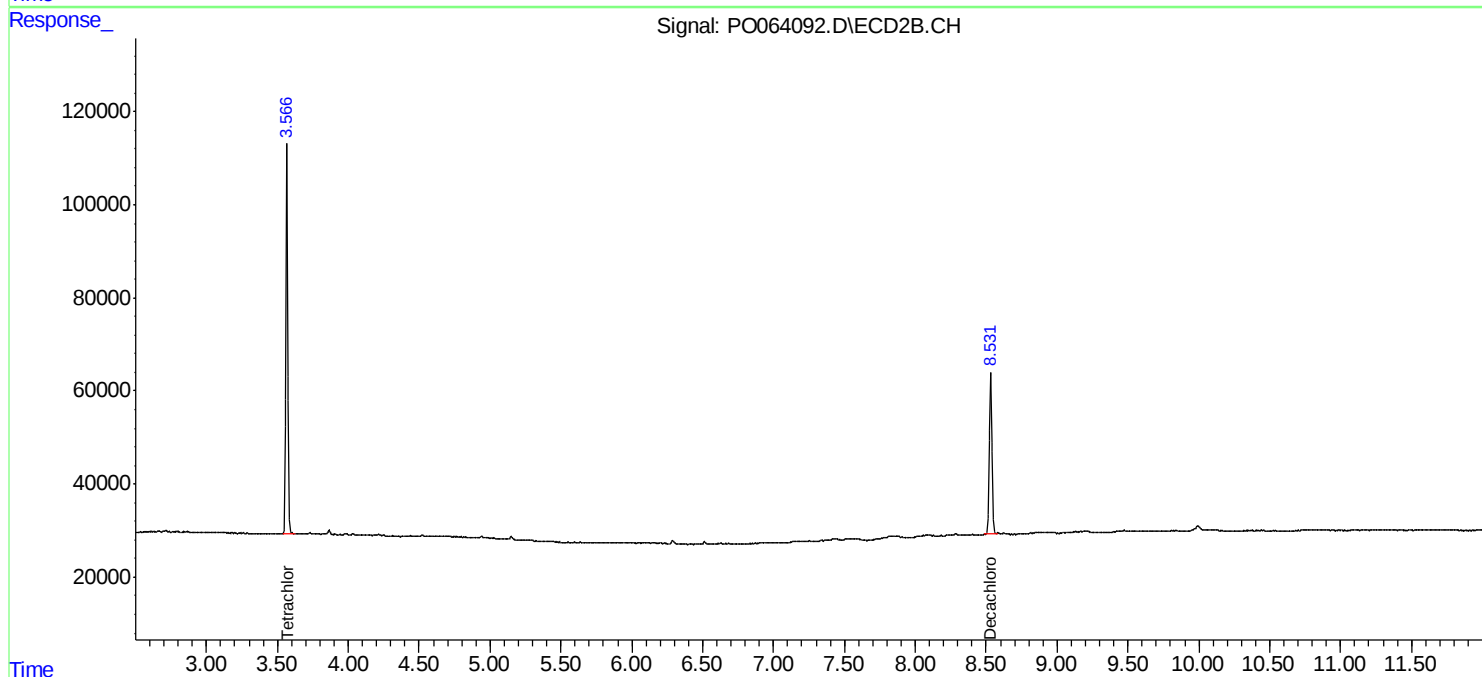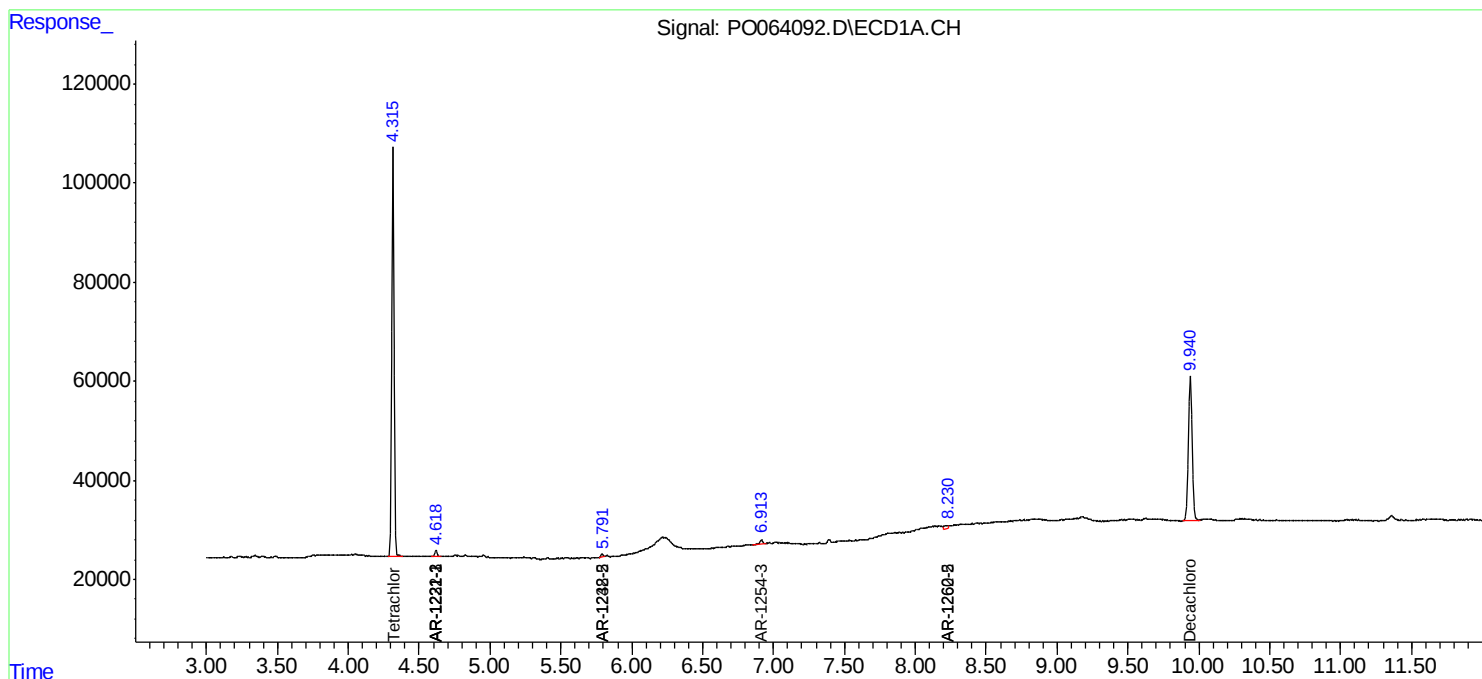


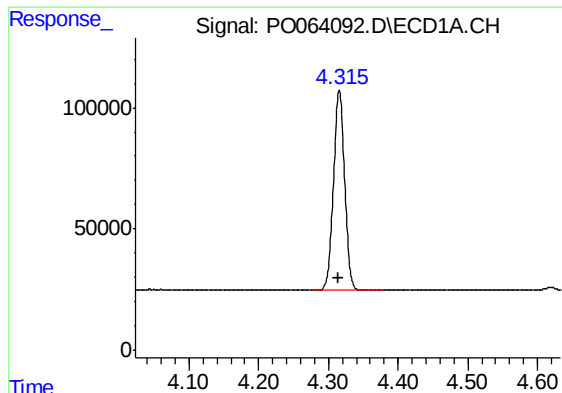

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 921114
Conc: 30.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

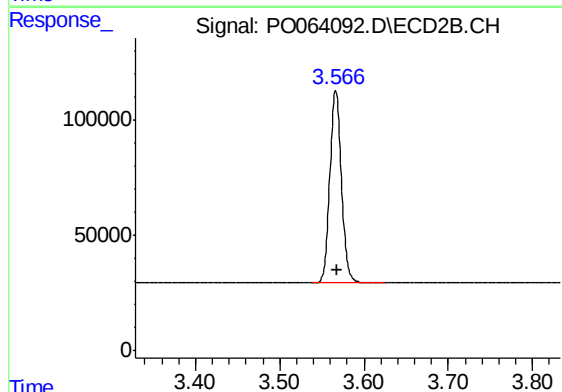


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.002 min
Response: 798039
Conc: 35.93 ng/ml

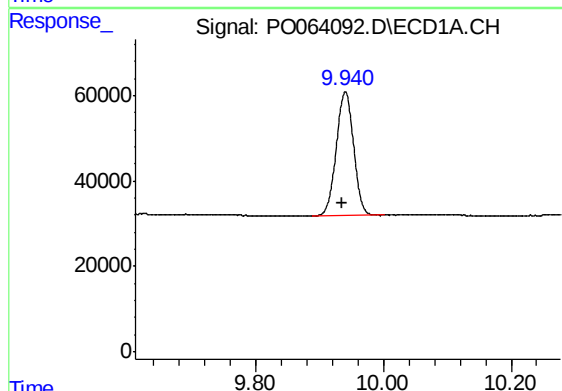


#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: 0.005 min
Response: 548419
Conc: 13.50 ng/ml

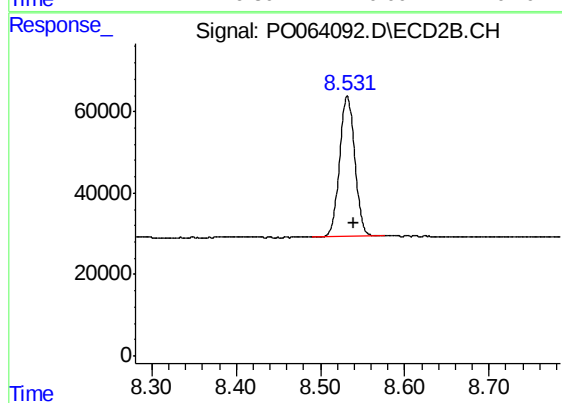

#2 Decachlorobiphenyl


R.T.: 8.532 min
Delta R.T.: -0.008 min
Response: 434021
Conc: 14.84 ng/ml

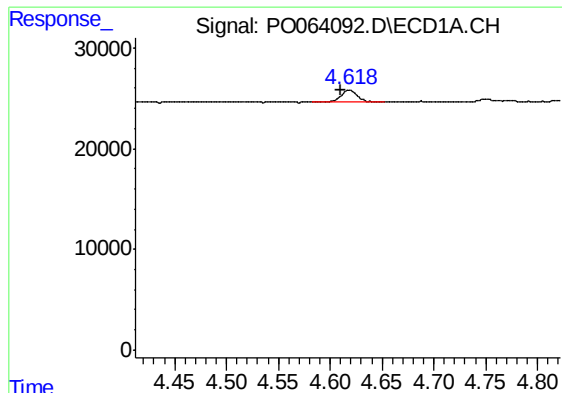

#9 AR-1221-2


R.T.: 4.618 min
Delta R.T.: 0.009 min
Response: 13295
Conc: 42.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

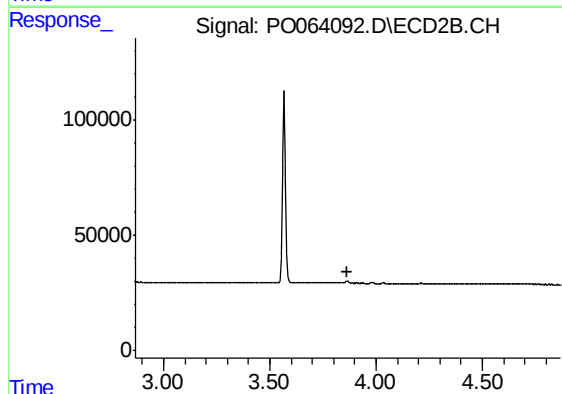


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.868 min
Response: 0
Conc: N.D.

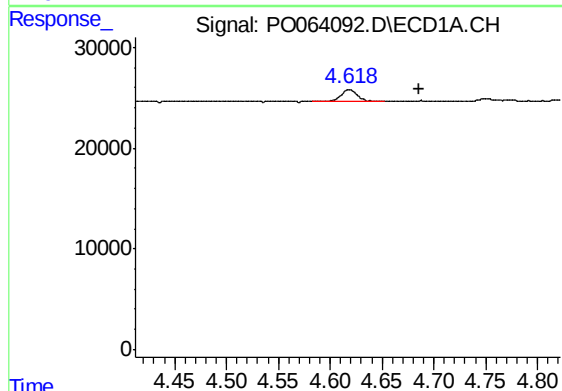


#10 AR-1221-3

R.T.: 4.618 min
Delta R.T.: -0.067 min
Response: 13295
Conc: 14.02 ng/ml

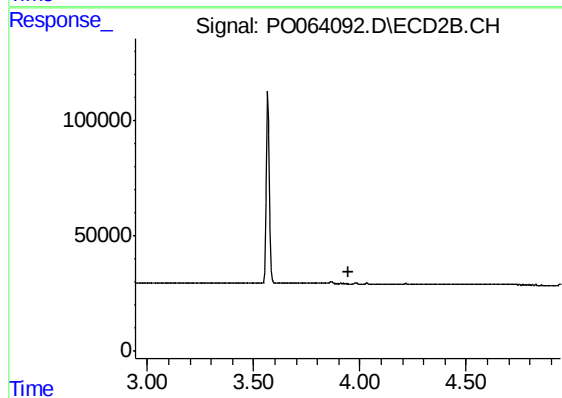

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.944 min
Response: 0
Conc: N.D.

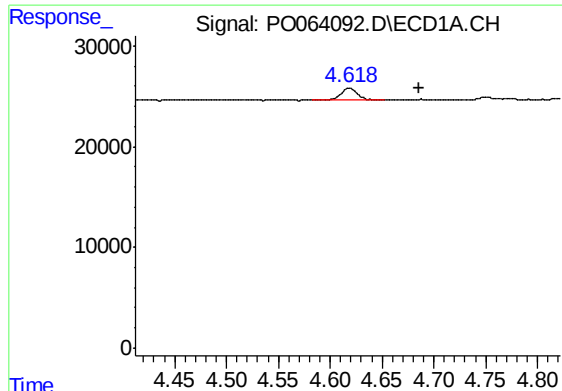

#11 AR-1232-1


R.T.: 4.618 min
Delta R.T.: -0.067 min
Response: 13295
Conc: 10.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

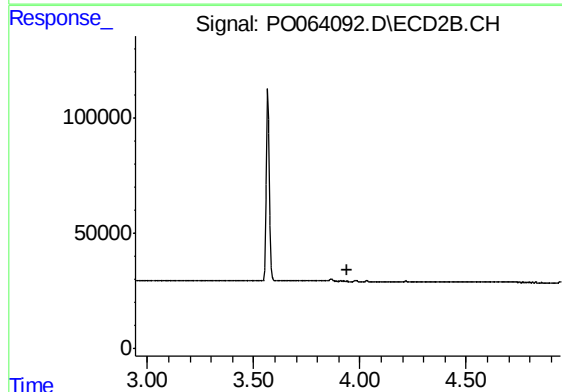


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.943 min
Response: 0
Conc: N.D.

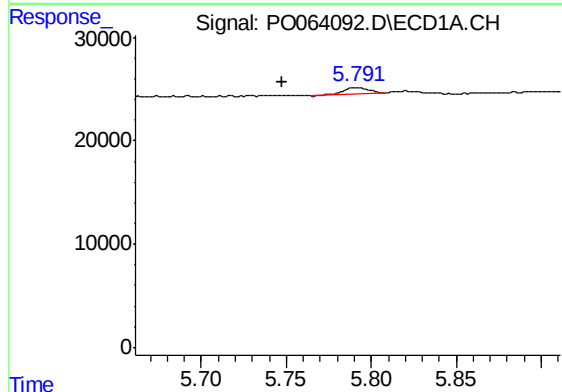


#15 AR-1232-5

R.T.: 5.791 min
Delta R.T.: 0.043 min
Response: 7013
Conc: 11.96 ng/ml

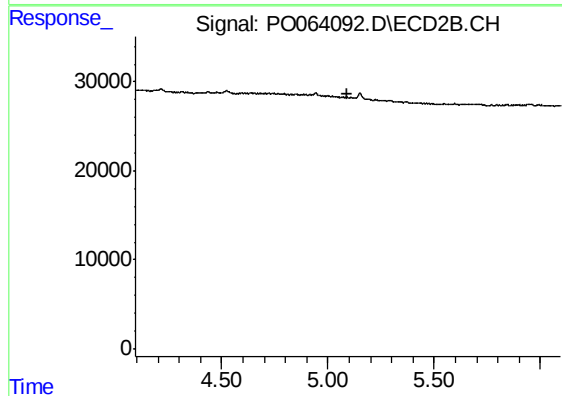

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.094 min
Response: 0
Conc: N.D.

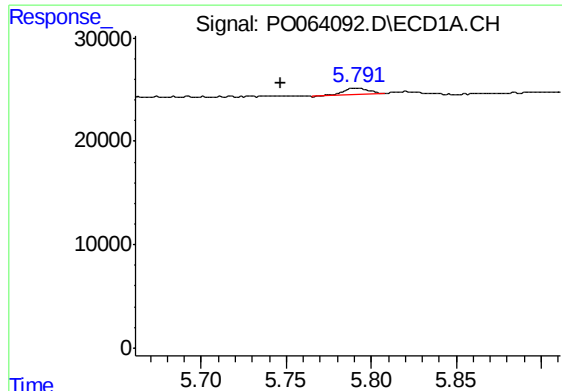

#22 AR-1248-2


R.T.: 5.791 min
Delta R.T.: 0.044 min
Response: 7013
Conc: 5.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

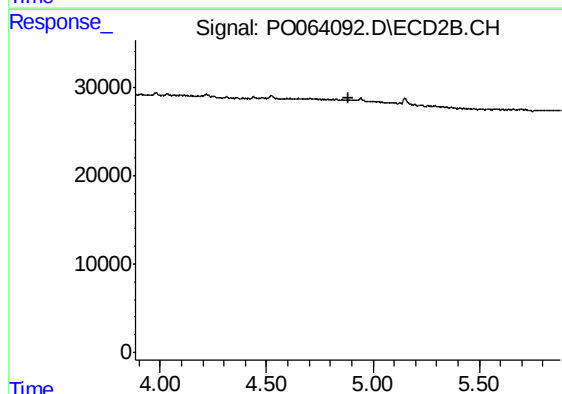


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 4.883 min
Response: 0
Conc: N.D.

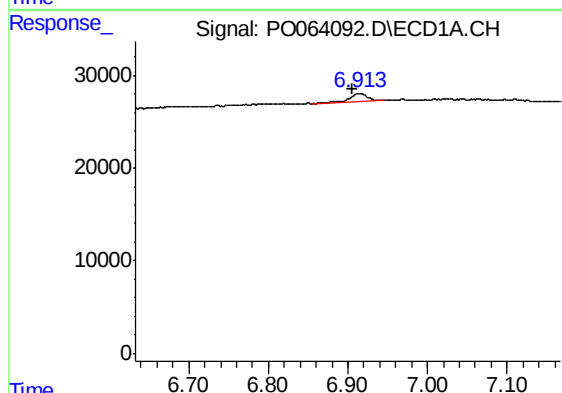


#28 AR-1254-3

R.T.: 6.913 min
Delta R.T.: 0.007 min
Response: 13115
Conc: 4.18 ng/ml

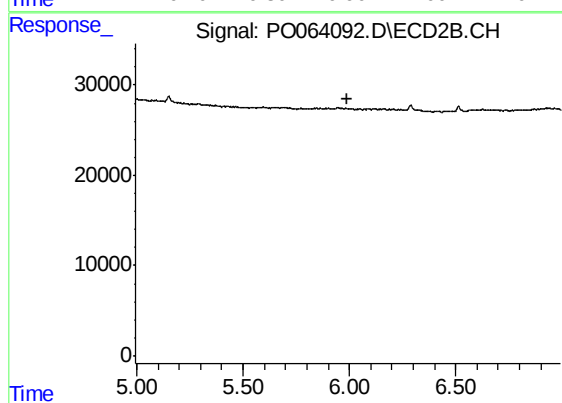

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

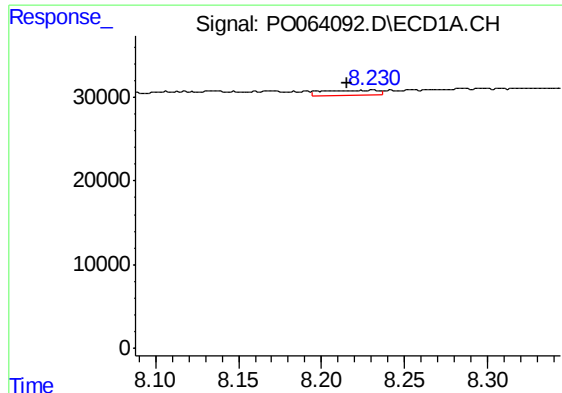

#35 AR-1260-5


R.T.: 8.231 min
Delta R.T.: 0.015 min
Response: 13524
Conc: 2.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

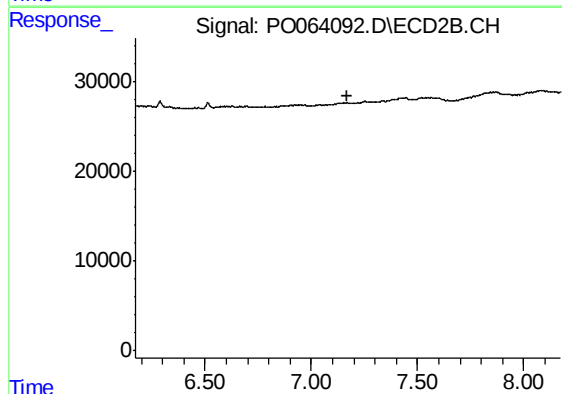


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

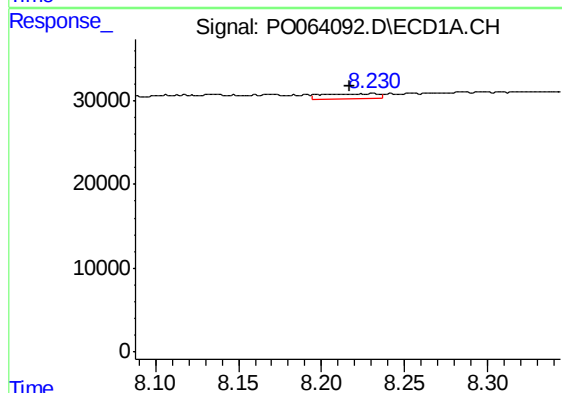

#37 AR-1262-2

R.T.: 8.231 min
Delta R.T.: 0.014 min
Response: 13524
Conc: 2.30 ng/ml

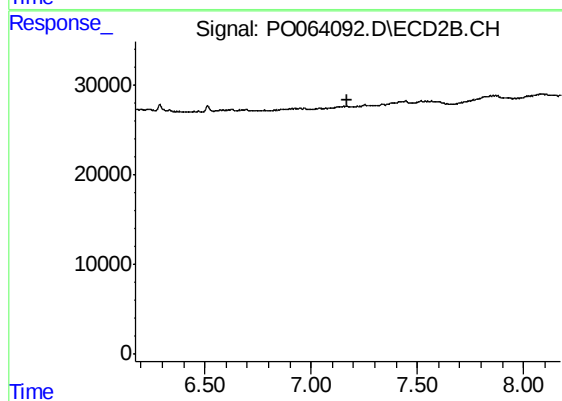

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.173 min
Response: 0
Conc: N.D.