

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112519\
 Data File : P0064060.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2019 11:59
 Operator : SM/AJ
 Sample : K5970-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-28-D

Manual Integrations
 APPROVED

Ankita
 11/26/2019 1:22:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:12:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.314	3.565	680254	529027	22.249	23.818
2) SA Decachlor...	9.941	8.531	762730	609844	18.770	20.852m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112519\
Data File : PO064060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2019 11:59
Operator : SM/AJ
Sample : K5970-07
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-28-D


Manual Integrations
APPROVED

Ankita
11/26/2019 1:22:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:12:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

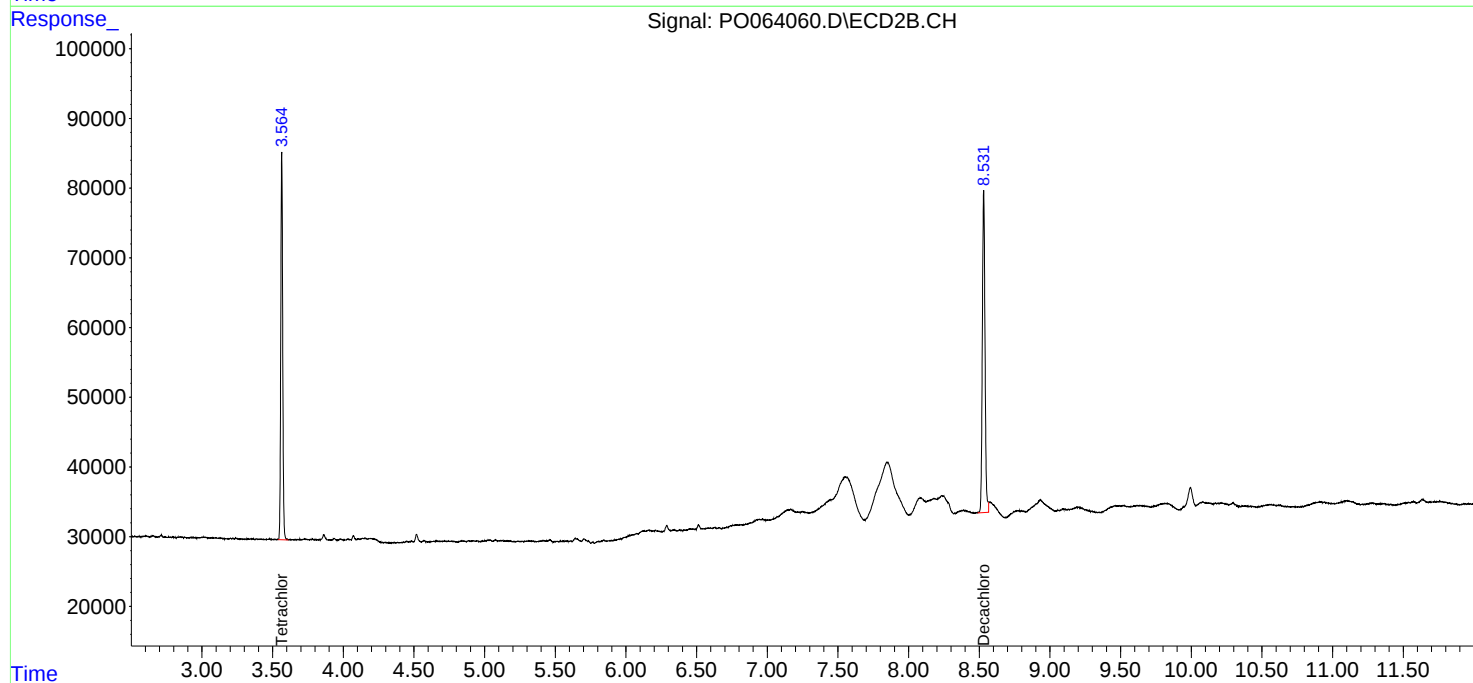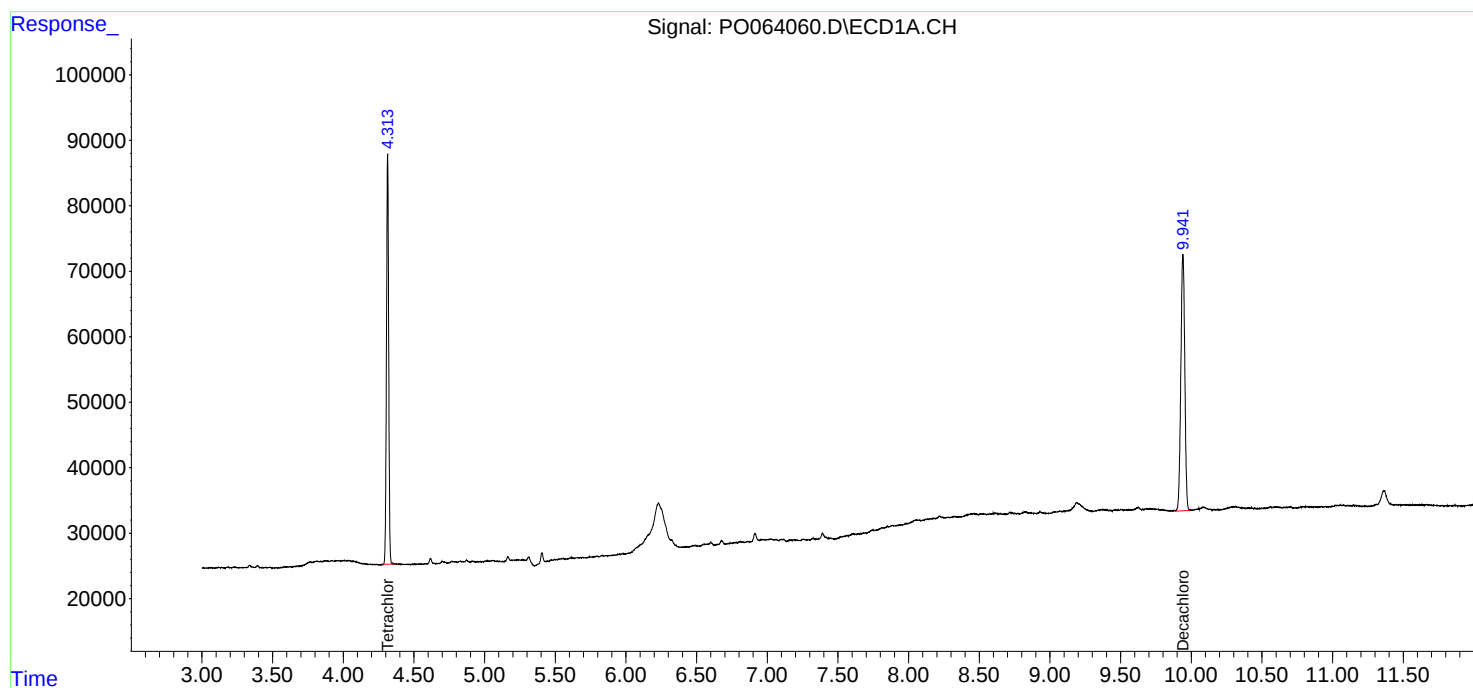

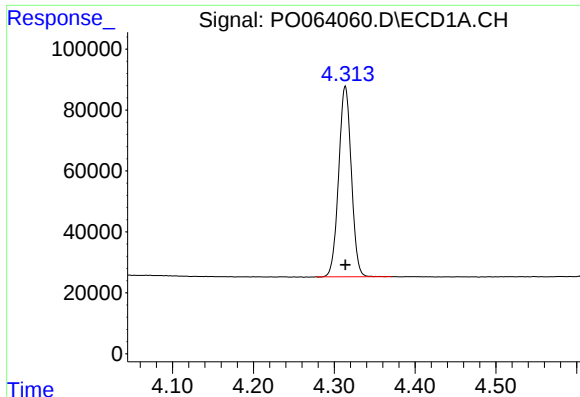


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: 0.000 min
Response: 680254
Conc: 22.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-28-D


Manual Integrations
APPROVED

Ankita
11/26/2019 1:22:33 PM

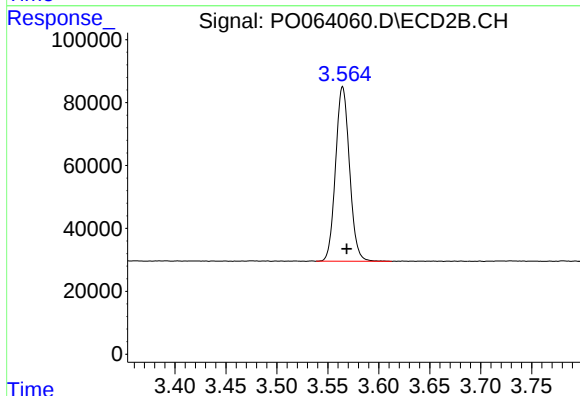


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.004 min
Response: 529027
Conc: 23.82 ng/ml

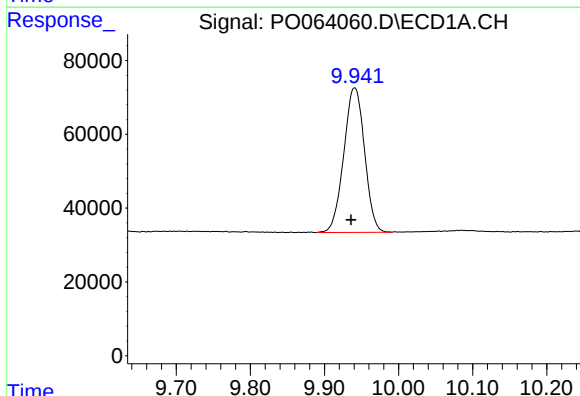

#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: 0.005 min
Response: 762730
Conc: 18.77 ng/ml

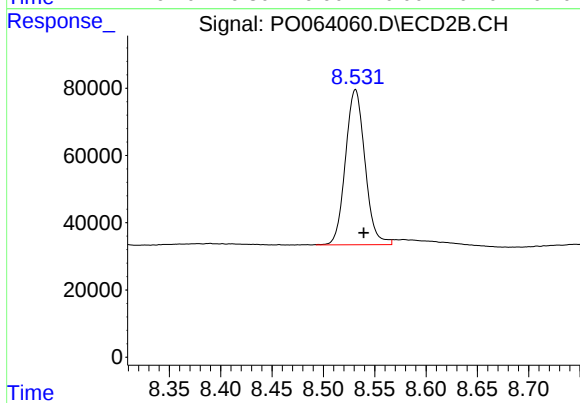

#2 Decachlorobiphenyl

R.T.: 8.531 min
Delta R.T.: -0.008 min
Response: 609844
Conc: 20.85 ng/ml m