

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
 Data File : PO073552.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 11:35
 Operator : DD\AJ
 Sample : L4892-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-48(8.0-8.5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 11:57:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.939	4.003	1947599	1099292	23.283	22.422
2) SA Decachlor...	10.960	9.270	1764431	986850	21.400	21.523

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
Data File : PO073552.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 11:35
Operator : DD\AJ
Sample : L4892-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-48(8.0-8.5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 11:57:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

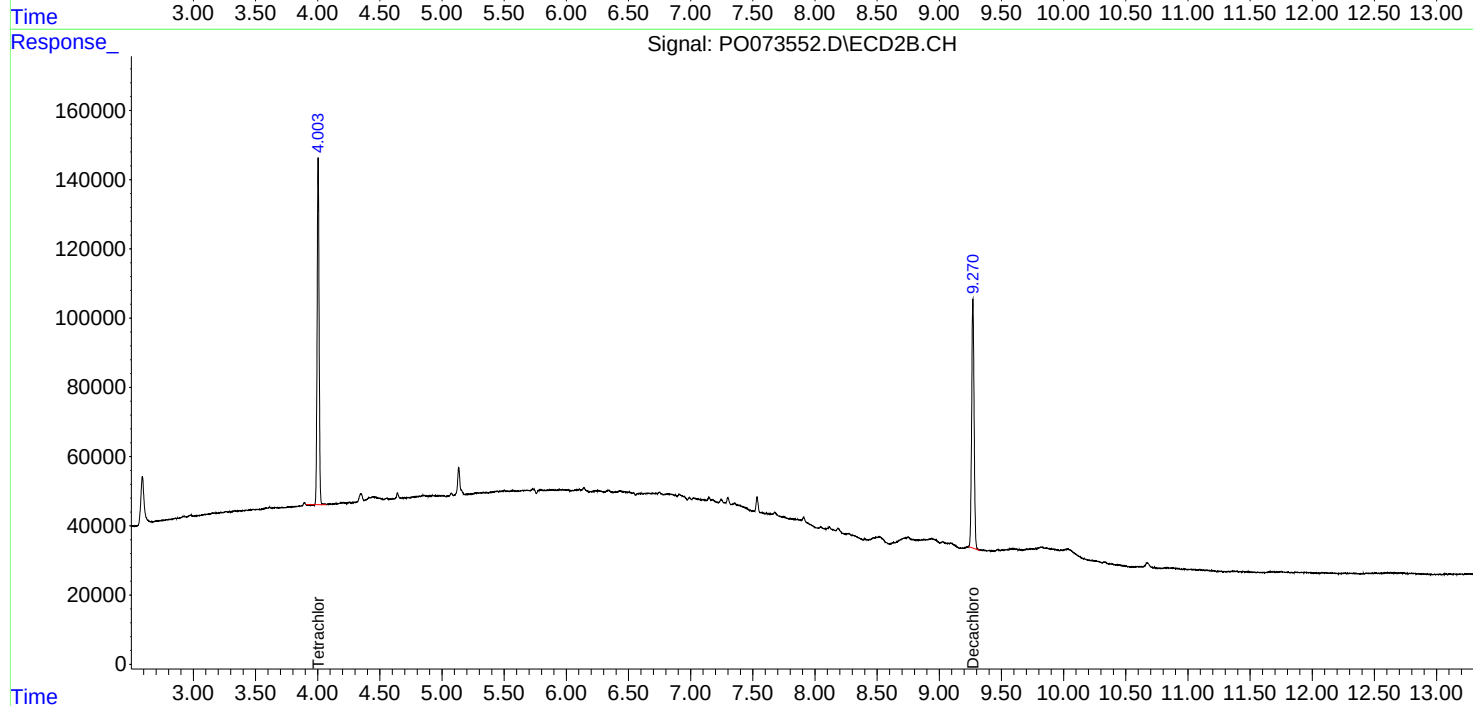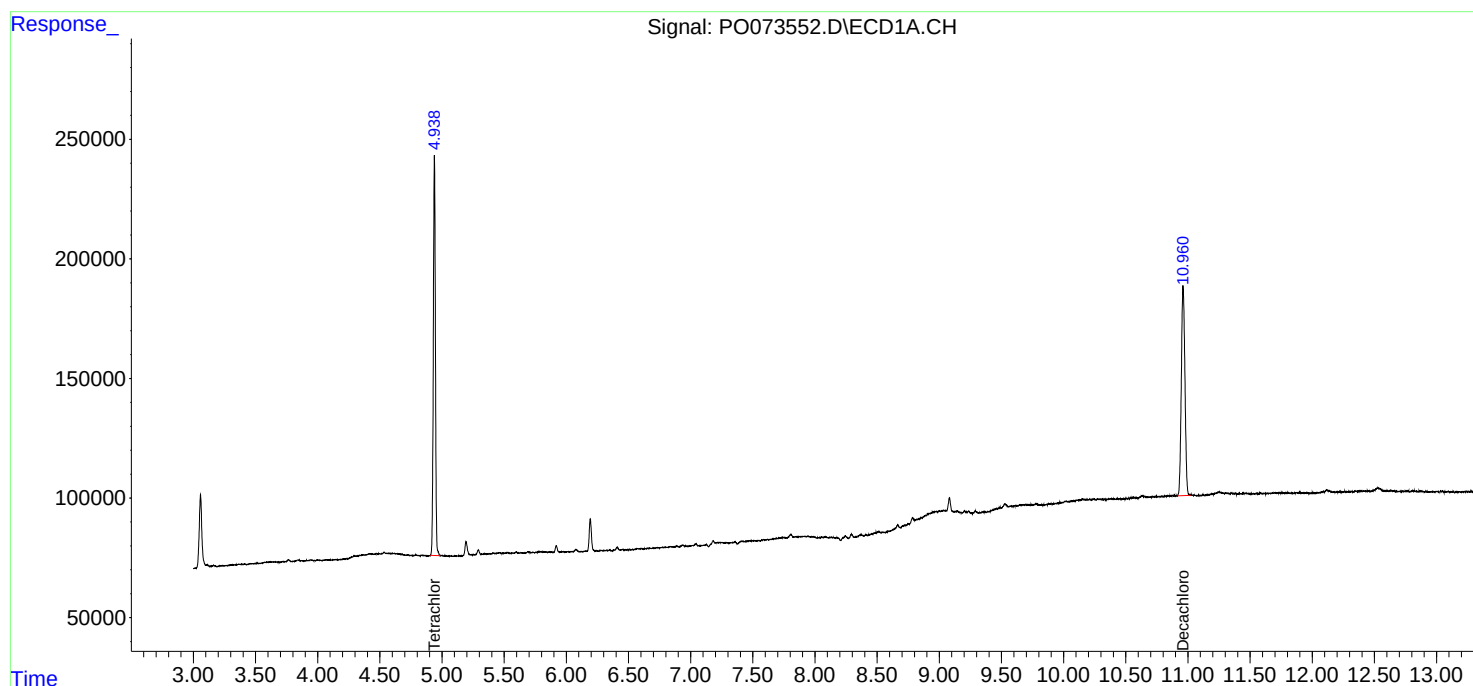


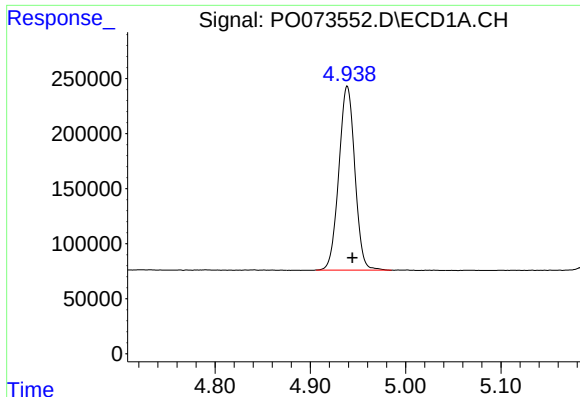

#1 Tetrachloro-m-xylene


R.T.: 4.939 min
Delta R.T.: -0.005 min
Response: 1947599
Conc: 23.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-48(8.0-8.5)

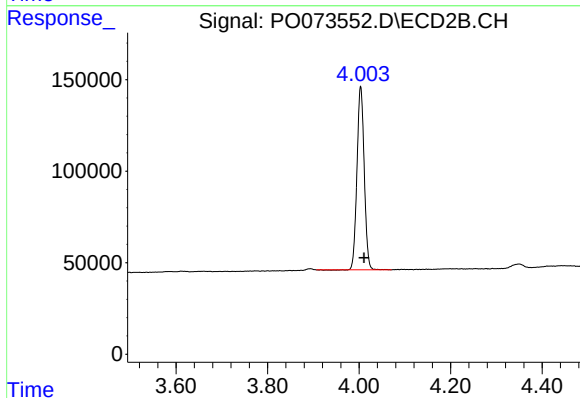


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.008 min
Response: 1099292
Conc: 22.42 ng/ml

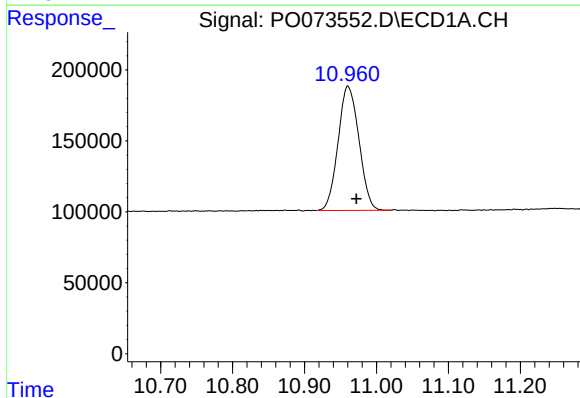

#2 Decachlorobiphenyl

R.T.: 10.960 min
Delta R.T.: -0.012 min
Response: 1764431
Conc: 21.40 ng/ml

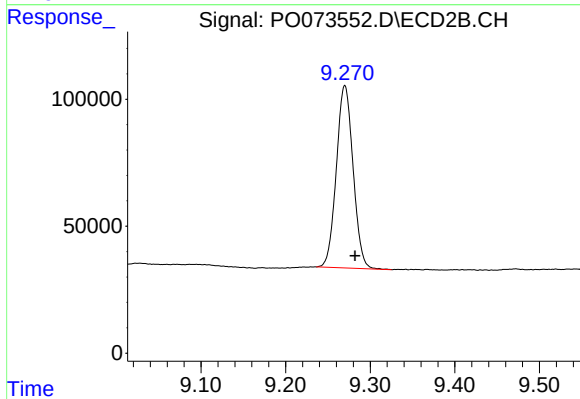

#2 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: -0.012 min
Response: 986850
Conc: 21.52 ng/ml