

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
 Data File : PO073573.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 18:11
 Operator : DD\AJ
 Sample : L4597-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BU-03-112320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:14:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.941	4.005	2051829	1281798	24.529	26.144
2) SA Decachlor...	10.964	9.271	1824475	1018223	22.128	22.207

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
Data File : PO073573.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 18:11
Operator : DD\AJ
Sample : L4597-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BU-03-112320

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:14:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

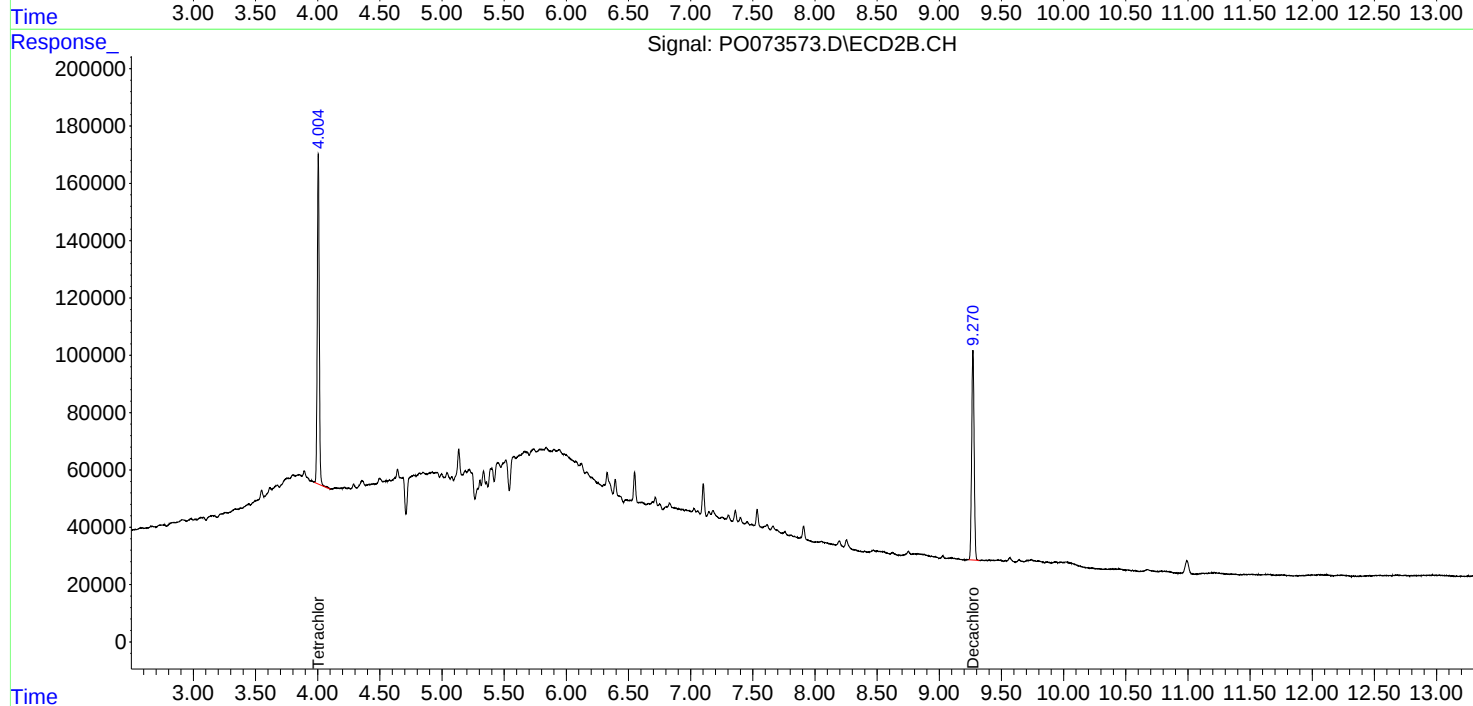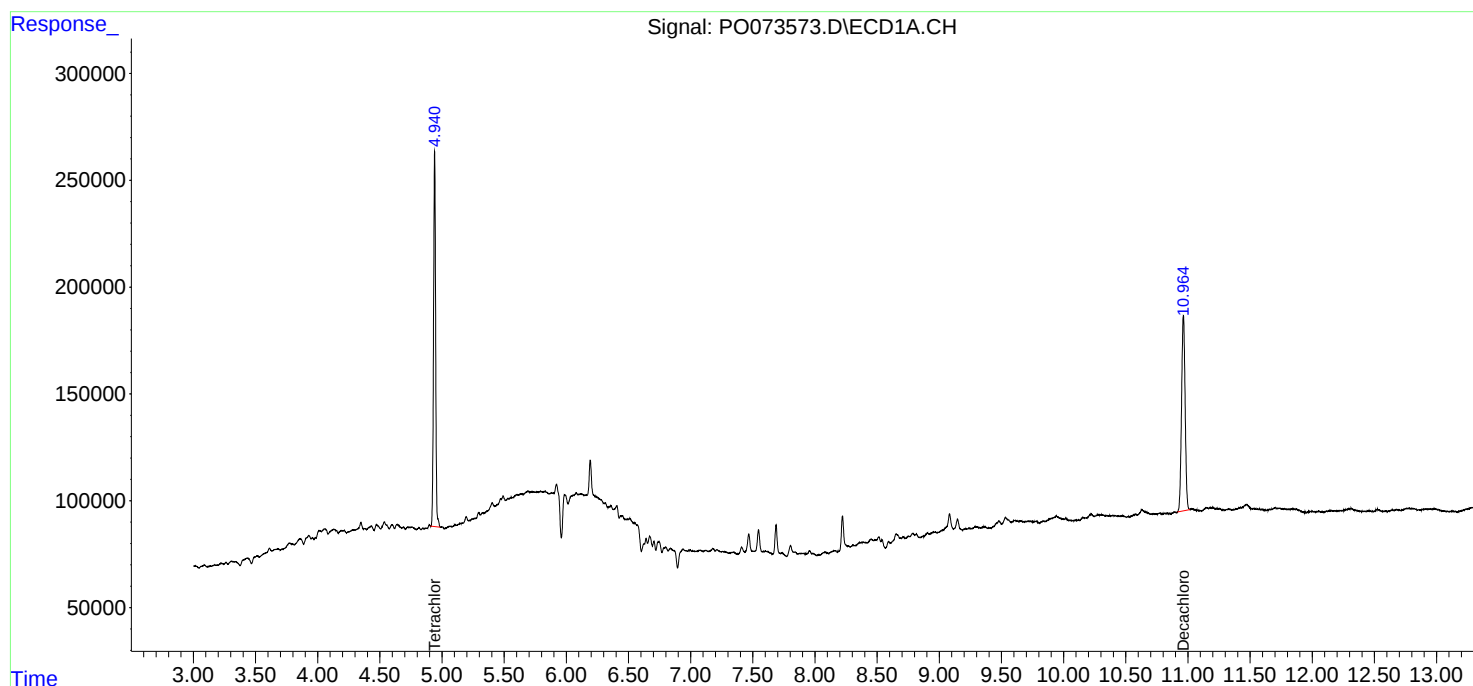


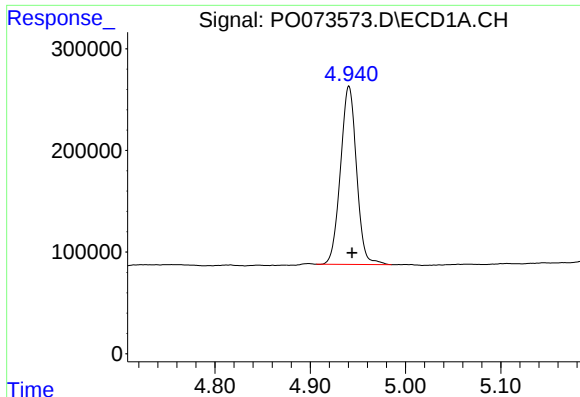

#1 Tetrachloro-m-xylene


R.T.: 4.941 min
Delta R.T.: -0.003 min
Response: 2051829
Conc: 24.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
BU-03-112320

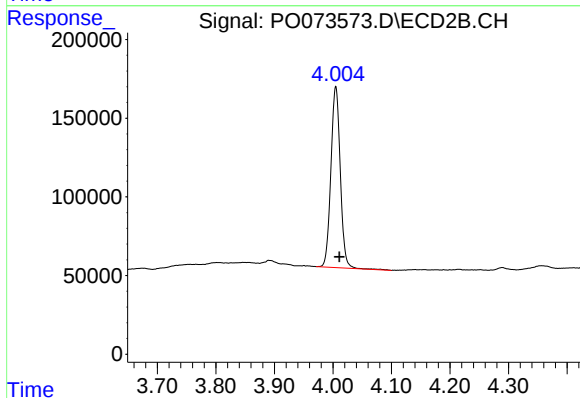


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.006 min
Response: 1281798
Conc: 26.14 ng/ml

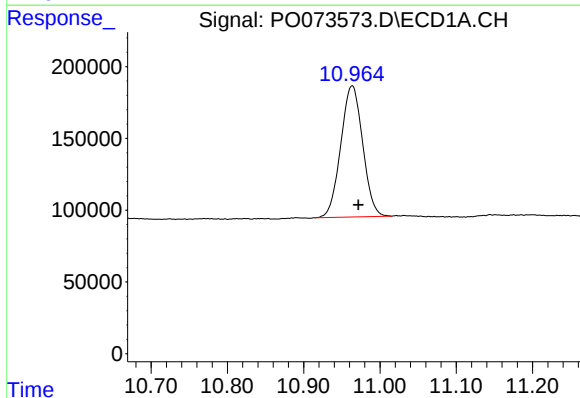

#2 Decachlorobiphenyl

R.T.: 10.964 min
Delta R.T.: -0.008 min
Response: 1824475
Conc: 22.13 ng/ml

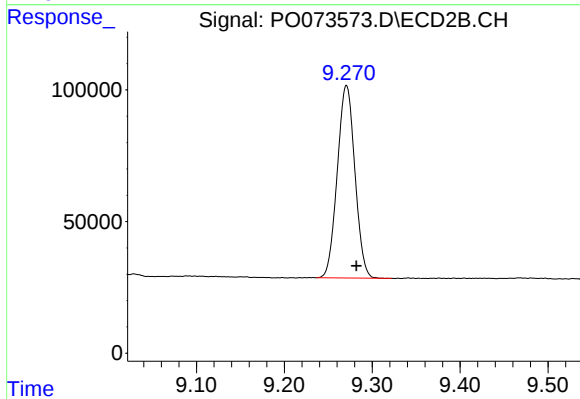

#2 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: -0.011 min
Response: 1018223
Conc: 22.21 ng/ml