

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112520\
 Data File : P0073574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 18:28
 Operator : DD\AJ
 Sample : L4871-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 32783

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:57:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:15:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.953	4.025	1600876	1111761	19.138m	22.676
2) SA Decachlor...	10.966	9.272	1724685	972784	20.918	21.216

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
Data File : PO073574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 18:28
Operator : DD\AJ
Sample : L4871-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
32783


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:15:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

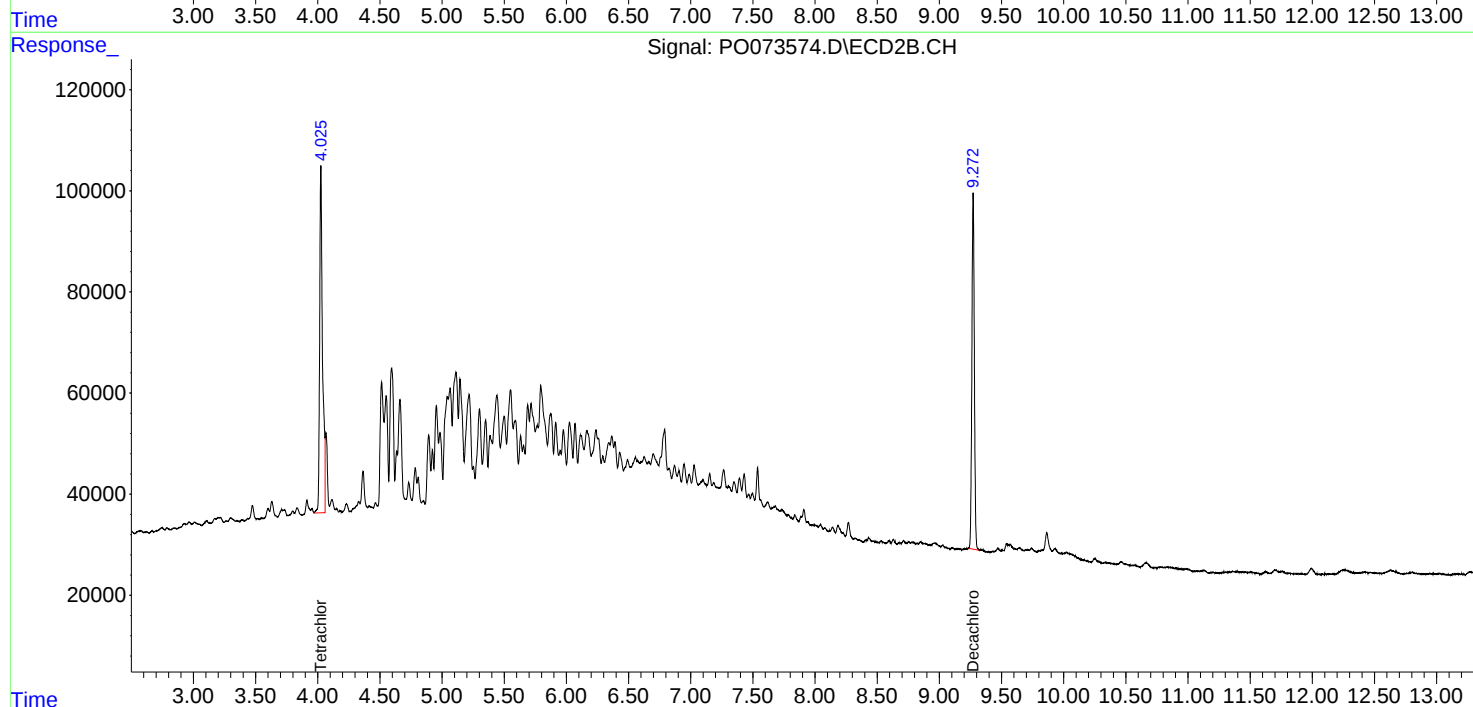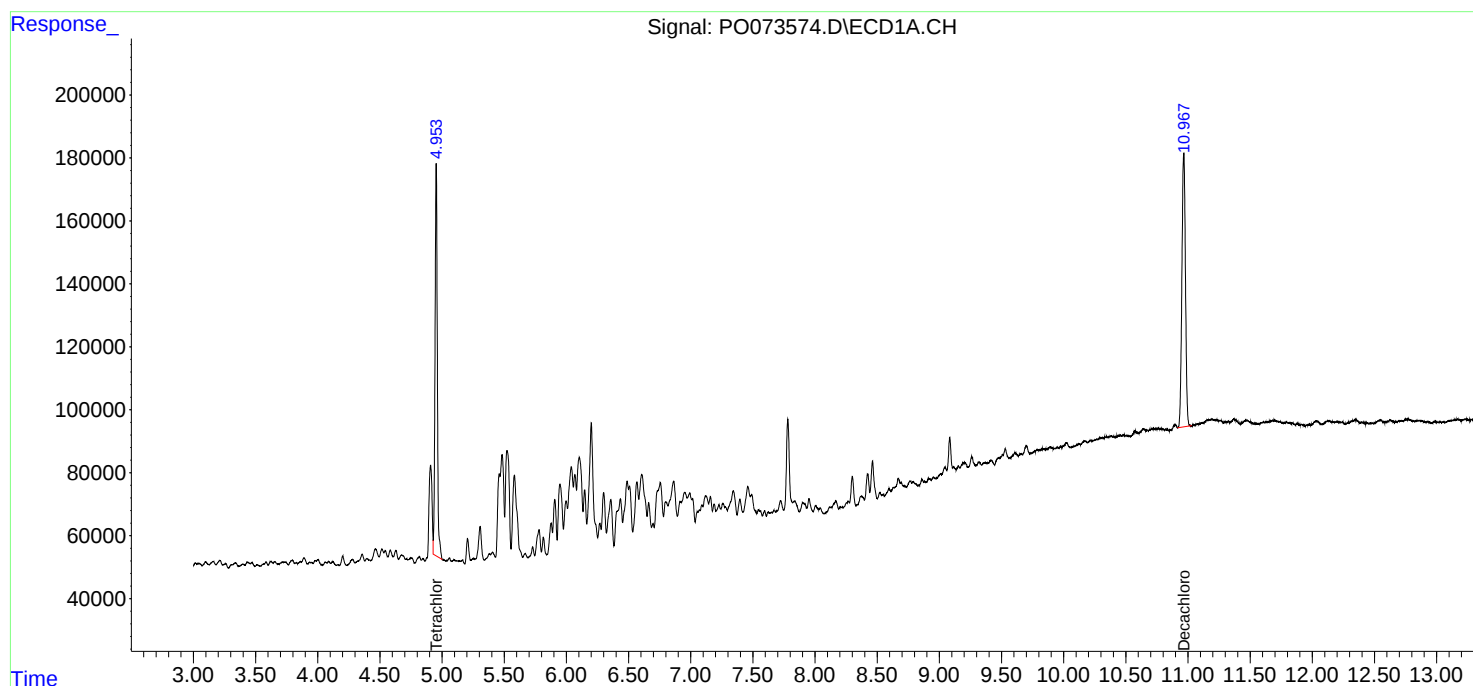

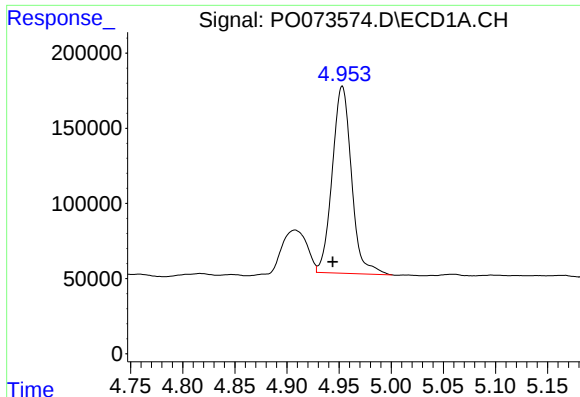


#1 Tetrachloro-m-xylene

R.T.: 4.953 min
Delta R.T.: 0.009 min
Response: 1600876
Conc: 19.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
32783


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:45 PM

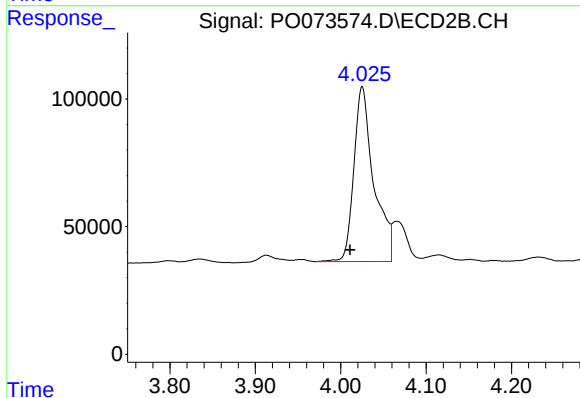


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.014 min
Response: 1111761
Conc: 22.68 ng/ml

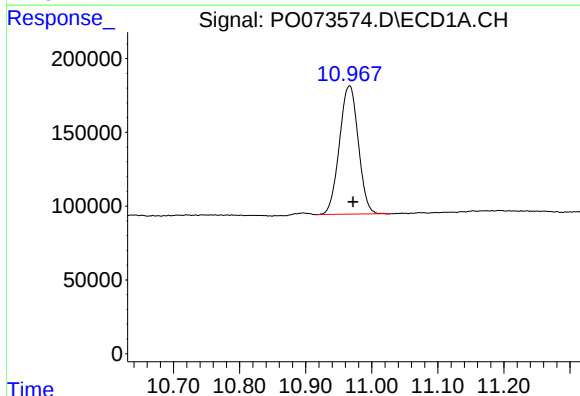

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: -0.006 min
Response: 1724685
Conc: 20.92 ng/ml

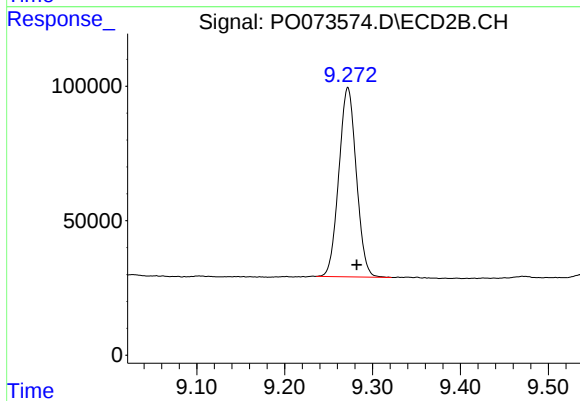

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: -0.010 min
Response: 972784
Conc: 21.22 ng/ml