

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
 Data File : PO073584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 21:36
 Operator : DD\AJ
 Sample : L4873-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-01-112320

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:57:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:22:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.940	4.006	1657256	1076226	19.812m	21.951
2) SA Decachlor...	10.966	9.273	1715100	966923	20.801	21.089

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
Data File : PO073584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 21:36
Operator : DD\AJ
Sample : L4873-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-01-112320


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:22:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

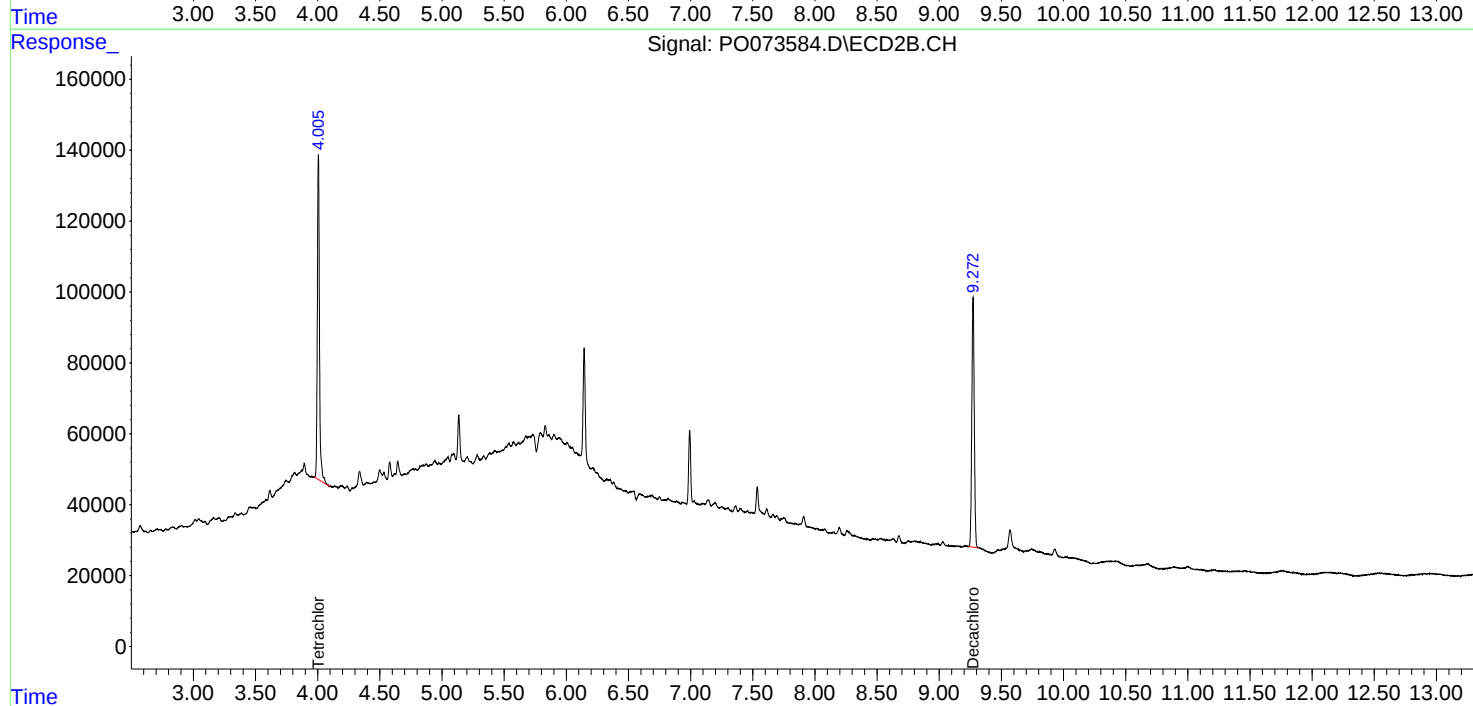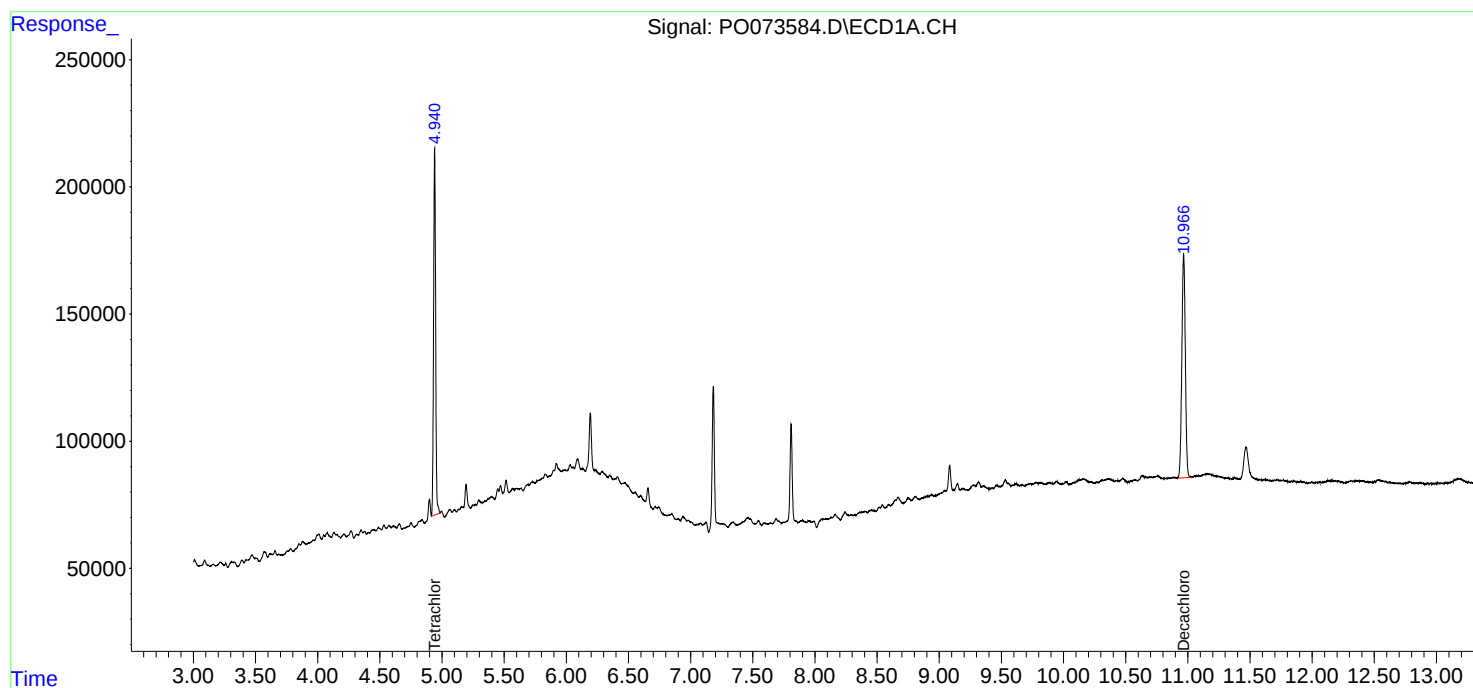

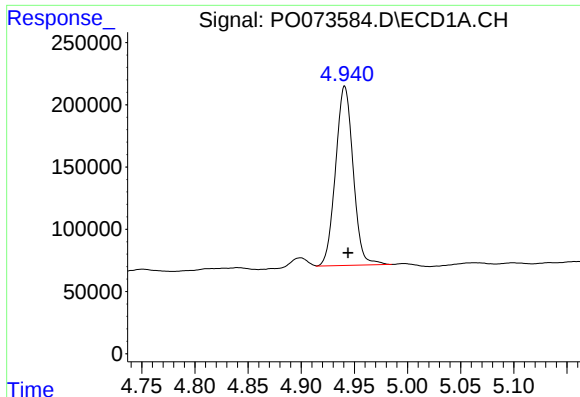


#1 Tetrachloro-m-xylene

R.T.: 4.940 min
Delta R.T.: -0.004 min
Response: 1657256
Conc: 19.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HR-01-112320


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:55 PM

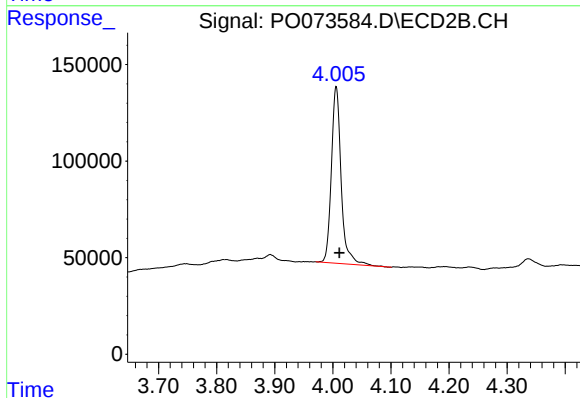


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.005 min
Response: 1076226
Conc: 21.95 ng/ml

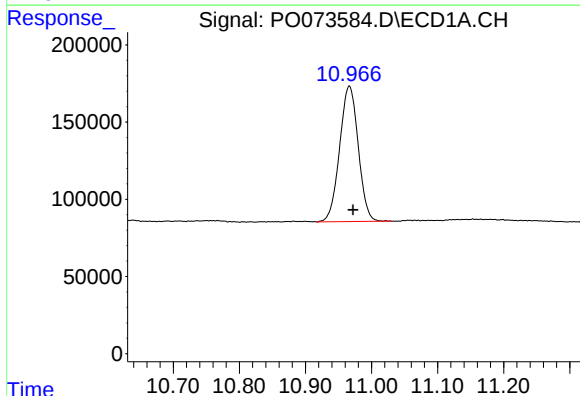

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: -0.006 min
Response: 1715100
Conc: 20.80 ng/ml

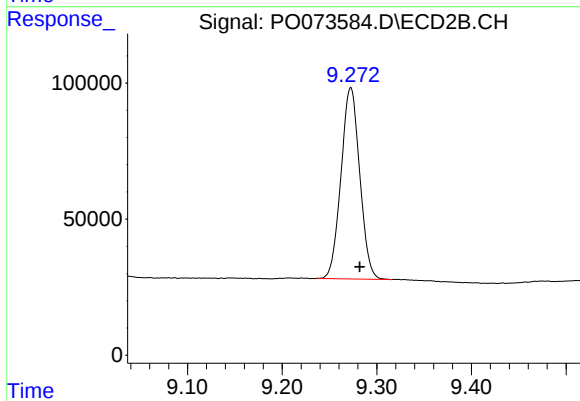

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.010 min
Response: 966923
Conc: 21.09 ng/ml