

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
 Data File : PO073585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 21:53
 Operator : DD\AJ
 Sample : L4875-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-08-112320

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:57:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:23:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	4.006	1580993	1039689	18.900	21.206m
2) SA Decachlor...	10.967	9.273	1355291	778277	16.438	16.974

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
Data File : PO073585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 21:53
Operator : DD\AJ
Sample : L4875-01
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-08-112320


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:23:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

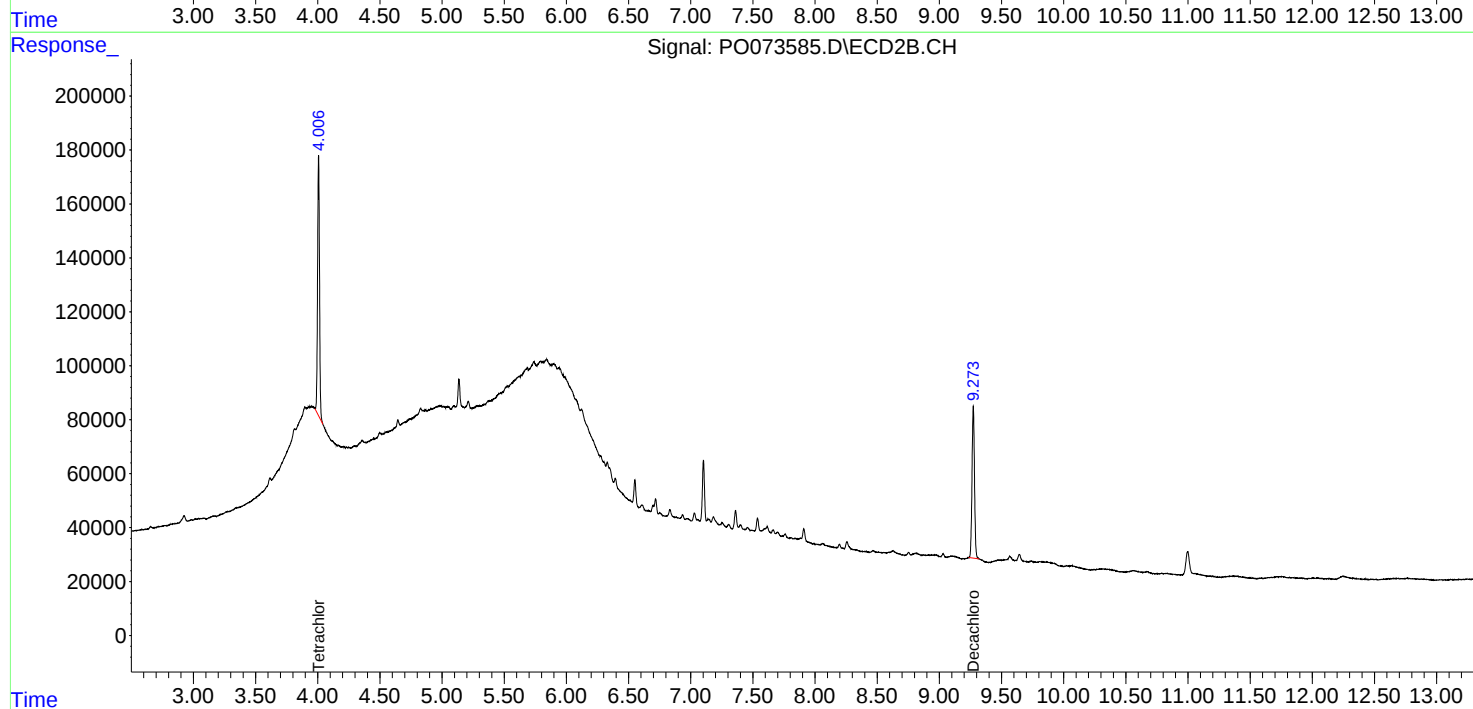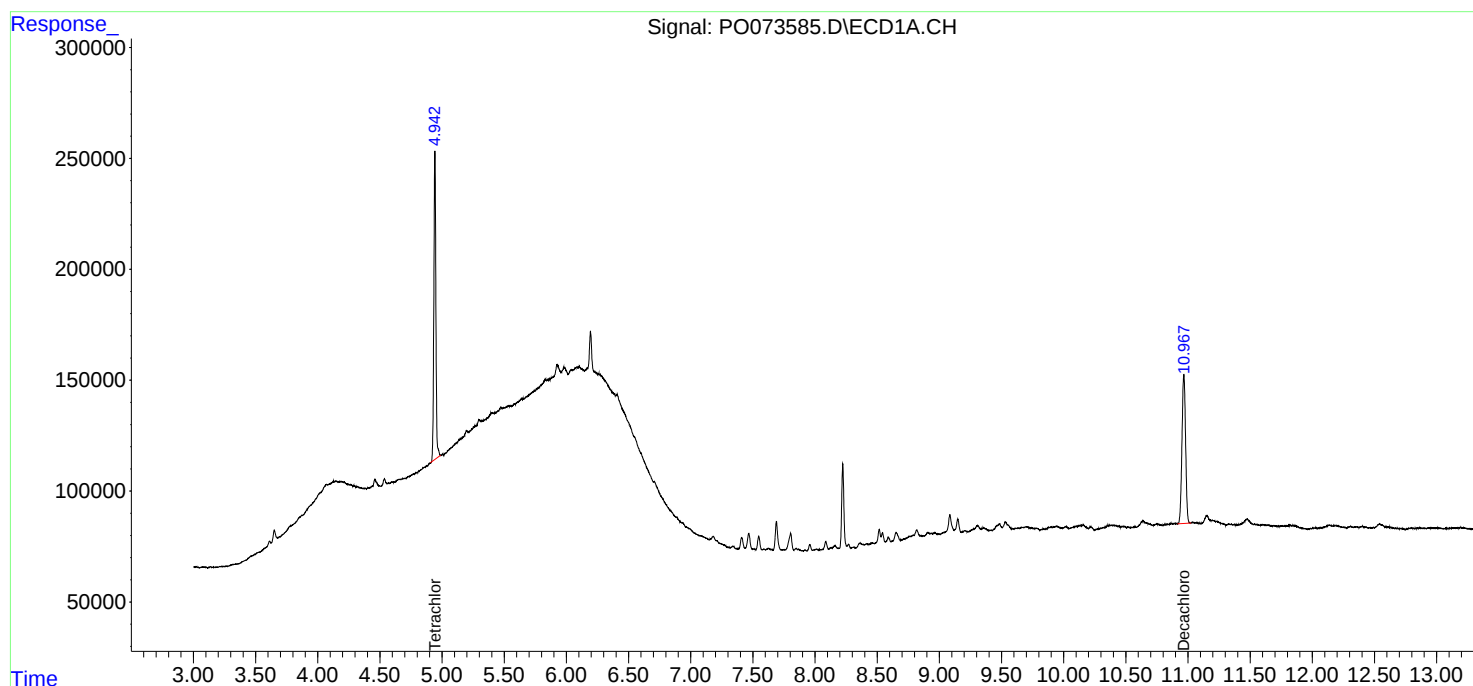

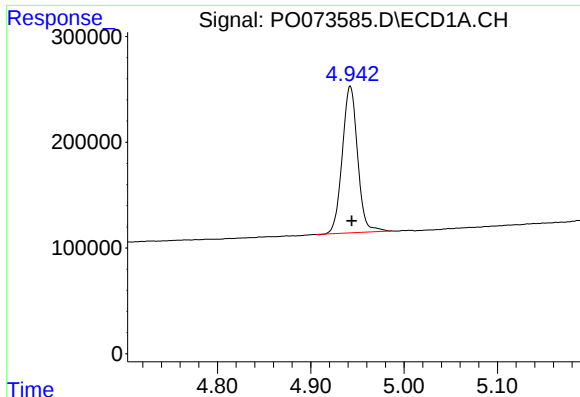


#1 Tetrachloro-m-xylene

R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 1580993
Conc: 18.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-08-112320


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:56 PM

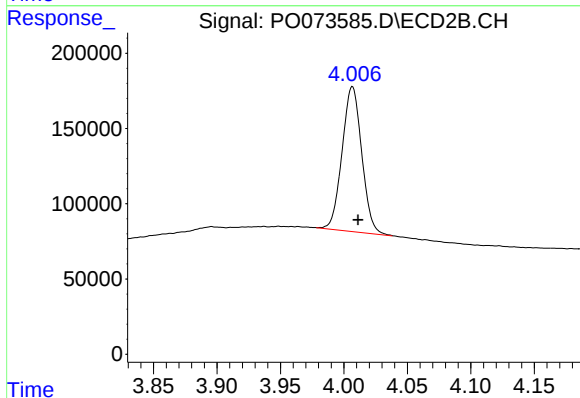


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.005 min
Response: 1039689
Conc: 21.21 ng/ml m

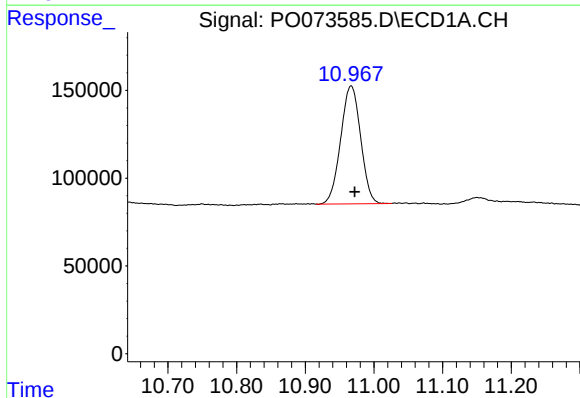

#2 Decachlorobiphenyl

R.T.: 10.967 min
Delta R.T.: -0.005 min
Response: 1355291
Conc: 16.44 ng/ml

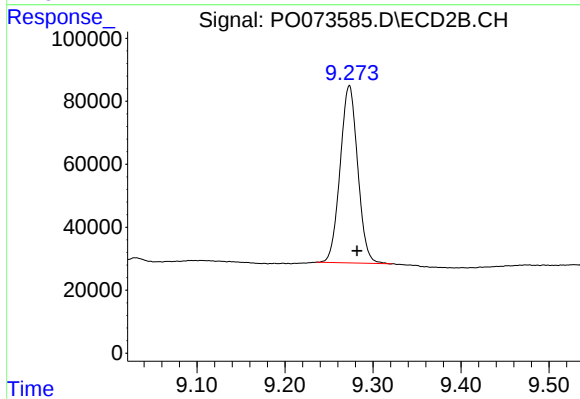

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: -0.009 min
Response: 778277
Conc: 16.97 ng/ml