

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
 Data File : PO073587.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Nov 2020 22:27
 Operator : DD\AJ
 Sample : L4886-01 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC248138-END-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:24:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 25 10:04:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.943	4.008	324924	232455	3.884	4.741
2) SA Decachlor...	10.969	9.276	264039	177912	3.202	3.880

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112520\
Data File : PO073587.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Nov 2020 22:27
Operator : DD\AJ
Sample : L4886-01 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC248138-END-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:24:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 25 10:04:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

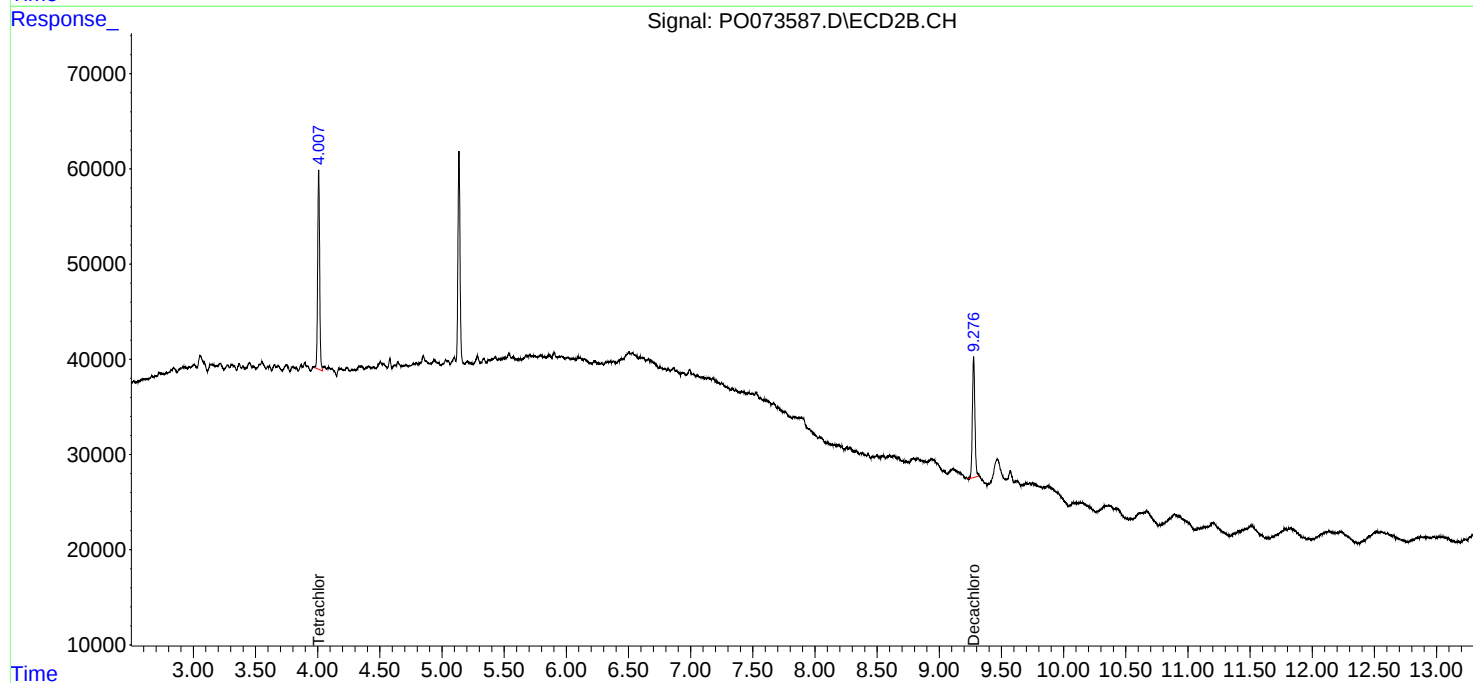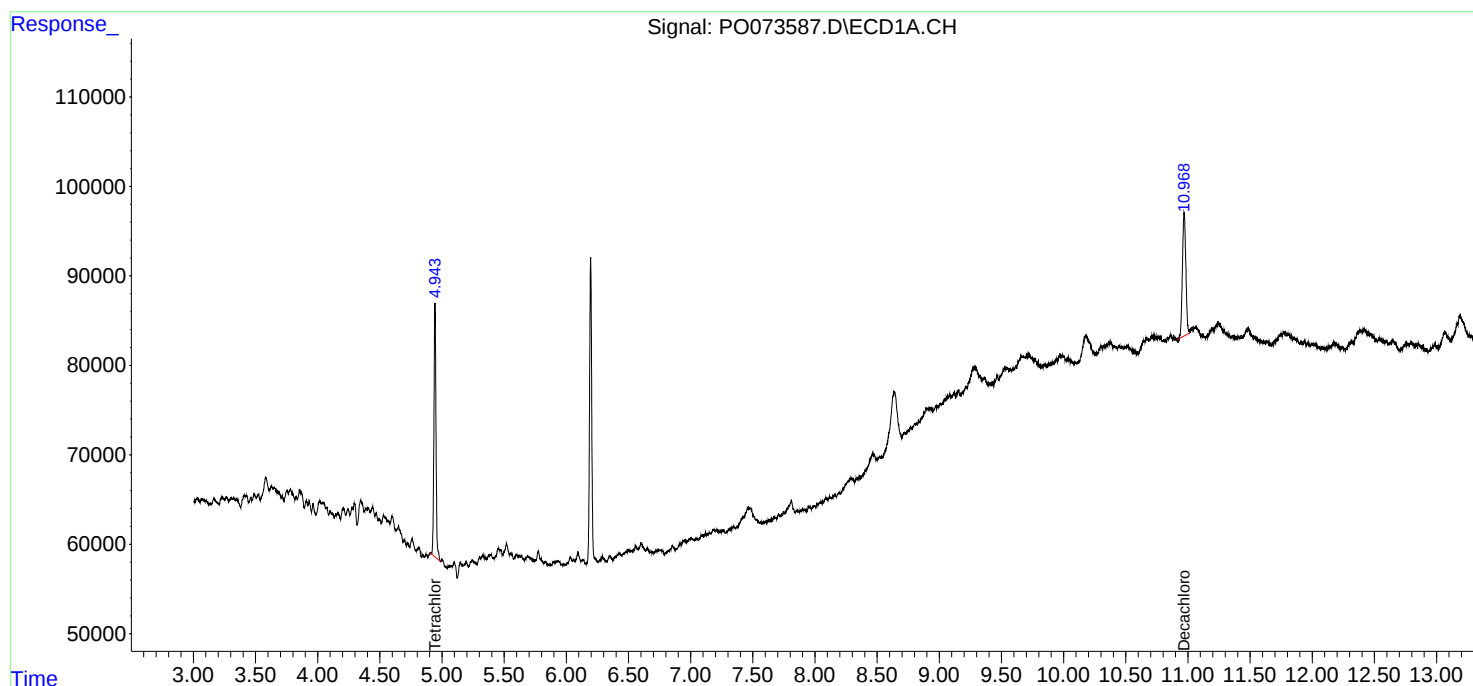


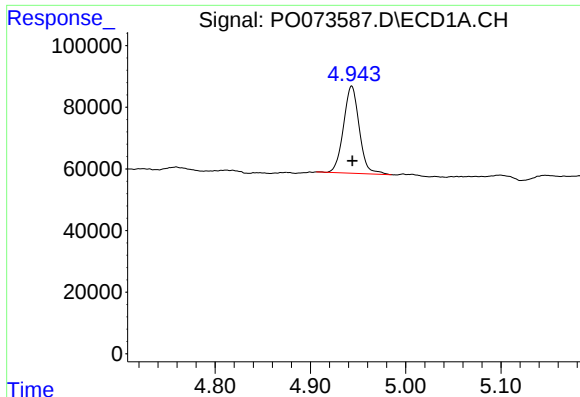

#1 Tetrachloro-m-xylene


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 324924
Conc: 3.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC248138-END-1

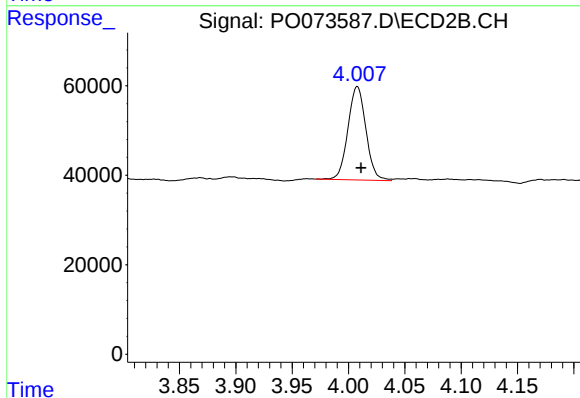


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.003 min
Response: 232455
Conc: 4.74 ng/ml

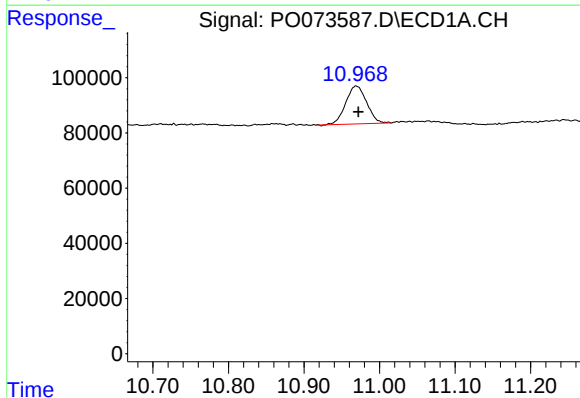

#2 Decachlorobiphenyl

R.T.: 10.969 min
Delta R.T.: -0.003 min
Response: 264039
Conc: 3.20 ng/ml

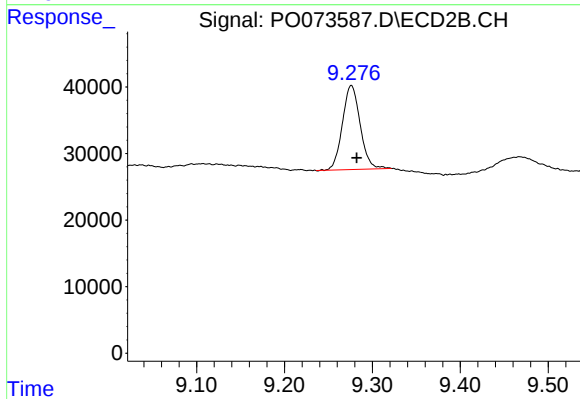

#2 Decachlorobiphenyl

R.T.: 9.276 min
Delta R.T.: -0.006 min
Response: 177912
Conc: 3.88 ng/ml