

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112525\
 Data File : PO115394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 11:17
 Operator : YP/AJ
 Sample : Q3707-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 V933

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/26/2025
 Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:35:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.642	183.9E6	114.9E6	26.129	25.713
2) SA Decachlor...	9.914	8.626	110.0E6	95646336	24.880m	24.501

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112525\
Data File : PO115394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 11:17
Operator : YP/AJ
Sample : Q3707-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
V933


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:35:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

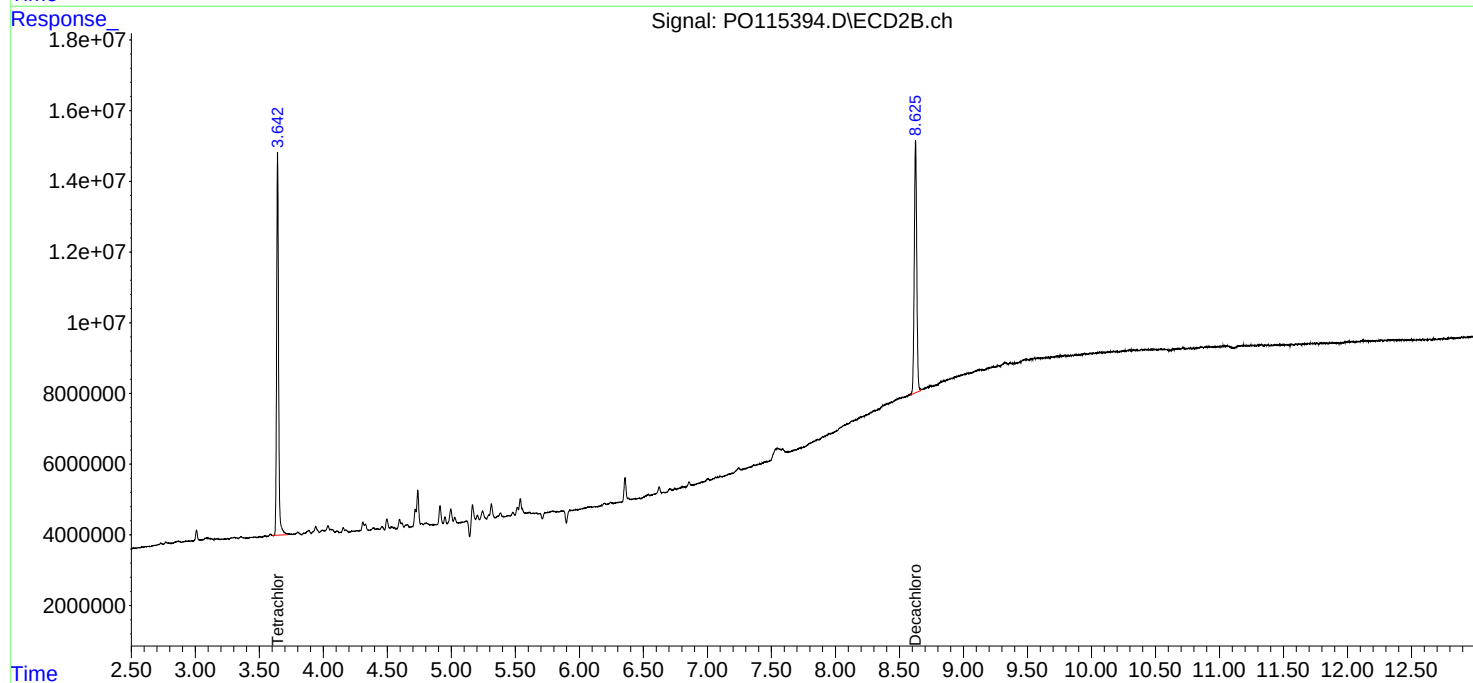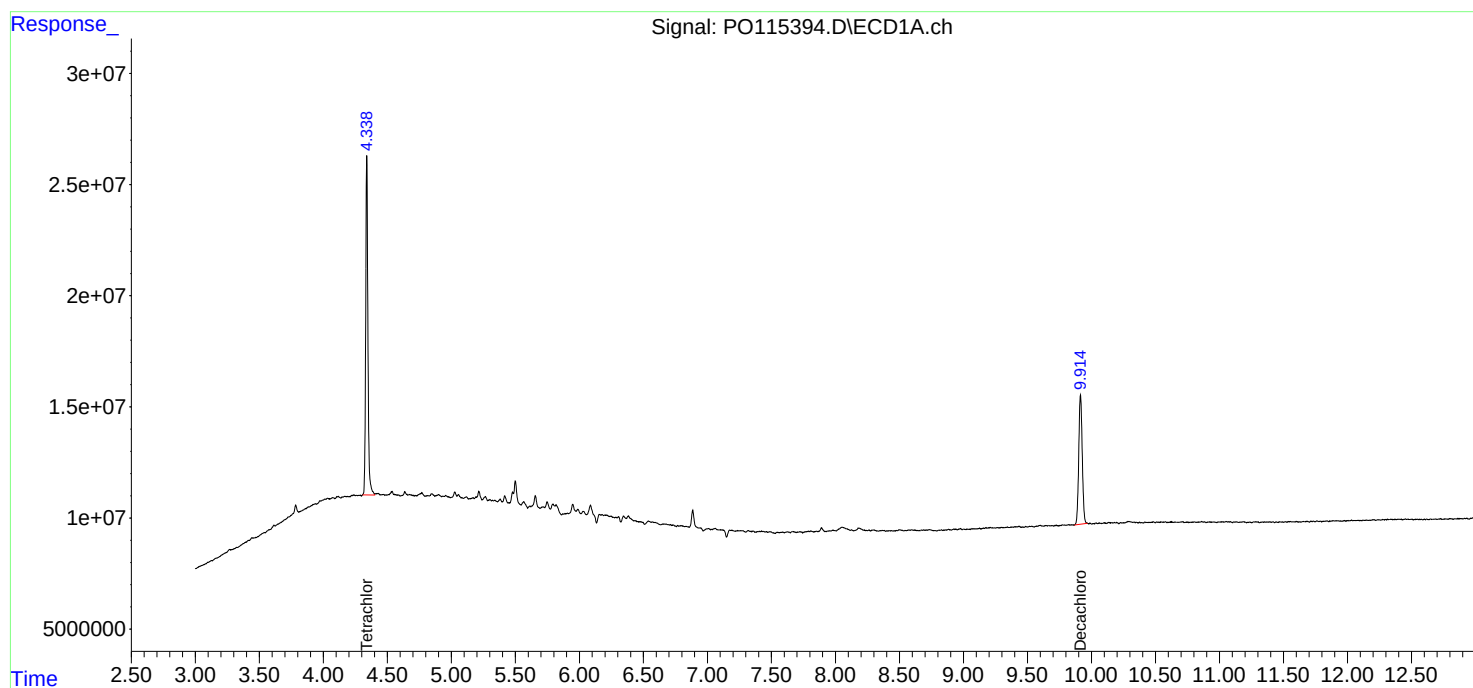

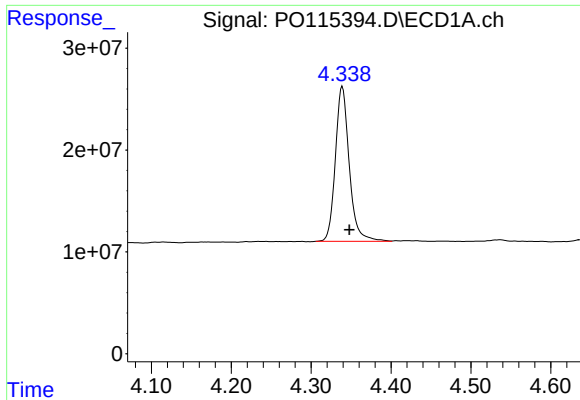


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.009 min
Response: 183901703
Conc: 26.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
V933


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

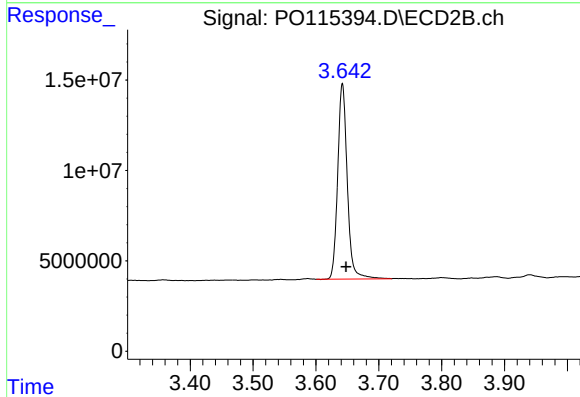


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.006 min
Response: 114855613
Conc: 25.71 ng/ml

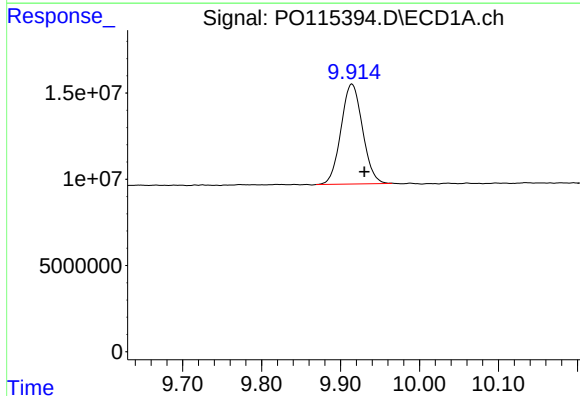

#2 Decachlorobiphenyl

R.T.: 9.914 min
Delta R.T.: -0.016 min
Response: 109977810
Conc: 24.88 ng/ml m

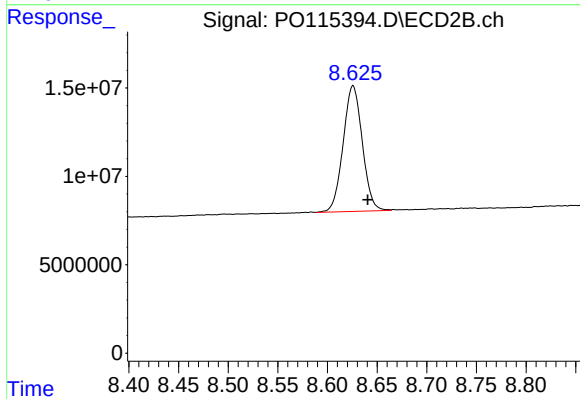

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.015 min
Response: 95646336
Conc: 24.50 ng/ml