

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112525\
 Data File : P0115395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 11:35
 Operator : YP/AJ
 Sample : Q3709-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LI-1-112125

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/26/2025
 Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 03:53:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.642	164.1E6	106.3E6	23.309	23.802
2) SA Decachlor...	9.912	8.625	84804017	73860259	19.185m	18.920

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO112525\
Data File : PO115395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 11:35
Operator : YP/AJ
Sample : Q3709-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LI-1-112125


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 03:53:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

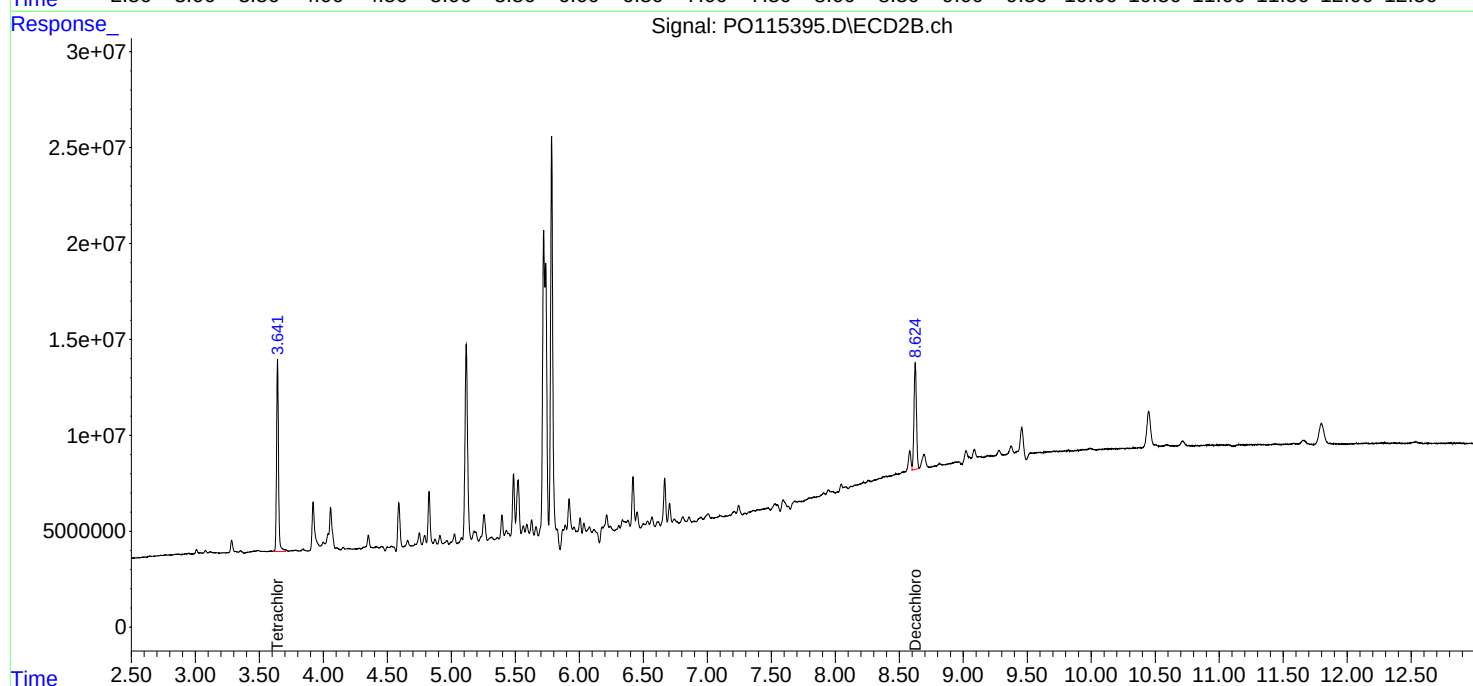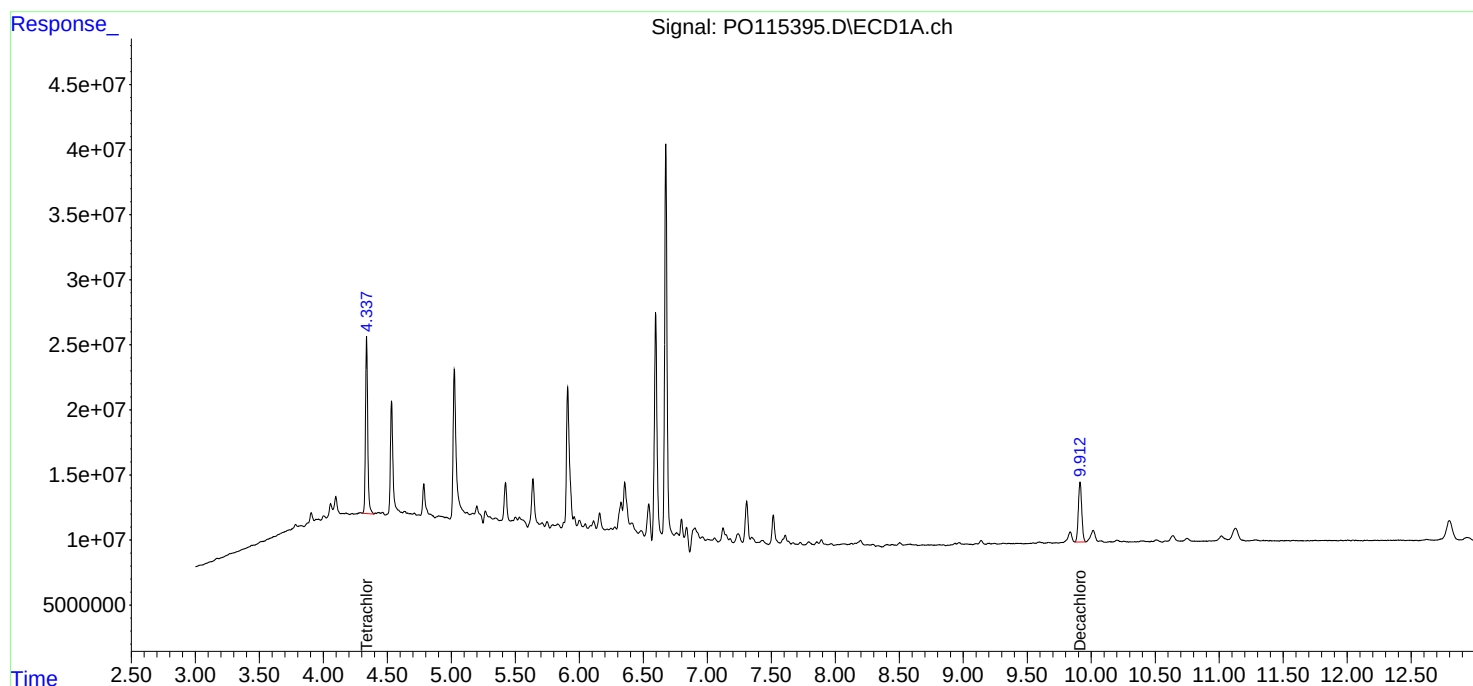

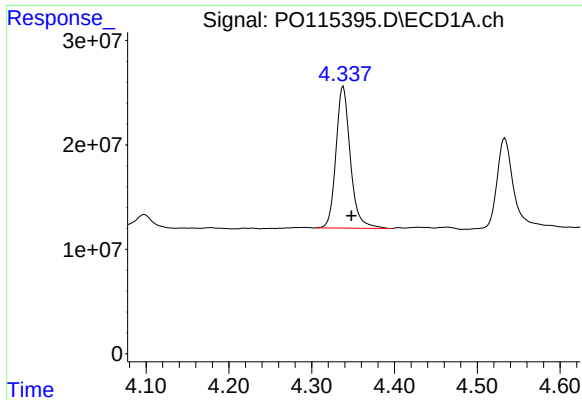


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.010 min
Response: 164051536
Conc: 23.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LI-1-112125


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

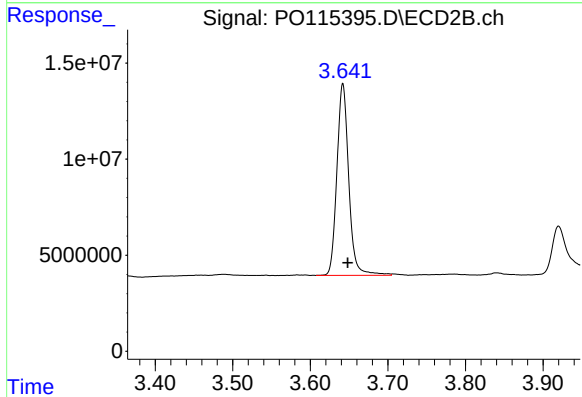


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.006 min
Response: 106320034
Conc: 23.80 ng/ml

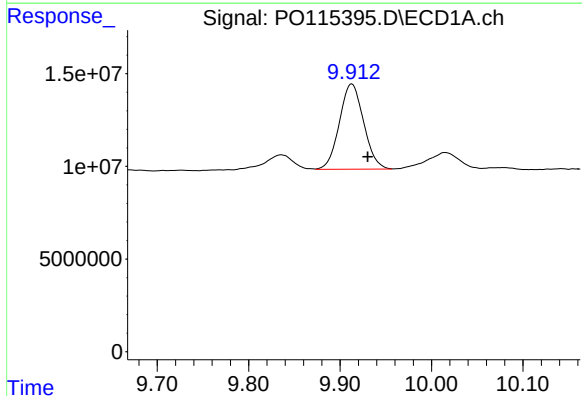

#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.018 min
Response: 84804017
Conc: 19.19 ng/ml m

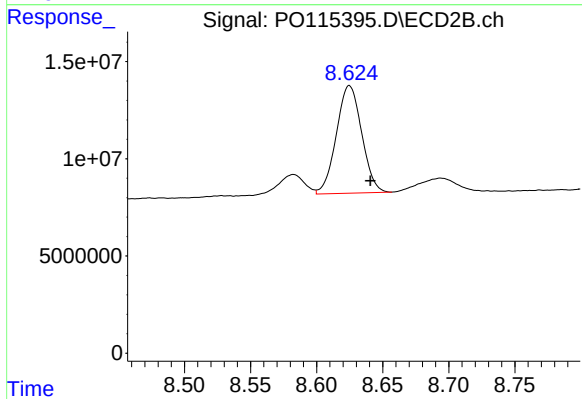

#2 Decachlorobiphenyl

R.T.: 8.625 min
Delta R.T.: -0.016 min
Response: 73860259
Conc: 18.92 ng/ml