

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112618\
 Data File : P0051812.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2018 5:54
 Operator : SM/SJ
 Sample : J6061-08
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112018-CHDE-E-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 07:21:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.307	3.313	20147982	5326299	30.885	22.559 #
2)	SA Decachlor...	9.920	8.032	9861889	4738105	23.650	23.948

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112618\
Data File : PO051812.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2018 5:54
Operator : SM/SJ
Sample : J6061-08
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
112018-CHDE-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 07:21:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

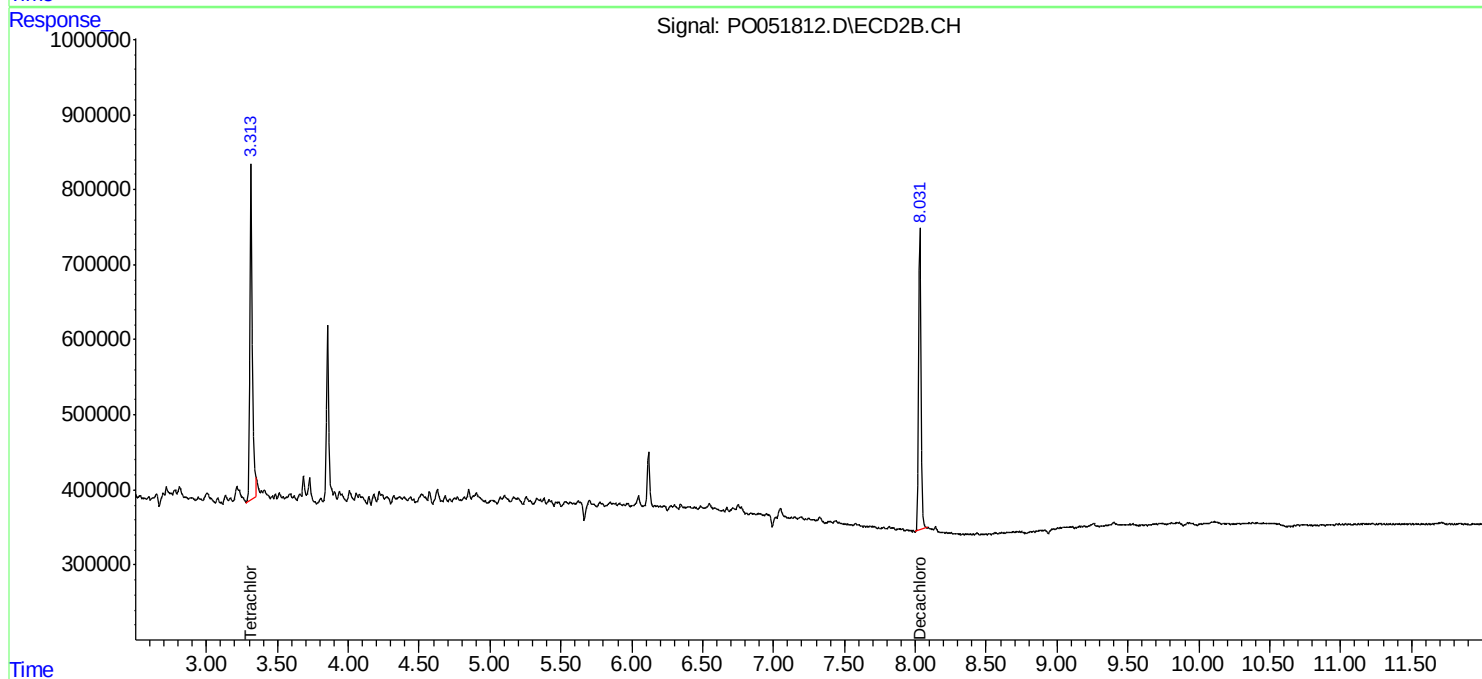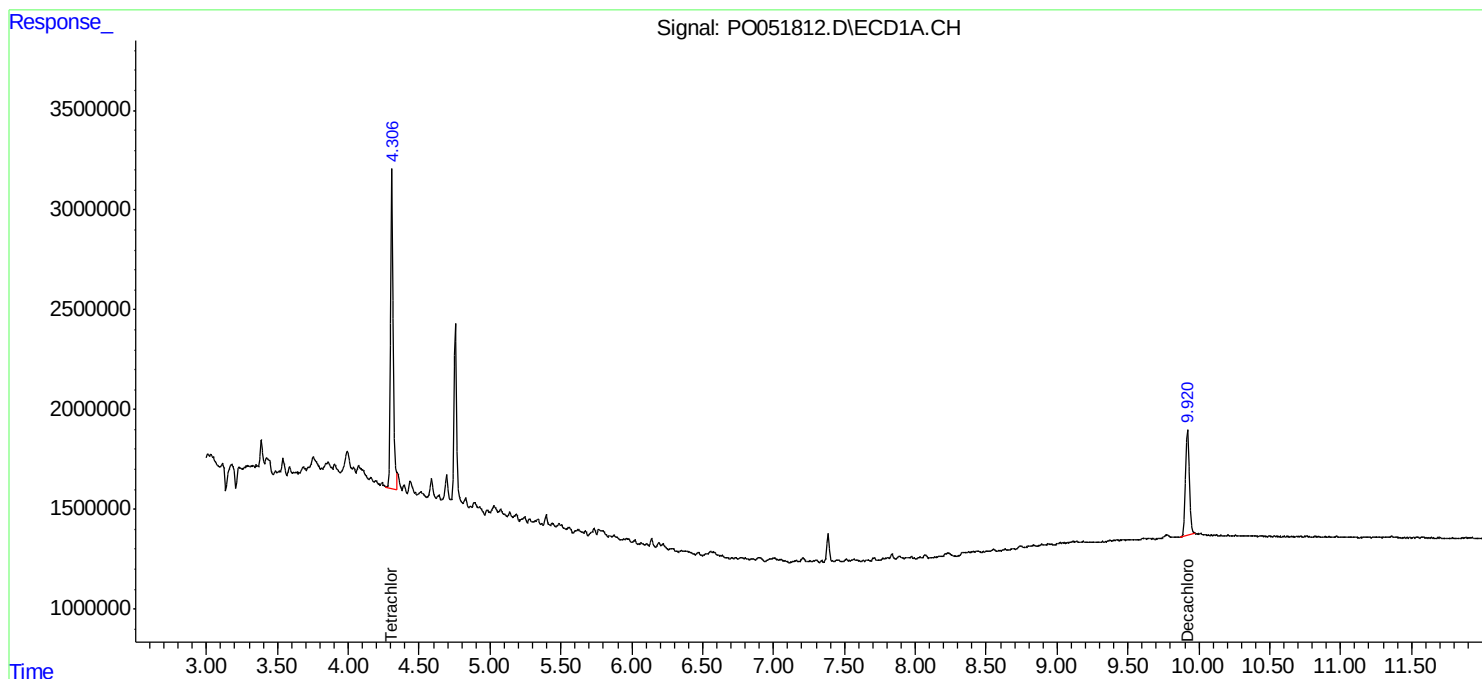


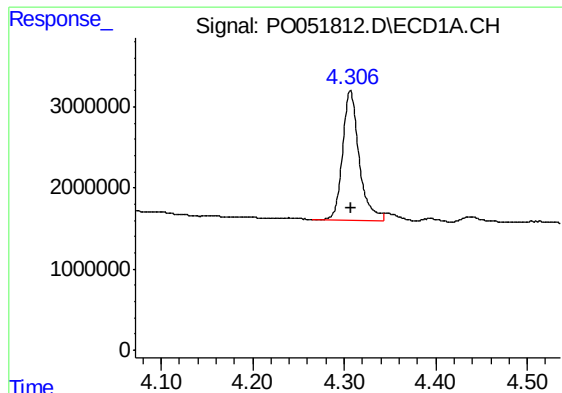

#1 Tetrachloro-m-xylene


R.T.: 4.307 min
Delta R.T.: -0.001 min
Response: 20147982
Conc: 30.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
112018-CHDE-E-D-S

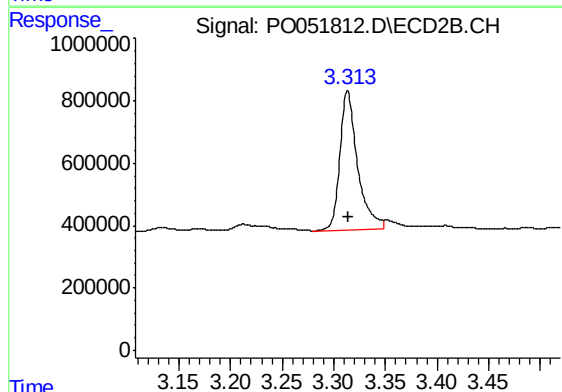


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 5326299
Conc: 22.56 ng/ml

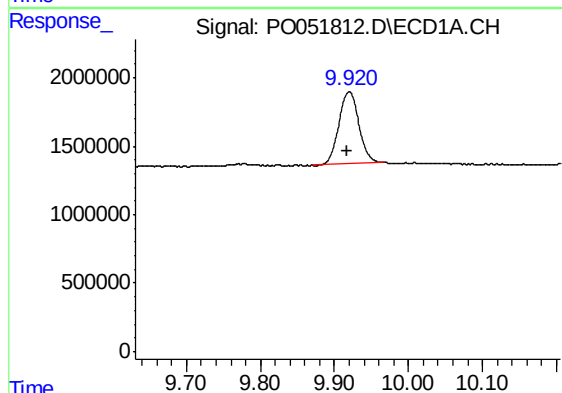

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: 0.003 min
Response: 9861889
Conc: 23.65 ng/ml

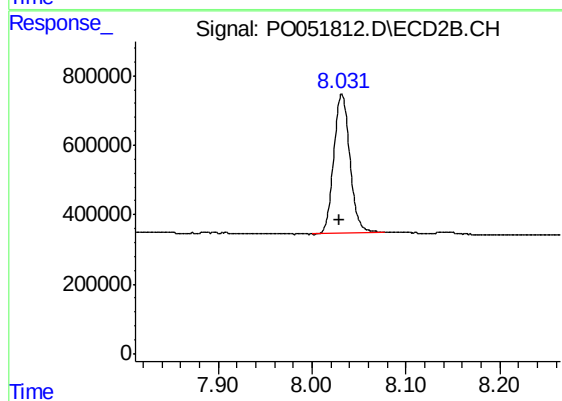

#2 Decachlorobiphenyl

R.T.: 8.032 min
Delta R.T.: 0.002 min
Response: 4738105
Conc: 23.95 ng/ml