

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112618\
 Data File : P0051818.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2018 7:36
 Operator : SM/SJ
 Sample : J6061-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112018-DBRI-E-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:06:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.313	18644005	4956815	28.579	20.995 #
2) SA Decachlor...	9.919	8.031	9287069	4565133	22.272	23.074

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112618\
Data File : PO051818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2018 7:36
Operator : SM/SJ
Sample : J6061-14
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
112018-DBRI-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:06:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

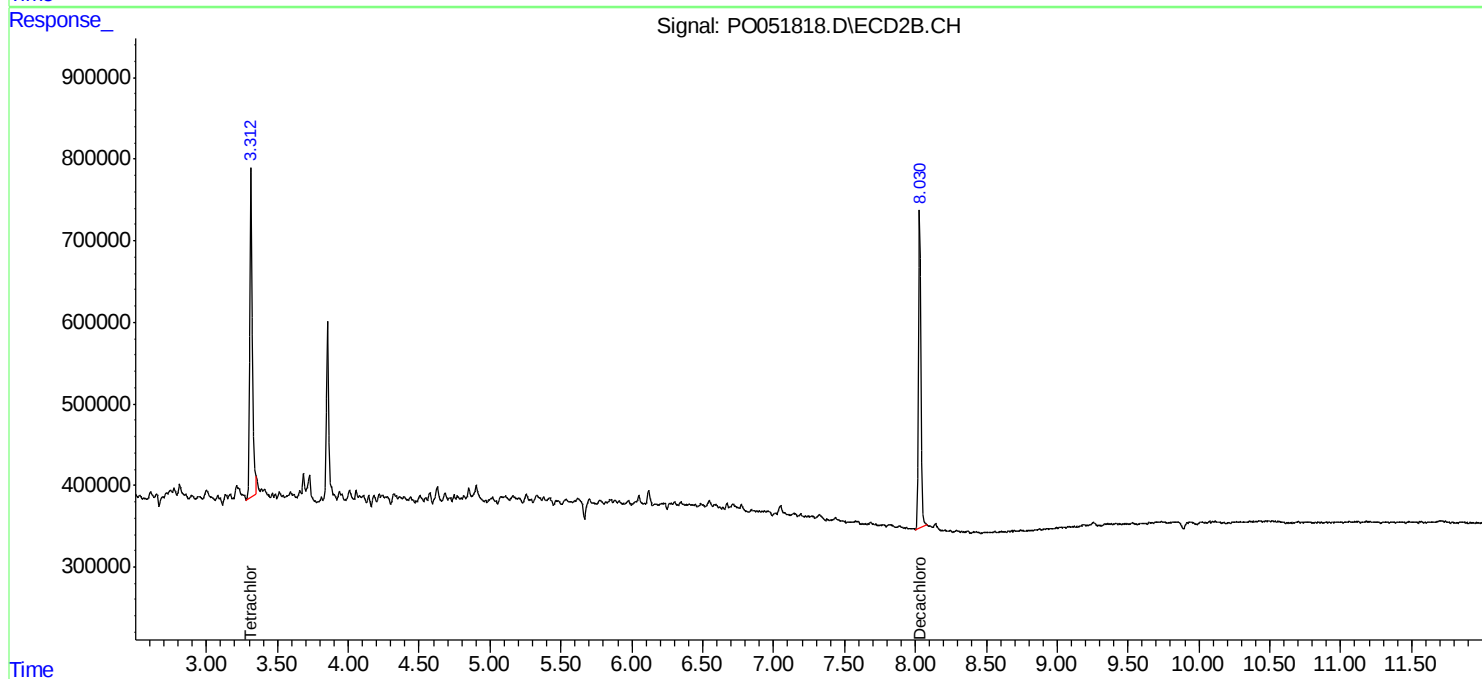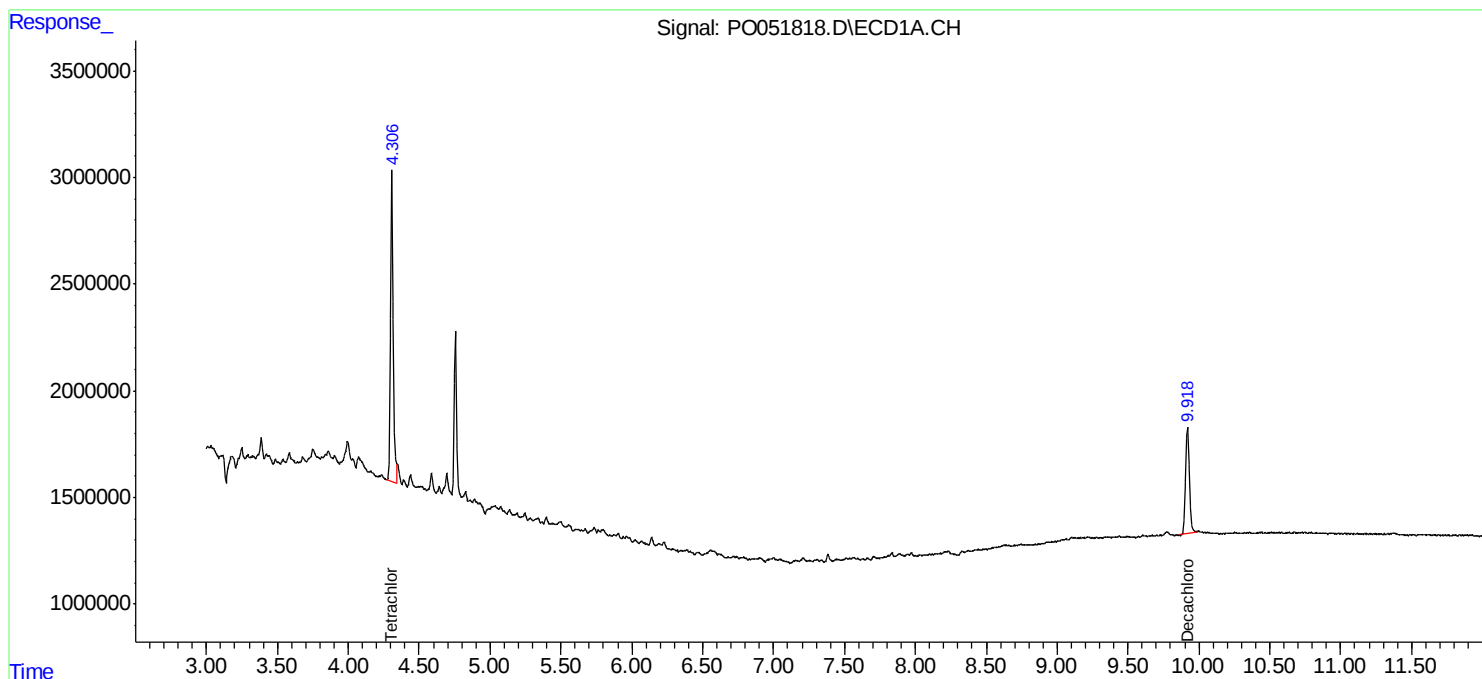


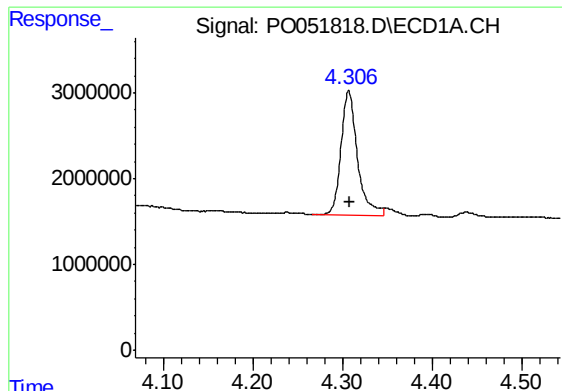

#1 Tetrachloro-m-xylene


R.T.: 4.307 min
Delta R.T.: -0.001 min
Response: 18644005
Conc: 28.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
112018-DBRI-E-D-S

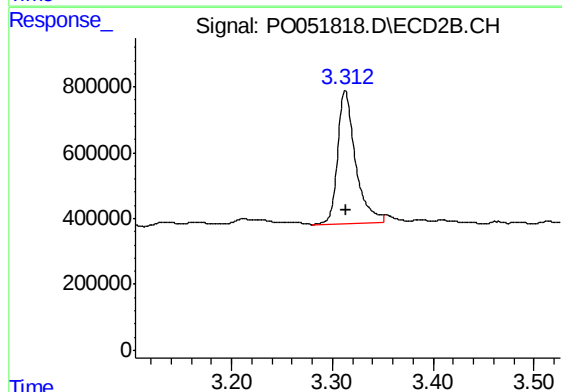


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.001 min
Response: 4956815
Conc: 20.99 ng/ml

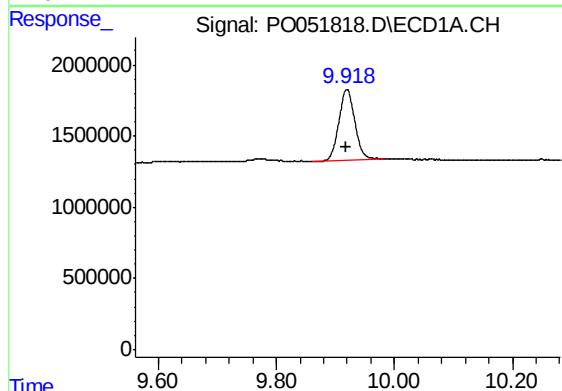

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: 0.001 min
Response: 9287069
Conc: 22.27 ng/ml

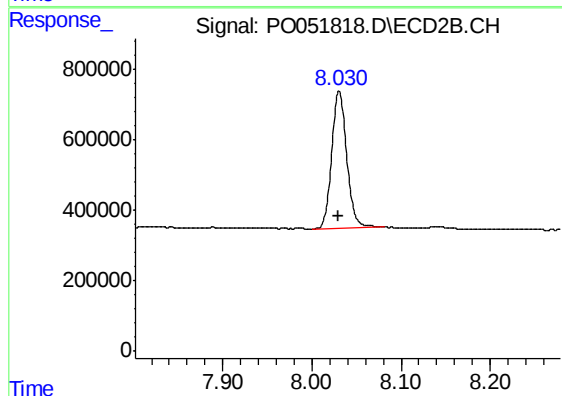

#2 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: 0.000 min
Response: 4565133
Conc: 23.07 ng/ml