

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112619\
 Data File : P0064150.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2019 1:56
 Operator : SM/AJ
 Sample : K6014-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 03:58:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.563	764189	582908	28.795	27.352
2)	SA Decachlor...	9.936	8.526	906240	837469	25.924	28.324
Target Compounds							
9)	L2 AR-1221-2	4.618	0.000	12409	0	46.480	N.D. #
10)	L2 AR-1221-3	4.618	0.000	12409	0	15.391	N.D. #
11)	L3 AR-1232-1	4.618	0.000	12409	0	10.022	N.D. #
28)	L6 AR-1254-3	6.914	0.000	16267	0	6.155	N.D. #
31)	L7 AR-1260-1	7.068	0.000	18765	0	10.645	N.D. #
32)	L7 AR-1260-2	7.389	0.000	13155	0	5.969	N.D. #
35)	L7 AR-1260-5	8.219	0.000	21731	0	5.130	N.D. #
37)	L8 AR-1262-2	8.219	0.000	21731	0	4.475	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : PO064150.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2019 1:56
Operator : SM/AJ
Sample : K6014-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CS-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 03:58:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

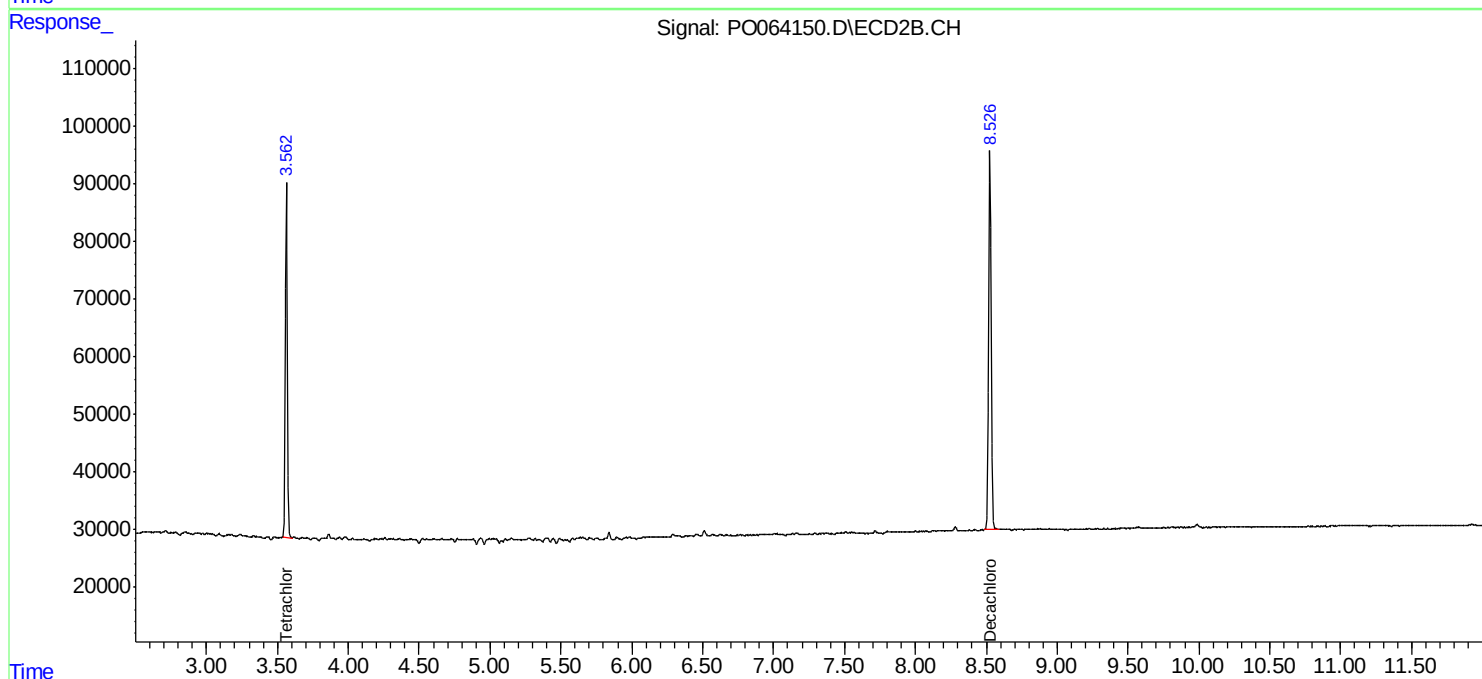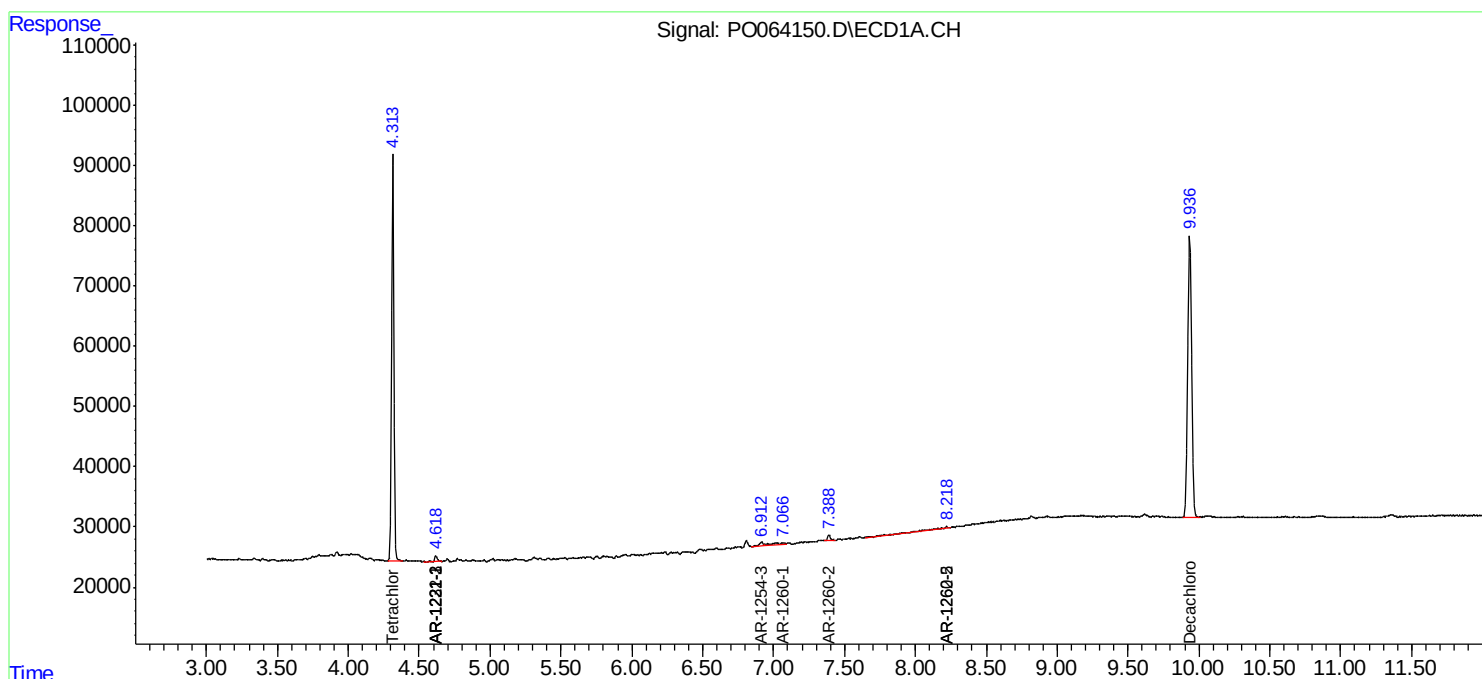


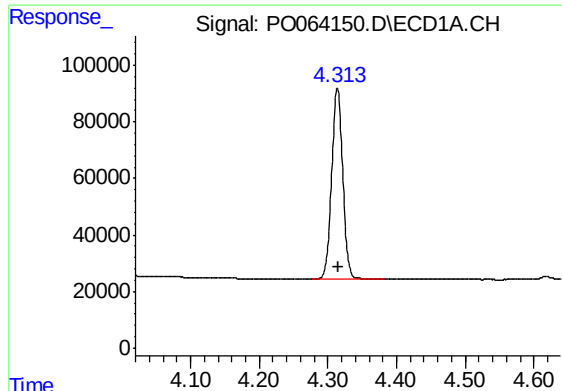

#1 Tetrachloro-m-xylene


R.T.: 4.314 min
Delta R.T.: -0.002 min
Response: 764189
Conc: 28.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-05

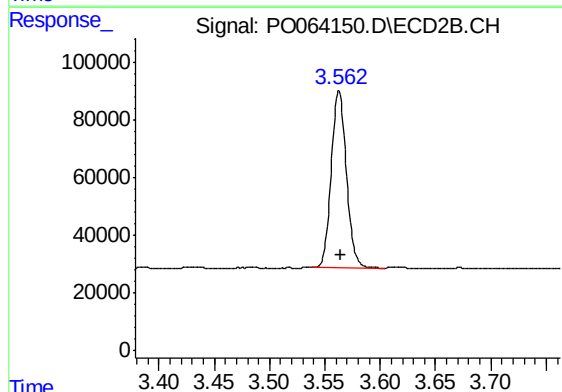


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.002 min
Response: 582908
Conc: 27.35 ng/ml

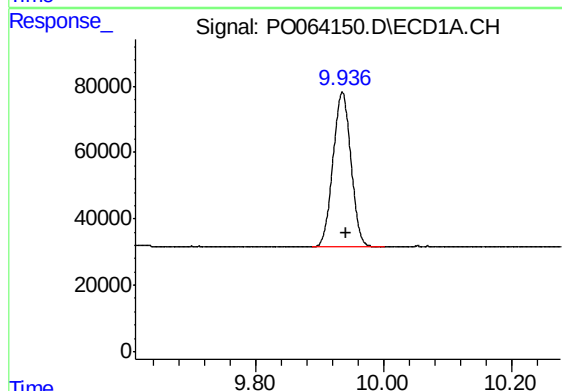


#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: -0.005 min
Response: 906240
Conc: 25.92 ng/ml

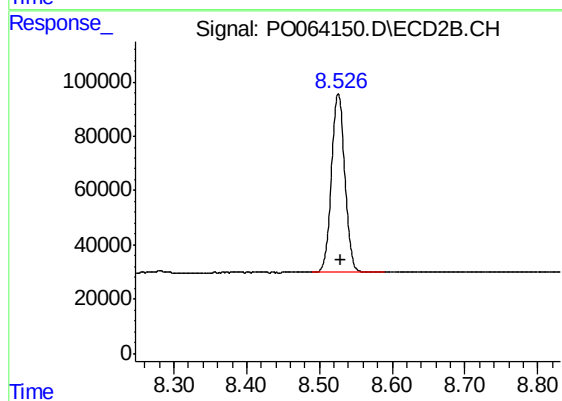

#2 Decachlorobiphenyl


R.T.: 8.526 min
Delta R.T.: -0.004 min
Response: 837469
Conc: 28.32 ng/ml

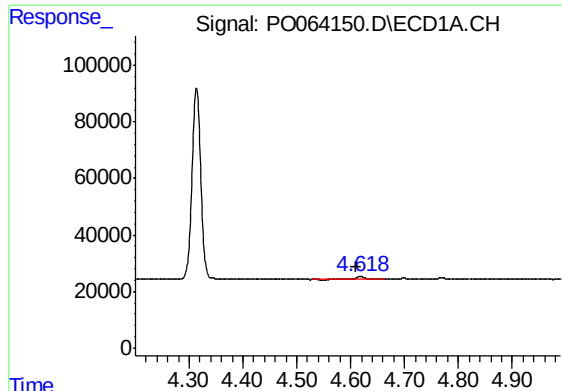

#9 AR-1221-2


R.T.: 4.618 min
Delta R.T.: 0.008 min
Response: 12409
Conc: 46.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-05

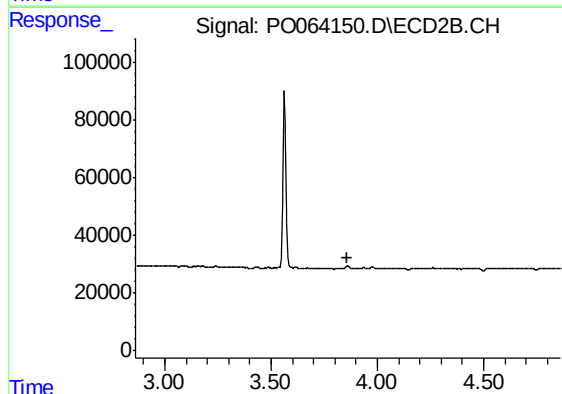


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

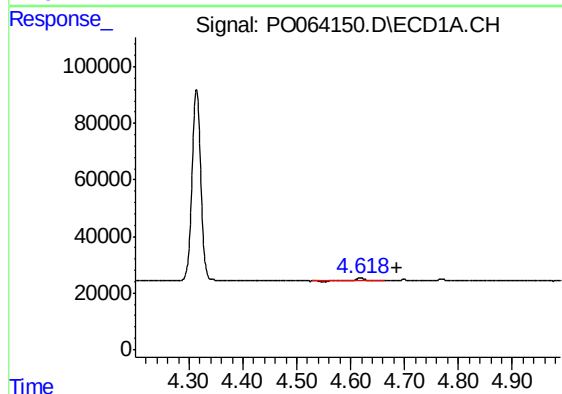


#10 AR-1221-3

R.T.: 4.618 min
Delta R.T.: -0.068 min
Response: 12409
Conc: 15.39 ng/ml

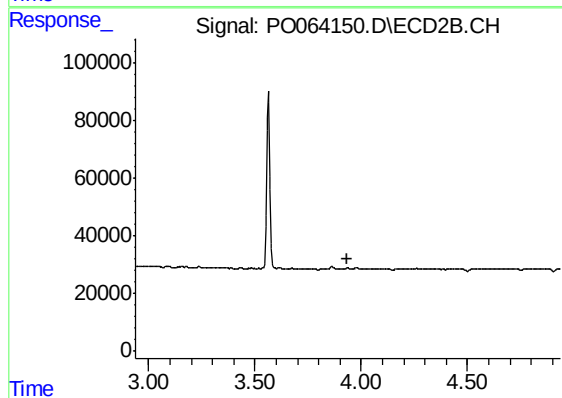

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.937 min
Response: 0
Conc: N.D.

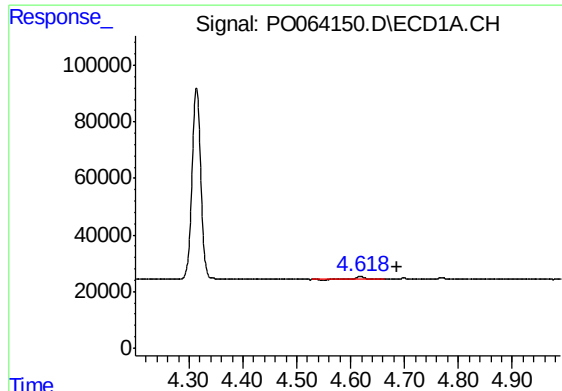

#11 AR-1232-1


R.T.: 4.618 min
Delta R.T.: -0.068 min
Response: 12409
Conc: 10.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-05

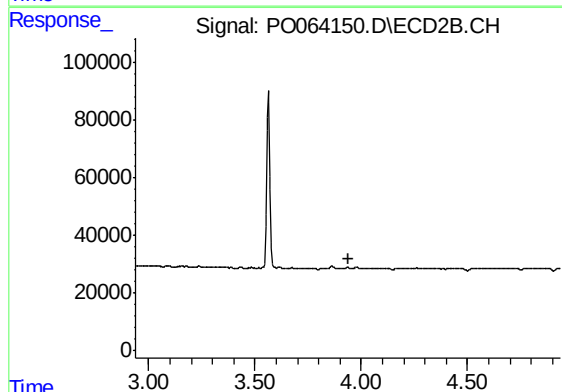


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.938 min
Response: 0
Conc: N.D.

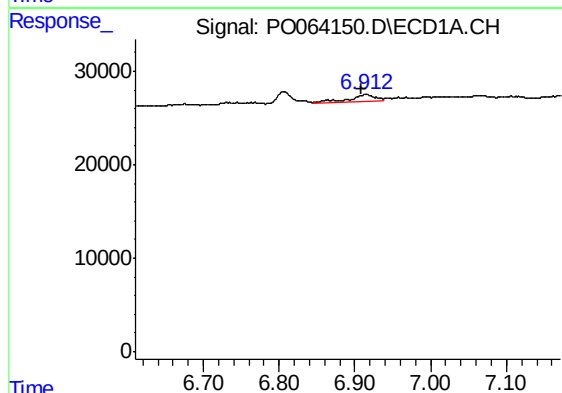


#28 AR-1254-3

R.T.: 6.914 min
Delta R.T.: 0.006 min
Response: 16267
Conc: 6.15 ng/ml

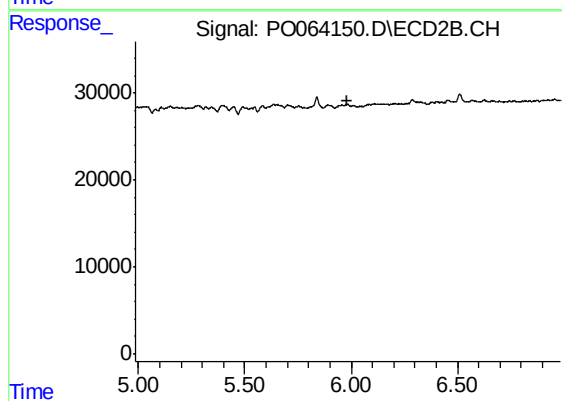

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.985 min
Response: 0
Conc: N.D.

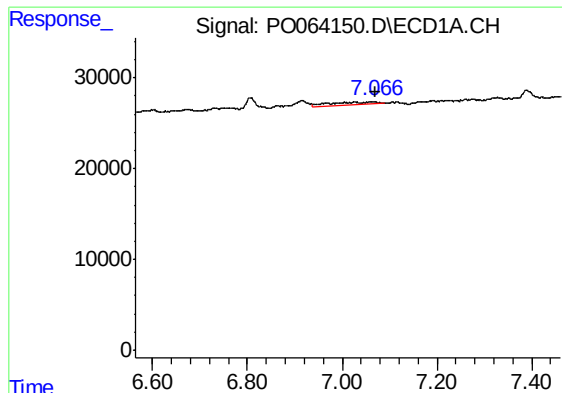

#31 AR-1260-1


R.T.: 7.068 min
Delta R.T.: -0.003 min
Response: 18765
Conc: 10.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-05

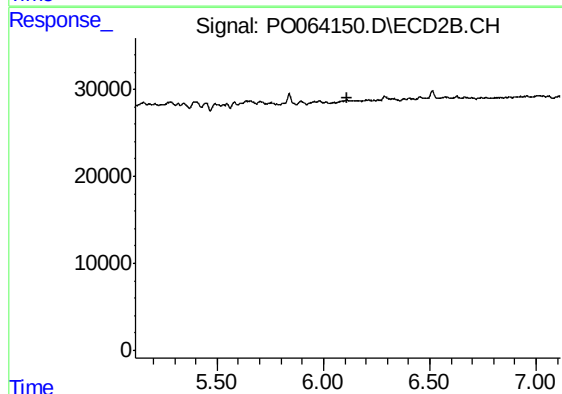


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

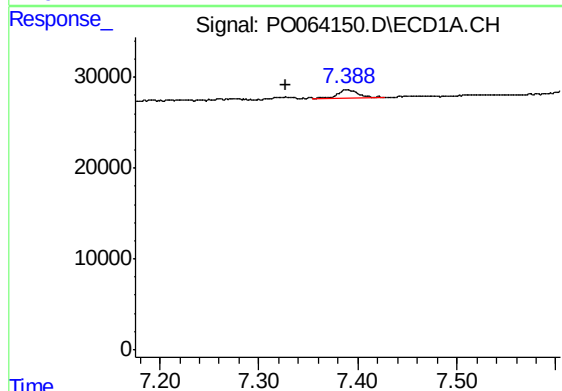


#32 AR-1260-2

R.T.: 7.389 min
Delta R.T.: 0.062 min
Response: 13155
Conc: 5.97 ng/ml

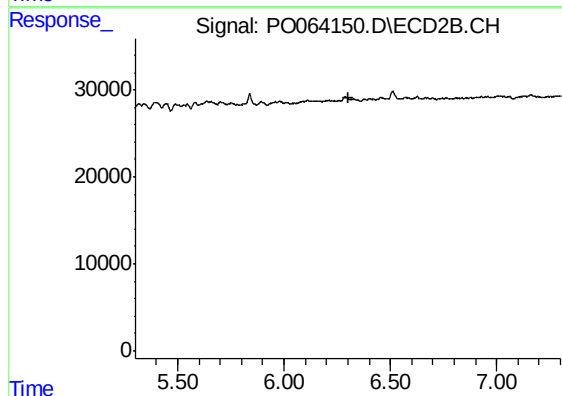

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

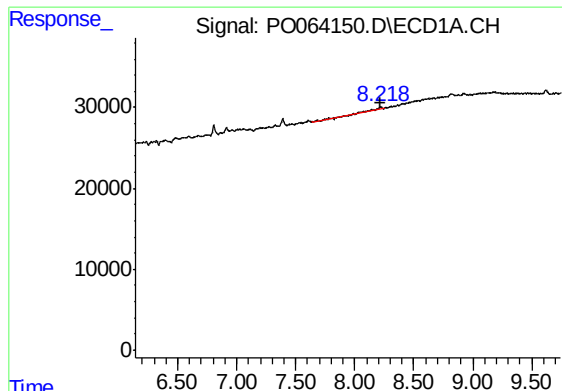

#35 AR-1260-5


R.T.: 8.219 min
Delta R.T.: -0.001 min
Response: 21731
Conc: 5.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-05

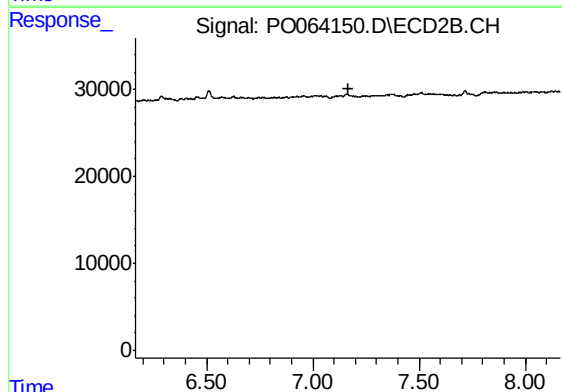


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.165 min
Response: 0
Conc: N.D.

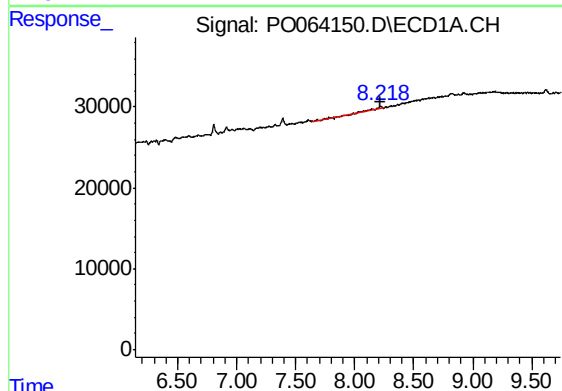

#37 AR-1262-2

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 21731
Conc: 4.47 ng/ml

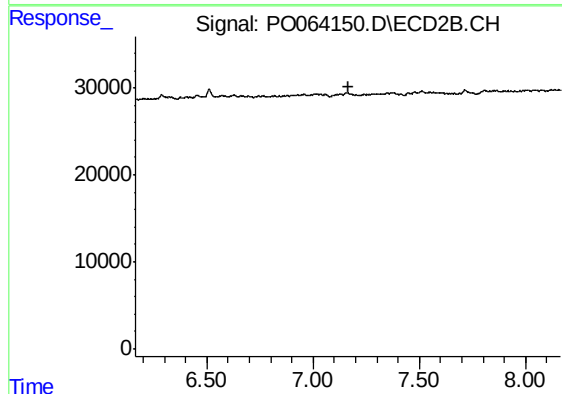

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.164 min
Response: 0
Conc: N.D.