

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112619\
 Data File : P0064154.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2019 3:03
 Operator : SM/AJ
 Sample : K6014-17
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 04:00:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.563	627700	511907	23.652	24.020
2)	SA Decachlor...	9.935	8.526	869819	811778	24.883	27.455
Target Compounds							
9)	L2 AR-1221-2	4.617	0.000	14547	0	54.488	N.D. #
10)	L2 AR-1221-3	4.617	0.000	14547	0	18.042	N.D. #
11)	L3 AR-1232-1	4.617	0.000	14547	0	11.749	N.D. #
28)	L6 AR-1254-3	6.912	0.000	11676	0	4.418	N.D. #
30)	L6 AR-1254-5	7.604	0.000	9831	0	4.595	N.D. #
32)	L7 AR-1260-2	7.326	0.000	23671	0	10.742	N.D. #
35)	L7 AR-1260-5	8.217	0.000	60566	0	14.298	N.D. #
37)	L8 AR-1262-2	8.217	0.000	60566	0	12.471	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : PO064154.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2019 3:03
Operator : SM/AJ
Sample : K6014-17
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CS-09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 04:00:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

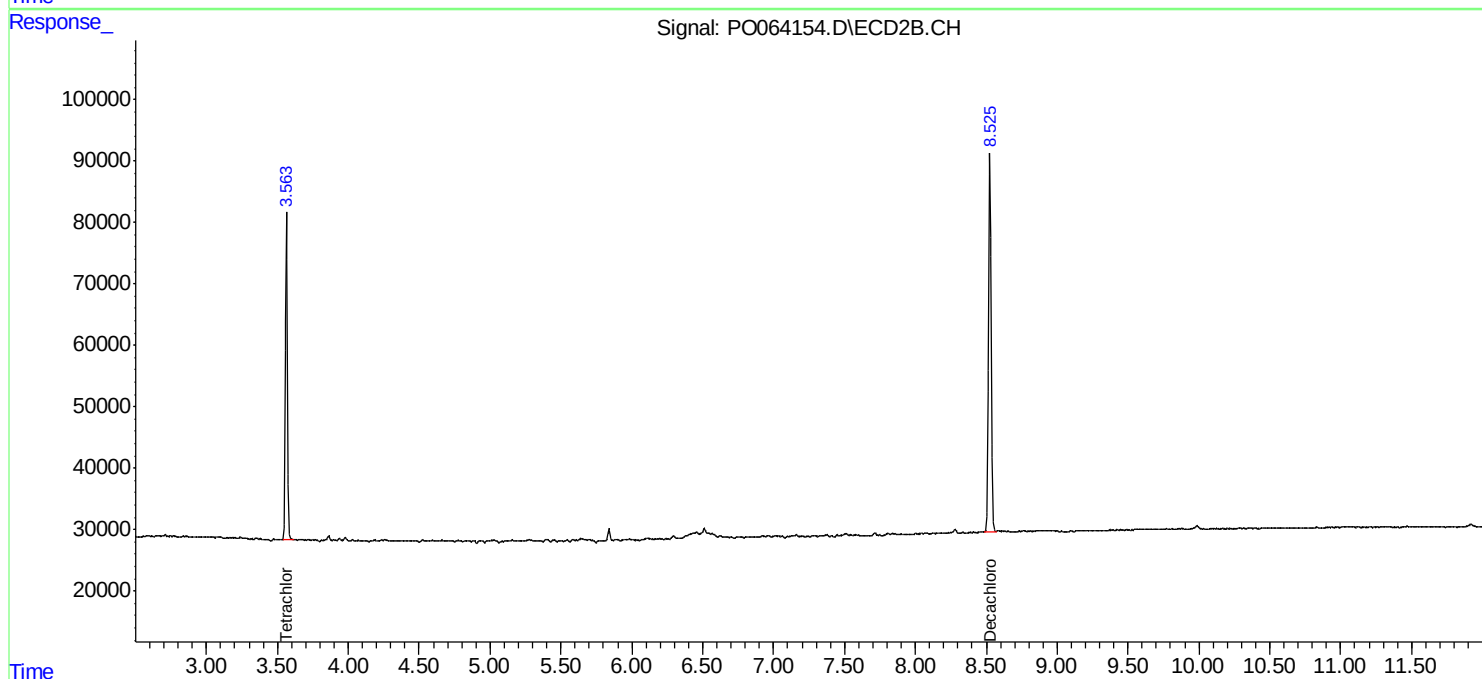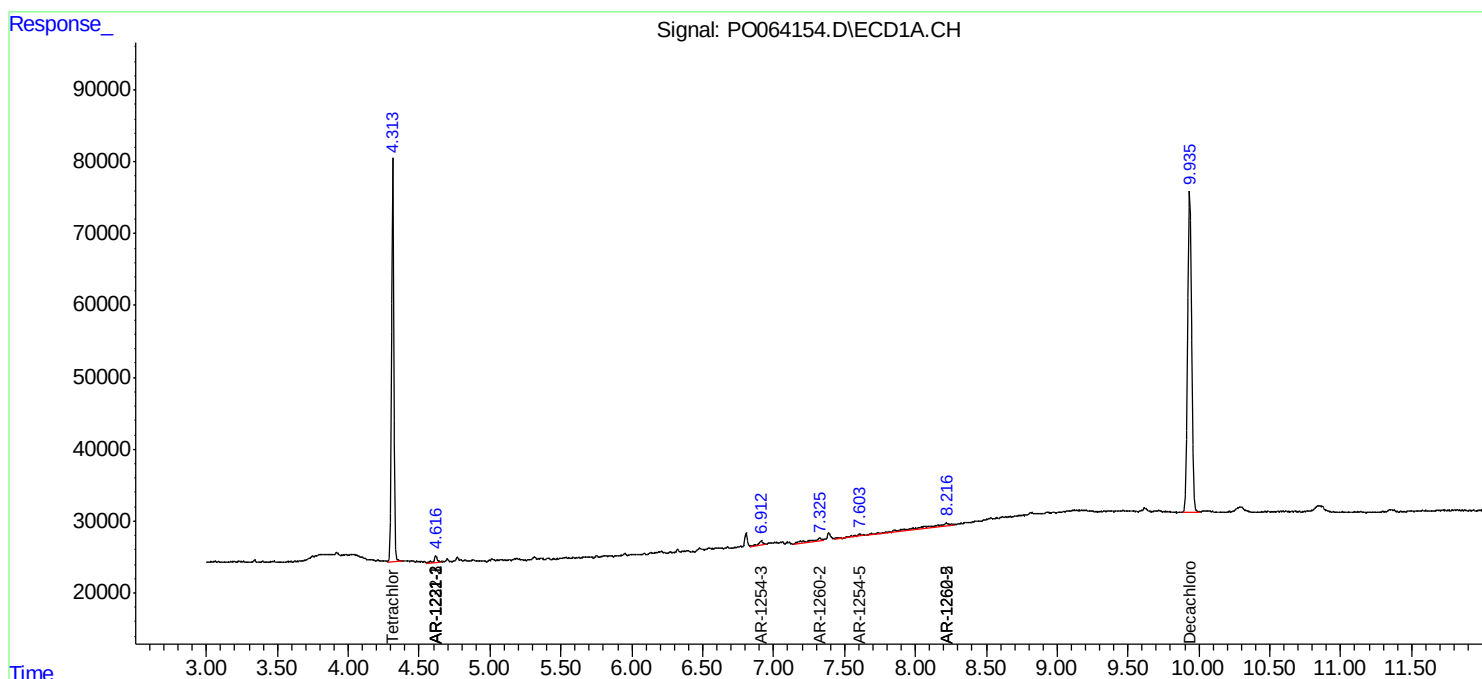


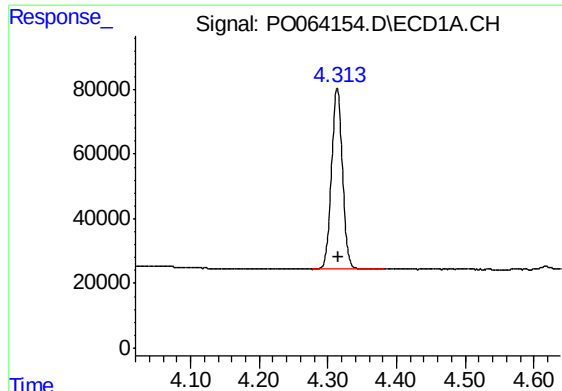

#1 Tetrachloro-m-xylene


R.T.: 4.314 min
Delta R.T.: -0.002 min
Response: 627700
Conc: 23.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-09

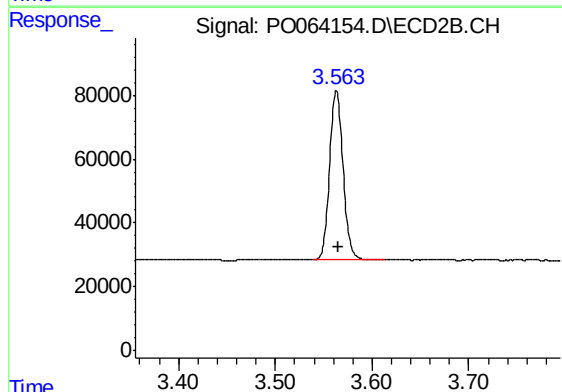


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.001 min
Response: 511907
Conc: 24.02 ng/ml

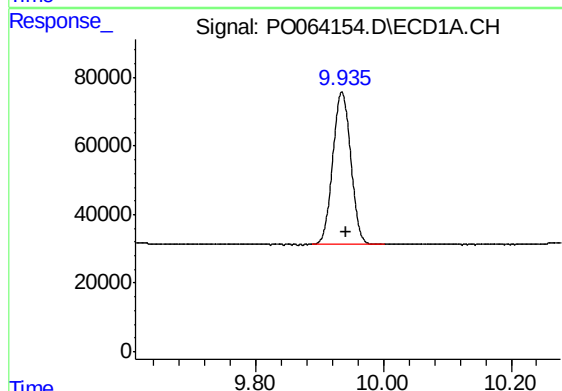


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.006 min
Response: 869819
Conc: 24.88 ng/ml

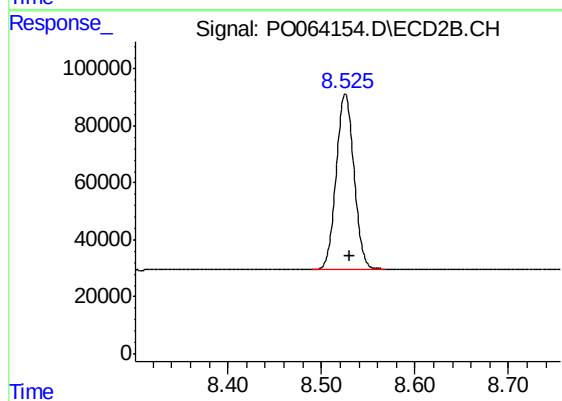

#2 Decachlorobiphenyl


R.T.: 8.526 min
Delta R.T.: -0.005 min
Response: 811778
Conc: 27.46 ng/ml

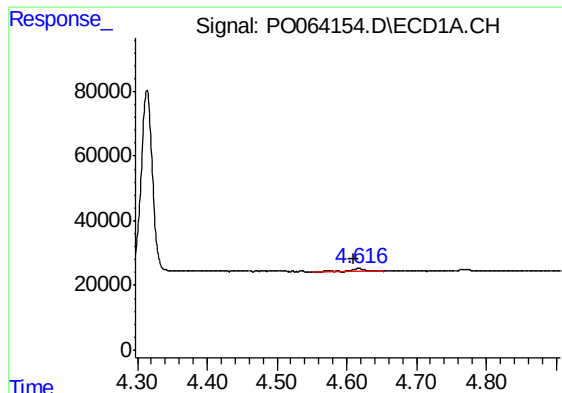

#9 AR-1221-2


R.T.: 4.617 min
Delta R.T.: 0.007 min
Response: 14547
Conc: 54.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-09

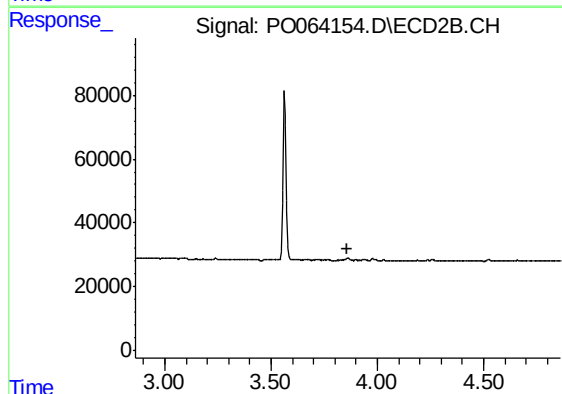


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

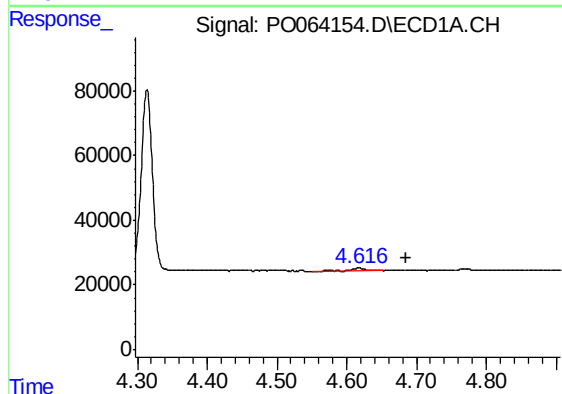


#10 AR-1221-3

R.T.: 4.617 min
Delta R.T.: -0.069 min
Response: 14547
Conc: 18.04 ng/ml

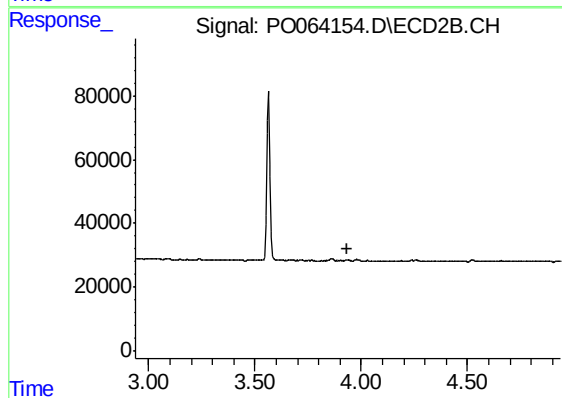

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.937 min
Response: 0
Conc: N.D.

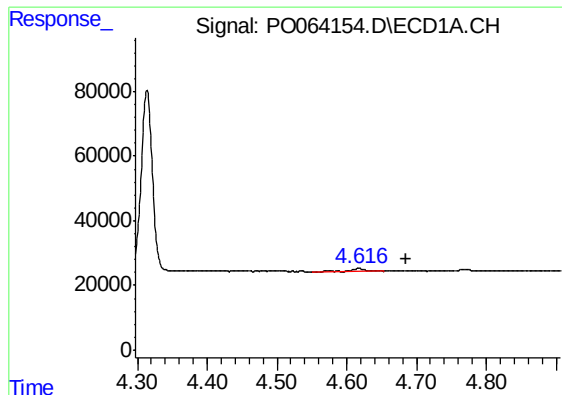

#11 AR-1232-1


R.T.: 4.617 min
Delta R.T.: -0.068 min
Response: 14547
Conc: 11.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-09

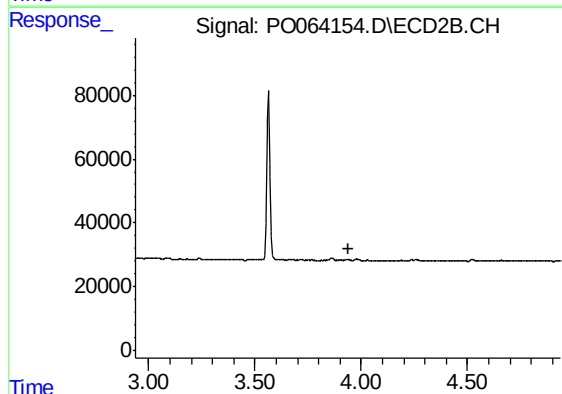


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.938 min
Response: 0
Conc: N.D.

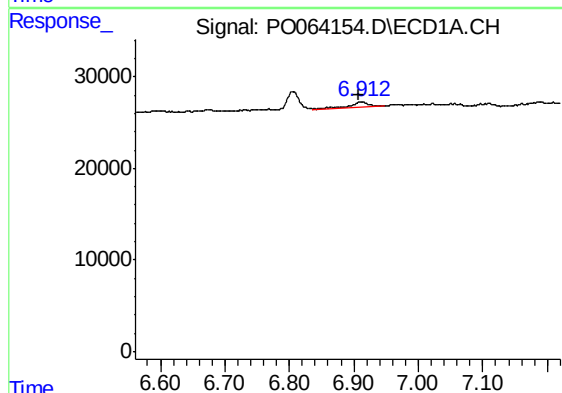


#28 AR-1254-3

R.T.: 6.912 min
Delta R.T.: 0.004 min
Response: 11676
Conc: 4.42 ng/ml

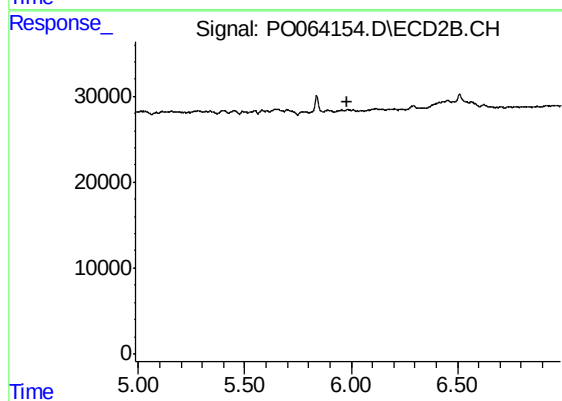

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.985 min
Response: 0
Conc: N.D.

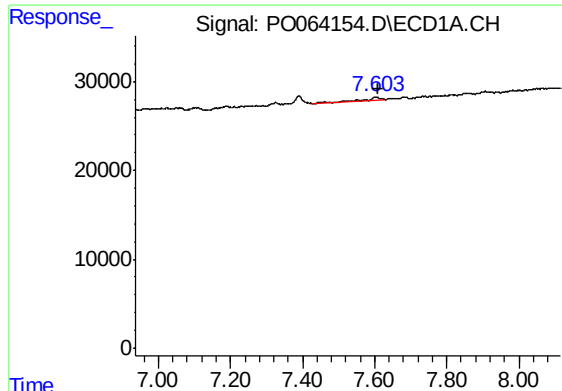

#30 AR-1254-5


R.T.: 7.604 min
Delta R.T.: -0.006 min
Response: 9831
Conc: 4.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-09

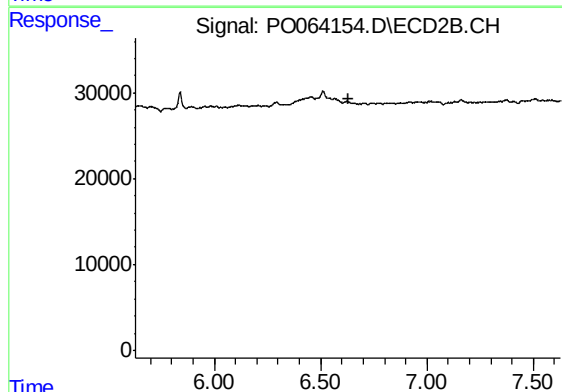


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.629 min
Response: 0
Conc: N.D.

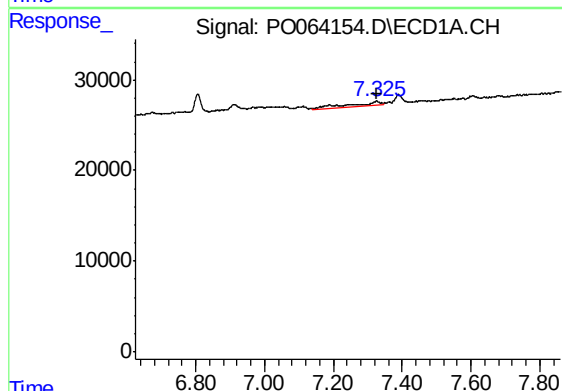


#32 AR-1260-2

R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 23671
Conc: 10.74 ng/ml

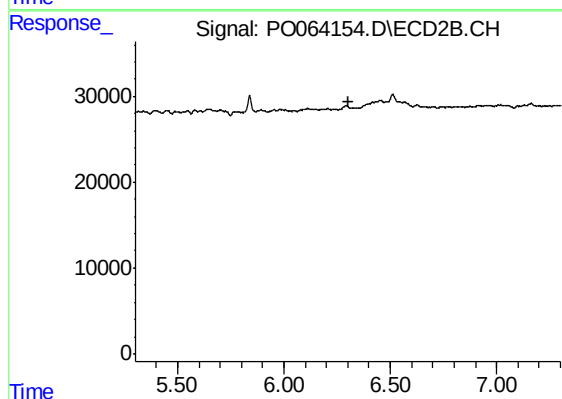

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

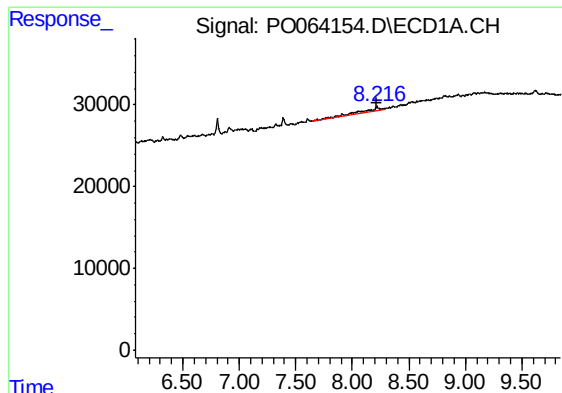

#35 AR-1260-5


R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 60566
Conc: 14.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-09

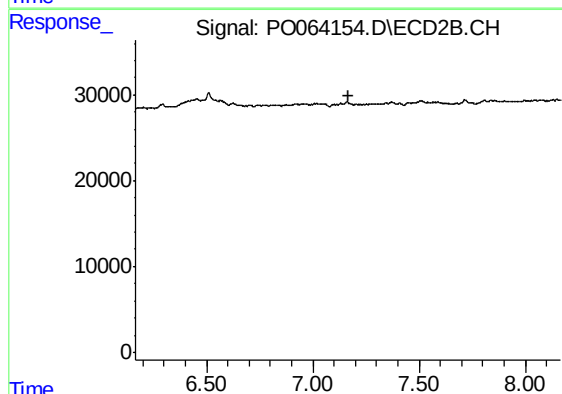


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.165 min
Response: 0
Conc: N.D.

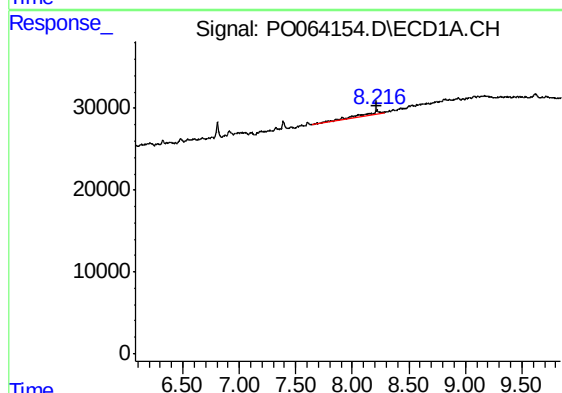

#37 AR-1262-2

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 60566
Conc: 12.47 ng/ml

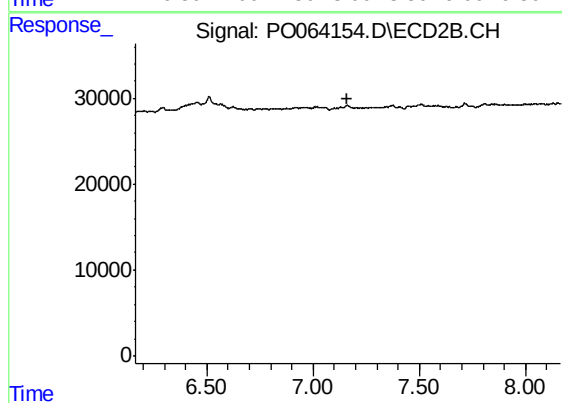

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.164 min
Response: 0
Conc: N.D.