

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112619\
 Data File : P0064119.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Nov 2019 16:28
 Operator : SM/AJ
 Sample : K6016-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

Ankita
 11/27/2019 1:22:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 03:43:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.314	3.562	1276767	616936	48.110m	28.949 #
2) SA Decachlor...	9.939	8.528	290984	211364	8.324	7.149

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : P0064119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Nov 2019 16:28
Operator : SM/AJ
Sample : K6016-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
11/27/2019 1:22:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 03:43:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

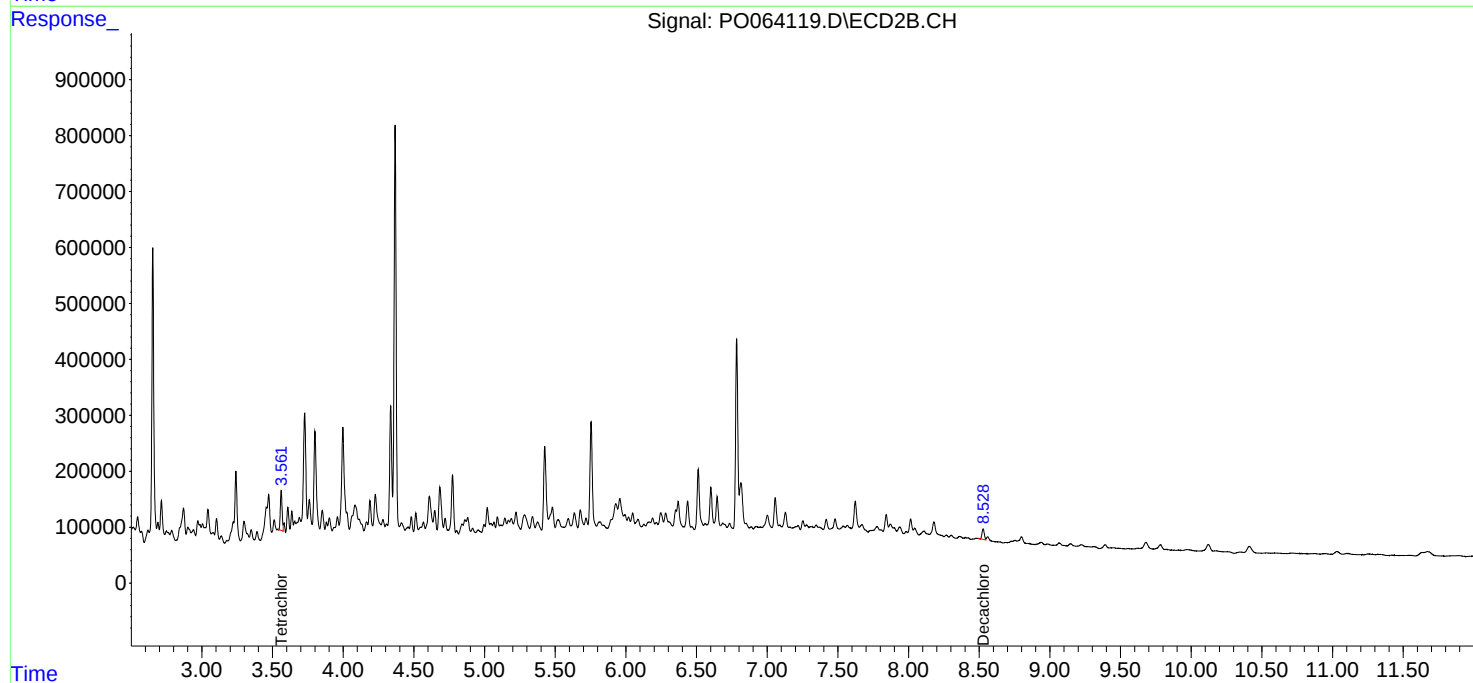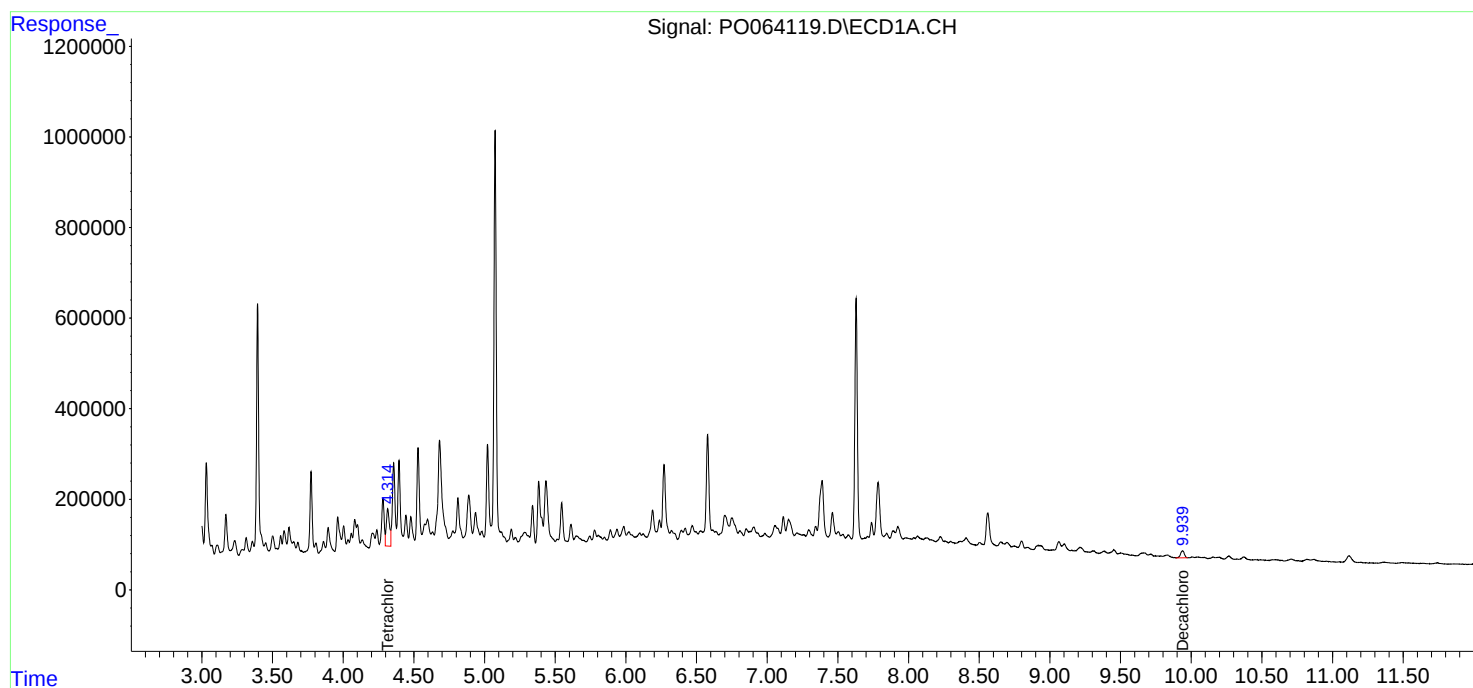

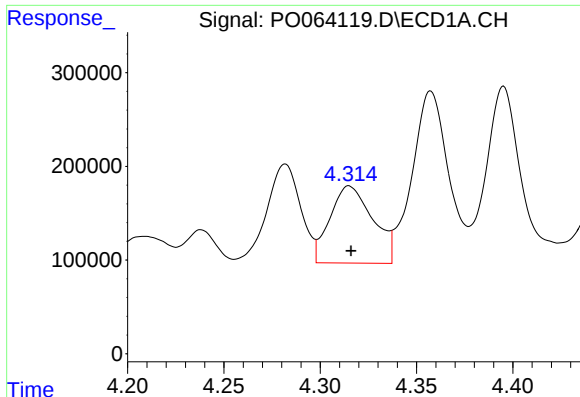


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.002 min
Response: 1276767
Conc: 48.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
11/27/2019 1:22:53 PM

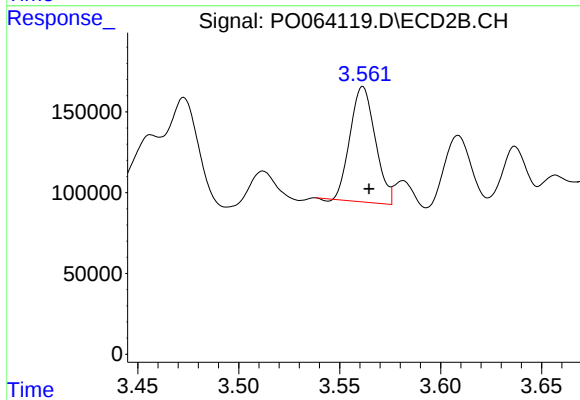


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.003 min
Response: 616936
Conc: 28.95 ng/ml

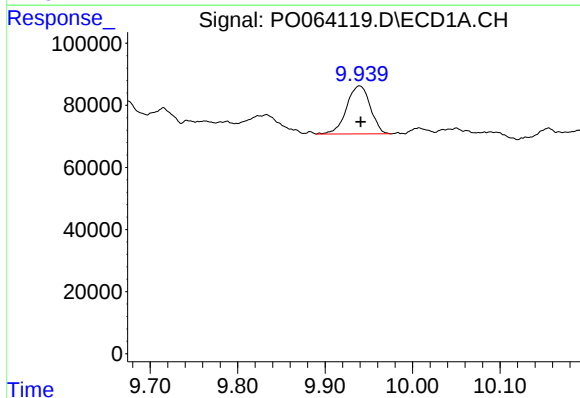

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: -0.001 min
Response: 290984
Conc: 8.32 ng/ml

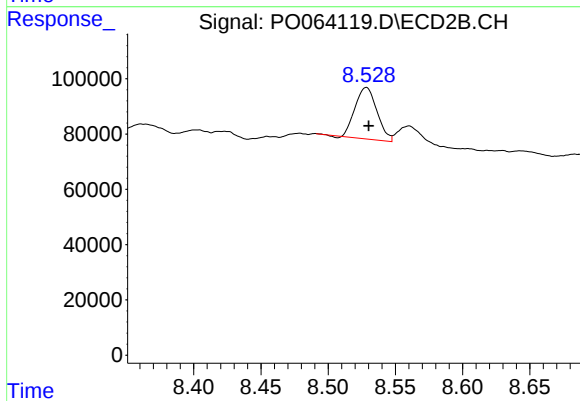

#2 Decachlorobiphenyl

R.T.: 8.528 min
Delta R.T.: -0.002 min
Response: 211364
Conc: 7.15 ng/ml