

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112619\
 Data File : P0064129.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Nov 2019 19:15
 Operator : SM/AJ
 Sample : K6022-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-15-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 03:48:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.564	813235	661210	30.644	31.026
2) SA Decachlor...	9.938	8.527	845315	720604	24.182	24.372

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : P0064129.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Nov 2019 19:15
Operator : SM/AJ
Sample : K6022-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-15-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 03:48:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

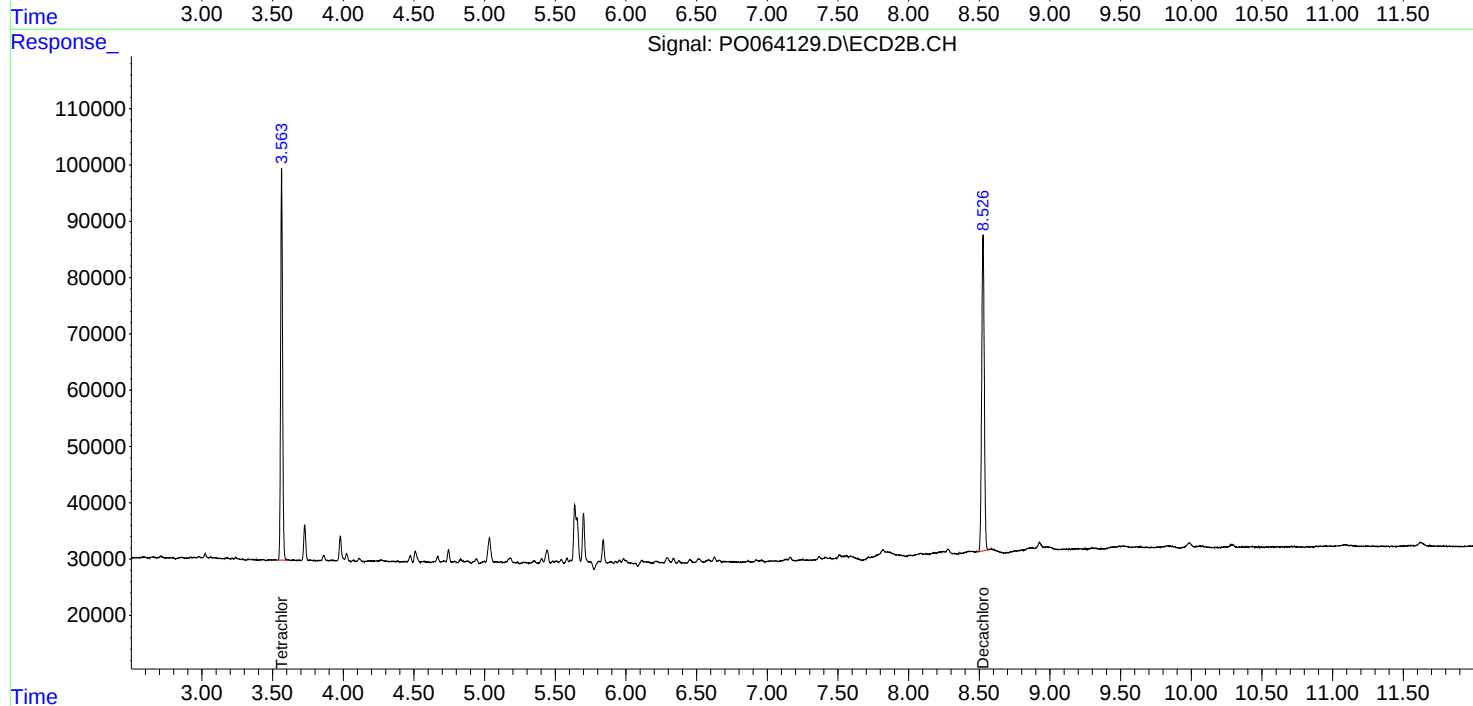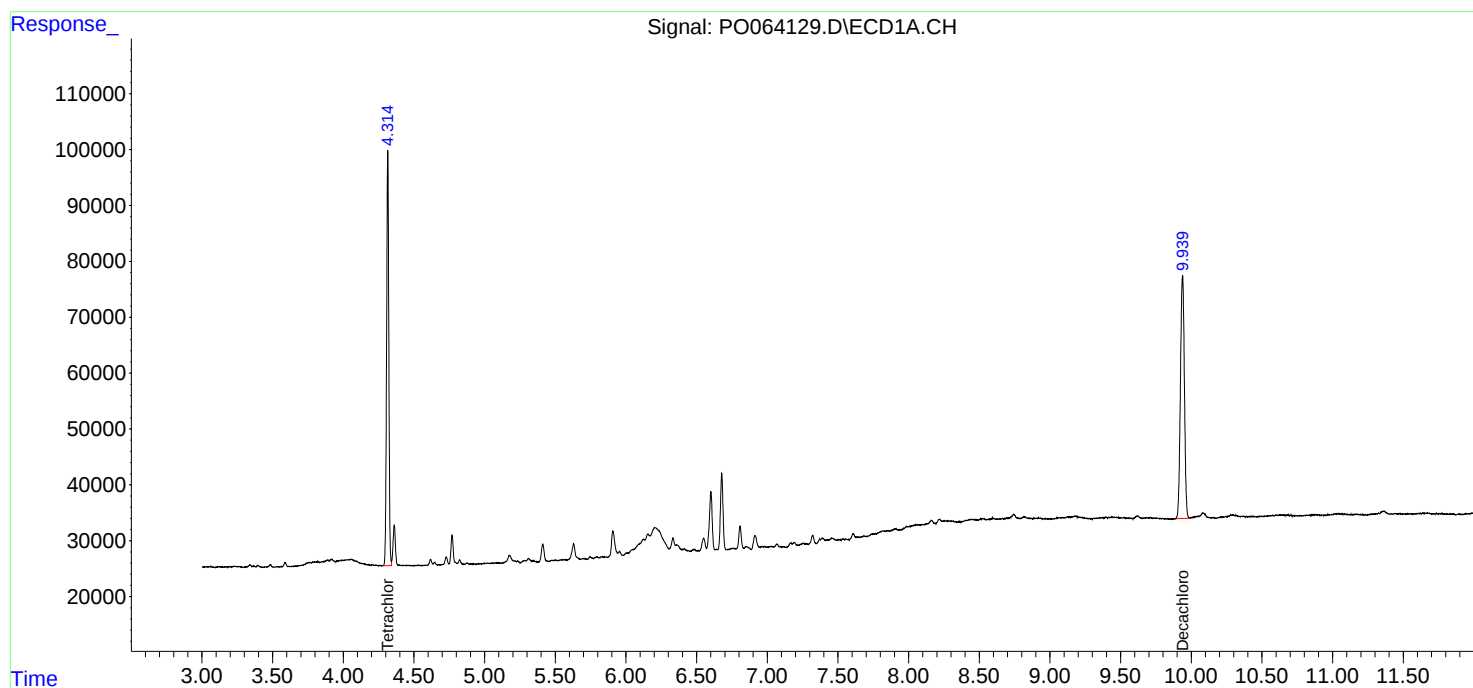


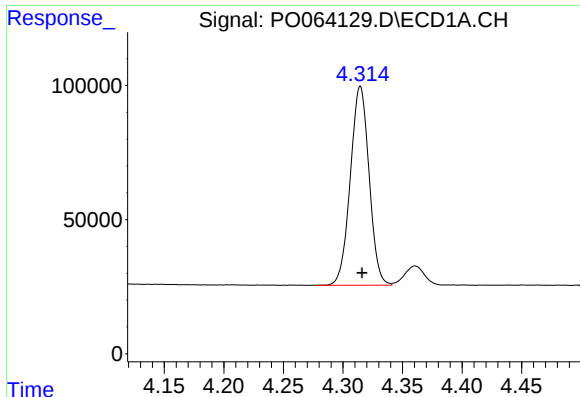

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: -0.001 min
Response: 813235
Conc: 30.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-15-S

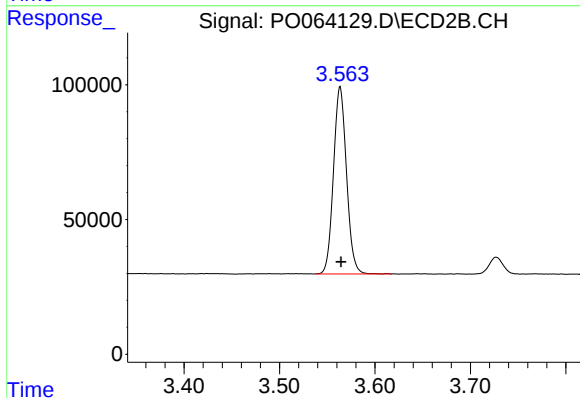


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 661210
Conc: 31.03 ng/ml

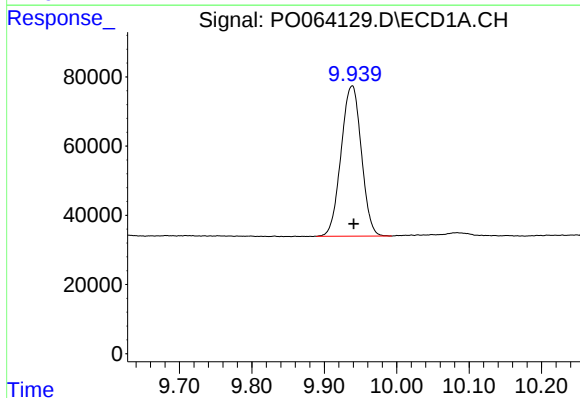

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.002 min
Response: 845315
Conc: 24.18 ng/ml

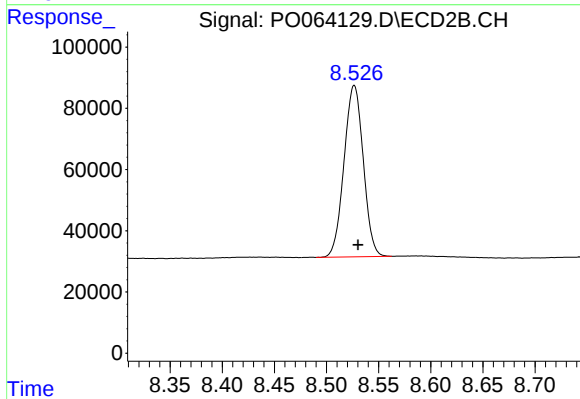

#2 Decachlorobiphenyl

R.T.: 8.527 min
Delta R.T.: -0.004 min
Response: 720604
Conc: 24.37 ng/ml