

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112619\
 Data File : P0064159.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2019 4:27
 Operator : SM/AJ
 Sample : K6008-01
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CALVTANK-1-20191121

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 05:41:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.564	620129	501046	23.367	23.511
2) SA Decachlor...	9.937	8.526	799823	745870	22.880	25.226

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : PO064159.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2019 4:27
Operator : SM/AJ
Sample : K6008-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CALVTANK-1-20191121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 05:41:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

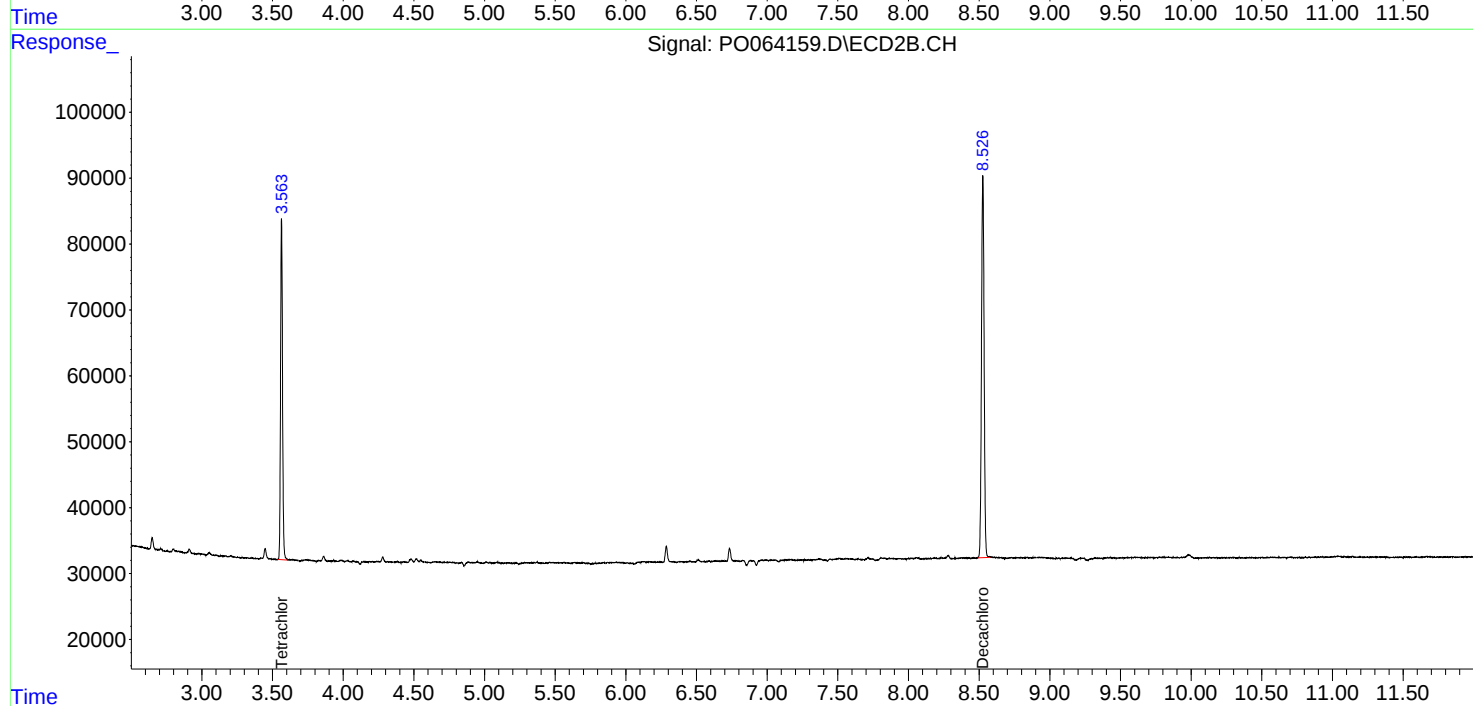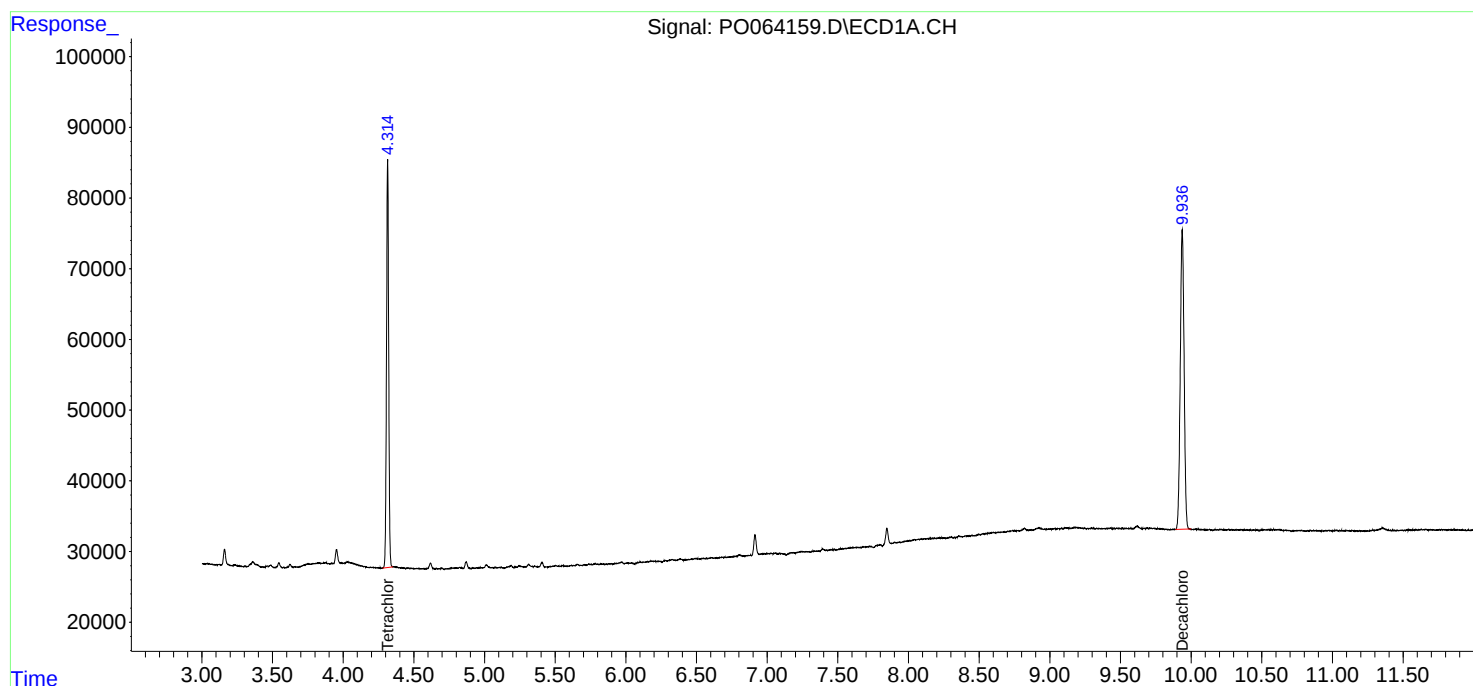


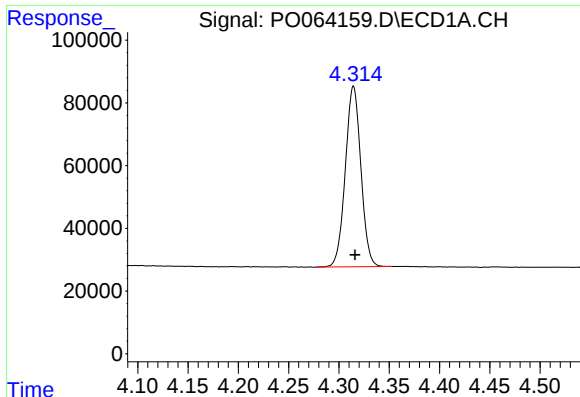

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: -0.001 min
Response: 620129
Conc: 23.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
CALVTANK-1-20191121

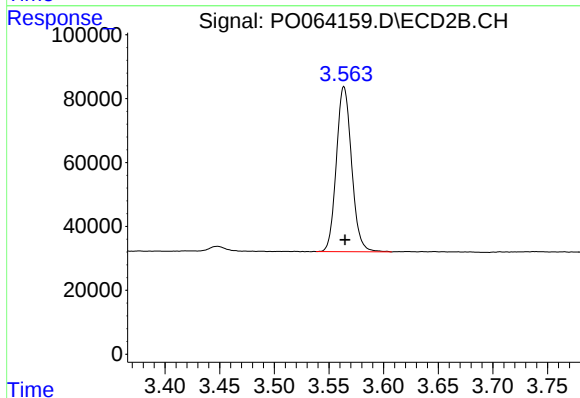


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 501046
Conc: 23.51 ng/ml

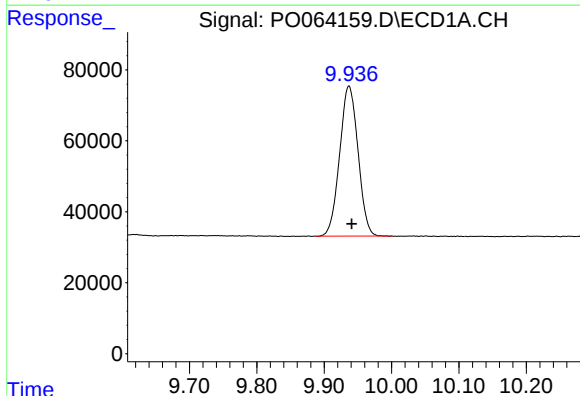

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.004 min
Response: 799823
Conc: 22.88 ng/ml

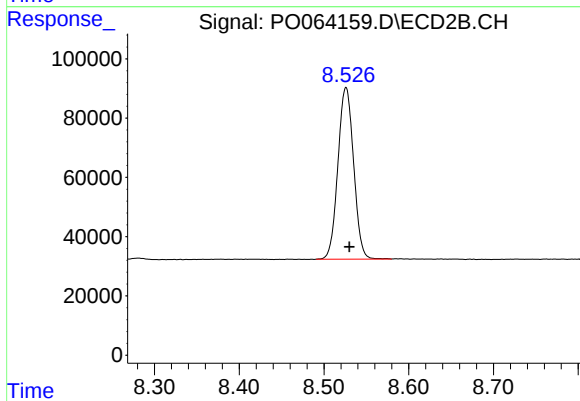

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: -0.004 min
Response: 745870
Conc: 25.23 ng/ml