

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0112619\
 Data File : P0064171.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2019 8:21
 Operator : SM/AJ
 Sample : K6006-03 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 11/27/2019 4:17:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 15:34:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.314	3.561	46320	89380	1.745m	4.194m#
2) SA Decachlor...	9.937	8.526	63565	59264	1.818	2.004
Target Compounds						
26) L6 AR-1254-1	6.322	5.434	124169	84731	85.193	50.802m#
27) L6 AR-1254-2	6.542	5.581	272281	100462	116.551	66.808m#
28) L6 AR-1254-3	6.907	5.982	285256	187438	107.930	73.550m#
29) L6 AR-1254-4	7.190	6.208	272055	125689	133.211	74.036m#
30) L6 AR-1254-5	7.607	6.626	257457	200824	120.323	82.617 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : P0064171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2019 8:21
Operator : SM/AJ
Sample : K6006-03 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 15:34:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

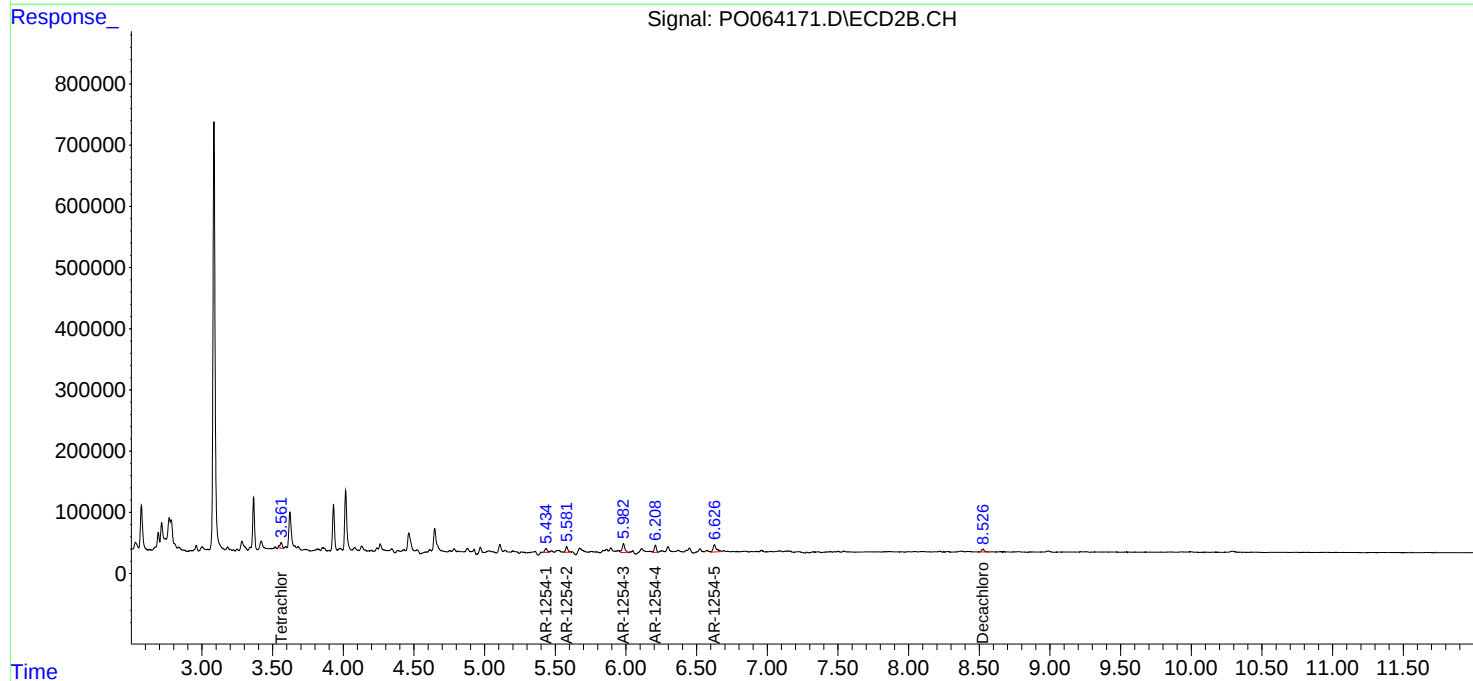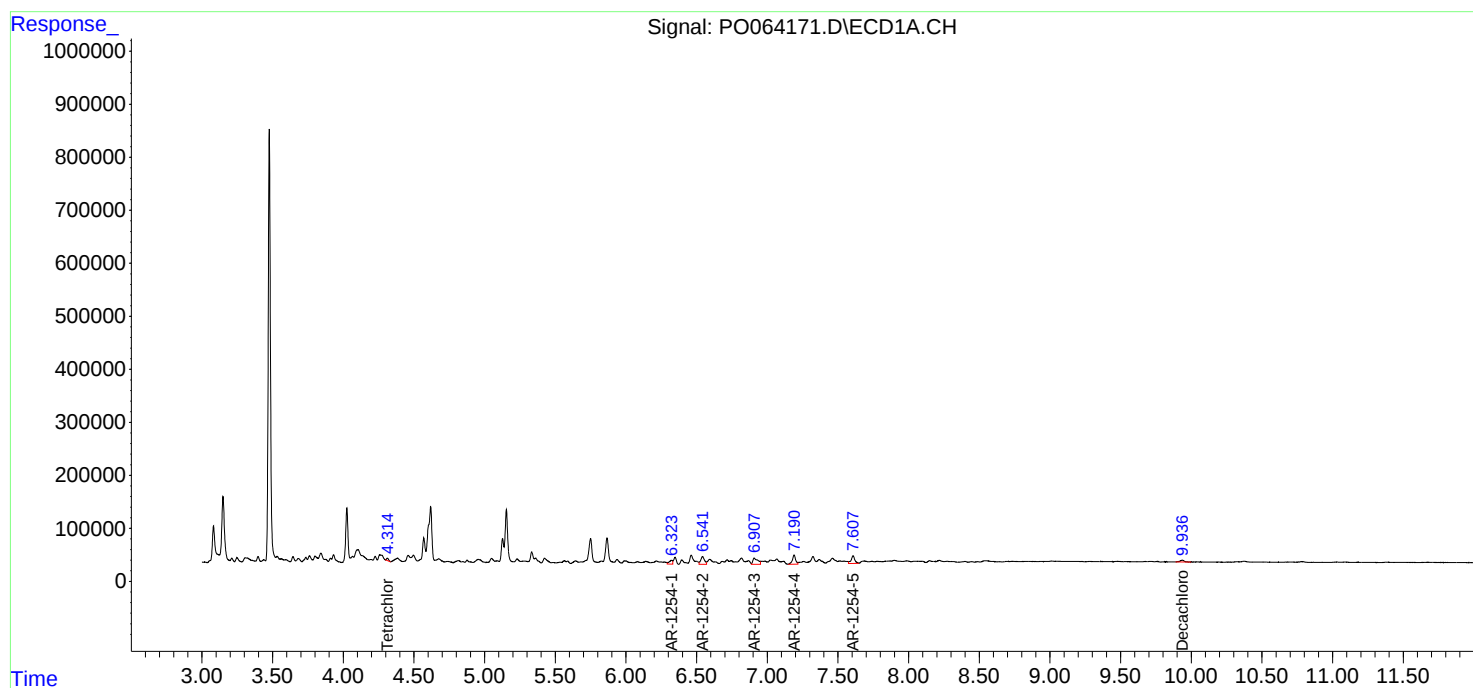

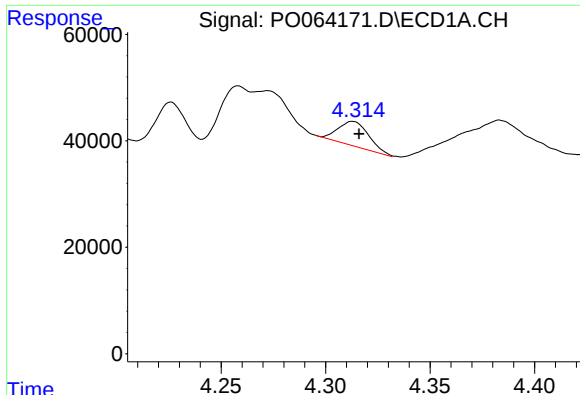


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.002 min
Response: 46320
Conc: 1.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:13 PM

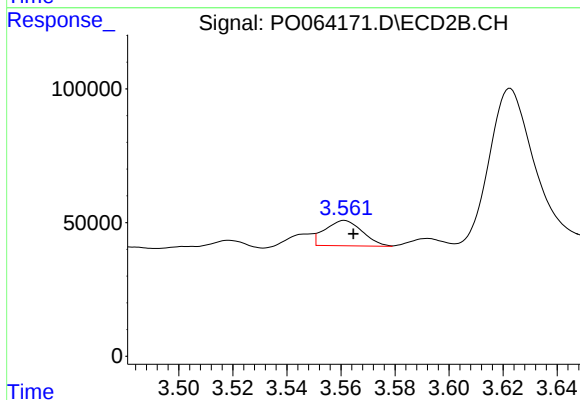


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.004 min
Response: 89380
Conc: 4.19 ng/ml m

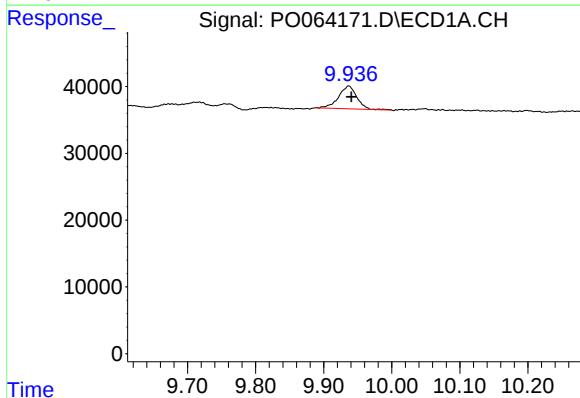


#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.004 min
Response: 63565
Conc: 1.82 ng/ml

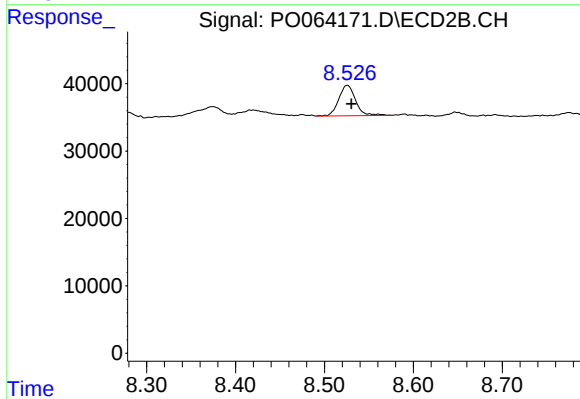

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: -0.005 min
Response: 59264
Conc: 2.00 ng/ml

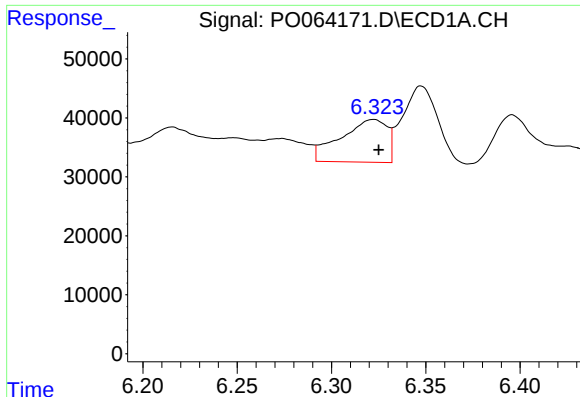


#26 AR-1254-1

R.T.: 6.322 min
Delta R.T.: -0.003 min
Response: 124169
Conc: 85.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:13 PM

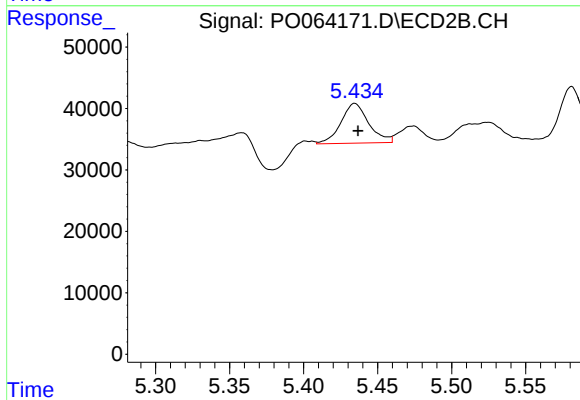


#26 AR-1254-1

R.T.: 5.434 min
Delta R.T.: -0.003 min
Response: 84731
Conc: 50.80 ng/ml m

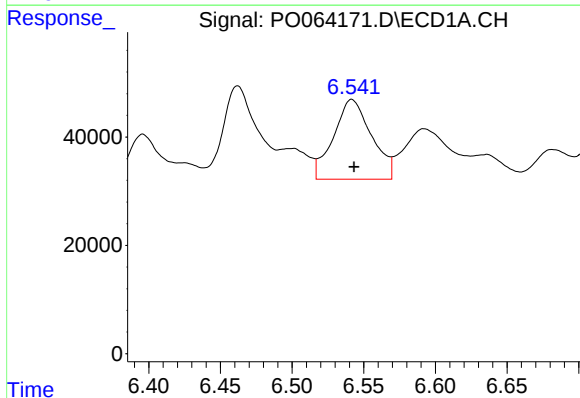


#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: -0.002 min
Response: 272281
Conc: 116.55 ng/ml

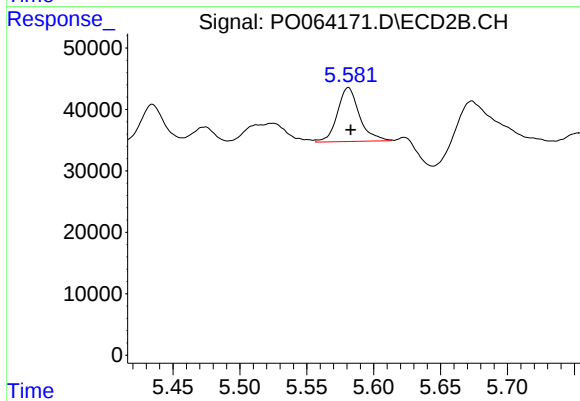

#27 AR-1254-2

R.T.: 5.581 min
Delta R.T.: -0.002 min
Response: 100462
Conc: 66.81 ng/ml m

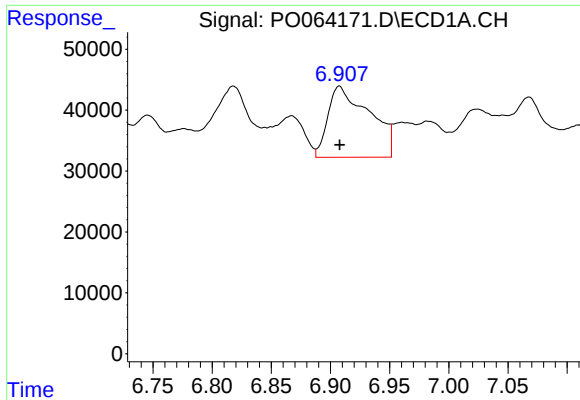


#28 AR-1254-3

R.T.: 6.907 min
Delta R.T.: 0.000 min
Response: 285256
Conc: 107.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:13 PM

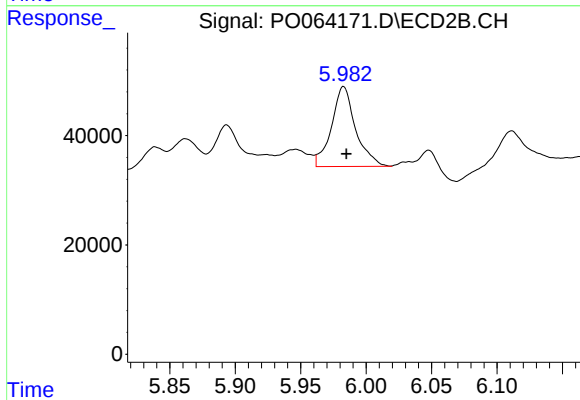


#28 AR-1254-3

R.T.: 5.982 min
Delta R.T.: -0.003 min
Response: 187438
Conc: 73.55 ng/ml m

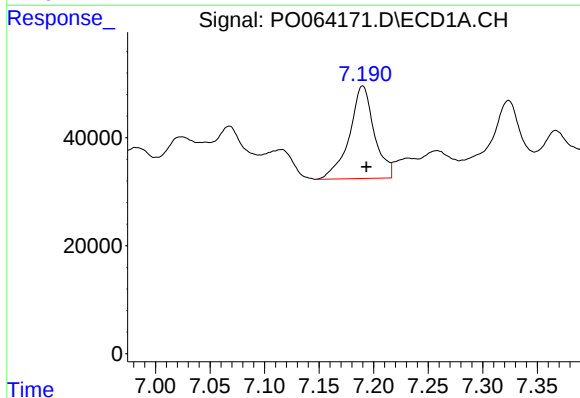


#29 AR-1254-4

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 272055
Conc: 133.21 ng/ml

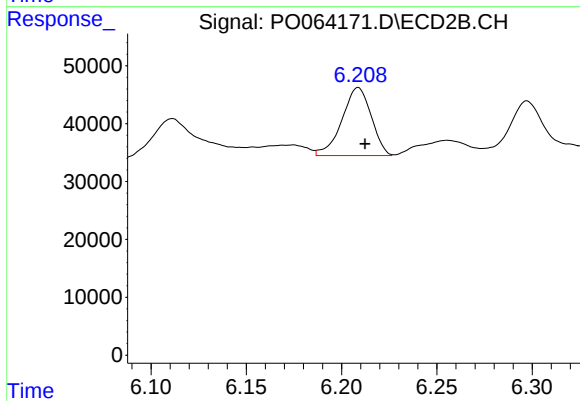

#29 AR-1254-4

R.T.: 6.208 min
Delta R.T.: -0.004 min
Response: 125689
Conc: 74.04 ng/ml m

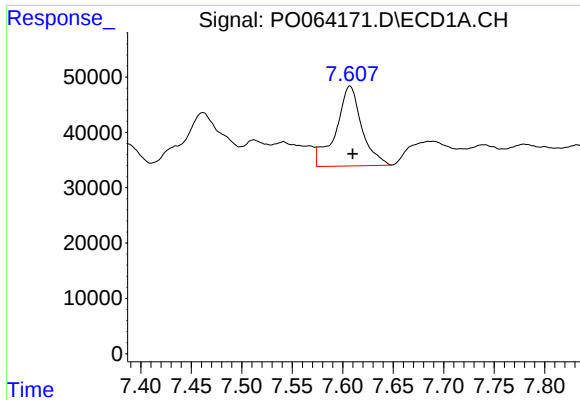


#30 AR-1254-5

R.T.: 7.607 min
Delta R.T.: -0.003 min
Response: 257457
Conc: 120.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C

Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:13 PM

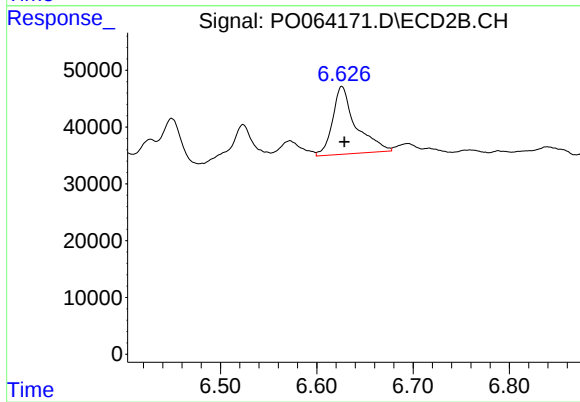

#30 AR-1254-5

R.T.: 6.626 min
Delta R.T.: -0.002 min
Response: 200824
Conc: 82.62 ng/ml