

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0112619\
 Data File : P0064175.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Nov 2019 9:28
 Operator : SM/AJ
 Sample : K6006-03RE 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 03-A-03-B-03-CRE

Manual Integrations
 APPROVED

Ankita
 11/27/2019 4:17:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 09:41:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0112619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 27 03:34:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.314	3.562	59686	42083	2.249m	1.975m
2) SA Decachlor...	9.939	8.526	58561	55983	1.675	1.893
Target Compounds						
26) L6 AR-1254-1	6.323	5.435	129564	73409	88.895	44.014m#
27) L6 AR-1254-2	6.542	5.581	278269	106061	119.115	70.531m#
28) L6 AR-1254-3	6.908	5.983	241694	177065	91.448	69.480m
29) L6 AR-1254-4	7.191	6.209	291961	124978	142.958	73.617m#
30) L6 AR-1254-5	7.608	6.627	283200	180379	132.354	74.206m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112619\
Data File : PO064175.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Nov 2019 9:28
Operator : SM/AJ
Sample : K6006-03RE 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 09:41:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 27 03:34:17 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

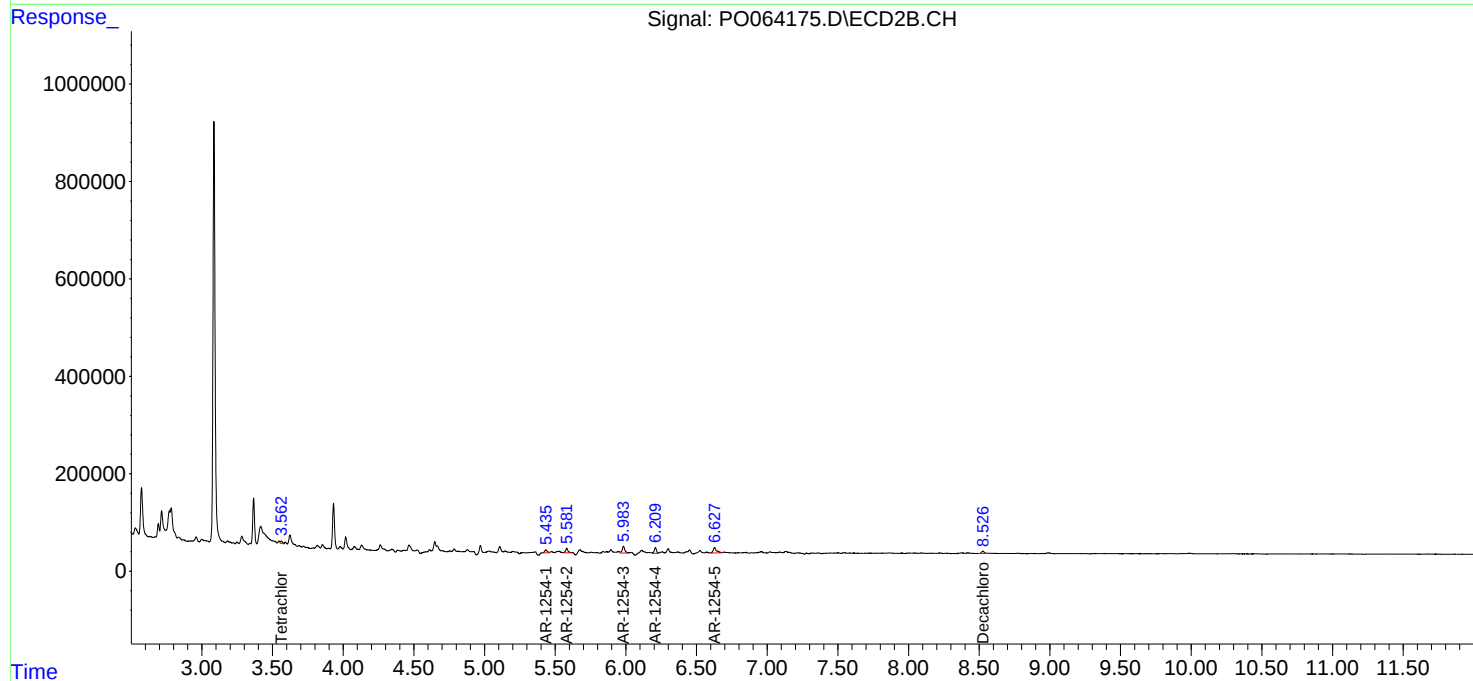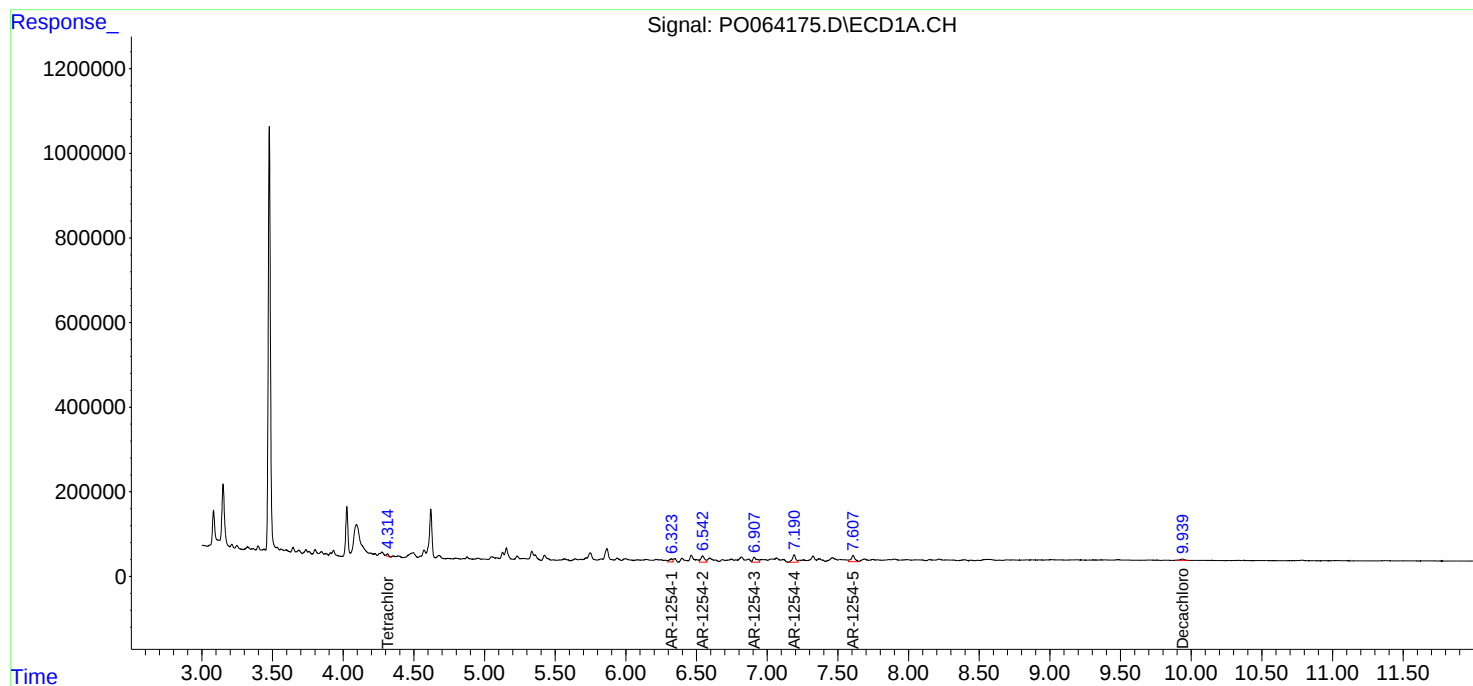

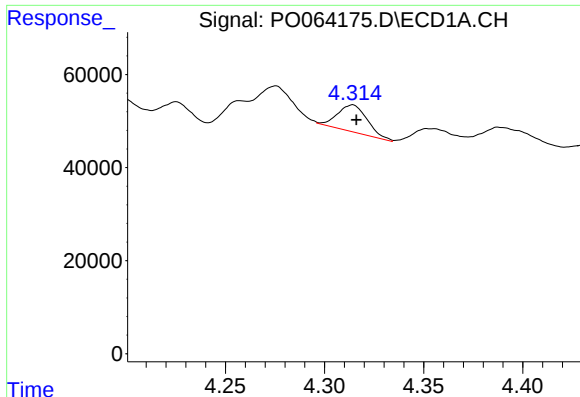


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: -0.002 min
Response: 59686
Conc: 2.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:14 PM

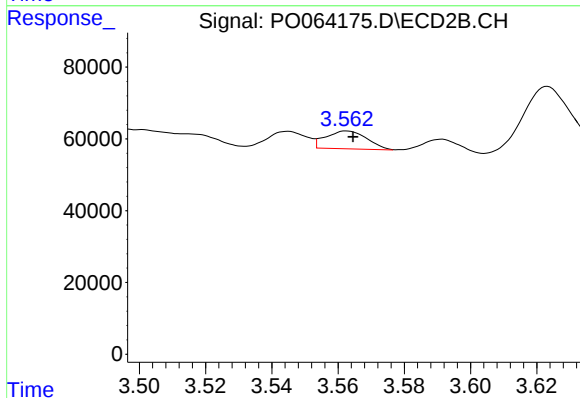


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.003 min
Response: 42083
Conc: 1.97 ng/ml m

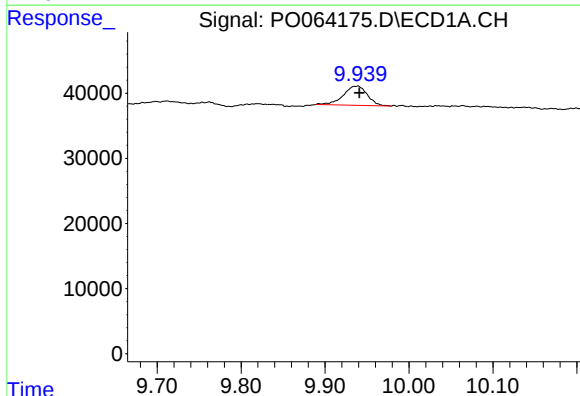


#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: -0.002 min
Response: 58561
Conc: 1.68 ng/ml

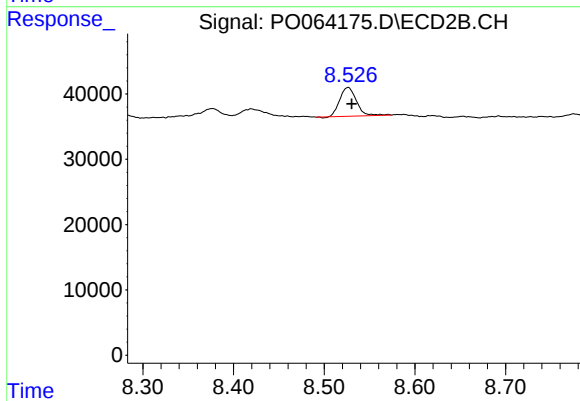

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: -0.004 min
Response: 55983
Conc: 1.89 ng/ml

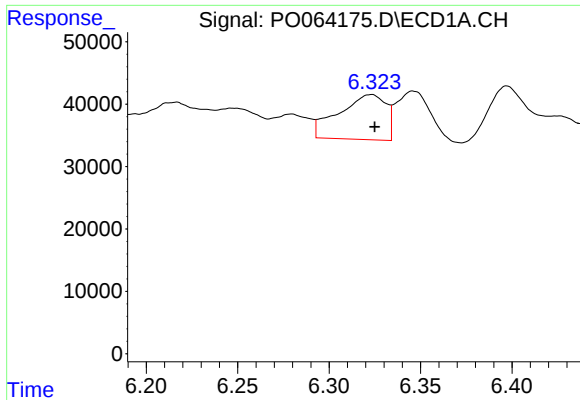


#26 AR-1254-1

R.T.: 6.323 min
Delta R.T.: -0.002 min
Response: 129564
Conc: 88.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:14 PM

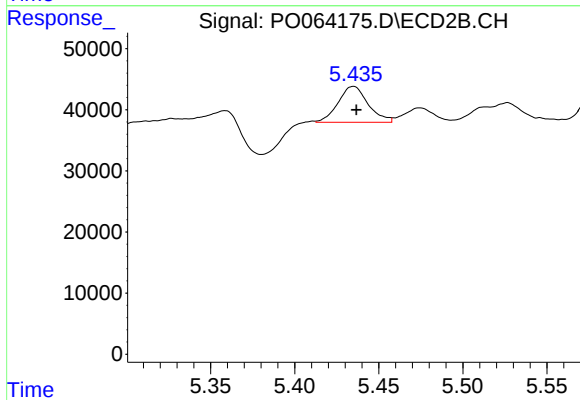


#26 AR-1254-1

R.T.: 5.435 min
Delta R.T.: -0.002 min
Response: 73409
Conc: 44.01 ng/ml m

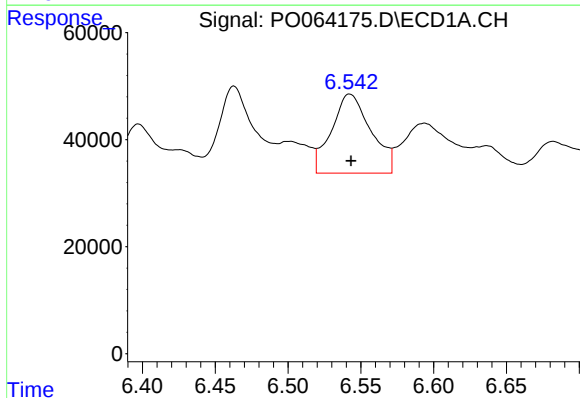


#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: 0.000 min
Response: 278269
Conc: 119.11 ng/ml

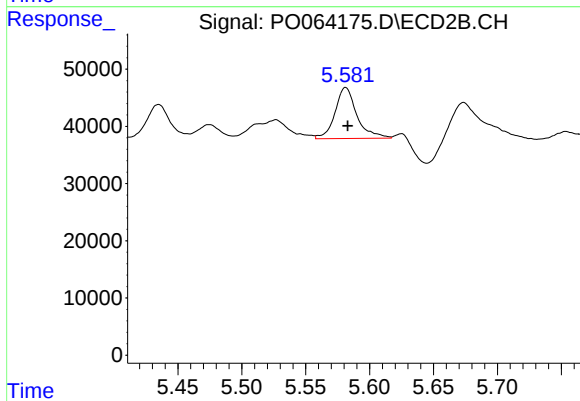

#27 AR-1254-2

R.T.: 5.581 min
Delta R.T.: -0.002 min
Response: 106061
Conc: 70.53 ng/ml m

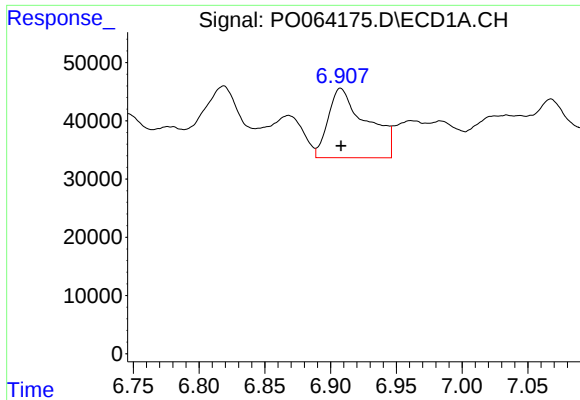


#28 AR-1254-3

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 241694
Conc: 91.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:14 PM

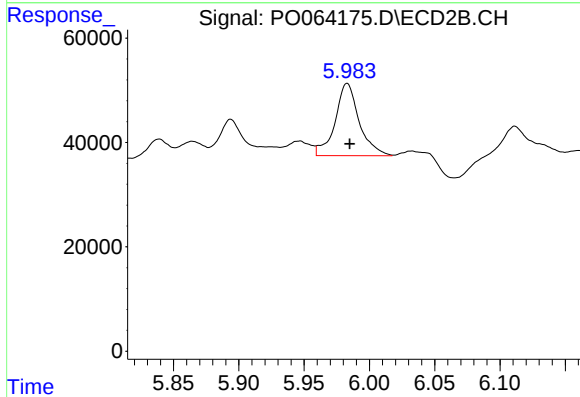


#28 AR-1254-3

R.T.: 5.983 min
Delta R.T.: -0.002 min
Response: 177065
Conc: 69.48 ng/ml m

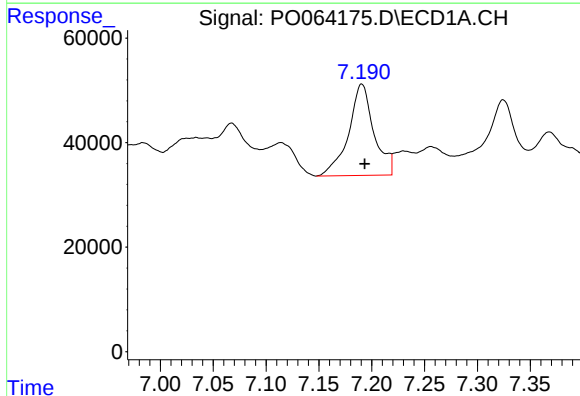


#29 AR-1254-4

R.T.: 7.191 min
Delta R.T.: -0.003 min
Response: 291961
Conc: 142.96 ng/ml

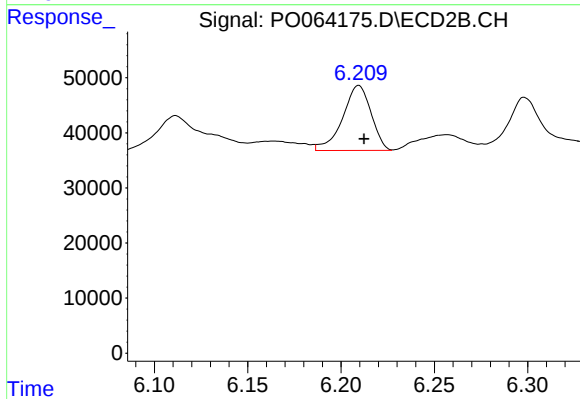

#29 AR-1254-4

R.T.: 6.209 min
Delta R.T.: -0.003 min
Response: 124978
Conc: 73.62 ng/ml m

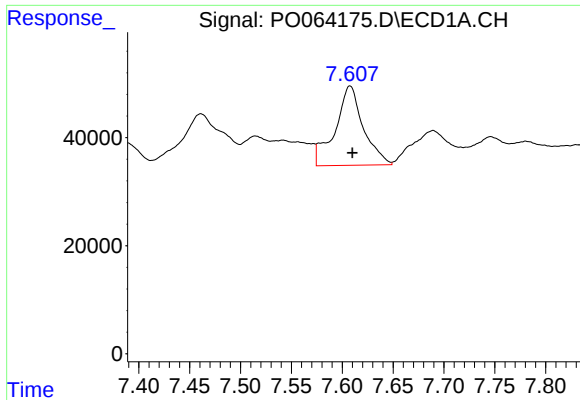


#30 AR-1254-5

R.T.: 7.608 min
Delta R.T.: -0.002 min
Response: 283200
Conc: 132.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE

Manual Integrations
APPROVED

Ankita
11/27/2019 4:17:14 PM

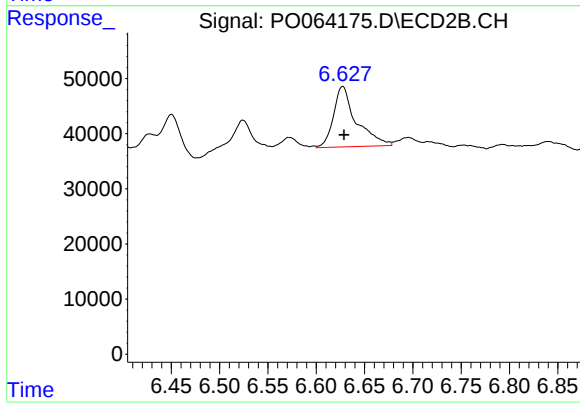

#30 AR-1254-5

R.T.: 6.627 min
Delta R.T.: -0.001 min
Response: 180379
Conc: 74.21 ng/ml m