

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112624\
 Data File : P0108228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2024 14:03
 Operator : YP/AJ
 Sample : P4985-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-740-WC

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :Ankita Jodhani 11/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 14:37:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.380	3.637	185.5E6	71898571	21.308	21.206
2) SA Decachlor...	10.110	8.637	57240523	52601582	18.742m	15.463

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112624\
Data File : PO108228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2024 14:03
Operator : YP/AJ
Sample : P4985-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MH-740-WC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :Ankita Jodhani 11/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 14:37:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

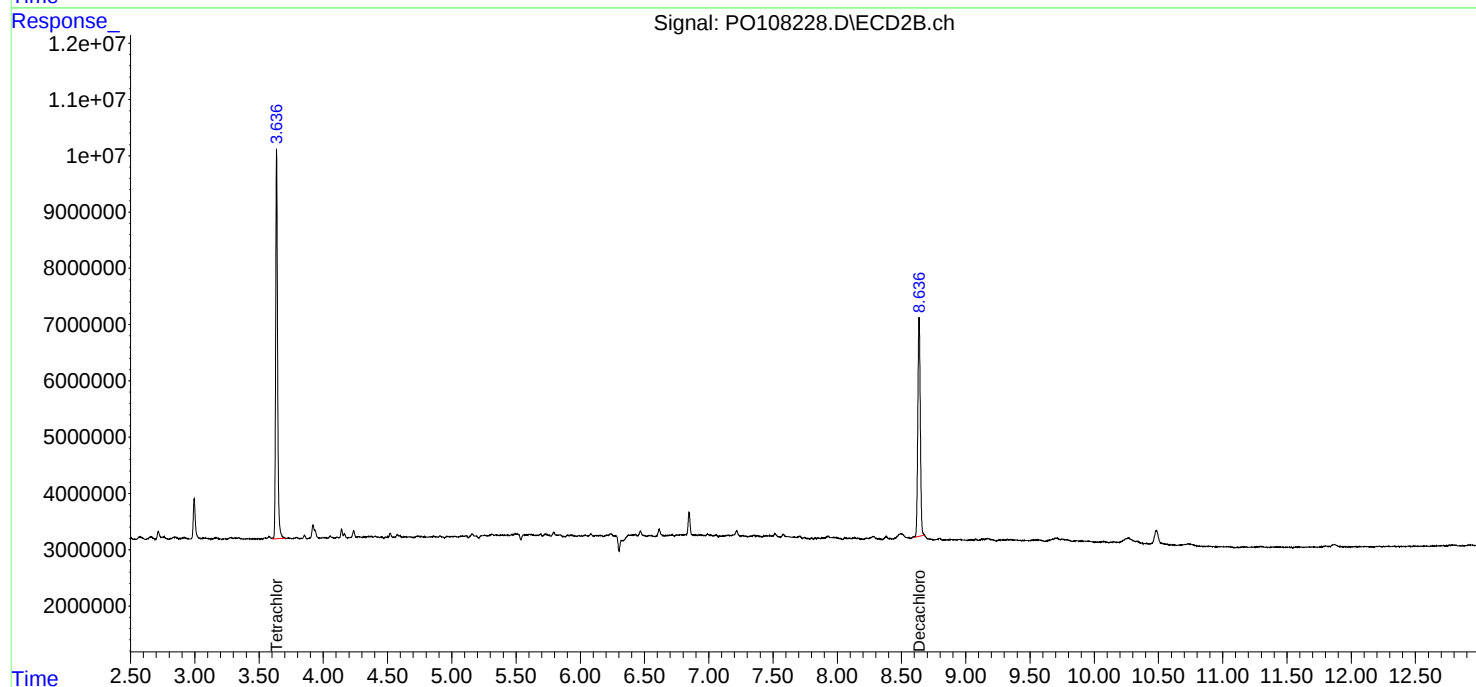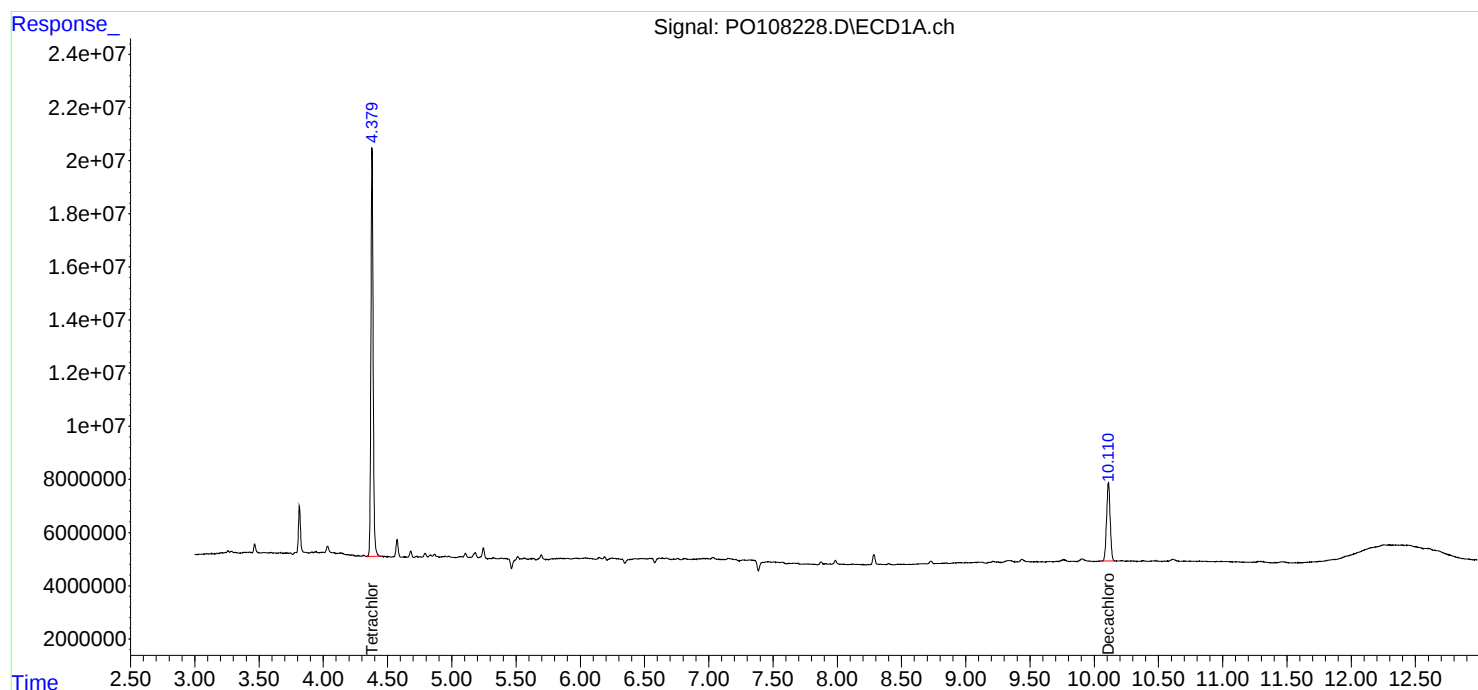

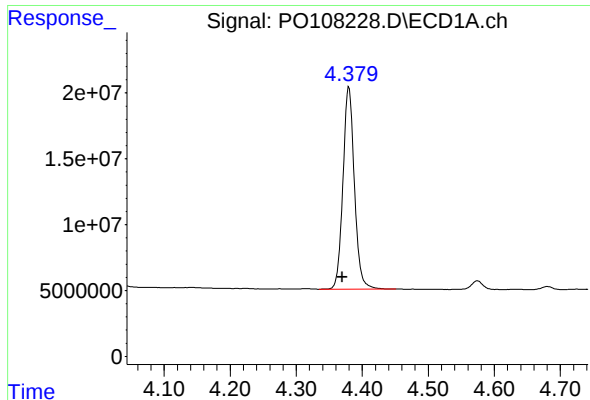


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: 0.010 min
Response: 185509904
Conc: 21.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-740-WC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :Ankita Jodhani 11/27/2024

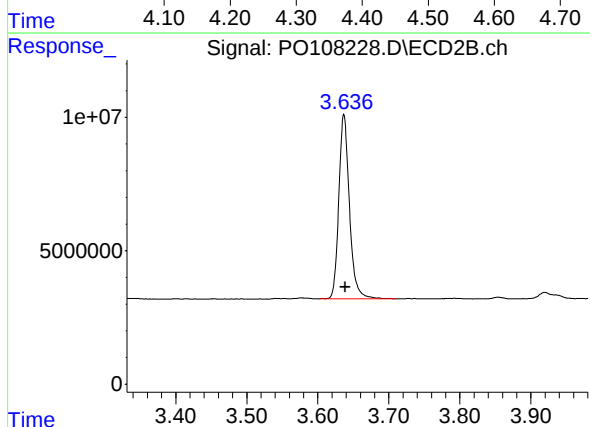


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 71898571
Conc: 21.21 ng/ml

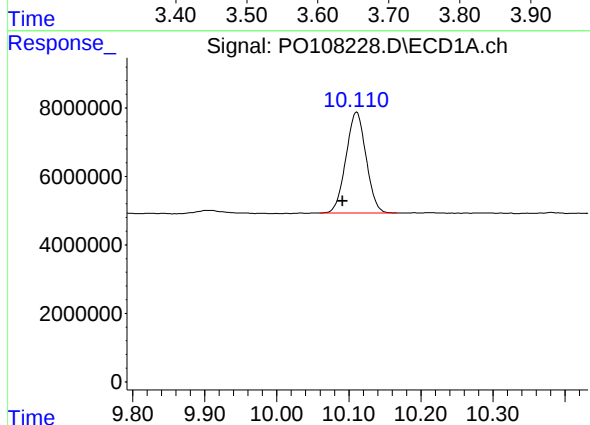

#2 Decachlorobiphenyl

R.T.: 10.110 min
Delta R.T.: 0.019 min
Response: 57240523
Conc: 18.74 ng/ml m

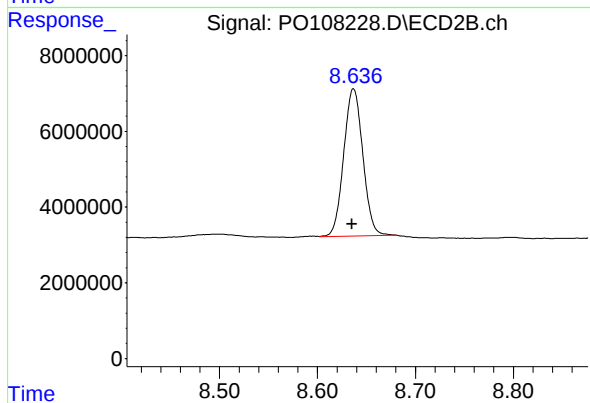

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: 0.001 min
Response: 52601582
Conc: 15.46 ng/ml